

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042700.D
 Acq On : 29 Jul 2024 18:56
 Operator : JC/MD
 Sample : P3328-16ME 20X
 Misc : 7.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20L9ME

Quant Time: Jul 30 01:12:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jul 30 00:49:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	153839	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	135441	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	50547	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	35750	38.251	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	76.500%		
7) Chloroethane-d5	1.648	69	17108	44.421	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.840%		
11) 1,1-Dichloroethene-d2	2.294	65	19283	41.874	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.740%		
21) 2-Butanone-d5	4.464	46	84293	121.686	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	121.690%		
24) Chloroform-d	5.056	84	104370	51.019	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	102.040%		
26) 1,2-Dichloroethane-d4	5.952	65	74101	56.146	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	112.300%		
32) Benzene-d6	5.970	84	197137	52.445	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	104.880%		
36) 1,2-Dichloropropane-d6	7.311	67	64201	57.709	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	115.420%		
41) Toluene-d8	8.647	98	163995	48.659	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.320%		
43) trans-1,3-Dichloroprop...	8.951	79	23994	46.088	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.180%		
47) 2-Hexanone-d5	9.390	63	58807	118.229	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	118.230%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	91903	57.375	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	114.740%		
66) 1,2-Dichlorobenzene-d4	12.323	152	54806	57.372	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	114.740%		
Target Compounds						Qvalue
34) Trichloroethene	7.129	95	7728	6.979	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042700.D
Acq On : 29 Jul 2024 18:56
Operator : JC/MD
Sample : P3328-16ME 20X
Misc : 7.48g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20L9ME

Quant Time: Jul 30 01:12:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jul 30 00:49:01 2024
Response via : Initial Calibration

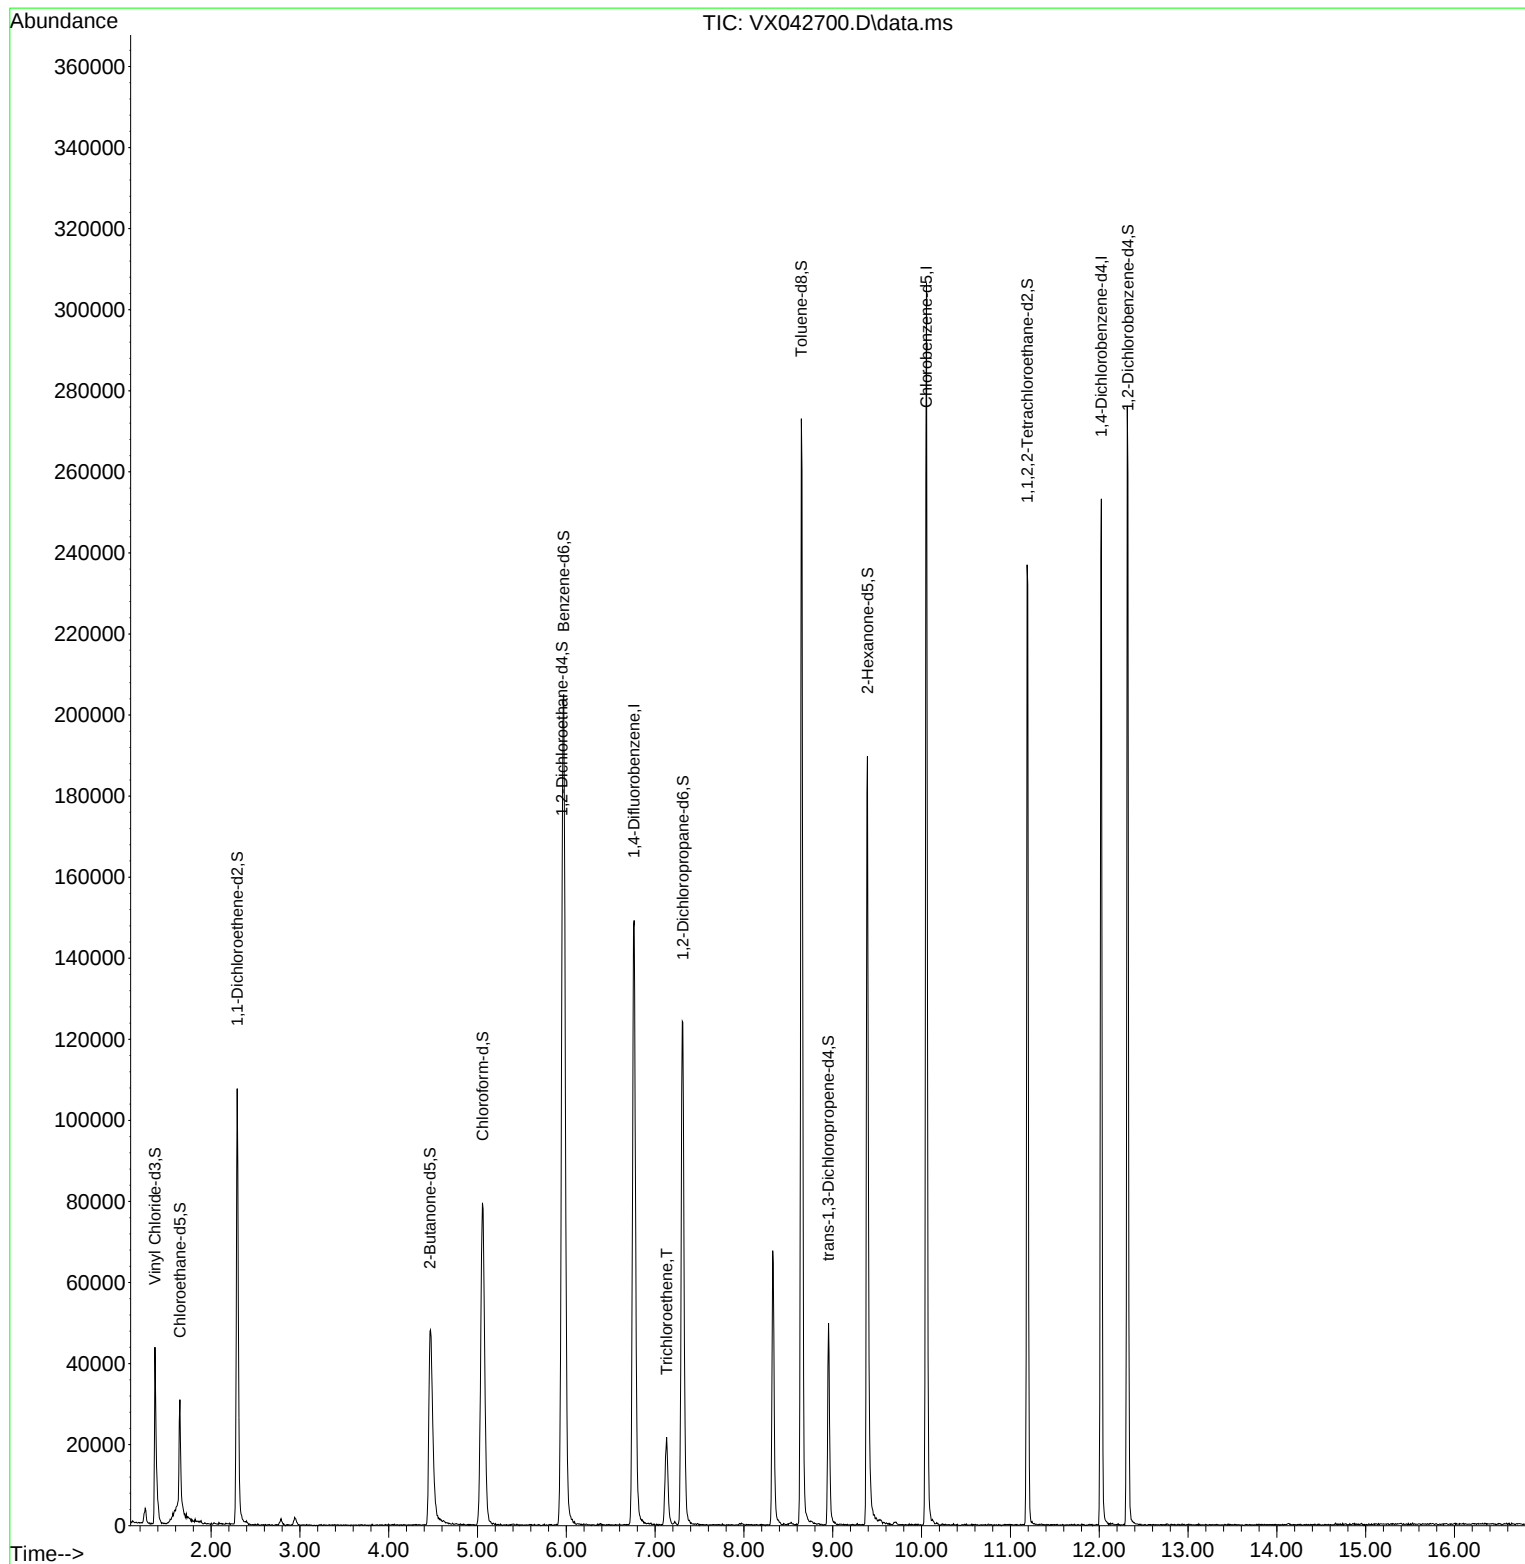

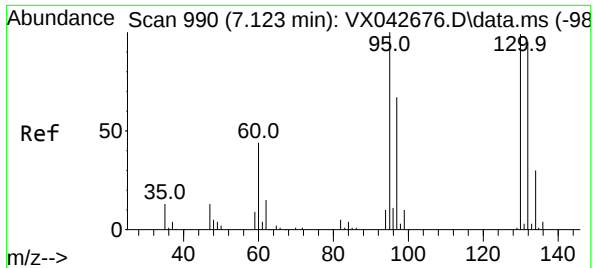

#34
 Trichloroethene
 Concen: 6.979 ug/L
 RT: 7.129 min Scan# 991
 Delta R.T. 0.006 min
 Lab File: VX042700.D
 Acq: 29 Jul 2024 18:56

Instrument :
 MSVOA_X
 ClientSampleId :
 E20L9ME

Tgt Ion: 95 Resp: 7728

Ion	Ratio	Lower	Upper
95	100		
97	58.7	46.3	86.1
132	87.1	64.3	119.5
130	90.9	67.0	124.4

