

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042681.D
 Acq On : 29 Jul 2024 11:38
 Operator : JC/MD
 Sample : P3370-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042681.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	17	rVB2	2353	3023	0.46%	0.061%
2	1.264	24	29	32	rBV3	3113	4874	0.74%	0.099%
3	1.368	43	46	57	rVB	55113	73061	11.13%	1.479%
4	1.447	57	59	62	rBV3	926	949	0.14%	0.019%
5	1.648	88	92	101	rVB	31667	47209	7.19%	0.956%
6	2.203	180	183	186	rBV3	440	740	0.11%	0.015%
7	2.294	193	198	209	rBV	127877	204179	31.11%	4.134%
8	2.508	229	233	237	rVB2	471	812	0.12%	0.016%
9	2.556	237	241	242	rBV2	266	384	0.06%	0.008%
10	2.617	250	251	253	rBV2	282	244	0.04%	0.005%
11	2.782	274	278	279	rBV	1117	1034	0.16%	0.021%
12	2.940	299	304	308	rBV2	1086	1931	0.29%	0.039%
13	3.117	330	333	336	rBB2	243	235	0.04%	0.005%
14	3.142	336	337	339	rBV2	241	241	0.04%	0.005%
15	3.355	369	372	374	rBV	258	238	0.04%	0.005%
16	3.434	380	385	391	rBV3	558	1033	0.16%	0.021%
17	3.501	394	396	399	rBV	245	318	0.05%	0.006%
18	3.702	426	429	430	rBV	215	228	0.03%	0.005%
19	3.788	440	443	445	rVB	243	293	0.04%	0.006%
20	3.831	445	450	453	rBV2	204	350	0.05%	0.007%
21	3.916	462	464	467	rBV2	195	244	0.04%	0.005%
22	4.123	496	498	504	rBV	231	253	0.04%	0.005%
23	4.465	546	554	572	rBV	49078	149425	22.77%	3.026%
24	4.934	627	631	636	rVB2	241	486	0.07%	0.010%
25	5.056	636	651	665	rBV2	87189	273187	41.62%	5.531%
26	5.312	690	693	695	rBV2	243	386	0.06%	0.008%
27	5.385	701	705	707	rBV3	487	745	0.11%	0.015%
28	5.556	729	733	734	rBV3	788	924	0.14%	0.019%
29	5.818	773	776	780	rVB2	236	327	0.05%	0.007%
30	5.964	790	800	820	rBV2	222767	656369	100.00%	13.290%
31	6.543	892	895	896	rBV	331	255	0.04%	0.005%
32	6.757	921	930	946	rBV	184539	454414	69.23%	9.201%
33	6.934	957	959	962	rBV2	286	356	0.05%	0.007%
34	7.129	982	991	995	rBV6	1702	4049	0.62%	0.082%
35	7.196	1001	1002	1004	rBV	372	296	0.05%	0.006%
36	7.305	1011	1020	1032	rBV	133539	298603	45.49%	6.046%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042681.D
 Acq On : 29 Jul 2024 11:38
 Operator : JC/MD
 Sample : P3370-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.470	1045	1047	1050	rBV2	271	364	0.06%	0.007%
38	7.824	1100	1105	1114	rBV3	1771	3644	0.56%	0.074%
39	7.946	1123	1125	1129	rBV2	430	518	0.08%	0.010%
40	8.189	1161	1165	1167	rBV2	391	504	0.08%	0.010%
41	8.324	1181	1187	1199	rBV	80944	136849	20.85%	2.771%
42	8.494	1214	1215	1218	rBV	312	351	0.05%	0.007%
43	8.519	1218	1219	1222	rVB2	473	450	0.07%	0.009%
44	8.574	1227	1228	1231	rVB2	379	275	0.04%	0.006%
45	8.647	1234	1240	1250	rBV	313939	501364	76.38%	10.151%
46	8.952	1285	1290	1302	rVV	57802	87058	13.26%	1.763%
47	9.275	1339	1343	1348	rVV2	1546	2125	0.32%	0.043%
48	9.384	1356	1361	1380	rBV	213221	316683	48.25%	6.412%
49	9.519	1380	1383	1392	rVB3	4889	9264	1.41%	0.188%
50	9.836	1432	1435	1437	rVB2	238	257	0.04%	0.005%
51	9.915	1446	1448	1451	rBV	152	236	0.04%	0.005%
52	10.055	1465	1471	1490	rVV	381786	517307	78.81%	10.474%
53	10.256	1501	1504	1505	rBV3	258	252	0.04%	0.005%
54	10.311	1510	1513	1516	rVB2	593	896	0.14%	0.018%
55	10.640	1562	1567	1575	rBV	27977	39333	5.99%	0.796%
56	10.732	1580	1582	1584	rVV2	412	342	0.05%	0.007%
57	10.756	1584	1586	1588	rVB	401	288	0.04%	0.006%
58	10.799	1590	1593	1599	rVB4	1974	3062	0.47%	0.062%
59	10.884	1604	1607	1610	rBV2	262	353	0.05%	0.007%
60	10.957	1617	1619	1624	rVB3	395	652	0.10%	0.013%
61	11.067	1636	1637	1640	rBV3	354	315	0.05%	0.006%
62	11.189	1652	1657	1667	rBV	247412	321818	49.03%	6.516%
63	11.311	1673	1677	1681	rVB4	682	1230	0.19%	0.025%
64	11.512	1708	1710	1714	rVB2	238	308	0.05%	0.006%
65	11.561	1714	1718	1719	rBV	297	358	0.05%	0.007%
66	11.640	1729	1731	1735	rBV2	165	246	0.04%	0.005%
67	11.677	1735	1737	1739	rVV	240	251	0.04%	0.005%
68	11.719	1742	1744	1747	rVV2	235	240	0.04%	0.005%
69	11.823	1756	1761	1766	rBV2	406	655	0.10%	0.013%
70	11.939	1777	1780	1783	rVB4	1102	1269	0.19%	0.026%
71	12.024	1788	1794	1805	rBV	314189	407503	62.08%	8.251%
72	12.225	1823	1827	1830	rBV3	894	1261	0.19%	0.026%
73	12.317	1837	1842	1859	rBV	308074	388726	59.22%	7.871%
74	12.701	1903	1905	1908	rVB	240	224	0.03%	0.005%
75	12.737	1908	1911	1912	rBV2	231	251	0.04%	0.005%
76	12.811	1919	1923	1924	rVB	325	300	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042681.D
 Acq On : 29 Jul 2024 11:38
 Operator : JC/MD
 Sample : P3370-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.859	1928	1931	1938	rVB3	1591	2468	0.38%	0.050%
78	12.920	1940	1941	1944	rVB	347	241	0.04%	0.005%
79	13.182	1983	1984	1987	rBV2	324	233	0.04%	0.005%
80	13.560	2043	2046	2048	rBV	284	331	0.05%	0.007%
81	13.597	2048	2052	2053	rBV2	244	295	0.04%	0.006%
82	13.652	2058	2061	2062	rBV	206	221	0.03%	0.004%
83	13.756	2075	2078	2079	rBV	308	286	0.04%	0.006%
84	13.780	2080	2082	2085	rVB2	308	301	0.05%	0.006%
85	13.932	2105	2107	2110	rBV2	244	228	0.03%	0.005%
86	13.999	2117	2118	2121	rBV	340	422	0.06%	0.009%
87	14.054	2124	2127	2130	rBV2	234	303	0.05%	0.006%
88	14.085	2130	2132	2135	rBV	267	290	0.04%	0.006%
89	14.121	2137	2138	2141	rVV	554	565	0.09%	0.011%
90	14.213	2150	2153	2157	rBV2	223	426	0.06%	0.009%
91	14.560	2208	2210	2213	rBV2	191	223	0.03%	0.005%
92	14.633	2220	2222	2225	rVV	235	248	0.04%	0.005%
93	14.841	2254	2256	2258	rVB	532	409	0.06%	0.008%
94	14.865	2258	2260	2261	rBV	393	299	0.05%	0.006%
95	14.883	2261	2263	2266	rVV	311	263	0.04%	0.005%
96	14.914	2266	2268	2272	rVV2	299	321	0.05%	0.006%
97	15.219	2316	2318	2321	rBV2	263	336	0.05%	0.007%
98	15.444	2353	2355	2360	rBV3	314	511	0.08%	0.010%
99	15.664	2390	2391	2393	rBV	293	304	0.05%	0.006%
100	16.462	2520	2522	2524	rBV2	315	239	0.04%	0.005%

Sum of corrected areas: 4938840




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042681.D
Acq On : 29 Jul 2024 11:38
Operator : JC/MD
Sample : P3370-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

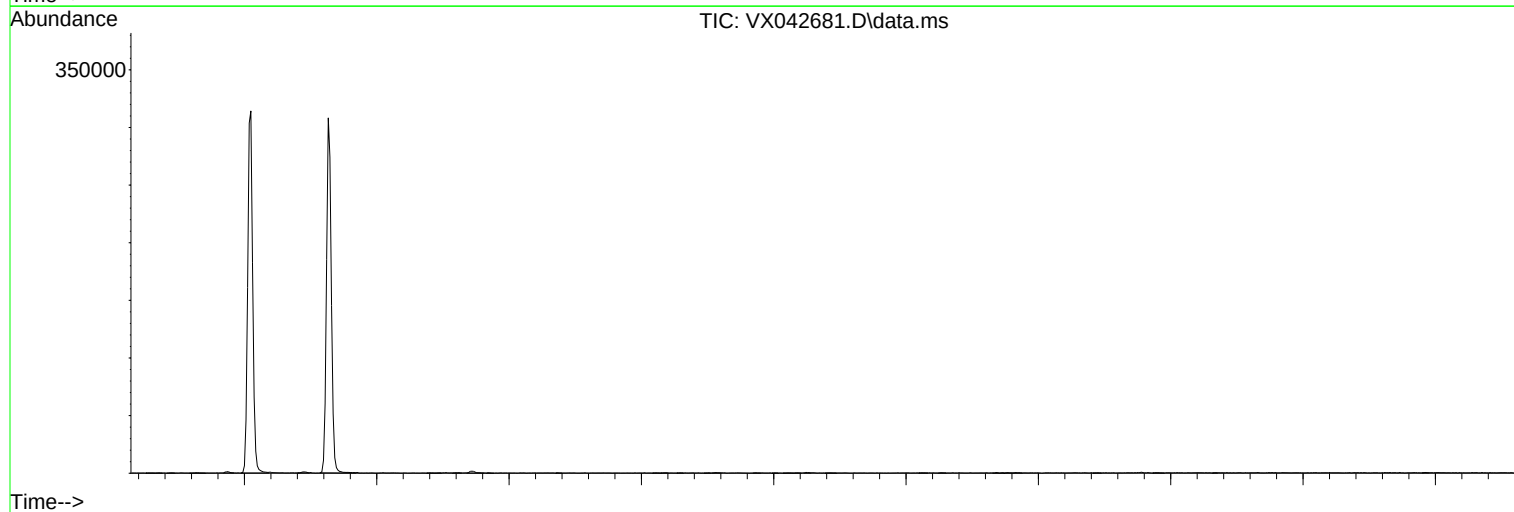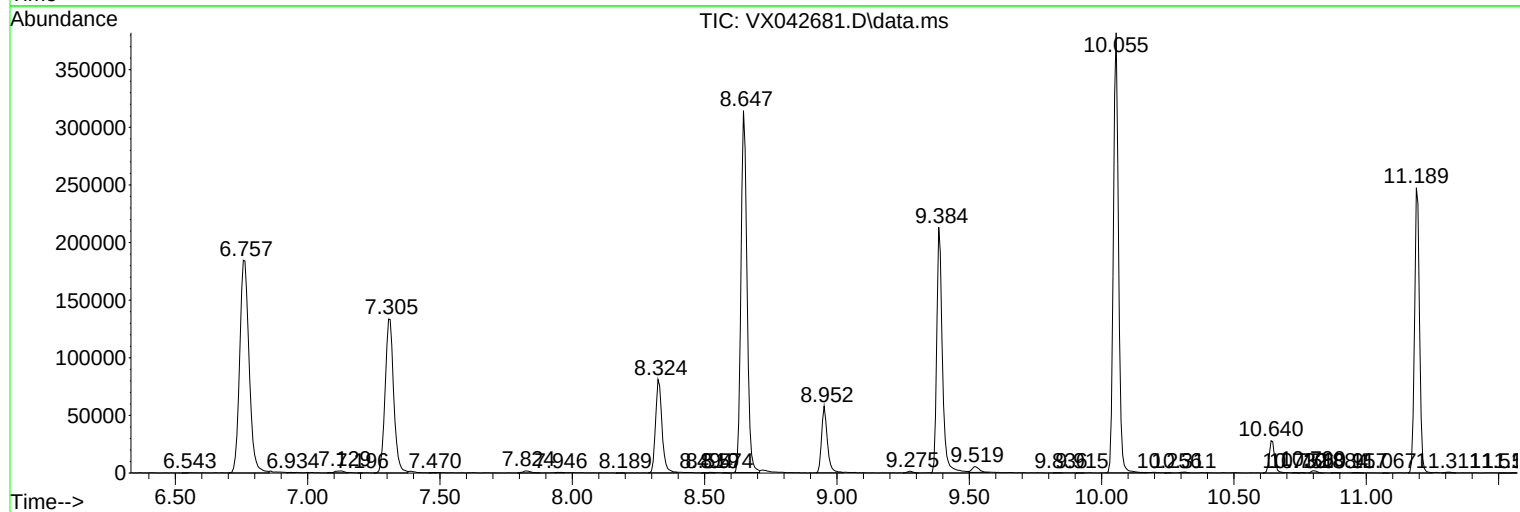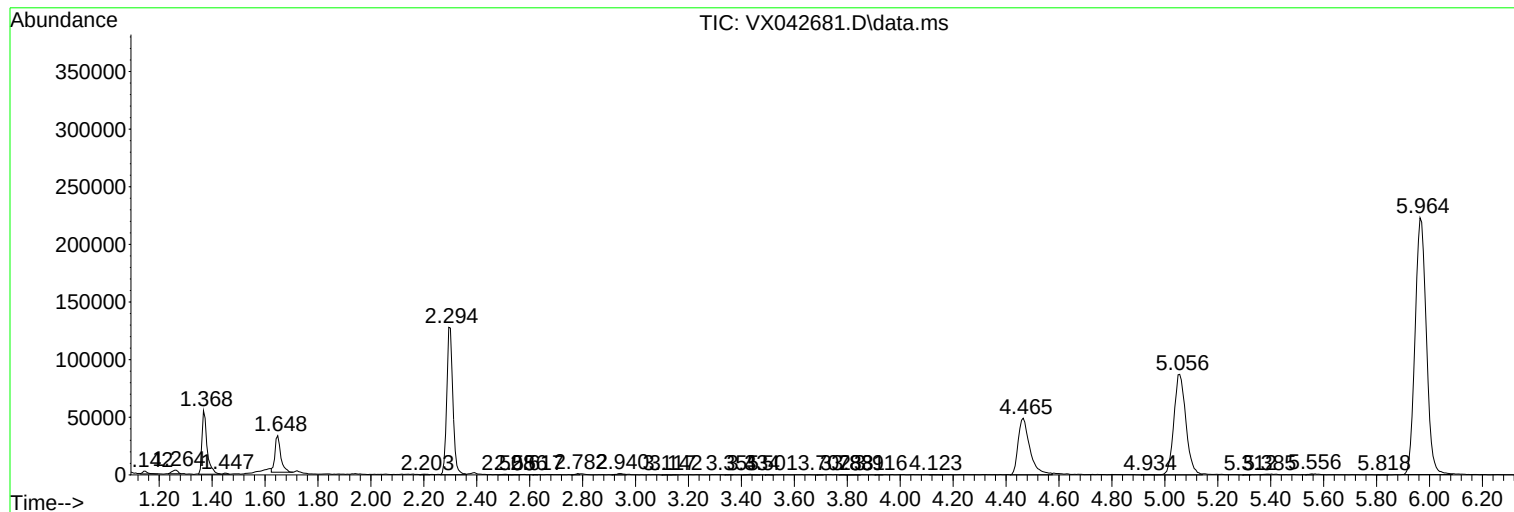

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042681.D
Acq On : 29 Jul 2024 11:38
Operator : JC/MD
Sample : P3370-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042681.D
Acq On : 29 Jul 2024 11:38
Operator : JC/MD
Sample : P3370-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc