

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042682.D
 Acq On : 29 Jul 2024 12:01
 Operator : JC/MD
 Sample : P3388-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042682.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	23	28	34	rVB3	3077	5233	0.82%	0.116%
2	1.368	43	46	59	rBV	50692	67351	10.51%	1.498%
3	1.648	88	92	101	rVB	33401	45614	7.11%	1.014%
4	2.294	192	198	209	rBV	121586	194994	30.41%	4.336%
5	2.386	211	213	218	rVB	1747	2224	0.35%	0.049%
6	2.496	228	231	235	rBV2	423	547	0.09%	0.012%
7	2.593	245	247	252	rVB2	204	293	0.05%	0.007%
8	2.660	256	258	260	rBV	274	234	0.04%	0.005%
9	2.776	276	277	279	rBV2	603	453	0.07%	0.010%
10	2.794	279	280	282	rVB	528	264	0.04%	0.006%
11	2.947	299	305	309	rBV4	955	1957	0.31%	0.044%
12	3.087	322	328	333	rBV3	541	1059	0.17%	0.024%
13	3.160	336	340	343	rVB2	185	296	0.05%	0.007%
14	3.367	373	374	376	rBV2	278	242	0.04%	0.005%
15	3.514	395	398	401	rBV	204	243	0.04%	0.005%
16	3.697	424	428	432	rBV2	194	243	0.04%	0.005%
17	3.758	432	438	441	rBV	230	319	0.05%	0.007%
18	3.886	456	459	461	rBB	280	317	0.05%	0.007%
19	3.922	461	465	467	rBV2	319	471	0.07%	0.010%
20	3.983	471	475	479	rBB2	250	493	0.08%	0.011%
21	4.257	516	520	521	rBV2	194	237	0.04%	0.005%
22	4.312	527	529	532	rVB	283	304	0.05%	0.007%
23	4.361	535	537	539	rBV	221	223	0.03%	0.005%
24	4.465	546	554	571	rBV2	48089	140980	21.99%	3.135%
25	4.702	591	593	597	rVB2	365	341	0.05%	0.008%
26	4.891	622	624	626	rBV2	231	224	0.03%	0.005%
27	5.056	640	651	669	rBV	83201	265455	41.40%	5.903%
28	5.269	682	686	687	rBV2	329	367	0.06%	0.008%
29	5.282	687	688	691	rVB	365	254	0.04%	0.006%
30	5.337	695	697	700	rBV	257	324	0.05%	0.007%
31	5.397	700	707	709	rBV	686	1255	0.20%	0.028%
32	5.465	716	718	722	rBV2	285	324	0.05%	0.007%
33	5.556	729	733	734	rBV2	439	616	0.10%	0.014%
34	5.964	789	800	817	rBV2	216531	641122	100.00%	14.258%
35	6.117	823	825	826	rVB2	593	323	0.05%	0.007%
36	6.135	826	828	830	rBV2	361	306	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042682.D
 Acq On : 29 Jul 2024 12:01
 Operator : JC/MD
 Sample : P3388-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.507	887	889	893	rVB2	311	441	0.07%	0.010%
38	6.763	921	931	944	rBV	147891	360220	56.19%	8.011%
39	6.897	951	953	959	rVV3	461	583	0.09%	0.013%
40	6.970	963	965	966	rBV	397	309	0.05%	0.007%
41	7.117	983	989	997	rBV5	1830	4331	0.68%	0.096%
42	7.232	1006	1008	1012	rVB2	608	568	0.09%	0.013%
43	7.306	1012	1020	1039	rBV2	130018	291755	45.51%	6.488%
44	7.830	1102	1106	1109	rBV	466	693	0.11%	0.015%
45	7.897	1114	1117	1118	rBV	209	236	0.04%	0.005%
46	8.220	1167	1170	1171	rBV	177	214	0.03%	0.005%
47	8.238	1171	1173	1176	rVB2	251	236	0.04%	0.005%
48	8.324	1182	1187	1199	rBV	73985	129255	20.16%	2.875%
49	8.647	1234	1240	1249	rBV	300771	479715	74.82%	10.668%
50	8.952	1285	1290	1302	rBV	56540	85722	13.37%	1.906%
51	9.275	1339	1343	1352	rVB4	1232	2282	0.36%	0.051%
52	9.385	1356	1361	1374	rBV	199026	302164	47.13%	6.720%
53	9.622	1398	1400	1403	rVB2	321	330	0.05%	0.007%
54	9.842	1433	1436	1437	rBV	270	244	0.04%	0.005%
55	9.860	1437	1439	1440	rVB	412	215	0.03%	0.005%
56	10.055	1465	1471	1484	rBV	293673	414287	64.62%	9.213%
57	10.311	1508	1513	1518	rVB3	849	1681	0.26%	0.037%
58	10.531	1547	1549	1551	rBV2	193	227	0.04%	0.005%
59	10.647	1565	1568	1571	rVV2	831	1173	0.18%	0.026%
60	10.866	1602	1604	1607	rVB	358	289	0.05%	0.006%
61	10.915	1607	1612	1613	rBV2	263	407	0.06%	0.009%
62	11.189	1652	1657	1665	rBV	244281	317100	49.46%	7.052%
63	11.317	1674	1678	1681	rVB3	1055	1323	0.21%	0.029%
64	11.378	1685	1688	1689	rBV	222	237	0.04%	0.005%
65	11.415	1693	1694	1699	rBV2	149	215	0.03%	0.005%
66	11.451	1699	1700	1703	rBV	293	223	0.03%	0.005%
67	11.756	1748	1750	1755	rVB2	617	748	0.12%	0.017%
68	11.927	1774	1778	1779	rBV	215	300	0.05%	0.007%
69	11.969	1783	1785	1788	rBV2	181	222	0.03%	0.005%
70	12.024	1788	1794	1803	rBV	252074	327715	51.12%	7.288%
71	12.085	1803	1804	1806	rVB	509	250	0.04%	0.006%
72	12.158	1814	1816	1817	rVB	415	245	0.04%	0.005%
73	12.226	1823	1827	1832	rVB2	899	1303	0.20%	0.029%
74	12.268	1832	1834	1837	rBV2	235	271	0.04%	0.006%
75	12.317	1837	1842	1851	rBV	302318	385678	60.16%	8.577%
76	12.536	1876	1878	1880	rBV2	175	218	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042682.D
 Acq On : 29 Jul 2024 12:01
 Operator : JC/MD
 Sample : P3388-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.616	1889	1891	1894	rVB	211	220	0.03%	0.005%
78	13.055	1960	1963	1965	rBV2	246	286	0.04%	0.006%
79	13.103	1968	1971	1972	rVB2	284	240	0.04%	0.005%
80	13.177	1981	1983	1986	rVB2	287	269	0.04%	0.006%
81	13.225	1989	1991	1993	rBV	193	213	0.03%	0.005%
82	13.305	2003	2004	2007	rBV	327	306	0.05%	0.007%
83	13.725	2071	2073	2075	rBV2	210	241	0.04%	0.005%
84	13.780	2079	2082	2087	rVB2	280	482	0.08%	0.011%
85	13.859	2094	2095	2099	rBV	219	263	0.04%	0.006%
86	13.896	2099	2101	2105	rBV2	204	284	0.04%	0.006%
87	14.134	2137	2140	2142	rVB2	402	397	0.06%	0.009%
88	14.201	2150	2151	2153	rBV2	325	305	0.05%	0.007%
89	14.530	2203	2205	2206	rVB2	330	218	0.03%	0.005%
90	14.731	2236	2238	2240	rVB2	399	318	0.05%	0.007%
91	14.768	2240	2244	2248	rBV2	295	405	0.06%	0.009%
92	15.048	2287	2290	2292	rBV	336	357	0.06%	0.008%
93	15.390	2344	2346	2348	rVB2	642	468	0.07%	0.010%
94	15.542	2370	2371	2373	rBV	399	286	0.04%	0.006%
95	15.572	2374	2376	2378	rVV	316	256	0.04%	0.006%
96	15.829	2416	2418	2421	rBV2	333	361	0.06%	0.008%
97	15.999	2443	2446	2447	rBV	293	248	0.04%	0.006%
98	16.237	2483	2485	2486	rVB2	530	306	0.05%	0.007%
99	16.475	2521	2524	2525	rBV2	299	245	0.04%	0.005%
100	16.591	2541	2543	2546	rBV2	366	476	0.07%	0.011%


Sum of corrected areas: 4496577

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042682.D
Acq On : 29 Jul 2024 12:01
Operator : JC/MD
Sample : P3388-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

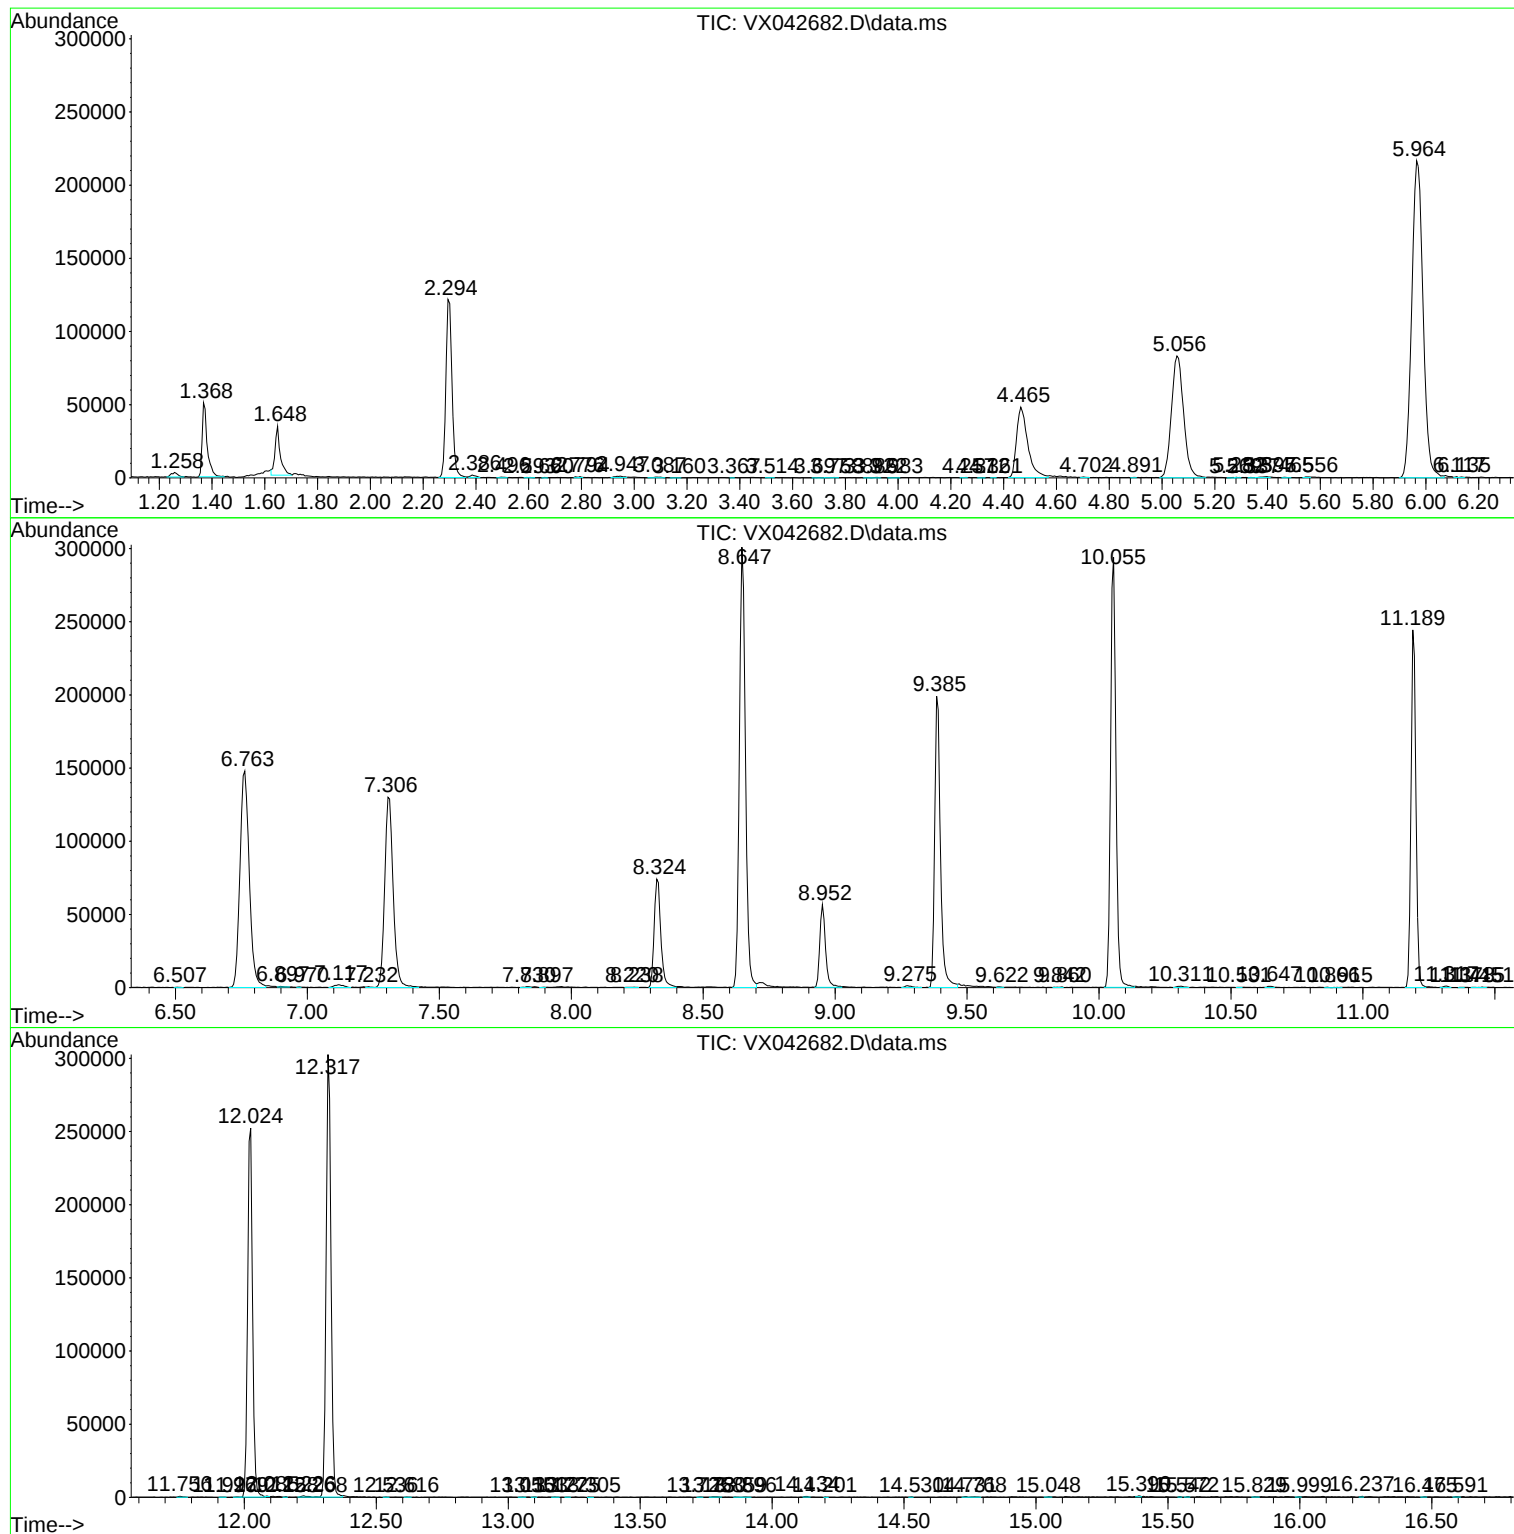

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042682.D
Acq On : 29 Jul 2024 12:01
Operator : JC/MD
Sample : P3388-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042682.D
Acq On : 29 Jul 2024 12:01
Operator : JC/MD
Sample : P3388-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc