

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042688.D
 Acq On : 29 Jul 2024 14:17
 Operator : JC/MD
 Sample : P3335-04DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20KODL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042688.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.251	23	27	33	rBV2	2884	4819	0.56%	0.090%
2	1.367	43	46	57	rBV	47297	65263	7.62%	1.216%
3	1.648	89	92	100	rVB	31076	40047	4.68%	0.746%
4	2.300	192	199	211	rBV	117799	191068	22.31%	3.561%
5	2.452	221	224	227	rBV	282	326	0.04%	0.006%
6	2.495	227	231	232	rVV	346	328	0.04%	0.006%
7	2.513	232	234	237	rVV2	171	220	0.03%	0.004%
8	2.739	270	271	274	rVB	447	344	0.04%	0.006%
9	2.788	274	279	288	rBV3	1877	4551	0.53%	0.085%
10	2.867	291	292	295	rBV	278	311	0.04%	0.006%
11	2.940	295	304	321	rVB	5515	13742	1.60%	0.256%
12	3.190	343	345	347	rVB	200	150	0.02%	0.003%
13	3.208	347	348	351	rBV	248	277	0.03%	0.005%
14	3.312	362	365	367	rVB	239	209	0.02%	0.004%
15	3.373	371	375	378	rBV2	286	502	0.06%	0.009%
16	3.483	391	393	396	rBV	187	192	0.02%	0.004%
17	3.635	416	418	420	rBV	204	171	0.02%	0.003%
18	3.769	438	440	441	rBV	227	175	0.02%	0.003%
19	4.038	479	484	485	rBV	204	317	0.04%	0.006%
20	4.086	489	492	493	rBV	290	325	0.04%	0.006%
21	4.227	513	515	517	rVV	189	189	0.02%	0.004%
22	4.361	534	537	539	rBV	198	184	0.02%	0.003%
23	4.470	546	555	570	rBV	48492	149950	17.51%	2.795%
24	5.056	639	651	665	rBV2	82718	258458	30.18%	4.817%
25	5.269	684	686	689	rVB	186	187	0.02%	0.003%
26	5.513	722	726	728	rBV	310	377	0.04%	0.007%
27	5.665	749	751	752	rVB	353	202	0.02%	0.004%
28	5.677	752	753	760	rVB2	245	439	0.05%	0.008%
29	5.757	760	766	767	rBV2	185	250	0.03%	0.005%
30	5.799	770	773	775	rBV2	226	276	0.03%	0.005%
31	5.964	789	800	820	rBV2	210032	630862	73.66%	11.758%
32	6.153	829	831	832	rBV2	240	180	0.02%	0.003%
33	6.214	839	841	844	rVB3	385	256	0.03%	0.005%
34	6.366	865	866	869	rVV	334	336	0.04%	0.006%
35	6.421	871	875	876	rBV2	212	287	0.03%	0.005%
36	6.513	887	890	892	rBV	217	282	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042688.D
 Acq On : 29 Jul 2024 14:17
 Operator : JC/MD
 Sample : P3335-04DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20KODL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.763	922	931	944	rBV	157668	379921	44.36%	7.081%
38	6.866	947	948	956	rVV	1230	1740	0.20%	0.032%
39	6.939	958	960	963	rBV2	410	423	0.05%	0.008%
40	7.049	977	978	981	rBV2	308	257	0.03%	0.005%
41	7.122	981	990	1012	rVV	388997	856436	100.00%	15.962%
42	7.305	1012	1020	1037	rVB	127577	290720	33.95%	5.418%
43	7.641	1072	1075	1076	rBV	244	206	0.02%	0.004%
44	7.671	1076	1080	1082	rVV2	170	186	0.02%	0.003%
45	7.775	1096	1097	1099	rBV	165	150	0.02%	0.003%
46	7.878	1112	1114	1118	rBV2	306	424	0.05%	0.008%
47	7.915	1118	1120	1123	rVV2	286	204	0.02%	0.004%
48	7.958	1125	1127	1131	rVV	430	600	0.07%	0.011%
49	8.098	1148	1150	1152	rBV	466	346	0.04%	0.006%
50	8.220	1168	1170	1172	rBV	191	181	0.02%	0.003%
51	8.323	1182	1187	1200	rBV	71310	125564	14.66%	2.340%
52	8.573	1226	1228	1230	rVB	202	144	0.02%	0.003%
53	8.646	1234	1240	1251	rBV	300612	474420	55.39%	8.842%
54	8.884	1277	1279	1282	rVB2	311	231	0.03%	0.004%
55	8.951	1285	1290	1306	rVV	54284	81980	9.57%	1.528%
56	9.274	1340	1343	1350	rVB3	2212	3291	0.38%	0.061%
57	9.384	1356	1361	1376	rBV	192392	304206	35.52%	5.670%
58	9.695	1411	1412	1417	rVB2	878	983	0.11%	0.018%
59	9.774	1423	1425	1430	rVB2	431	426	0.05%	0.008%
60	9.817	1430	1432	1434	rVB	191	171	0.02%	0.003%
61	9.921	1447	1449	1453	rBV2	225	370	0.04%	0.007%
62	10.006	1461	1463	1465	rBV	174	185	0.02%	0.003%
63	10.055	1465	1471	1483	rBV	319353	439562	51.32%	8.193%
64	10.408	1528	1529	1532	rBV2	176	207	0.02%	0.004%
65	10.475	1536	1540	1542	rBV2	168	225	0.03%	0.004%
66	10.536	1549	1550	1552	rBV	189	187	0.02%	0.003%
67	10.579	1555	1557	1558	rBV	191	157	0.02%	0.003%
68	10.591	1558	1559	1561	rVB	247	147	0.02%	0.003%
69	10.853	1601	1602	1604	rBV	230	151	0.02%	0.003%
70	10.890	1604	1608	1612	rVB2	238	489	0.06%	0.009%
71	11.189	1652	1657	1666	rBV	236449	310433	36.25%	5.786%
72	11.311	1675	1677	1678	rVB	283	150	0.02%	0.003%
73	11.463	1700	1702	1703	rBV	199	199	0.02%	0.004%
74	11.548	1713	1716	1718	rBV	223	257	0.03%	0.005%
75	11.615	1725	1727	1729	rBV	210	167	0.02%	0.003%
76	11.695	1738	1740	1743	rBV2	176	248	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042688.D
 Acq On : 29 Jul 2024 14:17
 Operator : JC/MD
 Sample : P3335-04DL 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20KODL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.762	1749	1751	1754	rBV2	216	167	0.02%	0.003%
78	11.859	1766	1767	1769	rBV2	265	208	0.02%	0.004%
79	12.024	1789	1794	1801	rBV	262880	342513	39.99%	6.384%
80	12.317	1837	1842	1853	rBV	284943	374457	43.72%	6.979%
81	12.506	1869	1873	1875	rBV	365	632	0.07%	0.012%
82	12.554	1879	1881	1883	rBV	189	182	0.02%	0.003%
83	12.621	1890	1892	1894	rVB	263	187	0.02%	0.003%
84	12.652	1894	1897	1898	rBV2	226	258	0.03%	0.005%
85	12.737	1907	1911	1912	rBV	151	207	0.02%	0.004%
86	13.097	1967	1970	1971	rBV2	295	306	0.04%	0.006%
87	13.133	1975	1976	1978	rVB	293	159	0.02%	0.003%
88	13.243	1991	1994	1995	rBV	227	285	0.03%	0.005%
89	13.664	2061	2063	2066	rBV2	167	156	0.02%	0.003%
90	14.042	2124	2125	2127	rBV	321	210	0.02%	0.004%
91	14.085	2130	2132	2134	rVV2	233	185	0.02%	0.003%
92	14.255	2157	2160	2162	rBV2	260	286	0.03%	0.005%
93	14.517	2200	2203	2204	rBV2	287	270	0.03%	0.005%
94	14.578	2212	2213	2215	rBV	168	158	0.02%	0.003%
95	14.865	2258	2260	2263	rBV2	286	303	0.04%	0.006%
96	15.078	2292	2295	2297	rBV2	283	373	0.04%	0.007%
97	15.426	2349	2352	2353	rBV	331	419	0.05%	0.008%
98	15.554	2371	2373	2374	rBV2	266	250	0.03%	0.005%
99	16.499	2527	2528	2531	rVB3	346	227	0.03%	0.004%
100	16.736	2561	2567	2568	rBV3	419	529	0.06%	0.010%




Sum of corrected areas: 5365323

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042688.D
Acq On : 29 Jul 2024 14:17
Operator : JC/MD
Sample : P3335-04DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20KODL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

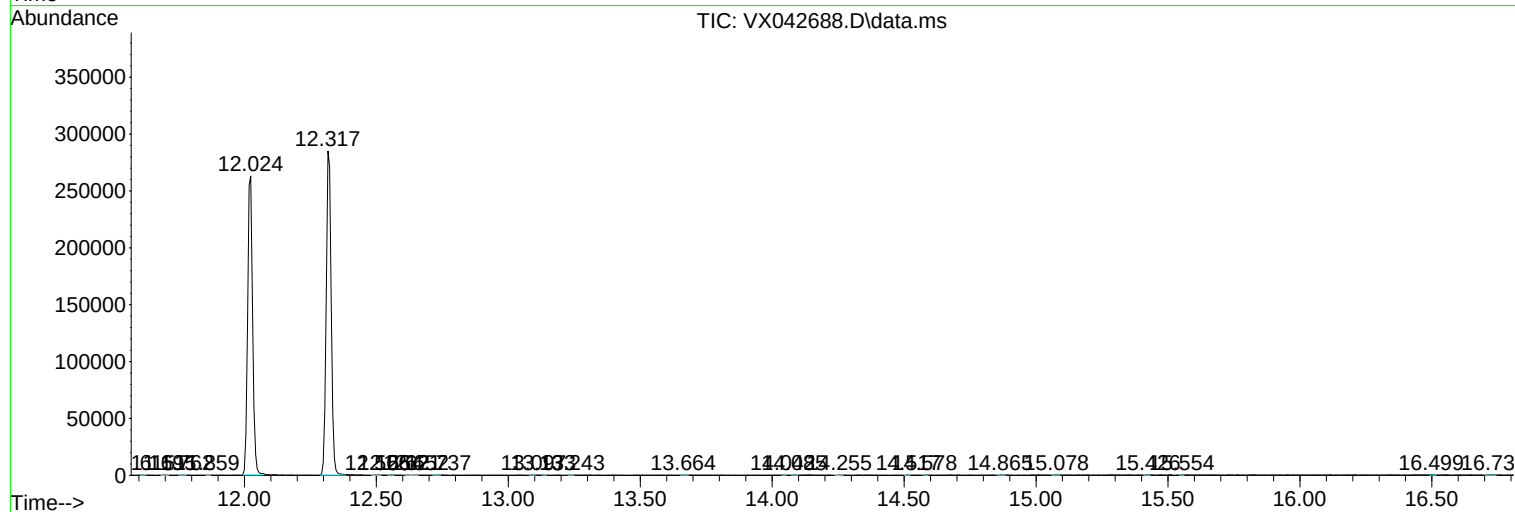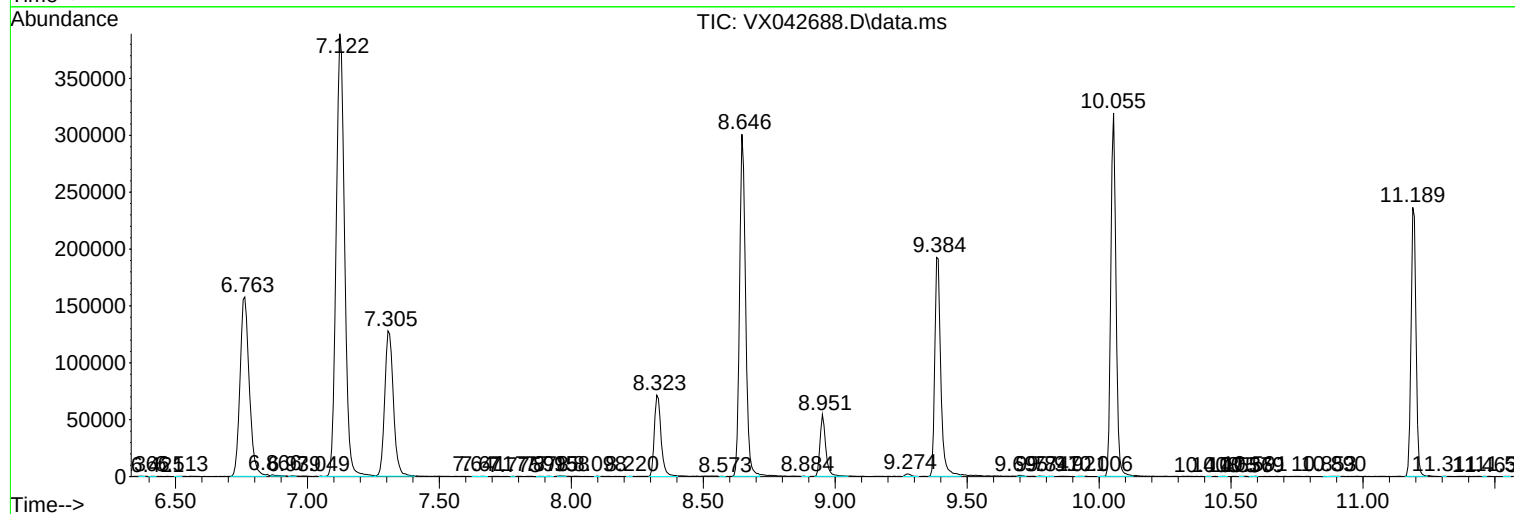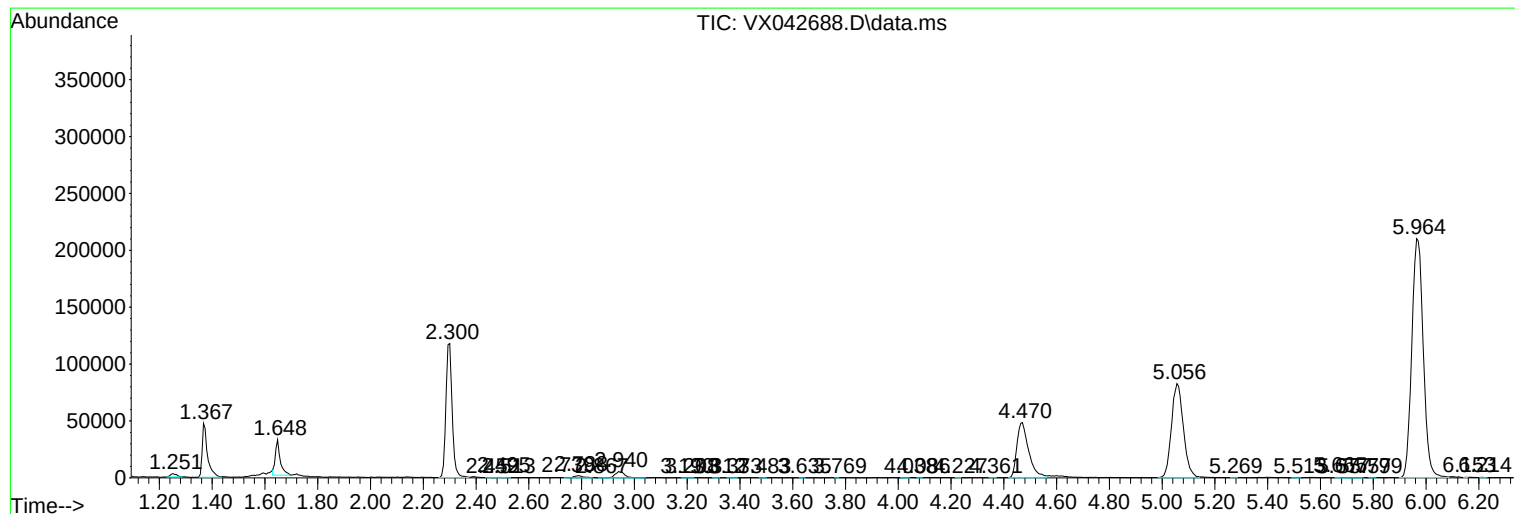

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042688.D
Acq On : 29 Jul 2024 14:17
Operator : JC/MD
Sample : P3335-04DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042688.D
Acq On : 29 Jul 2024 14:17
Operator : JC/MD
Sample : P3335-04DL 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc