

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042691.D
 Acq On : 29 Jul 2024 15:27
 Operator : JC/MD
 Sample : P3388-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	14	rBV3	1099	1398	0.22%	0.028%
2	1.264	23	29	34	rBV4	3877	6409	1.01%	0.128%
3	1.368	43	46	56	rBV	49865	63197	9.94%	1.265%
4	1.551	70	76	77	rBV2	1773	2230	0.35%	0.045%
5	1.648	88	92	100	rVB	29444	40584	6.39%	0.813%
6	1.874	126	129	130	rBV2	499	556	0.09%	0.011%
7	2.294	192	198	210	rBV	116624	187930	29.57%	3.763%
8	2.392	210	214	220	rVB5	1200	2812	0.44%	0.056%
9	2.441	220	222	224	rBV	301	411	0.06%	0.008%
10	2.563	239	242	243	rVB2	209	168	0.03%	0.003%
11	2.782	273	278	285	rBV4	1887	4279	0.67%	0.086%
12	2.849	287	289	291	rVB	355	238	0.04%	0.005%
13	2.947	294	305	313	rBV	4242	10152	1.60%	0.203%
14	3.087	324	328	334	rVB4	1190	2385	0.38%	0.048%
15	3.440	383	386	392	rBV	301	551	0.09%	0.011%
16	3.514	395	398	400	rBV2	265	352	0.06%	0.007%
17	3.593	410	411	414	rBV	323	317	0.05%	0.006%
18	3.660	420	422	426	rBV2	226	247	0.04%	0.005%
19	3.757	434	438	439	rVV	175	189	0.03%	0.004%
20	4.007	478	479	481	rBV	414	244	0.04%	0.005%
21	4.129	494	499	502	rBV2	212	383	0.06%	0.008%
22	4.471	545	555	572	rBV4	67968	230890	36.33%	4.623%
23	4.940	630	632	636	rBV2	219	278	0.04%	0.006%
24	5.056	640	651	666	rVV2	82848	259229	40.79%	5.191%
25	5.214	674	677	680	rVB3	582	759	0.12%	0.015%
26	5.263	680	685	687	rBV2	417	600	0.09%	0.012%
27	5.379	703	704	706	rBV2	323	256	0.04%	0.005%
28	5.440	710	714	718	rVB2	304	341	0.05%	0.007%
29	5.635	744	746	749	rBV	180	291	0.05%	0.006%
30	5.739	761	763	767	rBV	214	314	0.05%	0.006%
31	5.879	784	786	789	rBV2	230	256	0.04%	0.005%
32	5.970	789	801	817	rBV2	216739	635546	100.00%	12.726%
33	6.281	849	852	853	rBV2	195	174	0.03%	0.003%
34	6.483	883	885	888	rBV	231	350	0.06%	0.007%
35	6.763	922	931	945	rBV	165235	399149	62.80%	7.993%
36	6.964	962	964	965	rVV	331	179	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042691.D
 Acq On : 29 Jul 2024 15:27
 Operator : JC/MD
 Sample : P3388-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.989	966	968	971	rVB2	525	470	0.07%	0.009%
38	7.123	982	990	1002	rBV	154142	338706	53.29%	6.782%
39	7.306	1012	1020	1032	rBV	131540	291183	45.82%	5.831%
40	7.659	1075	1078	1080	rBV2	173	209	0.03%	0.004%
41	7.677	1080	1081	1086	rVV	288	269	0.04%	0.005%
42	7.958	1123	1127	1129	rVV2	564	693	0.11%	0.014%
43	8.147	1154	1158	1160	rBV2	216	335	0.05%	0.007%
44	8.208	1162	1168	1170	rBV2	215	372	0.06%	0.007%
45	8.324	1182	1187	1198	rBV	72379	124261	19.55%	2.488%
46	8.482	1211	1213	1214	rBV	265	161	0.03%	0.003%
47	8.519	1214	1219	1220	rBV2	388	541	0.09%	0.011%
48	8.647	1234	1240	1253	rBV	303868	474596	74.68%	9.503%
49	8.952	1285	1290	1304	rBV2	51232	82065	12.91%	1.643%
50	9.275	1342	1343	1346	rVB	373	299	0.05%	0.006%
51	9.330	1350	1352	1353	rVB	262	160	0.03%	0.003%
52	9.348	1353	1355	1356	rBV	268	260	0.04%	0.005%
53	9.384	1356	1361	1380	rBV	200379	313243	49.29%	6.272%
54	9.793	1426	1428	1429	rVB	481	215	0.03%	0.004%
55	9.811	1429	1431	1433	rBV	216	189	0.03%	0.004%
56	9.878	1440	1442	1444	rBV	199	236	0.04%	0.005%
57	10.055	1465	1471	1484	rBV	331971	458875	72.20%	9.189%
58	10.311	1510	1513	1515	rVB3	380	453	0.07%	0.009%
59	10.512	1544	1546	1550	rVB2	187	259	0.04%	0.005%
60	10.640	1565	1567	1569	rVB	248	230	0.04%	0.005%
61	10.872	1603	1605	1608	rBV	164	238	0.04%	0.005%
62	10.963	1618	1620	1625	rVB2	341	479	0.08%	0.010%
63	11.012	1625	1628	1629	rBV	295	246	0.04%	0.005%
64	11.043	1631	1633	1635	rVB2	288	228	0.04%	0.005%
65	11.189	1652	1657	1668	rVB	247360	316240	49.76%	6.332%
66	11.311	1675	1677	1678	rBV	239	193	0.03%	0.004%
67	11.780	1752	1754	1758	rBV2	201	183	0.03%	0.004%
68	11.847	1764	1765	1767	rBV	208	180	0.03%	0.004%
69	11.963	1781	1784	1788	rBV2	291	455	0.07%	0.009%
70	12.024	1788	1794	1805	rBV	277608	353042	55.55%	7.069%
71	12.219	1825	1826	1827	rBV	330	234	0.04%	0.005%
72	12.262	1830	1833	1836	rBV2	288	318	0.05%	0.006%
73	12.317	1837	1842	1857	rVB	280923	371881	58.51%	7.447%
74	12.646	1895	1896	1898	rVB2	360	182	0.03%	0.004%
75	12.738	1909	1911	1914	rBV2	185	194	0.03%	0.004%
76	13.128	1974	1975	1980	rBV2	283	230	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042691.D
 Acq On : 29 Jul 2024 15:27
 Operator : JC/MD
 Sample : P3388-07DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	13.164	1980	1981	1984	rVB	262	191	0.03%	0.004%
78	13.195	1984	1986	1988	rBV2	181	211	0.03%	0.004%
79	13.250	1993	1995	1997	rBV	385	365	0.06%	0.007%
80	13.439	2022	2026	2027	rBV2	200	296	0.05%	0.006%
81	13.554	2043	2045	2048	rBV2	223	246	0.04%	0.005%
82	13.750	2074	2077	2080	rBV2	308	431	0.07%	0.009%
83	13.774	2080	2081	2083	rBV2	168	161	0.03%	0.003%
84	13.878	2095	2098	2099	rBV2	363	394	0.06%	0.008%
85	13.981	2112	2115	2117	rBV	283	382	0.06%	0.008%
86	14.121	2136	2138	2145	rVB2	691	1062	0.17%	0.021%
87	14.762	2241	2243	2244	rBV	352	283	0.04%	0.006%
88	14.883	2261	2263	2264	rBV2	301	184	0.03%	0.004%
89	15.024	2285	2286	2287	rBV	417	176	0.03%	0.004%
90	15.042	2287	2289	2290	rVB	276	165	0.03%	0.003%
91	15.066	2292	2293	2296	rBV	228	210	0.03%	0.004%
92	15.097	2296	2298	2300	rBV	241	231	0.04%	0.005%
93	15.438	2352	2354	2355	rBV	216	160	0.03%	0.003%
94	15.457	2355	2357	2359	rVB2	297	244	0.04%	0.005%
95	15.609	2381	2382	2384	rBV2	281	228	0.04%	0.005%
96	15.810	2413	2415	2416	rBV2	296	236	0.04%	0.005%
97	15.950	2437	2438	2439	rBV	359	214	0.03%	0.004%
98	16.353	2502	2504	2509	rBV2	426	633	0.10%	0.013%
99	16.548	2535	2536	2539	rBV2	280	277	0.04%	0.006%
100	16.749	2567	2569	2573	rBV3	308	583	0.09%	0.012%




Sum of corrected areas: 4994010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042691.D
Acq On : 29 Jul 2024 15:27
Operator : JC/MD
Sample : P3388-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

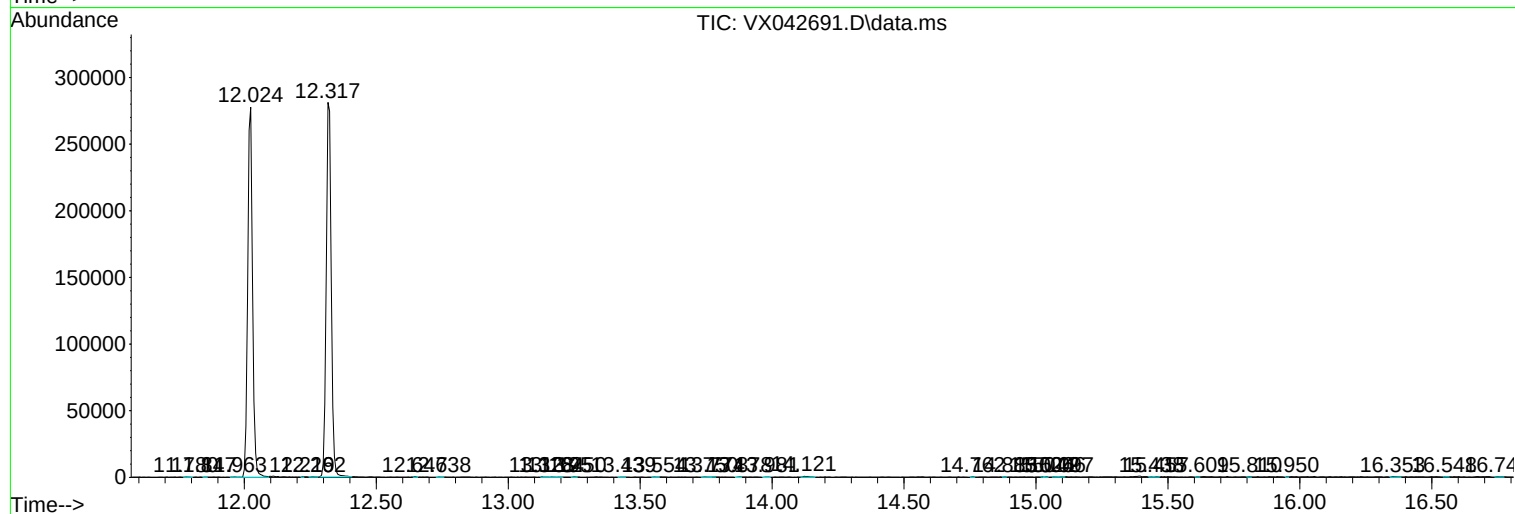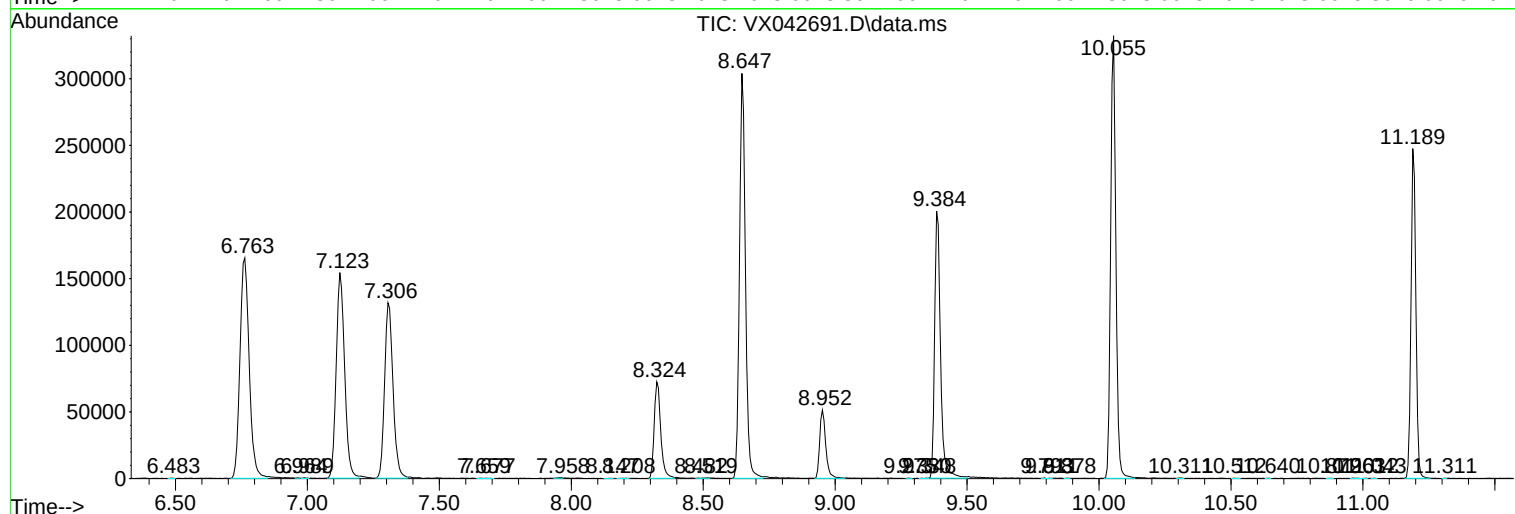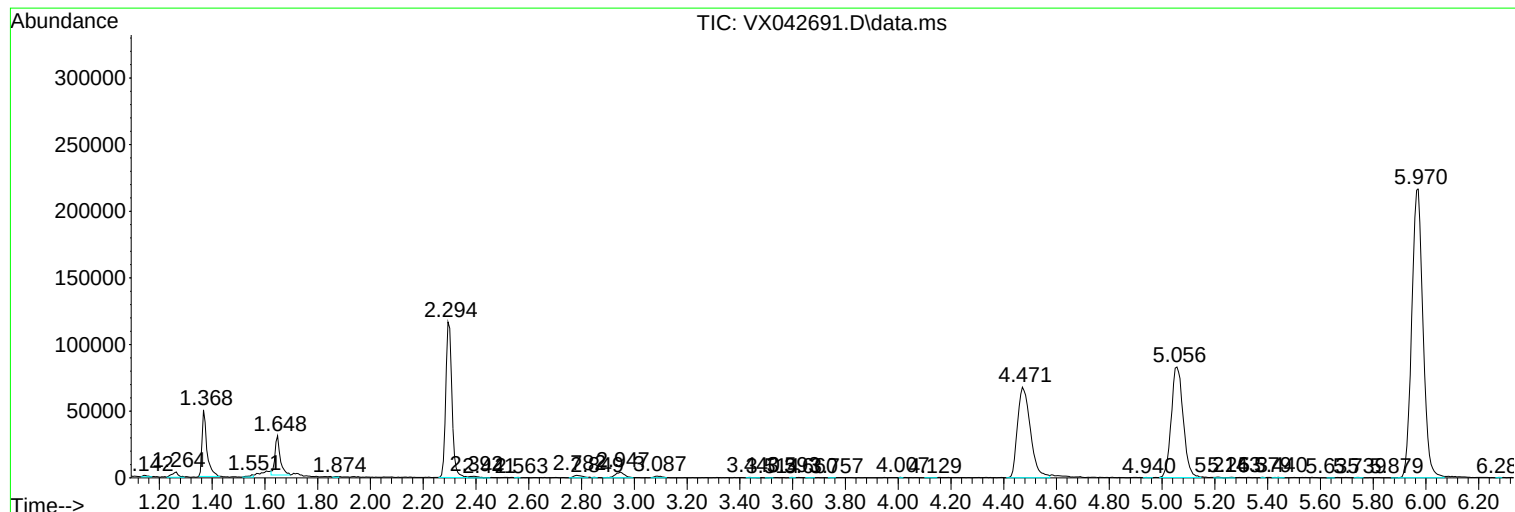

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042691.D
Acq On : 29 Jul 2024 15:27
Operator : JC/MD
Sample : P3388-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042691.D
Acq On : 29 Jul 2024 15:27
Operator : JC/MD
Sample : P3388-07DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------