

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042693.D
 Acq On : 29 Jul 2024 16:13
 Operator : JC/MD
 Sample : P3388-20DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	23	29	34	rBV3	3009	5417	0.89%	0.114%
2	1.368	42	46	57	rBV	46047	58682	9.61%	1.239%
3	1.648	89	92	101	rVB	26512	38614	6.33%	0.815%
4	1.819	118	120	123	rBV	441	499	0.08%	0.011%
5	2.185	178	180	182	rBV	389	385	0.06%	0.008%
6	2.300	192	199	211	rBV	108016	173562	28.43%	3.665%
7	2.386	211	213	219	rVB2	1214	1607	0.26%	0.034%
8	2.471	225	227	230	rBV2	264	269	0.04%	0.006%
9	2.496	230	231	234	rVB2	461	375	0.06%	0.008%
10	2.532	234	237	238	rBV	252	226	0.04%	0.005%
11	2.630	252	253	257	rBV	289	260	0.04%	0.005%
12	2.715	265	267	273	rVB2	241	466	0.08%	0.010%
13	2.782	273	278	285	rBV2	2819	5450	0.89%	0.115%
14	2.941	297	304	314	rVB	9031	20358	3.33%	0.430%
15	3.087	325	328	336	rVB2	765	1227	0.20%	0.026%
16	3.319	362	366	369	rBV	206	285	0.05%	0.006%
17	3.410	379	381	383	rVV2	207	225	0.04%	0.005%
18	3.581	406	409	411	rBV2	209	262	0.04%	0.006%
19	3.764	437	439	442	rBV2	152	204	0.03%	0.004%
20	3.892	457	460	463	rVB	204	209	0.03%	0.004%
21	3.959	469	471	475	rBV2	190	273	0.04%	0.006%
22	4.007	477	479	482	rBV2	163	189	0.03%	0.004%
23	4.044	482	485	487	rBV2	185	275	0.05%	0.006%
24	4.148	501	502	505	rVB	278	268	0.04%	0.006%
25	4.312	524	529	530	rBV2	246	341	0.06%	0.007%
26	4.471	546	555	568	rBV4	61043	195748	32.06%	4.133%
27	4.837	612	615	616	rBV2	233	272	0.04%	0.006%
28	5.056	638	651	668	rBV2	81225	249839	40.93%	5.276%
29	5.385	703	705	706	rBV	378	277	0.05%	0.006%
30	5.471	717	719	724	rVB2	213	333	0.05%	0.007%
31	5.519	724	727	729	rBV2	217	275	0.05%	0.006%
32	5.562	730	734	737	rVV2	381	649	0.11%	0.014%
33	5.635	744	746	750	rBV2	184	244	0.04%	0.005%
34	5.678	750	753	756	rVB2	263	319	0.05%	0.007%
35	5.714	756	759	760	rBV2	232	202	0.03%	0.004%
36	5.836	777	779	782	rVB2	179	195	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042693.D
 Acq On : 29 Jul 2024 16:13
 Operator : JC/MD
 Sample : P3388-20DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.971	789	801	819	rBV2	205586	610480	100.00%	12.891%
38	6.233	841	844	846	rBV2	293	267	0.04%	0.006%
39	6.385	866	869	871	rBV2	193	240	0.04%	0.005%
40	6.556	892	897	900	rBV	221	339	0.06%	0.007%
41	6.629	906	909	912	rBV	149	251	0.04%	0.005%
42	6.763	921	931	949	rBV	155494	378104	61.94%	7.984%
43	7.062	978	980	981	rBV	357	370	0.06%	0.008%
44	7.123	982	990	1009	rVV2	136900	297774	48.78%	6.288%
45	7.306	1012	1020	1034	rVV	123117	276587	45.31%	5.840%
46	7.556	1059	1061	1063	rVB	310	227	0.04%	0.005%
47	8.007	1133	1135	1137	rBV	261	222	0.04%	0.005%
48	8.324	1181	1187	1198	rBV	68608	118676	19.44%	2.506%
49	8.458	1207	1209	1212	rVB2	480	358	0.06%	0.008%
50	8.488	1212	1214	1215	rBV	409	304	0.05%	0.006%
51	8.568	1226	1227	1229	rVB	400	234	0.04%	0.005%
52	8.647	1234	1240	1258	rBV	280562	452399	74.11%	9.553%
53	8.952	1284	1290	1301	rBV	52590	78838	12.91%	1.665%
54	9.183	1326	1328	1332	rBV2	197	277	0.05%	0.006%
55	9.342	1350	1354	1356	rBV	306	390	0.06%	0.008%
56	9.385	1356	1361	1377	rBV	197607	299143	49.00%	6.317%
57	10.055	1465	1471	1484	rBV	314991	435276	71.30%	9.191%
58	10.201	1493	1495	1499	rBV4	494	523	0.09%	0.011%
59	10.372	1521	1523	1525	rBV	230	215	0.04%	0.005%
60	10.610	1559	1562	1564	rBV2	261	286	0.05%	0.006%
61	10.890	1602	1608	1610	rBV	329	610	0.10%	0.013%
62	11.122	1644	1646	1648	rBV	183	195	0.03%	0.004%
63	11.195	1652	1658	1672	rVB	241269	318241	52.13%	6.720%
64	11.335	1680	1681	1683	rVB	307	206	0.03%	0.004%
65	11.372	1683	1687	1692	rBV2	289	709	0.12%	0.015%
66	11.476	1701	1704	1706	rBV2	320	375	0.06%	0.008%
67	11.530	1711	1713	1715	rVB2	330	224	0.04%	0.005%
68	11.805	1755	1758	1761	rBV2	180	307	0.05%	0.006%
69	11.878	1765	1770	1771	rVB2	234	331	0.05%	0.007%
70	12.024	1788	1794	1801	rBV	257195	332455	54.46%	7.020%
71	12.225	1824	1827	1828	rBV2	445	377	0.06%	0.008%
72	12.317	1837	1842	1852	rBV	277360	362556	59.39%	7.656%
73	12.463	1865	1866	1868	rBV2	330	222	0.04%	0.005%
74	12.555	1879	1881	1884	rBV2	242	224	0.04%	0.005%
75	12.768	1914	1916	1919	rVB2	297	340	0.06%	0.007%
76	12.860	1929	1931	1933	rVV	373	232	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042693.D
 Acq On : 29 Jul 2024 16:13
 Operator : JC/MD
 Sample : P3388-20DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.927	1941	1942	1945	rBV2	225	247	0.04%	0.005%
78	13.426	2022	2024	2026	rVB	409	292	0.05%	0.006%
79	13.506	2035	2037	2041	rBV	178	265	0.04%	0.006%
80	13.591	2049	2051	2052	rVV	331	231	0.04%	0.005%
81	13.609	2052	2054	2056	rVB2	196	195	0.03%	0.004%
82	13.676	2063	2065	2066	rBV	388	263	0.04%	0.006%
83	13.841	2089	2092	2095	rBV2	216	303	0.05%	0.006%
84	14.024	2120	2122	2125	rVB2	248	221	0.04%	0.005%
85	14.128	2136	2139	2143	rVB2	819	1057	0.17%	0.022%
86	14.414	2184	2186	2187	rBV	207	180	0.03%	0.004%
87	14.725	2235	2237	2238	rVB2	342	205	0.03%	0.004%
88	14.749	2240	2241	2243	rBV2	228	175	0.03%	0.004%
89	14.768	2243	2244	2247	rBV3	326	264	0.04%	0.006%
90	15.103	2297	2299	2302	rBV2	352	434	0.07%	0.009%
91	15.219	2316	2318	2320	rBV2	251	285	0.05%	0.006%
92	15.255	2322	2324	2327	rVV3	317	315	0.05%	0.007%
93	15.286	2327	2329	2331	rVB2	295	230	0.04%	0.005%
94	15.396	2343	2347	2349	rBV4	552	819	0.13%	0.017%
95	15.786	2408	2411	2413	rBV2	337	395	0.06%	0.008%
96	15.865	2420	2424	2425	rVB2	276	274	0.04%	0.006%
97	15.914	2431	2432	2434	rVB2	408	268	0.04%	0.006%
98	16.206	2477	2480	2481	rBV2	477	392	0.06%	0.008%
99	16.450	2515	2520	2522	rBV3	411	614	0.10%	0.013%
100	16.609	2544	2546	2547	rVB	313	195	0.03%	0.004%




Sum of corrected areas: 4735784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042693.D
Acq On : 29 Jul 2024 16:13
Operator : JC/MD
Sample : P3388-20DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

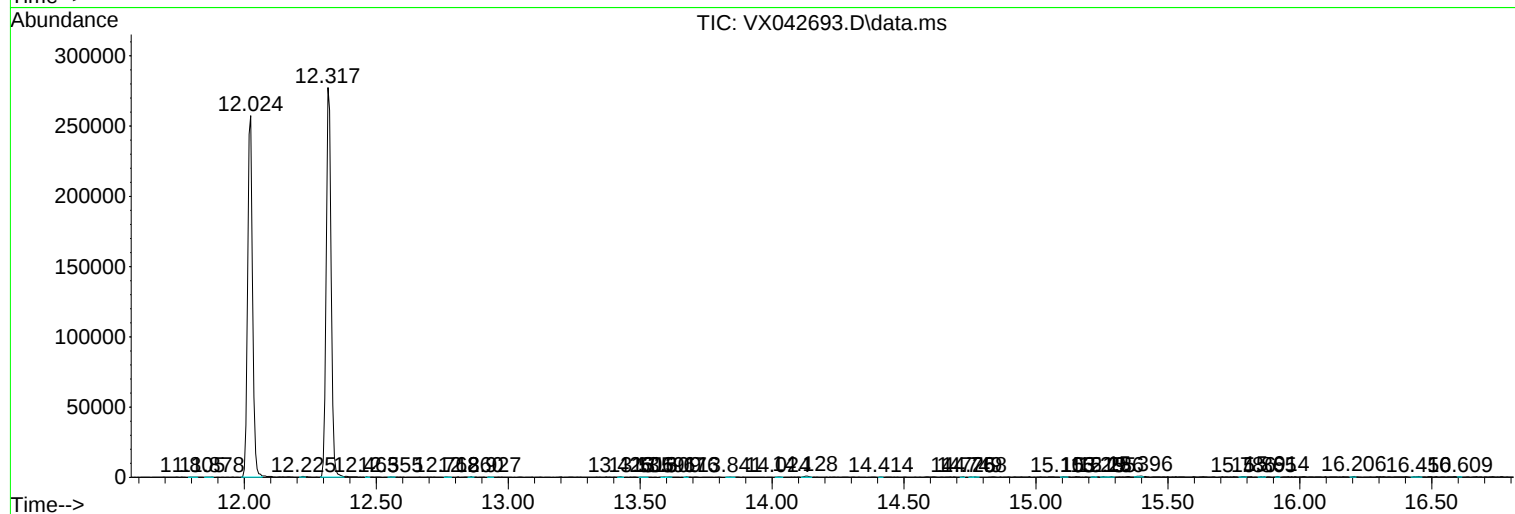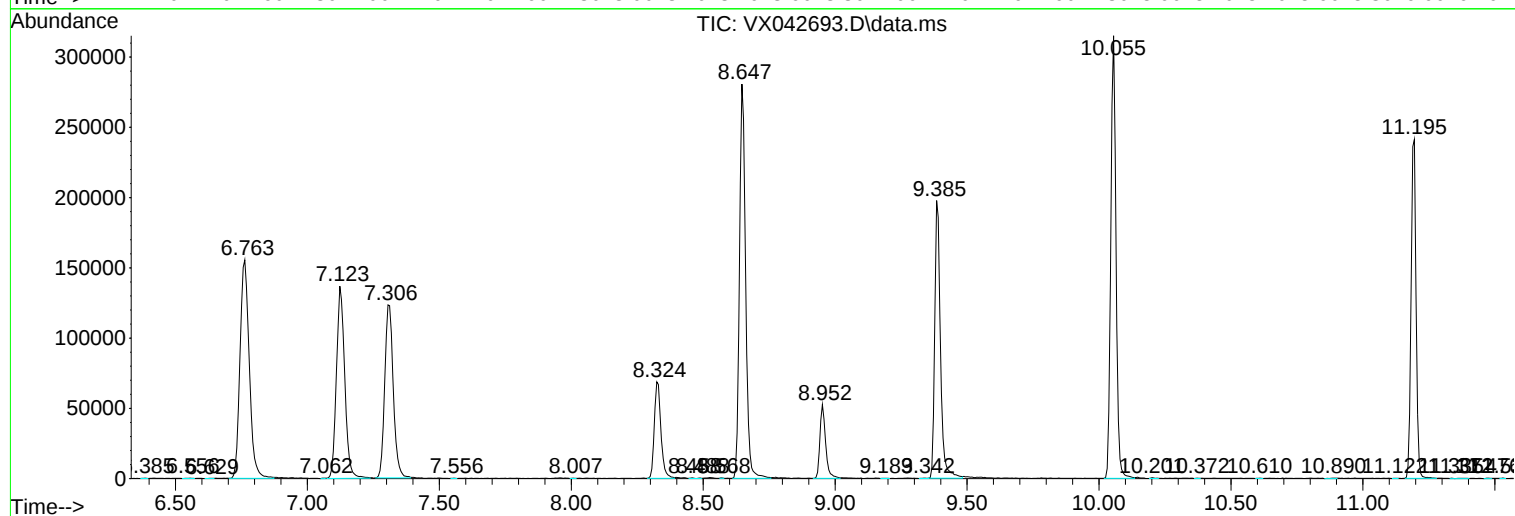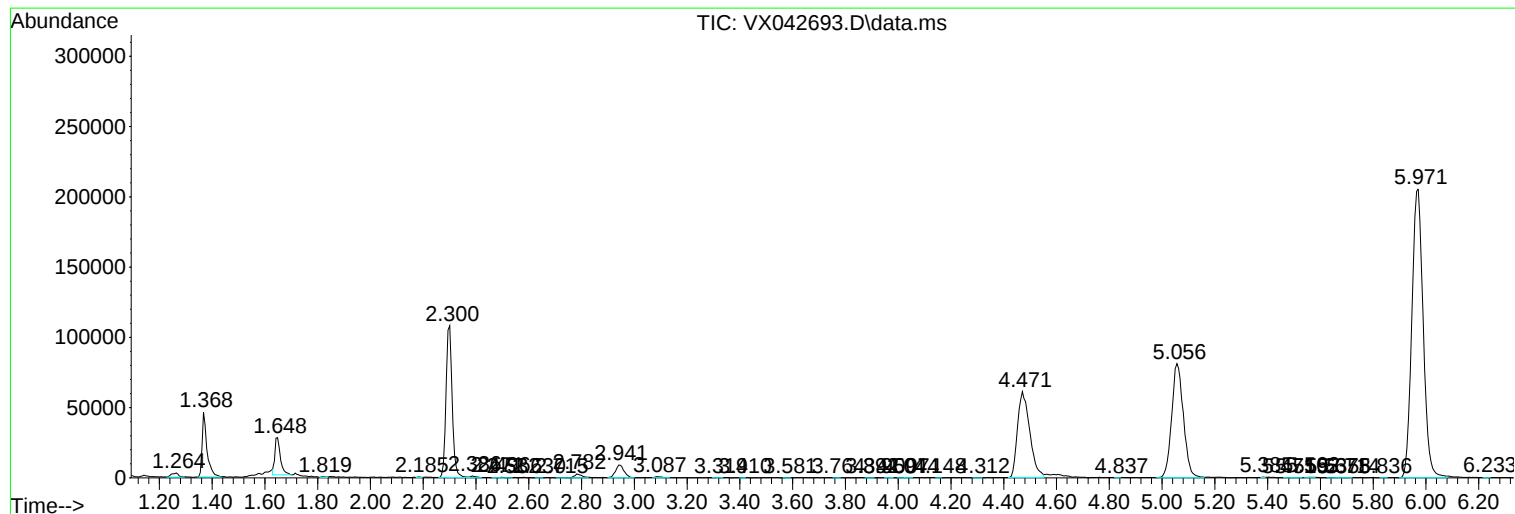

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042693.D
Acq On : 29 Jul 2024 16:13
Operator : JC/MD
Sample : P3388-20DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042693.D
Acq On : 29 Jul 2024 16:13
Operator : JC/MD
Sample : P3388-20DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------