

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042704.D
 Acq On : 29 Jul 2024 20:28
 Operator : JC/MD
 Sample : P3388-02DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042704.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rBV	37992	49179	9.06%	1.071%
2	1.648	89	92	101	rVB	30855	36307	6.69%	0.791%
3	2.032	153	155	157	rBV	440	417	0.08%	0.009%
4	2.056	157	159	163	rVV2	370	378	0.07%	0.008%
5	2.300	193	199	210	rBV	95131	149213	27.48%	3.249%
6	2.690	260	263	266	rBV	202	263	0.05%	0.006%
7	2.788	275	279	287	rBV3	2034	4483	0.83%	0.098%
8	2.861	289	291	293	rVB	430	255	0.05%	0.006%
9	2.886	293	295	296	rBV	239	163	0.03%	0.004%
10	2.953	298	306	312	rBV	5607	12371	2.28%	0.269%
11	3.038	318	320	322	rBV	161	184	0.03%	0.004%
12	3.215	347	349	353	rBV2	223	329	0.06%	0.007%
13	3.251	353	355	358	rVV	195	137	0.03%	0.003%
14	3.282	358	360	363	rBV	238	203	0.04%	0.004%
15	3.398	377	379	380	rVB	281	146	0.03%	0.003%
16	3.550	402	404	405	rBV	118	101	0.02%	0.002%
17	3.635	417	418	422	rBB	263	259	0.05%	0.006%
18	3.751	435	437	439	rBB	164	118	0.02%	0.003%
19	3.794	440	444	445	rBV	151	168	0.03%	0.004%
20	3.830	448	450	453	rVB	318	255	0.05%	0.006%
21	3.855	453	454	456	rBV	116	88	0.02%	0.002%
22	4.269	521	522	524	rBV	162	142	0.03%	0.003%
23	4.477	547	556	570	rBV	48091	156322	28.79%	3.404%
24	5.068	641	653	666	rBV	73713	219724	40.46%	4.785%
25	5.464	713	718	719	rBV	206	248	0.05%	0.005%
26	5.678	751	753	757	rVB2	187	164	0.03%	0.004%
27	5.745	762	764	767	rVB	181	208	0.04%	0.005%
28	5.787	767	771	773	rBB	274	309	0.06%	0.007%
29	5.824	774	777	779	rBV	154	195	0.04%	0.004%
30	5.976	790	802	824	rBV2	175062	518713	95.52%	11.295%
31	6.226	841	843	846	rBV2	332	333	0.06%	0.007%
32	6.385	866	869	873	rBV2	370	561	0.10%	0.012%
33	6.647	911	912	915	rVB	224	93	0.02%	0.002%
34	6.671	915	916	923	rBV2	159	297	0.05%	0.006%
35	6.769	923	932	948	rBV	162315	397470	73.20%	8.655%
36	7.007	969	971	973	rVB	301	223	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042704.D
 Acq On : 29 Jul 2024 20:28
 Operator : JC/MD
 Sample : P3388-02DL 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.025	973	974	977	rBV2	321	395	0.07%	0.009%
38	7.129	982	991	1006	rBV	248591	543026	100.00%	11.825%
39	7.312	1013	1021	1036	rBV	106521	238036	43.84%	5.183%
40	7.629	1069	1073	1074	rBV	225	210	0.04%	0.005%
41	7.683	1081	1082	1083	rBV	214	114	0.02%	0.002%
42	7.958	1124	1127	1129	rBV2	672	954	0.18%	0.021%
43	8.068	1144	1145	1146	rBV	229	137	0.03%	0.003%
44	8.214	1168	1169	1171	rBV	226	197	0.04%	0.004%
45	8.330	1182	1188	1196	rBV	60562	101248	18.65%	2.205%
46	8.653	1235	1241	1252	rBV	234189	379121	69.82%	8.256%
47	8.952	1285	1290	1299	rBV	39651	65075	11.98%	1.417%
48	9.208	1331	1332	1334	rBV	194	148	0.03%	0.003%
49	9.390	1357	1362	1373	rBV	177294	268552	49.45%	5.848%
50	9.701	1411	1413	1419	rVB3	1100	1474	0.27%	0.032%
51	9.756	1419	1422	1423	rBV2	200	199	0.04%	0.004%
52	9.805	1428	1430	1431	rBV	137	79	0.01%	0.002%
53	10.055	1465	1471	1483	rBV	339656	457936	84.33%	9.972%
54	10.305	1510	1512	1518	rVB3	440	634	0.12%	0.014%
55	10.354	1518	1520	1521	rBV	279	154	0.03%	0.003%
56	10.433	1531	1533	1536	rBV2	181	230	0.04%	0.005%
57	10.585	1557	1558	1560	rVB	141	101	0.02%	0.002%
58	10.963	1619	1620	1621	rBV	195	79	0.01%	0.002%
59	11.012	1626	1628	1629	rVB	220	109	0.02%	0.002%
60	11.195	1652	1658	1667	rBV	212537	284415	52.38%	6.193%
61	11.354	1681	1684	1686	rBV2	173	164	0.03%	0.004%
62	11.390	1686	1690	1694	rBV2	251	383	0.07%	0.008%
63	11.579	1720	1721	1722	rBV	128	82	0.02%	0.002%
64	11.610	1725	1726	1728	rBV	226	144	0.03%	0.003%
65	12.024	1789	1794	1806	rVB	280501	369986	68.13%	8.057%
66	12.256	1830	1832	1834	rVB	267	126	0.02%	0.003%
67	12.317	1837	1842	1854	rBV	245248	325518	59.95%	7.088%
68	12.597	1885	1888	1889	rBB	346	259	0.05%	0.006%
69	12.896	1934	1937	1939	rVB	261	350	0.06%	0.008%
70	12.932	1939	1943	1945	rBV2	223	337	0.06%	0.007%
71	13.018	1955	1957	1959	rBV	263	288	0.05%	0.006%
72	13.128	1973	1975	1978	rVB2	294	213	0.04%	0.005%
73	13.237	1991	1993	1995	rBV	165	131	0.02%	0.003%
74	13.256	1995	1996	1997	rBV	232	107	0.02%	0.002%
75	13.378	2015	2016	2017	rBV	204	80	0.01%	0.002%
76	13.664	2061	2063	2065	rBV	139	82	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042704.D
Acq On : 29 Jul 2024 20:28
Operator : JC/MD
Sample : P3388-02DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

77	13.682	2065	2066	2067	rVB	297	109	0.02%	0.002%
78	14.182	2146	2148	2151	rBV2	264	401	0.07%	0.009%
79	14.383	2178	2181	2182	rBV2	176	154	0.03%	0.003%
80	14.469	2192	2195	2196	rBV	209	229	0.04%	0.005%
81	14.585	2212	2214	2218	rVB3	259	214	0.04%	0.005%
82	14.707	2233	2234	2235	rBV3	332	198	0.04%	0.004%
83	15.335	2336	2337	2338	rBV	335	143	0.03%	0.003%




Sum of corrected areas: 4592340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042704.D
Acq On : 29 Jul 2024 20:28
Operator : JC/MD
Sample : P3388-02DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

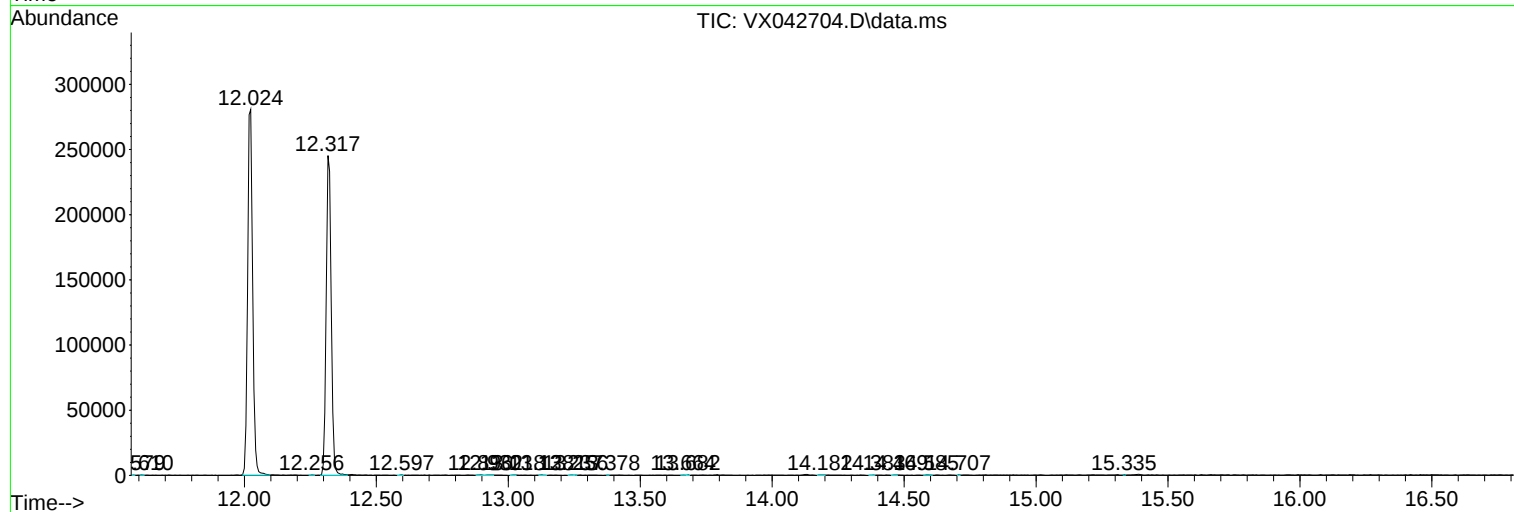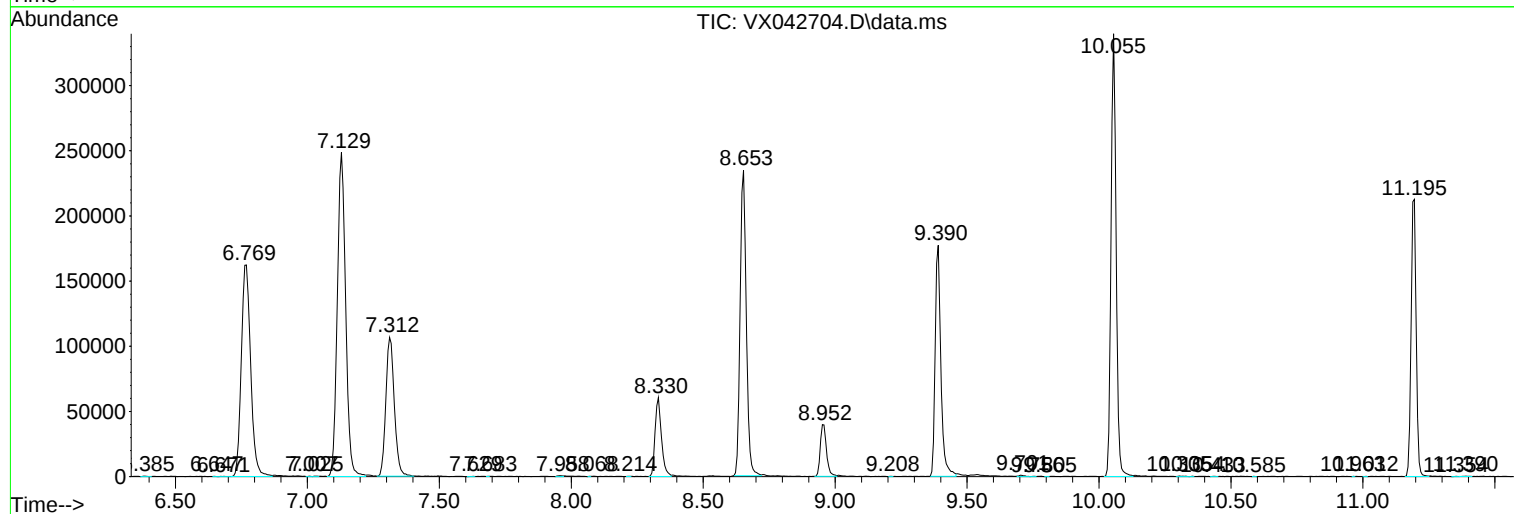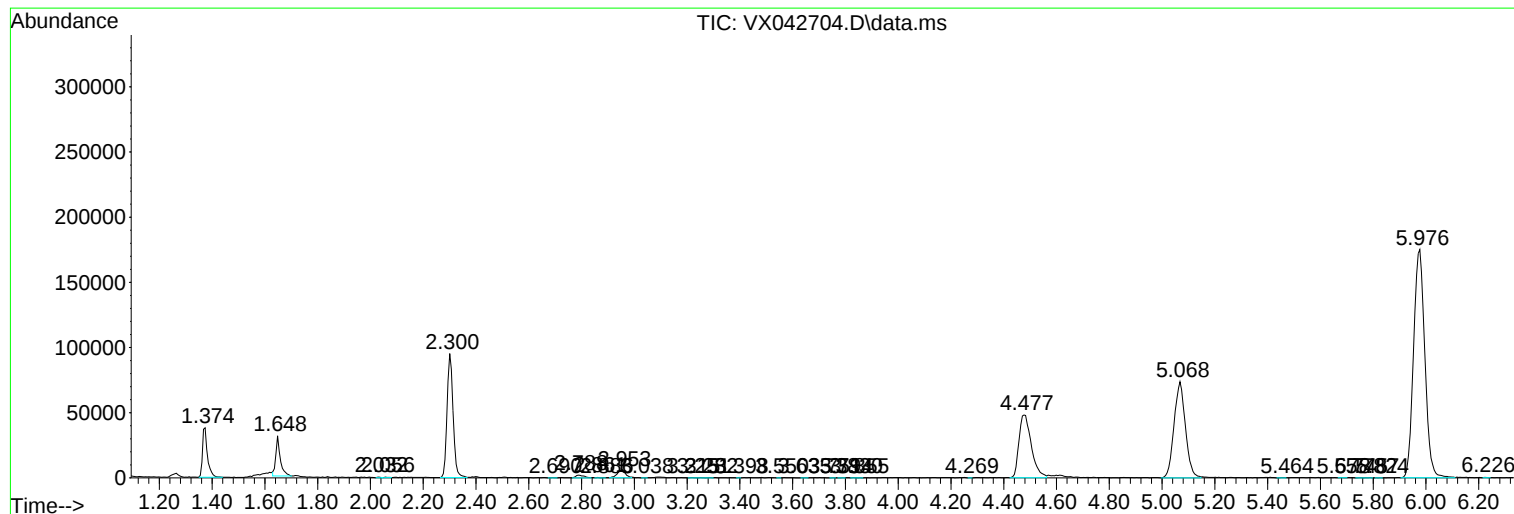

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042704.D
Acq On : 29 Jul 2024 20:28
Operator : JC/MD
Sample : P3388-02DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042704.D
Acq On : 29 Jul 2024 20:28
Operator : JC/MD
Sample : P3388-02DL 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
