

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042706.D
 Acq On : 29 Jul 2024 21:15
 Operator : JC/MD
 Sample : P3388-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	21	rVB	10215	13743	2.84%	0.369%
2	1.264	23	29	32	rBV3	7436	9643	1.99%	0.259%
3	1.368	43	46	56	rVB	36493	49448	10.21%	1.329%
4	1.563	75	78	80	rBV2	1362	1894	0.39%	0.051%
5	1.648	88	92	101	rVB	26794	34424	7.11%	0.925%
6	1.721	101	104	110	rVB3	3555	4796	0.99%	0.129%
7	1.935	135	139	145	rVB2	1662	2560	0.53%	0.069%
8	2.075	160	162	163	rBV	397	287	0.06%	0.008%
9	2.294	192	198	208	rBV	81148	127612	26.35%	3.431%
10	2.392	210	214	220	rVB	1702	3122	0.64%	0.084%
11	2.495	229	231	235	rBV	483	636	0.13%	0.017%
12	2.562	238	242	243	rBV3	334	406	0.08%	0.011%
13	2.703	262	265	267	rVB	297	268	0.06%	0.007%
14	2.782	274	278	280	rBV3	740	958	0.20%	0.026%
15	2.855	287	290	294	rBV3	337	431	0.09%	0.012%
16	2.916	298	300	301	rVV	313	232	0.05%	0.006%
17	2.947	301	305	311	rVB3	894	1953	0.40%	0.053%
18	3.026	315	318	324	rBV	141	246	0.05%	0.007%
19	3.099	326	330	332	rBV2	312	381	0.08%	0.010%
20	3.160	339	340	344	rBV	206	239	0.05%	0.006%
21	3.568	404	407	409	rVB	257	274	0.06%	0.007%
22	4.007	477	479	484	rVB2	275	359	0.07%	0.010%
23	4.245	515	518	521	rBV2	276	417	0.09%	0.011%
24	4.465	546	554	569	rBV2	43839	136179	28.12%	3.661%
25	4.812	607	611	612	rBV3	263	326	0.07%	0.009%
26	4.830	612	614	616	rVB	348	289	0.06%	0.008%
27	4.958	632	635	638	rBV	323	386	0.08%	0.010%
28	5.056	638	651	667	rBV3	64941	201610	41.62%	5.420%
29	5.239	680	681	683	rBV2	239	256	0.05%	0.007%
30	5.397	702	707	708	rVV2	300	327	0.07%	0.009%
31	5.458	714	717	721	rBV2	362	731	0.15%	0.020%
32	5.550	728	732	734	rBV3	431	581	0.12%	0.016%
33	5.568	734	735	739	rVB	498	405	0.08%	0.011%
34	5.964	789	800	822	rBV3	159116	484358	100.00%	13.022%
35	6.214	839	841	845	rVV2	223	261	0.05%	0.007%
36	6.623	907	908	913	rVB2	214	226	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042706.D
 Acq On : 29 Jul 2024 21:15
 Operator : JC/MD
 Sample : P3388-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.763	921	931	948	rBV	138574	344279	71.08%	9.256%
38	7.123	982	990	1002	rBV	39273	90050	18.59%	2.421%
39	7.306	1012	1020	1037	rBV	99241	227668	47.00%	6.121%
40	7.495	1048	1051	1054	rBV	415	529	0.11%	0.014%
41	7.543	1056	1059	1060	rVV2	290	285	0.06%	0.008%
42	7.592	1064	1067	1070	rVV2	250	380	0.08%	0.010%
43	7.677	1079	1081	1084	rVB	289	338	0.07%	0.009%
44	7.958	1123	1127	1130	rBV3	467	942	0.19%	0.025%
45	8.068	1142	1145	1148	rBV2	178	306	0.06%	0.008%
46	8.171	1160	1162	1165	rBV2	267	249	0.05%	0.007%
47	8.324	1182	1187	1205	rVV	53514	92663	19.13%	2.491%
48	8.500	1213	1216	1218	rBV2	260	363	0.07%	0.010%
49	8.525	1218	1220	1222	rBV2	270	280	0.06%	0.008%
50	8.647	1234	1240	1250	rBV	204799	328236	67.77%	8.824%
51	8.952	1285	1290	1301	rBV	37111	60190	12.43%	1.618%
52	9.275	1340	1343	1345	rBV2	268	305	0.06%	0.008%
53	9.384	1356	1361	1373	rBV	168892	268776	55.49%	7.226%
54	9.537	1383	1386	1389	rBV3	823	1272	0.26%	0.034%
55	9.647	1402	1404	1408	rBV2	273	386	0.08%	0.010%
56	9.756	1420	1422	1426	rVB	344	326	0.07%	0.009%
57	9.793	1426	1428	1431	rBV	194	244	0.05%	0.007%
58	9.945	1452	1453	1458	rVB2	241	232	0.05%	0.006%
59	10.055	1465	1471	1482	rBV	274596	381214	78.71%	10.249%
60	10.207	1492	1496	1501	rVV3	588	1046	0.22%	0.028%
61	10.311	1509	1513	1516	rBV3	951	1477	0.30%	0.040%
62	10.646	1566	1568	1572	rVV2	767	793	0.16%	0.021%
63	10.835	1595	1599	1600	rBV2	213	233	0.05%	0.006%
64	10.915	1610	1612	1615	rVB2	321	274	0.06%	0.007%
65	11.055	1634	1635	1638	rBV2	238	274	0.06%	0.007%
66	11.189	1652	1657	1668	rBV	199720	271870	56.13%	7.309%
67	11.354	1682	1684	1688	rVB	195	271	0.06%	0.007%
68	11.390	1688	1690	1694	rBV	239	324	0.07%	0.009%
69	11.652	1732	1733	1739	rVB	194	256	0.05%	0.007%
70	11.762	1747	1751	1755	rVB	592	751	0.16%	0.020%
71	11.829	1758	1762	1763	rBV	268	299	0.06%	0.008%
72	12.024	1788	1794	1804	rBV	222618	280467	57.90%	7.540%
73	12.116	1808	1809	1811	rBV	246	223	0.05%	0.006%
74	12.219	1822	1826	1832	rBV3	5529	7306	1.51%	0.196%
75	12.317	1837	1842	1851	rBV	200479	265570	54.83%	7.140%
76	12.451	1862	1864	1866	rBV2	328	318	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042706.D
 Acq On : 29 Jul 2024 21:15
 Operator : JC/MD
 Sample : P3388-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20R7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.926	1939	1942	1944	rBV2	260	255	0.05%	0.007%
78	13.115	1970	1973	1976	rBV	320	437	0.09%	0.012%
79	13.164	1978	1981	1984	rBV2	199	320	0.07%	0.009%
80	13.311	2002	2005	2007	rBV	238	286	0.06%	0.008%
81	13.426	2021	2024	2025	rBV	255	252	0.05%	0.007%
82	13.774	2077	2081	2082	rBV2	237	263	0.05%	0.007%
83	13.792	2082	2084	2086	rVV2	283	249	0.05%	0.007%
84	14.560	2207	2210	2213	rVB2	163	240	0.05%	0.006%
85	14.652	2223	2225	2228	rVB	263	225	0.05%	0.006%
86	14.682	2228	2230	2233	rBV	316	439	0.09%	0.012%
87	14.822	2249	2253	2254	rVB2	323	317	0.07%	0.009%
88	14.859	2257	2259	2261	rBV2	301	229	0.05%	0.006%
89	14.999	2278	2282	2284	rBV2	299	490	0.10%	0.013%
90	15.200	2313	2315	2318	rBV	304	294	0.06%	0.008%
91	15.231	2318	2320	2322	rBV	379	400	0.08%	0.011%
92	15.335	2332	2337	2338	rBV2	257	405	0.08%	0.011%
93	15.578	2376	2377	2381	rBV2	414	522	0.11%	0.014%
94	15.627	2384	2385	2388	rBV2	268	261	0.05%	0.007%
95	16.066	2455	2457	2459	rBV2	255	255	0.05%	0.007%
96	16.115	2463	2465	2466	rVB	510	295	0.06%	0.008%
97	16.401	2509	2512	2515	rBV2	390	619	0.13%	0.017%
98	16.456	2518	2521	2523	rBV3	399	409	0.08%	0.011%
99	16.529	2531	2533	2536	rBV2	220	308	0.06%	0.008%
100	16.700	2559	2561	2562	rBV	357	313	0.06%	0.008%




Sum of corrected areas: 3719612

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042706.D
Acq On : 29 Jul 2024 21:15
Operator : JC/MD
Sample : P3388-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

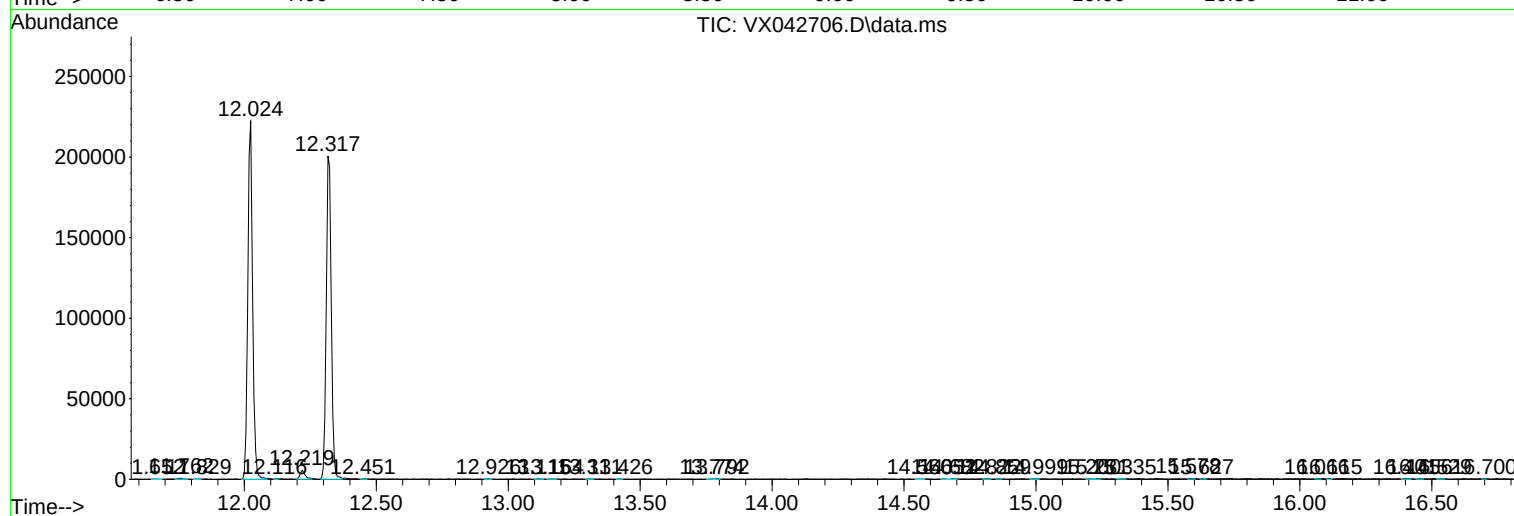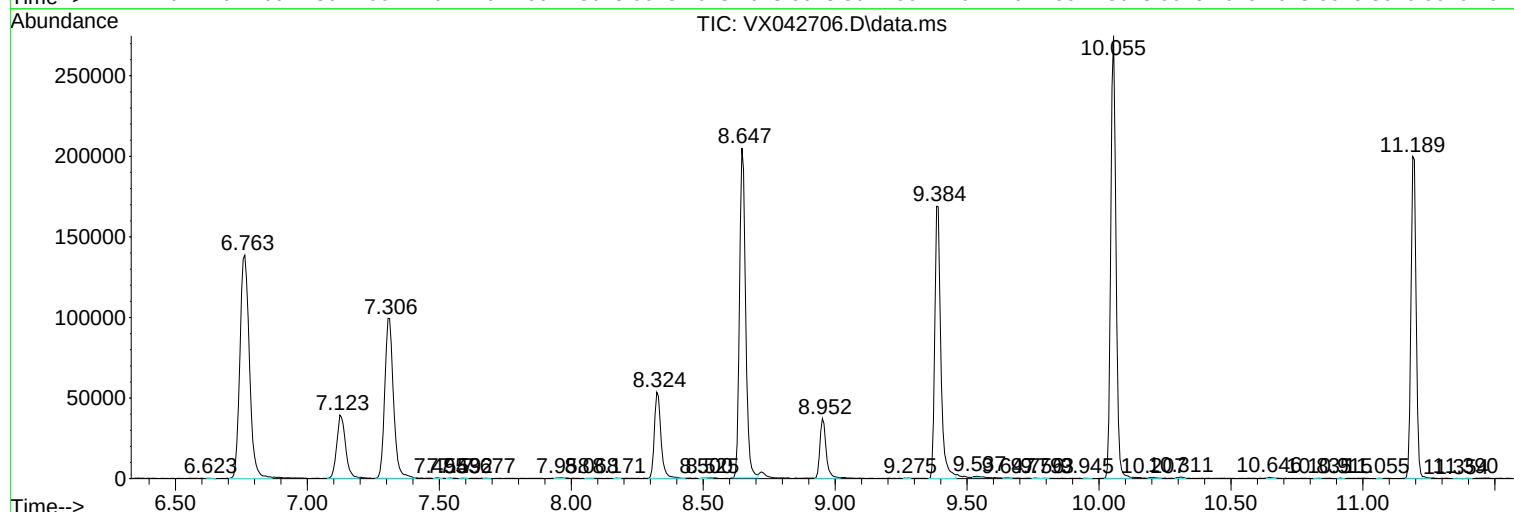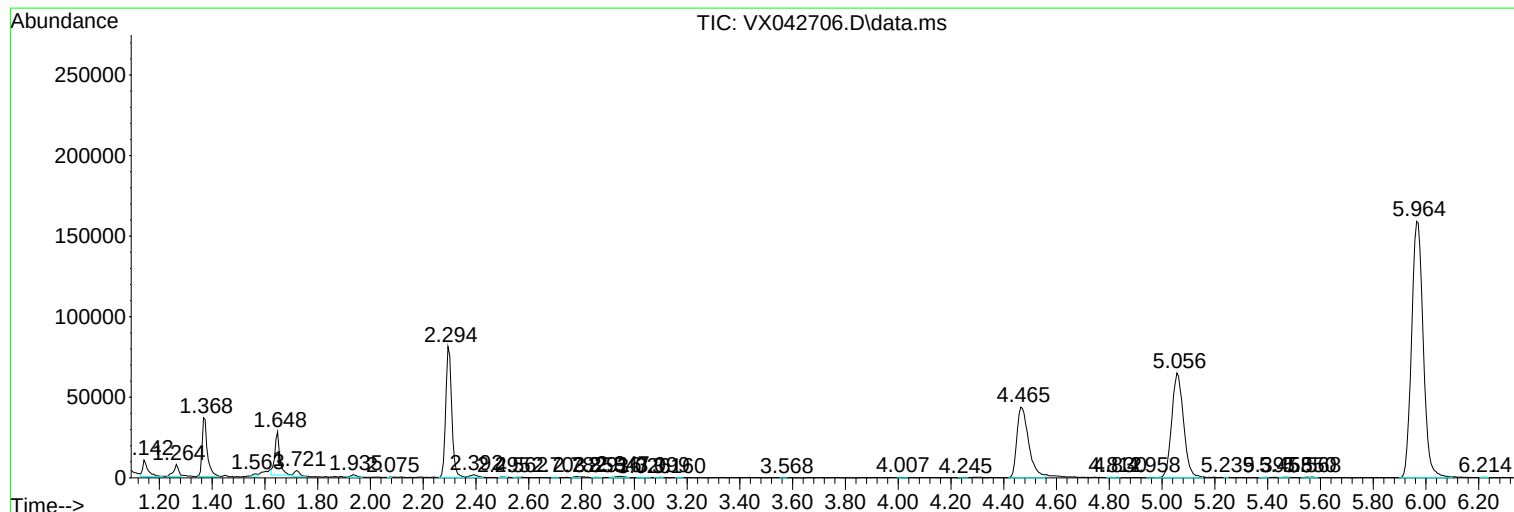

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042706.D
Acq On : 29 Jul 2024 21:15
Operator : JC/MD
Sample : P3388-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042706.D
Acq On : 29 Jul 2024 21:15
Operator : JC/MD
Sample : P3388-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20R7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc