

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042714.D
 Acq On : 30 Jul 2024 00:21
 Operator : JC/MD
 Sample : P3388-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042714.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	58	rVB	39377	48440	10.16%	1.311%
2	1.648	89	92	101	rVB	26969	34390	7.21%	0.930%
3	2.294	193	198	210	rBV	83955	131871	27.65%	3.568%
4	2.538	236	238	239	rBV	208	120	0.03%	0.003%
5	2.904	297	298	299	rBV	225	143	0.03%	0.004%
6	2.940	299	304	313	rVV3	987	2655	0.56%	0.072%
7	3.026	316	318	322	rBV	215	273	0.06%	0.007%
8	3.062	322	324	328	rVB	173	188	0.04%	0.005%
9	3.264	355	357	359	rBV	239	256	0.05%	0.007%
10	3.379	375	376	380	rVV	137	149	0.03%	0.004%
11	3.593	410	411	414	rBB	103	93	0.02%	0.003%
12	3.623	415	416	417	rBV	110	74	0.02%	0.002%
13	3.751	433	437	440	rBB2	264	415	0.09%	0.011%
14	3.855	451	454	455	rBV2	183	115	0.02%	0.003%
15	4.093	489	493	496	rBV2	256	331	0.07%	0.009%
16	4.257	518	520	521	rBV	218	183	0.04%	0.005%
17	4.465	546	554	569	rBV2	41015	122542	25.70%	3.315%
18	4.836	613	615	620	rVB	254	305	0.06%	0.008%
19	4.891	620	624	626	rBV	193	208	0.04%	0.006%
20	4.971	636	637	640	rBV	118	93	0.02%	0.003%
21	5.056	640	651	667	rBV	65195	200606	42.06%	5.427%
22	5.452	715	716	717	rVB	184	67	0.01%	0.002%
23	5.483	719	721	723	rVB	291	134	0.03%	0.004%
24	5.562	732	734	737	rBV2	207	260	0.05%	0.007%
25	5.696	755	756	759	rVV	235	135	0.03%	0.004%
26	5.720	759	760	764	rVB	232	149	0.03%	0.004%
27	5.769	765	768	770	rBV2	262	337	0.07%	0.009%
28	5.867	782	784	785	rBV	144	120	0.03%	0.003%
29	5.964	789	800	817	rBV3	162171	476906	100.00%	12.903%
30	6.251	845	847	849	rBV3	177	146	0.03%	0.004%
31	6.592	901	903	904	rBV	271	200	0.04%	0.005%
32	6.671	914	916	917	rVB	179	90	0.02%	0.002%
33	6.690	917	919	920	rVB	150	87	0.02%	0.002%
34	6.763	920	931	952	rBV	155885	384703	80.67%	10.408%
35	7.202	1001	1003	1004	rBV	346	310	0.07%	0.008%
36	7.305	1013	1020	1033	rBV	99641	220032	46.14%	5.953%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042714.D
 Acq On : 30 Jul 2024 00:21
 Operator : JC/MD
 Sample : P3388-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	7.482	1048	1049	1054	rVB	288	331	0.07%	0.009%
38	7.592	1065	1067	1073	rBV2	231	306	0.06%	0.008%
39	7.714	1086	1087	1092	rBV2	183	250	0.05%	0.007%
40	7.885	1113	1115	1116	rVB2	285	158	0.03%	0.004%
41	7.903	1116	1118	1119	rBB2	100	70	0.01%	0.002%
42	7.921	1119	1121	1123	rBV2	302	214	0.04%	0.006%
43	7.958	1123	1127	1130	rBV2	587	898	0.19%	0.024%
44	8.055	1142	1143	1147	rBV	269	295	0.06%	0.008%
45	8.092	1147	1149	1152	rVV2	242	288	0.06%	0.008%
46	8.153	1156	1159	1161	rVB2	103	91	0.02%	0.002%
47	8.275	1177	1179	1182	rBV	265	222	0.05%	0.006%
48	8.324	1182	1187	1203	rVV2	52465	89672	18.80%	2.426%
49	8.647	1234	1240	1251	rBV	217719	343168	71.96%	9.284%
50	8.952	1285	1290	1306	rBV	37986	60228	12.63%	1.629%
51	9.208	1331	1332	1333	rVB	341	125	0.03%	0.003%
52	9.232	1333	1336	1337	rBV	207	238	0.05%	0.006%
53	9.330	1351	1352	1354	rBV2	175	153	0.03%	0.004%
54	9.384	1356	1361	1379	rBV	165098	259221	54.35%	7.013%
55	9.738	1418	1419	1420	rBV	198	120	0.03%	0.003%
56	9.811	1427	1431	1432	rBV	308	433	0.09%	0.012%
57	9.896	1442	1445	1446	rBV	255	339	0.07%	0.009%
58	9.988	1458	1460	1463	rVB	231	167	0.04%	0.005%
59	10.055	1465	1471	1486	rBV	314695	434010	91.01%	11.742%
60	10.268	1504	1506	1508	rBV	153	137	0.03%	0.004%
61	10.305	1510	1512	1514	rBV	486	401	0.08%	0.011%
62	10.360	1519	1521	1522	rBV	279	180	0.04%	0.005%
63	10.409	1526	1529	1530	rBV	156	171	0.04%	0.005%
64	10.567	1553	1555	1556	rBV	229	163	0.03%	0.004%
65	10.811	1593	1595	1596	rBB	295	161	0.03%	0.004%
66	10.848	1596	1601	1603	rBV2	188	353	0.07%	0.010%
67	10.963	1617	1620	1625	rVB	209	391	0.08%	0.011%
68	11.006	1625	1627	1629	rBV2	263	236	0.05%	0.006%
69	11.134	1645	1648	1650	rBV2	230	232	0.05%	0.006%
70	11.189	1652	1657	1673	rVB	198728	265126	55.59%	7.173%
71	11.372	1686	1687	1690	rBV	146	166	0.03%	0.004%
72	11.457	1700	1701	1703	rBV	118	95	0.02%	0.003%
73	11.689	1737	1739	1740	rBV	211	124	0.03%	0.003%
74	11.750	1747	1749	1752	rBV2	474	507	0.11%	0.014%
75	11.805	1757	1758	1761	rVV	146	114	0.02%	0.003%
76	11.902	1772	1774	1775	rBV	173	105	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042714.D
 Acq On : 30 Jul 2024 00:21
 Operator : JC/MD
 Sample : P3388-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.957	1778	1783	1786	rBV	287	486	0.10%	0.013%
78	12.024	1789	1794	1807	rVB	243634	322510	67.63%	8.725%
79	12.152	1813	1815	1822	rVB3	275	514	0.11%	0.014%
80	12.219	1822	1826	1835	rBV2	3059	5028	1.05%	0.136%
81	12.317	1837	1842	1851	rBV	217770	276830	58.05%	7.490%
82	12.585	1884	1886	1888	rBV	292	258	0.05%	0.007%
83	12.640	1891	1895	1897	rBV2	152	237	0.05%	0.006%
84	12.713	1904	1907	1909	rBB2	233	243	0.05%	0.007%
85	12.744	1909	1912	1913	rBV2	284	278	0.06%	0.008%
86	12.853	1929	1930	1935	rBV2	220	316	0.07%	0.009%
87	12.945	1944	1945	1951	rBB2	204	294	0.06%	0.008%
88	13.000	1951	1954	1955	rBV	232	223	0.05%	0.006%
89	13.061	1961	1964	1965	rBV	201	191	0.04%	0.005%
90	13.213	1987	1989	1991	rBV	188	141	0.03%	0.004%
91	13.445	2025	2027	2028	rVB	217	118	0.02%	0.003%
92	13.469	2029	2031	2033	rBV	210	222	0.05%	0.006%
93	13.749	2076	2077	2078	rBV	197	94	0.02%	0.003%
94	14.194	2149	2150	2153	rBV	268	182	0.04%	0.005%
95	14.249	2158	2159	2160	rBV	178	98	0.02%	0.003%
96	14.426	2184	2188	2189	rBV	182	240	0.05%	0.006%
97	14.627	2219	2221	2222	rBV	167	160	0.03%	0.004%
98	14.640	2222	2223	2224	rVV	221	98	0.02%	0.003%
99	15.822	2414	2417	2419	rBV3	317	334	0.07%	0.009%
100	15.865	2422	2424	2425	rBV3	494	308	0.06%	0.008%




Sum of corrected areas: 3696188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042714.D
Acq On : 30 Jul 2024 00:21
Operator : JC/MD
Sample : P3388-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

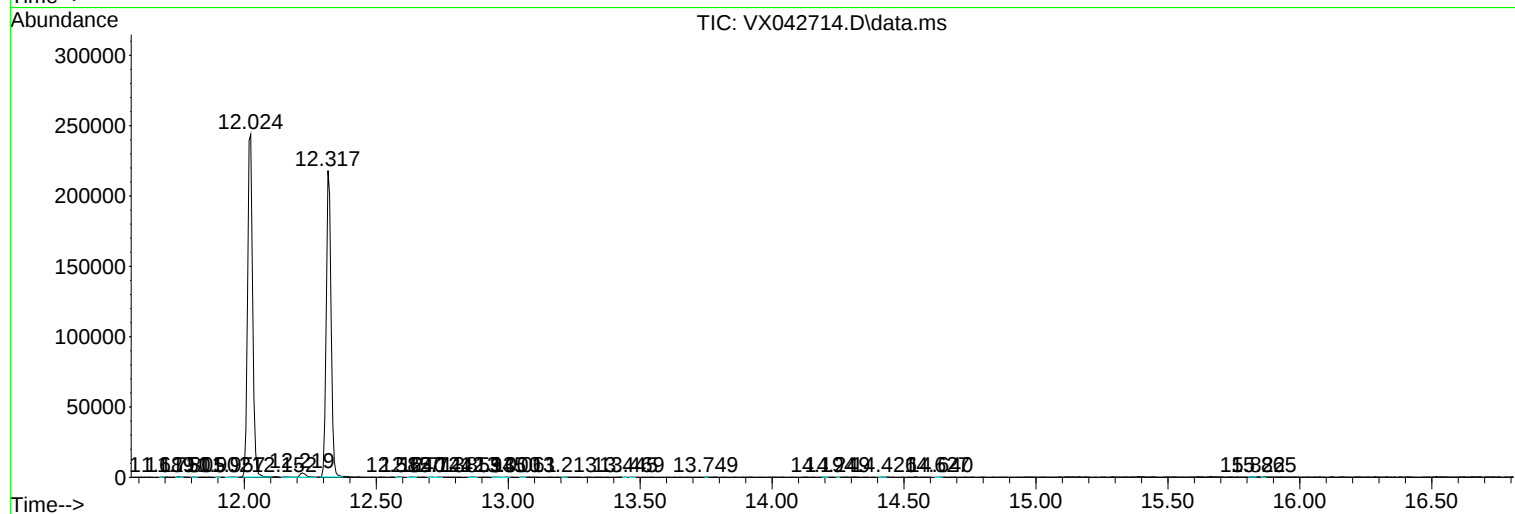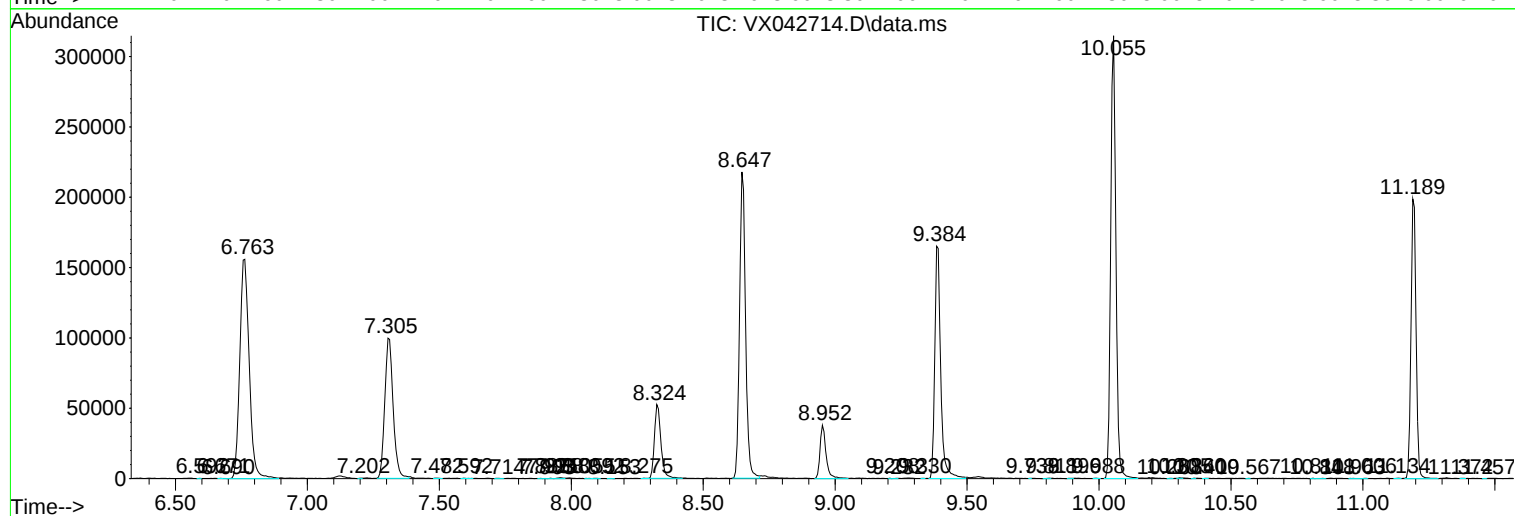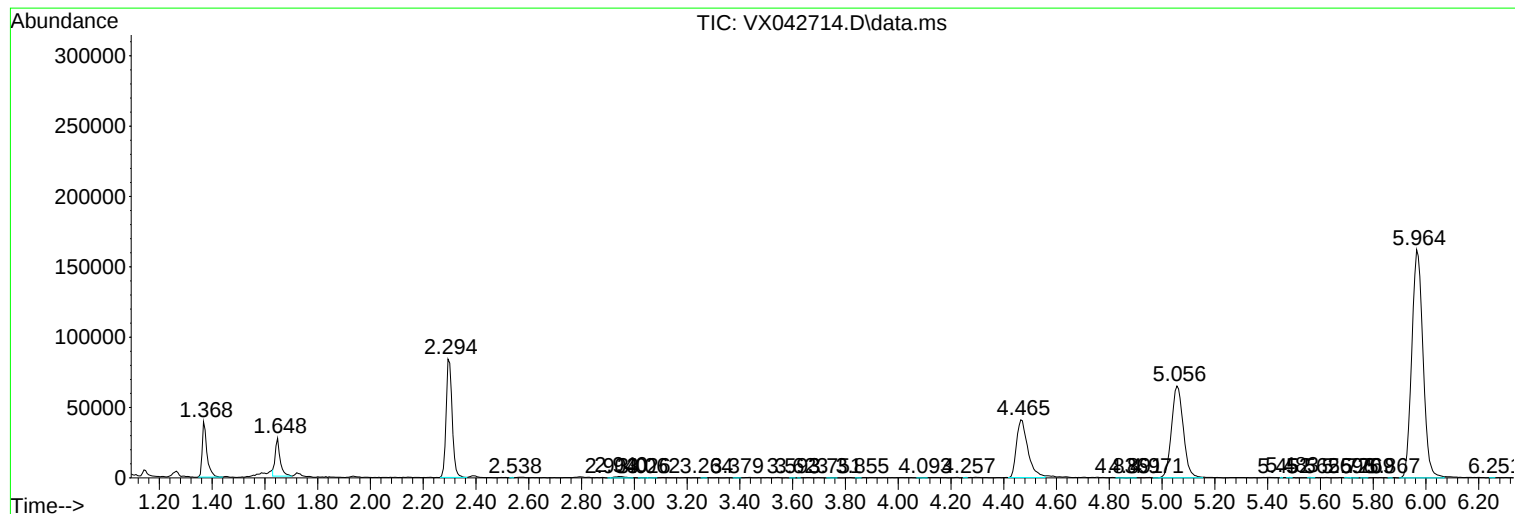

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042714.D
Acq On : 30 Jul 2024 00:21
Operator : JC/MD
Sample : P3388-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042714.D
Acq On : 30 Jul 2024 00:21
Operator : JC/MD
Sample : P3388-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------