

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042716.D
 Acq On : 30 Jul 2024 01:07
 Operator : JC/MD
 Sample : P3389-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042716.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	18	rVB2	8097	10308	2.20%	0.286%
2	1.368	43	46	57	rVB	38489	50198	10.73%	1.394%
3	1.544	70	75	76	rBV2	1158	1406	0.30%	0.039%
4	1.648	89	92	99	rVB	26089	32799	7.01%	0.911%
5	1.935	137	139	144	rVB	1874	2209	0.47%	0.061%
6	2.300	193	199	209	rVB	79904	128560	27.48%	3.571%
7	2.556	237	241	242	rBV	370	351	0.08%	0.010%
8	2.623	250	252	253	rBV	170	114	0.02%	0.003%
9	2.678	259	261	262	rBV	195	128	0.03%	0.004%
10	2.715	265	267	270	rBV	235	326	0.07%	0.009%
11	3.038	319	320	324	rVB	234	226	0.05%	0.006%
12	3.087	324	328	330	rBV3	592	709	0.15%	0.020%
13	3.190	341	345	346	rBB3	197	185	0.04%	0.005%
14	3.221	347	350	354	rBB	127	150	0.03%	0.004%
15	3.264	354	357	359	rBB	248	276	0.06%	0.008%
16	3.300	360	363	364	rBV	200	203	0.04%	0.006%
17	3.349	369	371	373	rVB	210	166	0.04%	0.005%
18	3.422	380	383	384	rBV	242	255	0.05%	0.007%
19	3.483	390	393	398	rBV	139	241	0.05%	0.007%
20	3.556	401	405	407	rBV	158	199	0.04%	0.006%
21	3.599	411	412	415	rVB2	224	235	0.05%	0.007%
22	3.629	415	417	420	rBB	176	196	0.04%	0.005%
23	3.672	420	424	426	rBV2	241	395	0.08%	0.011%
24	3.751	435	437	439	rVB	251	182	0.04%	0.005%
25	3.940	466	468	470	rBV	176	161	0.03%	0.004%
26	4.166	503	505	512	rVB	332	442	0.09%	0.012%
27	4.227	512	515	517	rBV	154	199	0.04%	0.006%
28	4.300	525	527	530	rVB2	386	363	0.08%	0.010%
29	4.465	546	554	573	rBV	40295	121230	25.91%	3.367%
30	4.836	612	615	617	rBV	175	172	0.04%	0.005%
31	4.861	617	619	621	rVB	325	241	0.05%	0.007%
32	4.879	621	622	627	rBV2	244	322	0.07%	0.009%
33	4.964	633	636	638	rBV	174	215	0.05%	0.006%
34	5.062	638	652	668	rVV	63830	200428	42.84%	5.567%
35	5.239	679	681	682	rBV	138	137	0.03%	0.004%
36	5.391	704	706	709	rBV3	222	330	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042716.D
 Acq On : 30 Jul 2024 01:07
 Operator : JC/MD
 Sample : P3389-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.446	713	715	716	rBV	242	118	0.03%	0.003%
38	5.672	749	752	754	rBV	216	324	0.07%	0.009%
39	5.970	790	801	822	rVB2	156720	467904	100.00%	12.996%
40	6.220	840	842	845	rBV2	237	218	0.05%	0.006%
41	6.330	859	860	862	rBV	119	124	0.03%	0.003%
42	6.458	877	881	882	rBV2	236	267	0.06%	0.007%
43	6.550	895	896	897	rBV2	185	135	0.03%	0.004%
44	6.671	915	916	919	rVB	262	185	0.04%	0.005%
45	6.763	919	931	943	rBV	151031	363852	77.76%	10.106%
46	7.129	984	991	998	rBV4	3716	9545	2.04%	0.265%
47	7.306	1013	1020	1036	rBV	95399	217924	46.57%	6.053%
48	7.610	1068	1070	1071	rBV	141	127	0.03%	0.004%
49	7.866	1109	1112	1117	rBV2	226	445	0.10%	0.012%
50	7.903	1117	1118	1120	rBV	239	179	0.04%	0.005%
51	8.232	1170	1172	1175	rBB2	180	214	0.05%	0.006%
52	8.324	1182	1187	1203	rVV	51557	87389	18.68%	2.427%
53	8.647	1234	1240	1249	rBV	204833	330150	70.56%	9.170%
54	8.952	1285	1290	1307	rVB2	37173	57677	12.33%	1.602%
55	9.256	1339	1340	1342	rBV2	333	291	0.06%	0.008%
56	9.384	1356	1361	1379	rBV	164052	255445	54.59%	7.095%
57	9.860	1435	1439	1440	rBV	345	254	0.05%	0.007%
58	9.909	1445	1447	1451	rVB	234	295	0.06%	0.008%
59	9.982	1458	1459	1460	rBV	171	118	0.03%	0.003%
60	10.055	1465	1471	1483	rBV	291488	406384	86.85%	11.287%
61	10.299	1509	1511	1521	rVB4	978	1724	0.37%	0.048%
62	10.482	1539	1541	1544	rBV	239	319	0.07%	0.009%
63	10.555	1551	1553	1554	rBV	189	119	0.03%	0.003%
64	10.701	1576	1577	1578	rBV	273	129	0.03%	0.004%
65	10.756	1584	1586	1588	rBV	306	156	0.03%	0.004%
66	10.811	1593	1595	1597	rBV	152	123	0.03%	0.003%
67	10.927	1612	1614	1618	rVB	308	388	0.08%	0.011%
68	10.969	1618	1621	1625	rBB	318	298	0.06%	0.008%
69	11.067	1634	1637	1640	rBV2	262	395	0.08%	0.011%
70	11.189	1652	1657	1668	rVV	200780	262735	56.15%	7.298%
71	11.445	1697	1699	1701	rBV	224	163	0.03%	0.005%
72	11.725	1743	1745	1748	rBV2	264	311	0.07%	0.009%
73	11.872	1767	1769	1770	rBV	217	167	0.04%	0.005%
74	11.982	1784	1787	1788	rBV2	276	250	0.05%	0.007%
75	12.018	1788	1793	1802	rBV	229203	298383	63.77%	8.288%
76	12.219	1822	1826	1833	rVB2	8054	10822	2.31%	0.301%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042716.D
 Acq On : 30 Jul 2024 01:07
 Operator : JC/MD
 Sample : P3389-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1853	rBV	203276	264247	56.47%	7.340%
78	12.457	1864	1865	1869	rVB	293	223	0.05%	0.006%
79	12.658	1896	1898	1899	rBV	190	136	0.03%	0.004%
80	12.933	1941	1943	1944	rBV	179	158	0.03%	0.004%
81	13.109	1969	1972	1973	rBV	270	296	0.06%	0.008%
82	13.262	1994	1997	1998	rBV	192	206	0.04%	0.006%
83	13.317	2004	2006	2007	rBV2	296	205	0.04%	0.006%
84	13.603	2051	2053	2058	rVB	338	444	0.09%	0.012%
85	13.670	2059	2064	2066	rBV	298	396	0.08%	0.011%
86	13.719	2071	2072	2073	rBV	222	133	0.03%	0.004%
87	13.780	2080	2082	2084	rBV2	249	256	0.05%	0.007%
88	13.865	2095	2096	2098	rVB	201	126	0.03%	0.003%
89	13.896	2098	2101	2102	rBV	347	290	0.06%	0.008%
90	13.945	2108	2109	2111	rBV	154	128	0.03%	0.004%
91	14.006	2116	2119	2120	rVV	306	189	0.04%	0.005%
92	14.024	2120	2122	2124	rVB	211	144	0.03%	0.004%
93	14.493	2196	2199	2200	rBV	298	255	0.05%	0.007%
94	14.713	2231	2235	2239	rBV2	329	473	0.10%	0.013%
95	14.780	2244	2246	2250	rVB2	373	338	0.07%	0.009%
96	14.865	2258	2260	2264	rBV2	321	267	0.06%	0.007%
97	14.896	2264	2265	2266	rBV	302	165	0.04%	0.005%
98	15.152	2306	2307	2308	rBV	368	196	0.04%	0.005%
99	15.292	2328	2330	2332	rBV	385	356	0.08%	0.010%
100	15.938	2435	2436	2441	rBV	408	386	0.08%	0.011%

Sum of corrected areas: 3600316




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042716.D
Acq On : 30 Jul 2024 01:07
Operator : JC/MD
Sample : P3389-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

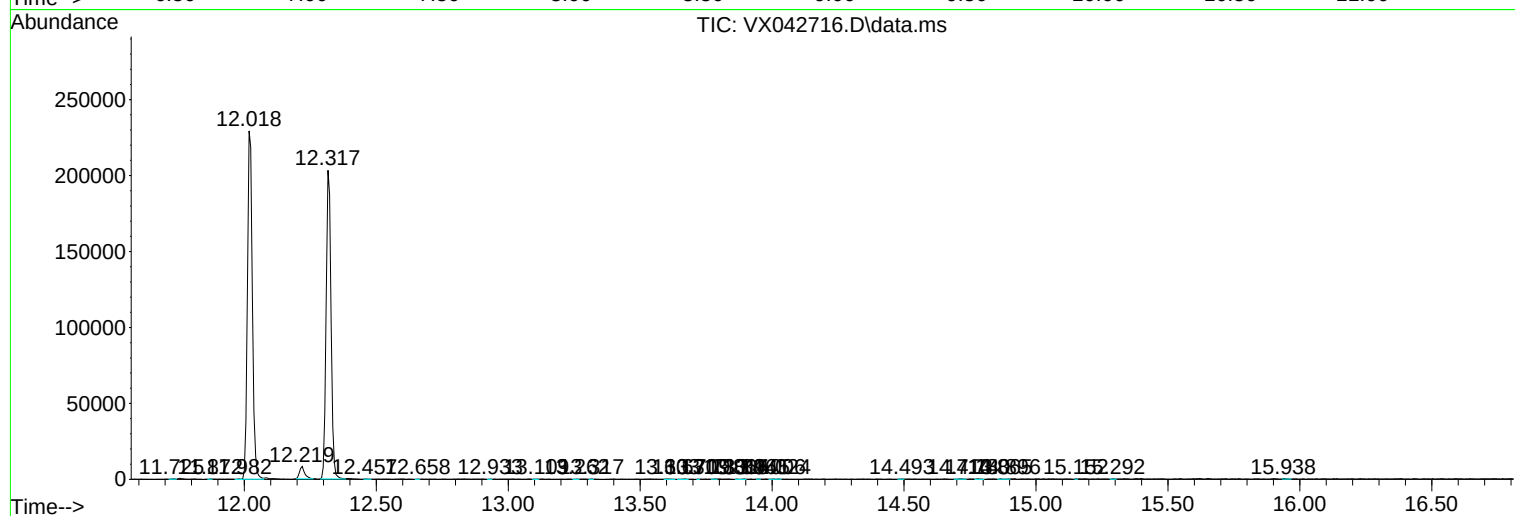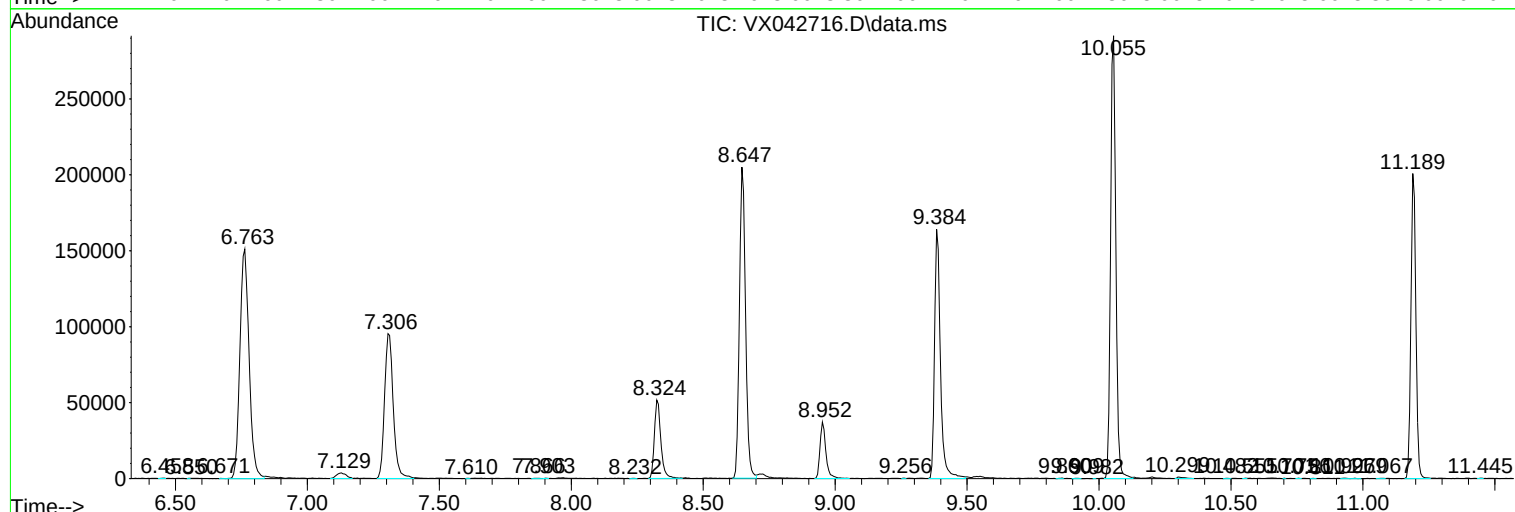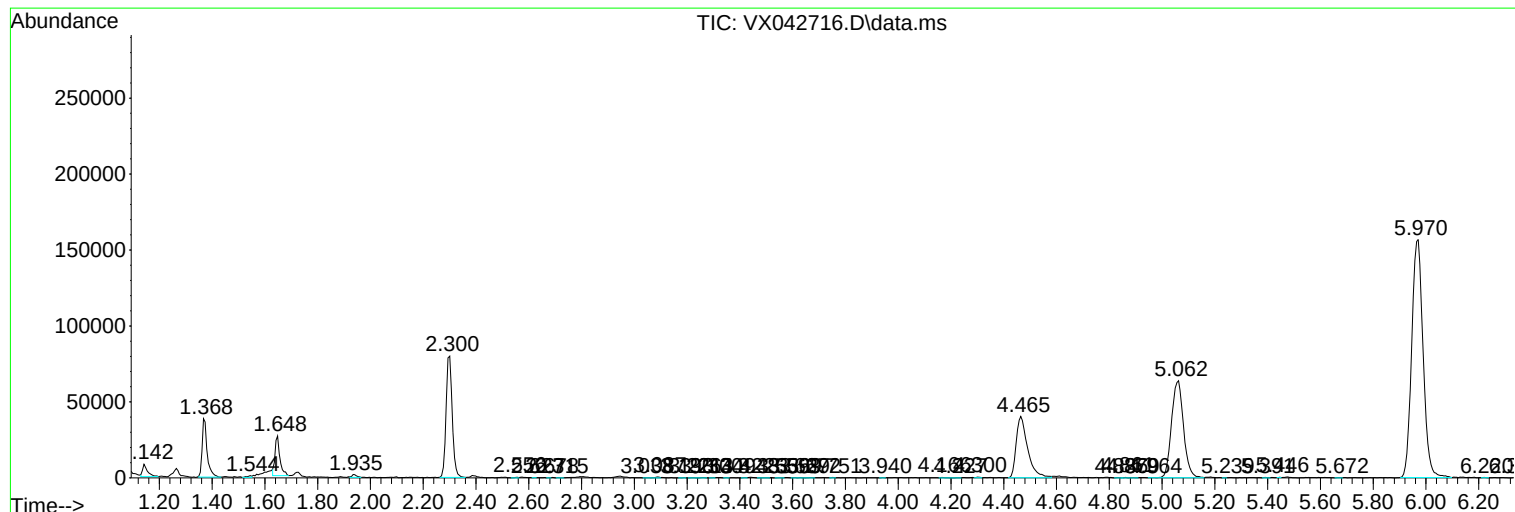

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042716.D
Acq On : 30 Jul 2024 01:07
Operator : JC/MD
Sample : P3389-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042716.D
Acq On : 30 Jul 2024 01:07
Operator : JC/MD
Sample : P3389-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc