

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042717.D
 Acq On : 30 Jul 2024 01:30
 Operator : JC/MD
 Sample : P3389-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	14	rVB	4760	5479	1.19%	0.151%
2	1.368	43	46	57	rVB	33581	44422	9.66%	1.223%
3	1.648	89	92	101	rVB	24230	31810	6.92%	0.875%
4	2.099	164	166	168	rBV	502	284	0.06%	0.008%
5	2.300	193	199	208	rVB	81955	124184	27.01%	3.418%
6	2.575	238	244	247	rBV3	734	1387	0.30%	0.038%
7	2.666	257	259	263	rVB	174	251	0.05%	0.007%
8	2.721	265	268	269	rBV	161	123	0.03%	0.003%
9	2.745	269	272	273	rBV	108	97	0.02%	0.003%
10	2.782	276	278	282	rVV	462	426	0.09%	0.012%
11	2.916	296	300	301	rBV2	263	343	0.07%	0.009%
12	2.934	301	303	304	rBV	1063	948	0.21%	0.026%
13	3.105	328	331	333	rVB	266	259	0.06%	0.007%
14	3.221	347	350	351	rBV	96	111	0.02%	0.003%
15	3.239	351	353	354	rBV	194	102	0.02%	0.003%
16	3.446	385	387	388	rVB	197	111	0.02%	0.003%
17	3.471	388	391	392	rBV	195	165	0.04%	0.005%
18	3.684	425	426	429	rVV	139	121	0.03%	0.003%
19	3.751	434	437	438	rBV	227	206	0.04%	0.006%
20	3.830	447	450	453	rBB2	237	314	0.07%	0.009%
21	3.885	457	459	460	rBV2	143	107	0.02%	0.003%
22	4.038	481	484	488	rBV	229	360	0.08%	0.010%
23	4.074	488	490	493	rBV2	249	266	0.06%	0.007%
24	4.147	500	502	506	rVB	126	98	0.02%	0.003%
25	4.184	506	508	511	rVB	218	196	0.04%	0.005%
26	4.233	511	516	519	rBB2	146	284	0.06%	0.008%
27	4.269	519	522	523	rBV	307	263	0.06%	0.007%
28	4.373	535	539	542	rBV	239	426	0.09%	0.012%
29	4.465	546	554	574	rBV	37661	118172	25.70%	3.252%
30	4.855	617	618	621	rBV	200	176	0.04%	0.005%
31	4.891	621	624	627	rVB	310	318	0.07%	0.009%
32	5.062	641	652	673	rVB2	63718	193006	41.98%	5.312%
33	5.294	689	690	692	rVB2	237	160	0.03%	0.004%
34	5.379	701	704	705	rBV	374	312	0.07%	0.009%
35	5.464	714	718	719	rBV2	382	442	0.10%	0.012%
36	5.659	749	750	754	rBV	157	163	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042717.D
 Acq On : 30 Jul 2024 01:30
 Operator : JC/MD
 Sample : P3389-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.757	764	766	768	rBV	145	104	0.02%	0.003%
38	5.824	776	777	780	rBV	114	142	0.03%	0.004%
39	5.970	788	801	819	rBV2	155165	459754	100.00%	12.653%
40	6.348	861	863	864	rVV	285	166	0.04%	0.005%
41	6.379	867	868	871	rVV	301	180	0.04%	0.005%
42	6.403	871	872	876	rVB2	181	200	0.04%	0.006%
43	6.495	886	887	888	rBV2	156	104	0.02%	0.003%
44	6.543	892	895	896	rBV	231	186	0.04%	0.005%
45	6.610	903	906	908	rBV	163	176	0.04%	0.005%
46	6.659	912	914	916	rVB	245	168	0.04%	0.005%
47	6.763	922	931	943	rBV	159654	382044	83.10%	10.514%
48	7.123	985	990	999	rVB3	4339	10465	2.28%	0.288%
49	7.312	1012	1021	1030	rBV	96533	210570	45.80%	5.795%
50	7.488	1048	1050	1051	rBV2	398	311	0.07%	0.009%
51	7.824	1103	1105	1106	rBV	147	111	0.02%	0.003%
52	7.939	1123	1124	1126	rBV	277	238	0.05%	0.007%
53	7.958	1126	1127	1130	rVV3	294	362	0.08%	0.010%
54	8.202	1165	1167	1168	rBV3	164	129	0.03%	0.004%
55	8.324	1180	1187	1202	rBV	47970	85198	18.53%	2.345%
56	8.513	1215	1218	1219	rBV3	390	406	0.09%	0.011%
57	8.647	1234	1240	1249	rBV	201378	328359	71.42%	9.037%
58	8.909	1281	1283	1285	rBV2	253	244	0.05%	0.007%
59	8.952	1285	1290	1302	rVV	35249	55427	12.06%	1.525%
60	9.269	1339	1342	1348	rBV2	538	965	0.21%	0.027%
61	9.384	1356	1361	1376	rBV	163605	245800	53.46%	6.765%
62	9.720	1414	1416	1417	rBV	342	247	0.05%	0.007%
63	9.957	1451	1455	1457	rBV	291	263	0.06%	0.007%
64	10.006	1462	1463	1465	rBV	251	259	0.06%	0.007%
65	10.055	1465	1471	1481	rBV	315003	436541	94.95%	12.014%
66	10.195	1492	1494	1498	rVB3	492	615	0.13%	0.017%
67	10.427	1530	1532	1534	rVB	169	132	0.03%	0.004%
68	10.482	1539	1541	1543	rBV	201	175	0.04%	0.005%
69	10.500	1543	1544	1547	rBV	146	142	0.03%	0.004%
70	10.549	1551	1552	1554	rBV2	211	119	0.03%	0.003%
71	10.579	1556	1557	1561	rBV2	241	376	0.08%	0.010%
72	10.713	1577	1579	1582	rBV2	225	262	0.06%	0.007%
73	10.976	1619	1622	1624	rBV2	304	396	0.09%	0.011%
74	11.189	1652	1657	1665	rBV	197567	259853	56.52%	7.151%
75	11.439	1694	1698	1700	rBV	207	265	0.06%	0.007%
76	11.512	1709	1710	1711	rBV	190	127	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042717.D
 Acq On : 30 Jul 2024 01:30
 Operator : JC/MD
 Sample : P3389-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.677	1735	1737	1739	rBV	104	109	0.02%	0.003%
78	11.762	1748	1751	1752	rBV2	300	352	0.08%	0.010%
79	11.823	1758	1761	1766	rBB	223	380	0.08%	0.010%
80	11.872	1766	1769	1772	rBV	219	324	0.07%	0.009%
81	12.024	1789	1794	1803	rBV	250357	329852	71.75%	9.078%
82	12.219	1822	1826	1837	rVB	9013	12420	2.70%	0.342%
83	12.317	1837	1842	1854	rBV	214503	279037	60.69%	7.679%
84	12.640	1893	1895	1896	rBV	204	126	0.03%	0.003%
85	12.884	1934	1935	1938	rBV2	259	241	0.05%	0.007%
86	12.932	1942	1943	1945	rBV	221	132	0.03%	0.004%
87	12.987	1951	1952	1954	rBV	195	154	0.03%	0.004%
88	13.036	1957	1960	1961	rBV	201	227	0.05%	0.006%
89	13.176	1982	1983	1984	rBV	232	129	0.03%	0.004%
90	13.256	1994	1996	1998	rBV	230	257	0.06%	0.007%
91	13.292	1998	2002	2003	rVV	162	166	0.04%	0.005%
92	13.402	2018	2020	2022	rBV	131	128	0.03%	0.004%
93	13.768	2075	2080	2081	rBV	231	373	0.08%	0.010%
94	13.804	2084	2086	2088	rBV	128	113	0.02%	0.003%
95	13.920	2104	2105	2106	rBV	176	113	0.02%	0.003%
96	14.030	2120	2123	2127	rBV	226	341	0.07%	0.009%
97	14.194	2148	2150	2151	rBV	203	207	0.05%	0.006%
98	14.280	2163	2164	2166	rBV	209	163	0.04%	0.004%
99	14.463	2190	2194	2197	rBV2	202	325	0.07%	0.009%
100	15.572	2374	2376	2380	rBV2	495	496	0.11%	0.014%


Sum of corrected areas: 3633638

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042717.D
Acq On : 30 Jul 2024 01:30
Operator : JC/MD
Sample : P3389-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

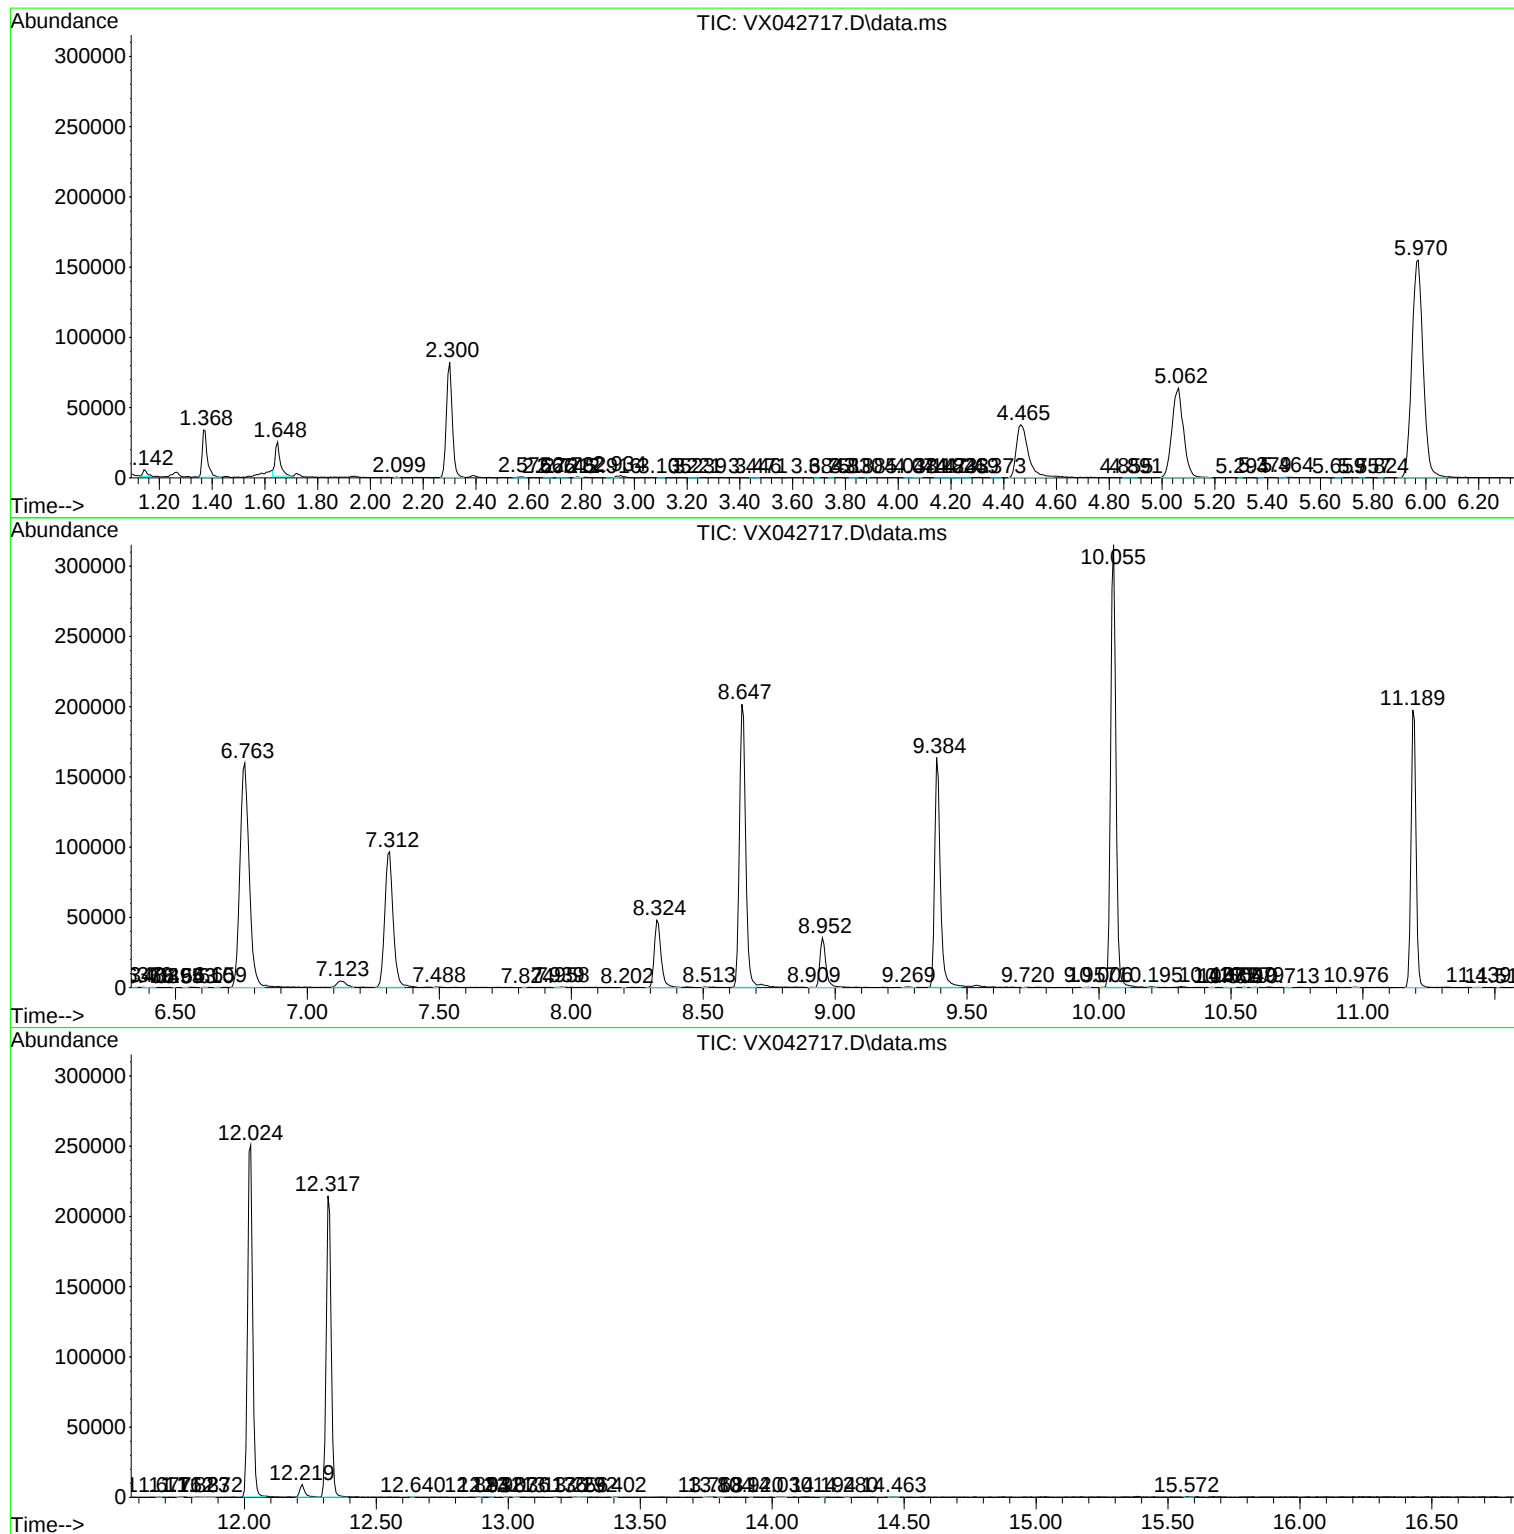

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042717.D
Acq On : 30 Jul 2024 01:30
Operator : JC/MD
Sample : P3389-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042717.D
Acq On : 30 Jul 2024 01:30
Operator : JC/MD
Sample : P3389-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------