

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042718.D
 Acq On : 30 Jul 2024 01:53
 Operator : JC/MD
 Sample : P3389-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042718.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	16	rVB	4901	5816	1.25%	0.160%
2	1.368	43	46	58	rVB	35816	44218	9.51%	1.215%
3	1.648	89	92	101	rVB	22536	33740	7.26%	0.927%
4	2.142	172	173	174	rBV	256	141	0.03%	0.004%
5	2.300	193	199	209	rVB	80182	128604	27.66%	3.535%
6	2.569	237	243	247	rBV2	808	1240	0.27%	0.034%
7	2.782	275	278	279	rBV	710	538	0.12%	0.015%
8	2.940	297	304	311	rBB2	1280	3266	0.70%	0.090%
9	2.995	311	313	316	rBV2	208	311	0.07%	0.009%
10	3.081	325	327	331	rVB3	418	461	0.10%	0.013%
11	3.227	349	351	353	rBB3	167	147	0.03%	0.004%
12	3.392	377	378	381	rVB	327	196	0.04%	0.005%
13	3.434	383	385	388	rBV	270	228	0.05%	0.006%
14	3.471	388	391	392	rBV	179	142	0.03%	0.004%
15	3.544	402	403	406	rVB	145	128	0.03%	0.004%
16	3.587	407	410	411	rBV	118	135	0.03%	0.004%
17	3.599	411	412	415	rBV2	179	136	0.03%	0.004%
18	3.696	424	428	429	rBB	149	129	0.03%	0.004%
19	3.721	429	432	434	rBB	198	218	0.05%	0.006%
20	3.751	435	437	439	rBV	245	222	0.05%	0.006%
21	3.849	450	453	454	rBV	133	135	0.03%	0.004%
22	4.068	488	489	492	rVB	237	198	0.04%	0.005%
23	4.093	492	493	497	rBV	161	195	0.04%	0.005%
24	4.190	508	509	510	rBV	180	131	0.03%	0.004%
25	4.343	532	534	537	rBV	212	259	0.06%	0.007%
26	4.465	544	554	573	rBV	39847	122382	26.32%	3.364%
27	4.897	623	625	626	rBV	151	137	0.03%	0.004%
28	4.952	630	634	637	rBB2	204	304	0.07%	0.008%
29	5.056	640	651	669	rBV2	66187	195271	42.00%	5.368%
30	5.355	697	700	702	rBV2	175	222	0.05%	0.006%
31	5.507	723	725	726	rBV	220	166	0.04%	0.005%
32	5.574	734	736	737	rBV	176	118	0.03%	0.003%
33	5.599	738	740	741	rVV	227	154	0.03%	0.004%
34	5.635	745	746	747	rBV	162	118	0.03%	0.003%
35	5.690	752	755	757	rBV	164	157	0.03%	0.004%
36	5.788	767	771	773	rBV	147	217	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042718.D
 Acq On : 30 Jul 2024 01:53
 Operator : JC/MD
 Sample : P3389-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.873	783	785	786	rBV	165	136	0.03%	0.004%
38	5.964	790	800	817	rBV2	155712	464972	100.00%	12.781%
39	6.318	855	858	860	rBV	314	311	0.07%	0.009%
40	6.385	867	869	871	rBV	209	195	0.04%	0.005%
41	6.507	888	889	892	rBV	137	157	0.03%	0.004%
42	6.562	895	898	901	rVV	152	204	0.04%	0.006%
43	6.763	922	931	945	rBV2	157012	380057	81.74%	10.447%
44	7.043	976	977	980	rBB2	381	241	0.05%	0.007%
45	7.129	983	991	1001	rVV7	5652	14541	3.13%	0.400%
46	7.306	1012	1020	1036	rBV2	95668	215522	46.35%	5.924%
47	7.446	1041	1043	1045	rVB	403	292	0.06%	0.008%
48	7.482	1045	1049	1051	rBB	413	476	0.10%	0.013%
49	7.604	1064	1069	1072	rBV2	272	550	0.12%	0.015%
50	7.763	1094	1095	1096	rBV2	187	108	0.02%	0.003%
51	7.824	1104	1105	1109	rBV	179	280	0.06%	0.008%
52	8.086	1145	1148	1149	rBV2	175	150	0.03%	0.004%
53	8.165	1159	1161	1162	rBV2	223	211	0.05%	0.006%
54	8.324	1181	1187	1198	rBV	49098	84513	18.18%	2.323%
55	8.494	1213	1215	1217	rBV	328	261	0.06%	0.007%
56	8.568	1226	1227	1229	rVB	213	116	0.02%	0.003%
57	8.647	1234	1240	1249	rBV	205150	328061	70.56%	9.018%
58	8.891	1276	1280	1282	rBV2	262	340	0.07%	0.009%
59	8.952	1285	1290	1305	rVV	34880	55036	11.84%	1.513%
60	9.281	1340	1344	1346	rVB3	702	856	0.18%	0.024%
61	9.384	1356	1361	1378	rVV	163030	250646	53.91%	6.890%
62	9.787	1424	1427	1429	rBV2	271	394	0.08%	0.011%
63	9.848	1435	1437	1440	rBV2	182	252	0.05%	0.007%
64	9.939	1448	1452	1454	rBV2	253	377	0.08%	0.010%
65	10.055	1465	1471	1479	rBV	308182	428365	92.13%	11.775%
66	10.506	1543	1545	1548	rBV	330	299	0.06%	0.008%
67	10.640	1566	1567	1570	rBV2	332	408	0.09%	0.011%
68	10.957	1614	1619	1622	rBV	345	567	0.12%	0.016%
69	10.988	1622	1624	1627	rVV	199	132	0.03%	0.004%
70	11.037	1631	1632	1634	rBV	252	130	0.03%	0.004%
71	11.189	1652	1657	1666	rBV	199280	257090	55.29%	7.067%
72	11.616	1725	1727	1729	rVB	158	119	0.03%	0.003%
73	11.756	1748	1750	1754	rBV	304	474	0.10%	0.013%
74	11.933	1776	1779	1782	rBV2	191	295	0.06%	0.008%
75	12.024	1789	1794	1803	rBV	251706	323855	69.65%	8.902%
76	12.158	1815	1816	1819	rBV	358	399	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042718.D
 Acq On : 30 Jul 2024 01:53
 Operator : JC/MD
 Sample : P3389-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.219	1822	1826	1831	rBV3	4908	6819	1.47%	0.187%
78	12.317	1837	1842	1856	rVB	212664	273992	58.93%	7.531%
79	12.408	1856	1857	1859	rVB	430	220	0.05%	0.006%
80	12.427	1859	1860	1861	rBV	331	200	0.04%	0.005%
81	12.512	1872	1874	1876	rVB	291	201	0.04%	0.006%
82	12.683	1900	1902	1906	rBV	230	374	0.08%	0.010%
83	12.713	1906	1907	1909	rBV	160	152	0.03%	0.004%
84	12.878	1933	1934	1935	rBV	291	166	0.04%	0.005%
85	13.055	1960	1963	1965	rVB	196	165	0.04%	0.005%
86	13.079	1965	1967	1970	rBV	225	227	0.05%	0.006%
87	13.207	1985	1988	1991	rBB2	214	292	0.06%	0.008%
88	13.237	1991	1993	1997	rBV	248	315	0.07%	0.009%
89	13.573	2046	2048	2049	rBV	242	148	0.03%	0.004%
90	13.792	2082	2084	2086	rBV2	237	222	0.05%	0.006%
91	13.853	2091	2094	2097	rBV2	215	304	0.07%	0.008%
92	14.054	2125	2127	2129	rBV	207	240	0.05%	0.007%
93	14.127	2136	2139	2141	rBV2	276	246	0.05%	0.007%
94	14.152	2141	2143	2146	rVB	384	354	0.08%	0.010%
95	14.195	2146	2150	2152	rBV2	303	460	0.10%	0.013%
96	14.274	2161	2163	2164	rBV	175	111	0.02%	0.003%
97	14.475	2192	2196	2199	rBV2	324	652	0.14%	0.018%
98	14.566	2209	2211	2213	rBV2	228	274	0.06%	0.008%
99	14.865	2258	2260	2261	rBV2	121	107	0.02%	0.003%
100	14.975	2277	2278	2280	rBV	270	195	0.04%	0.005%

Sum of corrected areas: 3638004




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042718.D
Acq On : 30 Jul 2024 01:53
Operator : JC/MD
Sample : P3389-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

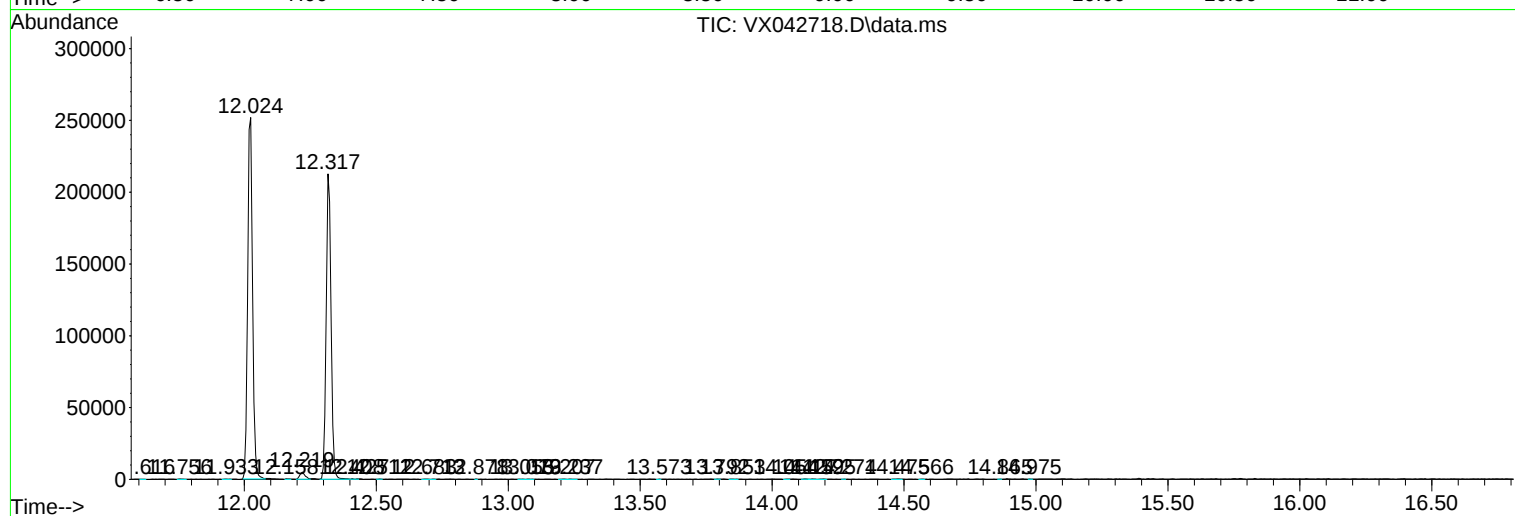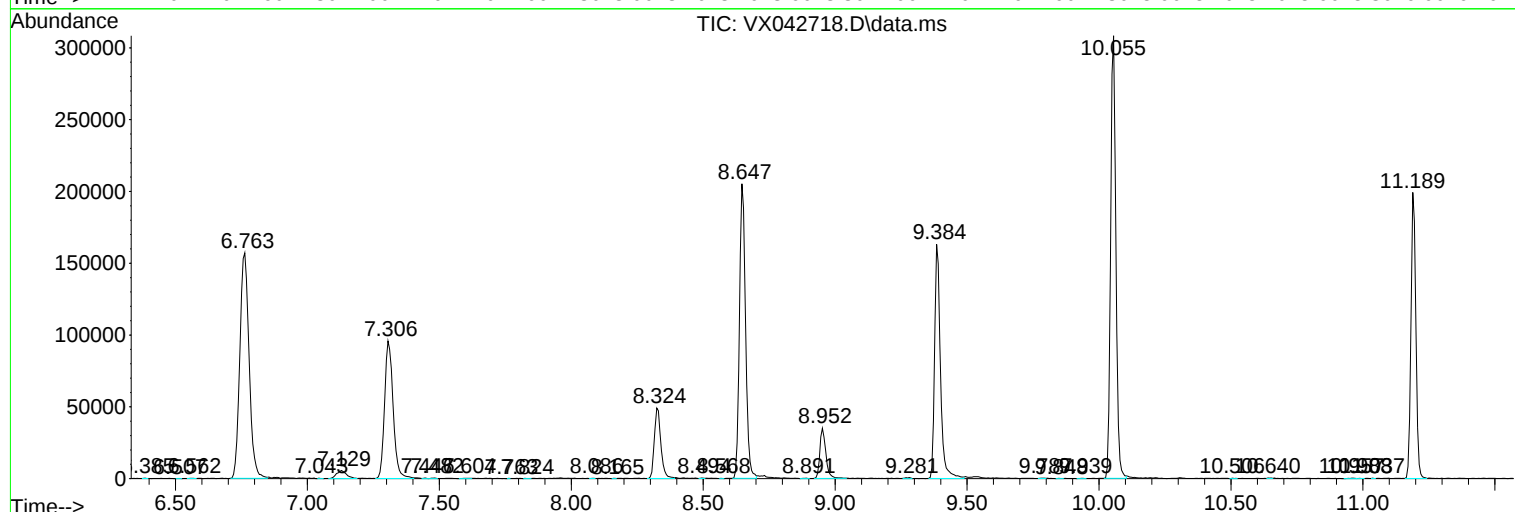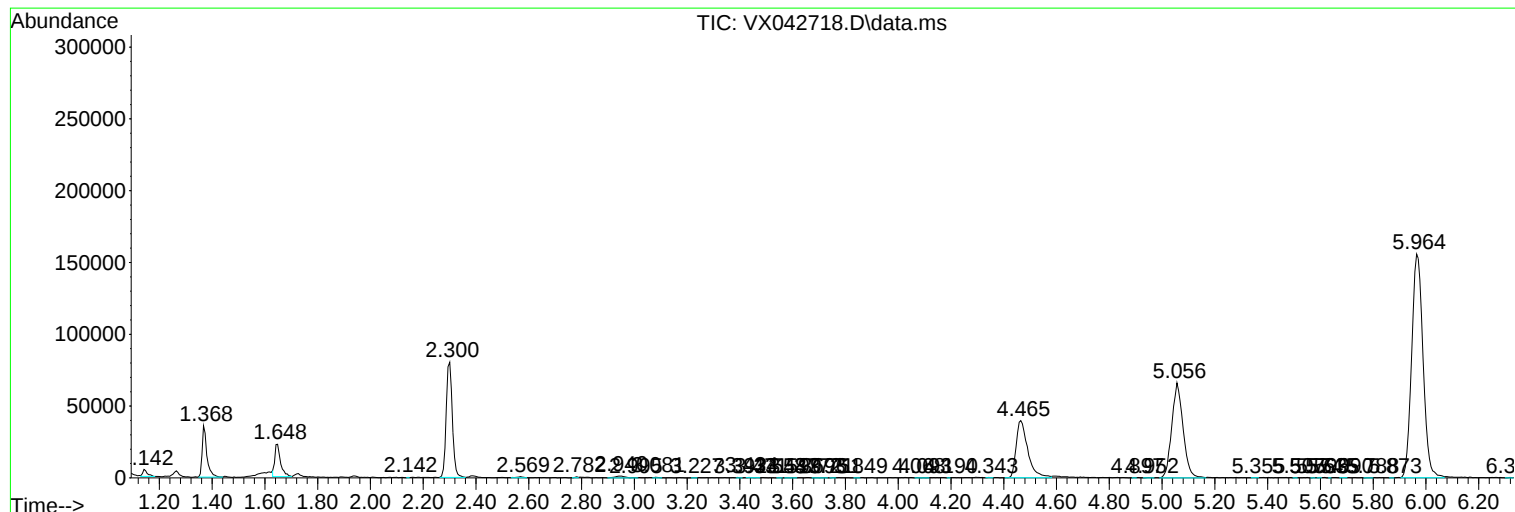

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042718.D
Acq On : 30 Jul 2024 01:53
Operator : JC/MD
Sample : P3389-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042718.D
Acq On : 30 Jul 2024 01:53
Operator : JC/MD
Sample : P3389-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc