

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042721.D
 Acq On : 30 Jul 2024 03:03
 Operator : JC/MD
 Sample : P3388-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	19	rVB	10752	13162	0.45%	0.199%
2	1.368	43	46	58	rVB	34479	45965	1.56%	0.695%
3	2.166	175	177	178	rBV	468	226	0.01%	0.003%
4	2.300	192	199	209	rBV	76374	120754	4.10%	1.827%
5	2.477	225	228	229	rBV	198	180	0.01%	0.003%
6	2.532	236	237	238	rBV	229	146	0.00%	0.002%
7	2.550	238	240	241	rVV	290	184	0.01%	0.003%
8	2.660	257	258	263	rBV	214	235	0.01%	0.004%
9	2.709	264	266	271	rVB2	305	229	0.01%	0.003%
10	2.776	271	277	281	rBV2	956	1799	0.06%	0.027%
11	2.940	300	304	305	rBV2	644	823	0.03%	0.012%
12	3.008	313	315	317	rBV	235	231	0.01%	0.003%
13	3.099	322	330	336	rVV4	2475	4993	0.17%	0.076%
14	3.172	341	342	344	rBV4	139	139	0.00%	0.002%
15	3.337	367	369	370	rBV	220	128	0.00%	0.002%
16	3.379	374	376	378	rBV	144	148	0.01%	0.002%
17	3.398	378	379	380	rBV	241	98	0.00%	0.001%
18	3.440	383	386	387	rBV	582	526	0.02%	0.008%
19	3.562	405	406	408	rVB	268	125	0.00%	0.002%
20	3.593	408	411	414	rVB	253	321	0.01%	0.005%
21	3.629	414	417	419	rBV	161	207	0.01%	0.003%
22	3.709	429	430	433	rBB	127	122	0.00%	0.002%
23	3.739	433	435	439	rBB	195	195	0.01%	0.003%
24	3.824	445	449	451	rBB	107	138	0.00%	0.002%
25	3.934	465	467	470	rBV	271	209	0.01%	0.003%
26	3.965	470	472	473	rBV	231	131	0.00%	0.002%
27	4.111	493	496	498	rVB2	271	313	0.01%	0.005%
28	4.129	498	499	501	rBV	176	105	0.00%	0.002%
29	4.160	501	504	505	rBV	185	136	0.00%	0.002%
30	4.306	522	528	532	rBV3	673	1486	0.05%	0.022%
31	4.483	546	557	578	rBV3	99164	329420	11.17%	4.983%
32	4.849	614	617	622	rBV	217	421	0.01%	0.006%
33	5.056	638	651	670	rBV	63211	192435	6.53%	2.911%
34	5.294	688	690	691	rBV	218	111	0.00%	0.002%
35	5.330	694	696	698	rBV	164	148	0.01%	0.002%
36	5.458	713	717	720	rBV3	645	1026	0.03%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042721.D
 Acq On : 30 Jul 2024 03:03
 Operator : JC/MD
 Sample : P3388-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.507	724	725	728	rVB3	359	188	0.01%	0.003%
38	5.556	729	733	735	rBV	404	448	0.02%	0.007%
39	5.659	748	750	753	rBV	225	283	0.01%	0.004%
40	5.885	784	787	789	rBV	250	350	0.01%	0.005%
41	5.964	790	800	818	rVV2	149779	455070	15.43%	6.884%
42	6.422	871	875	878	rBV2	240	367	0.01%	0.006%
43	6.452	878	880	884	rVV2	239	199	0.01%	0.003%
44	6.519	889	891	895	rBV2	235	325	0.01%	0.005%
45	6.665	912	915	916	rBV	162	173	0.01%	0.003%
46	6.763	922	931	949	rBV	148277	359182	12.18%	5.433%
47	7.123	980	990	1012	rBV	1342891	2948526	100.00%	44.602%
48	7.306	1014	1020	1030	rVV	94200	202406	6.86%	3.062%
49	7.604	1068	1069	1070	rBV	157	104	0.00%	0.002%
50	7.915	1118	1120	1122	rBV	194	134	0.00%	0.002%
51	8.025	1137	1138	1141	rBV2	297	206	0.01%	0.003%
52	8.214	1166	1169	1170	rBV2	235	270	0.01%	0.004%
53	8.324	1182	1187	1201	rBV	49299	84262	2.86%	1.275%
54	8.476	1210	1212	1214	rBV	229	249	0.01%	0.004%
55	8.647	1234	1240	1249	rBV	195984	313050	10.62%	4.735%
56	8.952	1285	1290	1300	rBV	35234	54419	1.85%	0.823%
57	9.159	1323	1324	1325	rBV	181	108	0.00%	0.002%
58	9.281	1340	1344	1346	rBV2	851	1002	0.03%	0.015%
59	9.384	1356	1361	1376	rBV	169661	257575	8.74%	3.896%
60	9.878	1440	1442	1443	rBV	288	157	0.01%	0.002%
61	9.927	1447	1450	1453	rBV2	268	311	0.01%	0.005%
62	10.055	1465	1471	1482	rBV	284682	400248	13.57%	6.055%
63	10.305	1509	1512	1516	rVB3	1492	2086	0.07%	0.032%
64	10.415	1529	1530	1532	rBV3	166	110	0.00%	0.002%
65	10.537	1548	1550	1551	rBV	173	109	0.00%	0.002%
66	10.622	1562	1564	1565	rBV	198	120	0.00%	0.002%
67	10.652	1565	1569	1575	rVB4	933	1383	0.05%	0.021%
68	10.884	1605	1607	1609	rVB	199	105	0.00%	0.002%
69	11.152	1648	1651	1652	rBV	218	206	0.01%	0.003%
70	11.189	1652	1657	1668	rVV	202323	261139	8.86%	3.950%
71	11.305	1674	1676	1678	rBV	460	299	0.01%	0.005%
72	11.384	1686	1689	1690	rBV2	316	298	0.01%	0.005%
73	11.793	1754	1756	1758	rBV	270	223	0.01%	0.003%
74	11.811	1758	1759	1761	rBV	205	130	0.00%	0.002%
75	11.872	1767	1769	1771	rBV	223	193	0.01%	0.003%
76	11.921	1774	1777	1781	rBV	363	472	0.02%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042721.D
 Acq On : 30 Jul 2024 03:03
 Operator : JC/MD
 Sample : P3388-11
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20S6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.969	1781	1785	1788	rBV2	184	289	0.01%	0.004%
78	12.024	1788	1794	1801	rBV	214705	286907	9.73%	4.340%
79	12.219	1822	1826	1831	rBV2	4164	5465	0.19%	0.083%
80	12.317	1837	1842	1852	rBV	183770	248288	8.42%	3.756%
81	12.475	1865	1868	1873	rBV	245	432	0.01%	0.007%
82	12.524	1875	1876	1878	rVV	226	152	0.01%	0.002%
83	12.567	1880	1883	1885	rBV	249	250	0.01%	0.004%
84	12.707	1903	1906	1908	rBV2	280	334	0.01%	0.005%
85	12.829	1924	1926	1928	rBV	229	229	0.01%	0.003%
86	13.085	1966	1968	1975	rVB	449	537	0.02%	0.008%
87	13.146	1975	1978	1981	rBV2	306	405	0.01%	0.006%
88	13.274	1997	1999	2001	rBV	197	167	0.01%	0.003%
89	13.323	2006	2007	2009	rBV	168	169	0.01%	0.003%
90	13.469	2027	2031	2032	rBV	175	215	0.01%	0.003%
91	13.853	2092	2094	2096	rBV	233	223	0.01%	0.003%
92	13.871	2096	2097	2098	rBV	242	126	0.00%	0.002%
93	14.067	2127	2129	2130	rBV	197	111	0.00%	0.002%
94	14.109	2134	2136	2138	rVB	326	230	0.01%	0.003%
95	14.146	2138	2142	2144	rBV2	267	489	0.02%	0.007%
96	14.664	2225	2227	2228	rBV	189	165	0.01%	0.002%
97	14.896	2261	2265	2266	rBV2	255	372	0.01%	0.006%
98	16.145	2466	2470	2473	rBV2	481	742	0.03%	0.011%
99	16.536	2531	2534	2536	rBV	396	465	0.02%	0.007%
100	16.639	2549	2551	2554	rBV	385	451	0.02%	0.007%


Sum of corrected areas: 6610713

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042721.D
Acq On : 30 Jul 2024 03:03
Operator : JC/MD
Sample : P3388-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

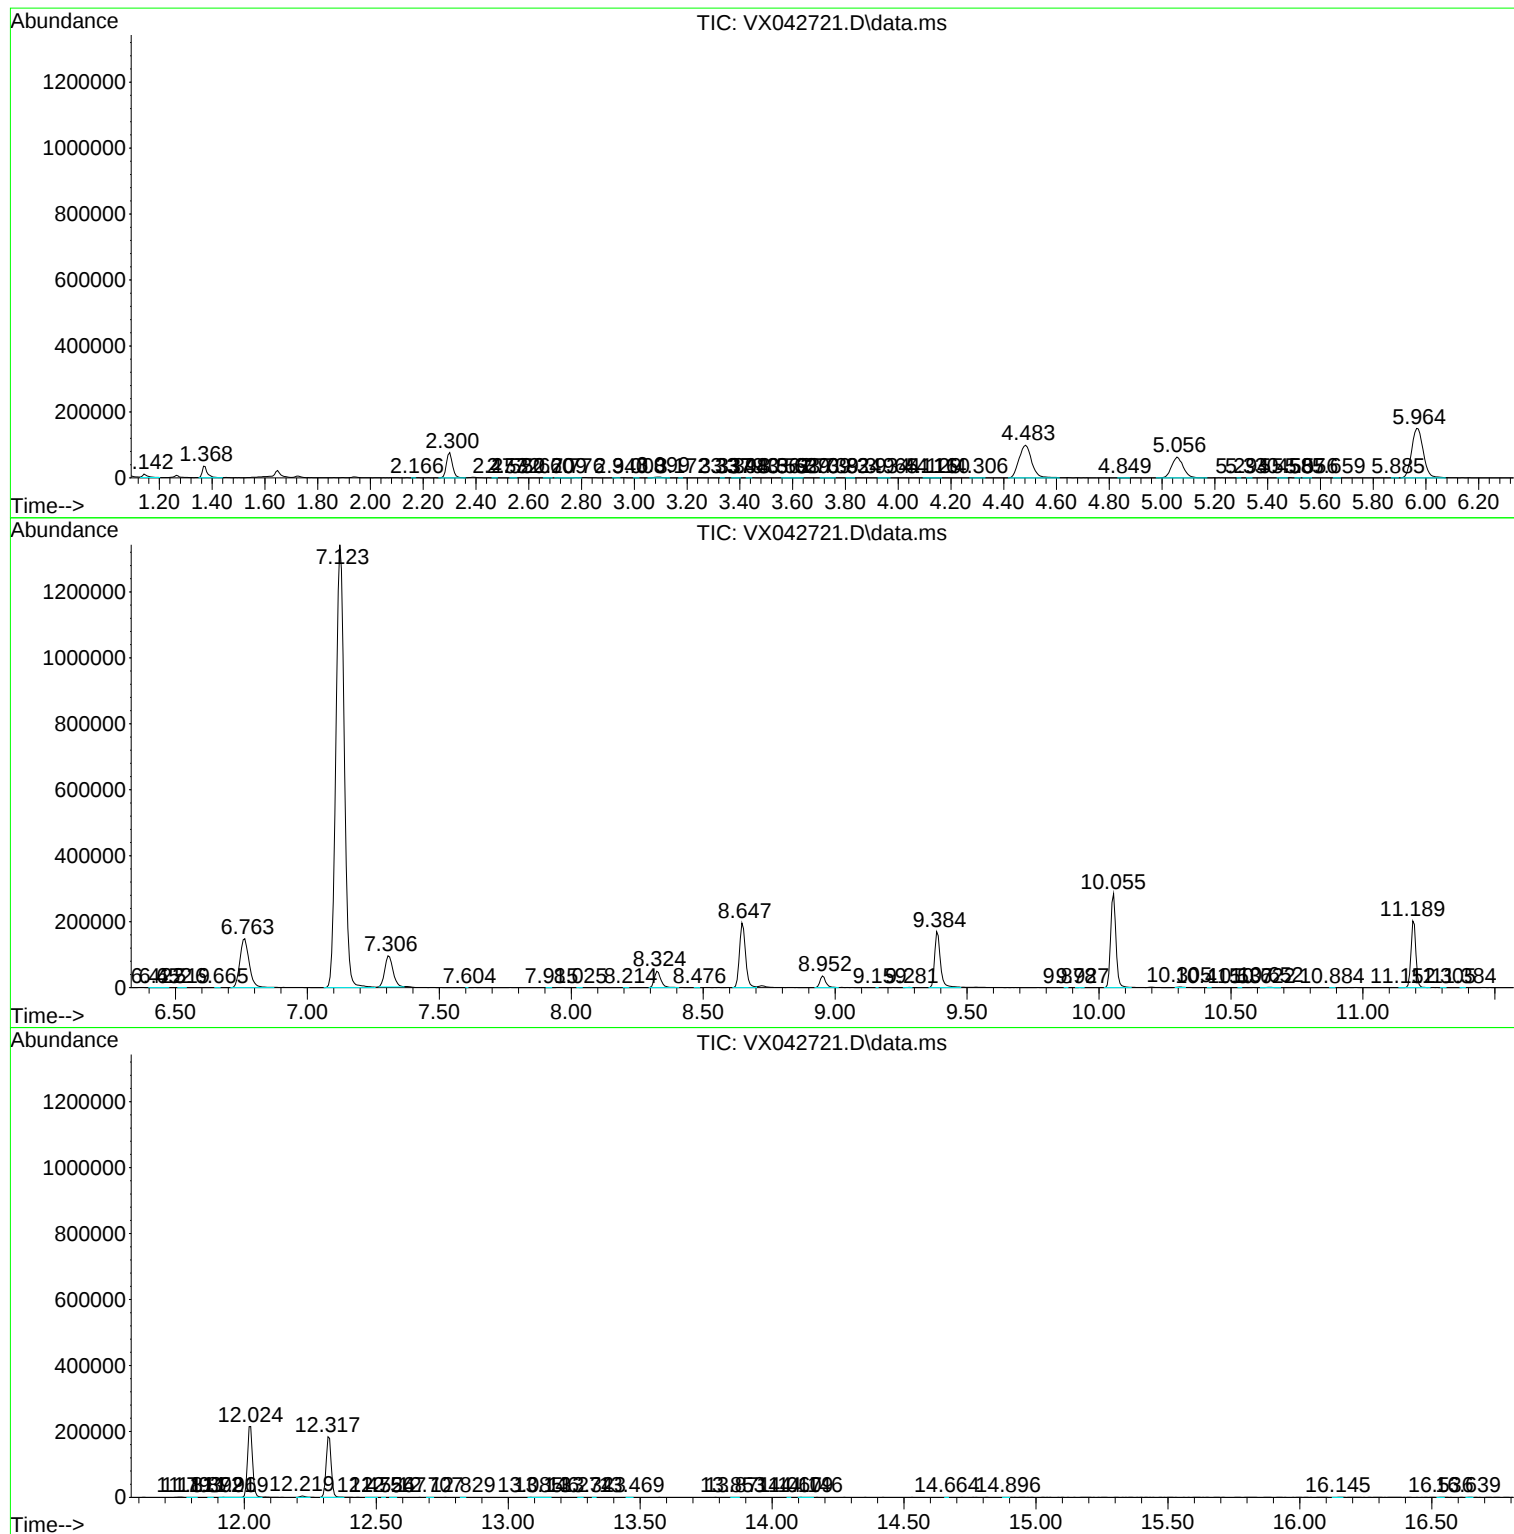

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042721.D
Acq On : 30 Jul 2024 03:03
Operator : JC/MD
Sample : P3388-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042721.D
Acq On : 30 Jul 2024 03:03
Operator : JC/MD
Sample : P3388-11
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20S6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc