

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042723.D
 Acq On : 30 Jul 2024 03:49
 Operator : JC/MD
 Sample : P3388-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042723.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	20	rVB	11368	14377	0.47%	0.196%
2	1.368	43	46	58	rVB	34803	47558	1.54%	0.649%
3	1.648	89	92	100	rVB	26497	33675	1.09%	0.459%
4	2.300	192	199	210	rVB	79180	129810	4.20%	1.771%
5	2.508	230	233	241	rVB2	484	1099	0.04%	0.015%
6	2.575	241	244	246	rBB	224	240	0.01%	0.003%
7	2.605	246	249	253	rBV2	254	512	0.02%	0.007%
8	2.733	267	270	271	rBV2	177	210	0.01%	0.003%
9	2.794	274	280	282	rBV3	760	1428	0.05%	0.019%
10	2.947	298	305	311	rBV4	1166	2689	0.09%	0.037%
11	3.087	322	328	338	rVB3	7837	15831	0.51%	0.216%
12	3.227	348	351	354	rBV	163	191	0.01%	0.003%
13	3.300	358	363	364	rBV	273	325	0.01%	0.004%
14	3.373	370	375	376	rBV	237	334	0.01%	0.005%
15	3.446	382	387	391	rVB3	534	1137	0.04%	0.016%
16	3.538	400	402	406	rBV	150	183	0.01%	0.002%
17	3.672	423	424	430	rBV2	199	347	0.01%	0.005%
18	3.782	440	442	443	rBV2	172	146	0.00%	0.002%
19	3.855	452	454	457	rBB2	149	172	0.01%	0.002%
20	3.971	471	473	474	rBV	291	249	0.01%	0.003%
21	4.026	481	482	485	rBV	287	271	0.01%	0.004%
22	4.050	485	486	489	rVV	248	198	0.01%	0.003%
23	4.129	494	499	500	rBV2	183	228	0.01%	0.003%
24	4.233	512	516	518	rBV2	215	247	0.01%	0.003%
25	4.294	520	526	527	rBV2	556	782	0.03%	0.011%
26	4.483	546	557	574	rBV2	251477	714201	23.12%	9.743%
27	4.733	596	598	599	rBV	485	261	0.01%	0.004%
28	4.928	628	630	633	rVB	279	267	0.01%	0.004%
29	5.062	638	652	667	rBV2	62879	195863	6.34%	2.672%
30	5.342	695	698	701	rBV	384	520	0.02%	0.007%
31	5.666	748	751	756	rBV2	264	486	0.02%	0.007%
32	5.830	776	778	779	rVB	271	164	0.01%	0.002%
33	5.964	790	800	814	rBV2	152735	458444	14.84%	6.254%
34	6.190	836	837	838	rBV2	324	171	0.01%	0.002%
35	6.330	858	860	863	rBV2	207	208	0.01%	0.003%
36	6.440	877	878	881	rBV2	192	168	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042723.D
 Acq On : 30 Jul 2024 03:49
 Operator : JC/MD
 Sample : P3388-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.574	898	900	902	rBV2	216	189	0.01%	0.003%
38	6.684	917	918	920	rBV2	181	136	0.00%	0.002%
39	6.763	922	931	943	rBV	155457	374389	12.12%	5.107%
40	7.123	979	990	1013	rBV	1433270	3088475	100.00%	42.131%
41	7.312	1014	1021	1037	rVV	97535	223083	7.22%	3.043%
42	7.440	1040	1042	1043	rBV2	483	322	0.01%	0.004%
43	7.696	1082	1084	1086	rBV	217	199	0.01%	0.003%
44	7.714	1086	1087	1091	rVV	226	253	0.01%	0.003%
45	8.007	1133	1135	1138	rVB	372	239	0.01%	0.003%
46	8.135	1151	1156	1160	rBV2	189	364	0.01%	0.005%
47	8.189	1163	1165	1167	rVV	198	198	0.01%	0.003%
48	8.250	1172	1175	1178	rBV	252	332	0.01%	0.005%
49	8.324	1181	1187	1206	rVV	49871	86749	2.81%	1.183%
50	8.488	1210	1214	1215	rBV2	243	305	0.01%	0.004%
51	8.525	1218	1220	1225	rVB2	659	769	0.02%	0.010%
52	8.567	1225	1227	1228	rBV	288	235	0.01%	0.003%
53	8.647	1234	1240	1250	rBV	204996	331810	10.74%	4.526%
54	8.903	1281	1282	1285	rBV	181	166	0.01%	0.002%
55	8.952	1285	1290	1299	rBV	35201	55090	1.78%	0.751%
56	9.159	1321	1324	1327	rBV3	624	856	0.03%	0.012%
57	9.275	1341	1343	1346	rVB	448	445	0.01%	0.006%
58	9.384	1356	1361	1373	rBV	157102	242896	7.86%	3.313%
59	9.781	1424	1426	1428	rBV2	303	309	0.01%	0.004%
60	9.915	1447	1448	1450	rBV	197	133	0.00%	0.002%
61	10.000	1461	1462	1464	rBV	216	150	0.00%	0.002%
62	10.055	1465	1471	1489	rVV	305619	425593	13.78%	5.806%
63	10.189	1491	1493	1498	rBV2	649	907	0.03%	0.012%
64	10.311	1508	1513	1520	rBV3	747	1333	0.04%	0.018%
65	10.396	1525	1527	1530	rBV	271	185	0.01%	0.003%
66	10.488	1540	1542	1543	rBV2	196	147	0.00%	0.002%
67	10.579	1552	1557	1559	rBV	289	493	0.02%	0.007%
68	10.701	1576	1577	1580	rVB	206	194	0.01%	0.003%
69	10.793	1590	1592	1593	rBV	199	146	0.00%	0.002%
70	10.896	1608	1609	1612	rVB	383	292	0.01%	0.004%
71	10.933	1612	1615	1617	rBV	178	246	0.01%	0.003%
72	10.963	1619	1620	1624	rVB	289	301	0.01%	0.004%
73	11.006	1624	1627	1628	rBV	301	351	0.01%	0.005%
74	11.189	1652	1657	1668	rBV	199774	256259	8.30%	3.496%
75	11.732	1741	1746	1747	rBV	232	342	0.01%	0.005%
76	11.750	1748	1749	1755	rVB2	455	626	0.02%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
 Data File : VX042723.D
 Acq On : 30 Jul 2024 03:49
 Operator : JC/MD
 Sample : P3388-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.805	1755	1758	1760	rBV	246	275	0.01%	0.004%
78	12.018	1788	1793	1803	rBV	246971	324839	10.52%	4.431%
79	12.170	1815	1818	1819	rBV	216	224	0.01%	0.003%
80	12.219	1822	1826	1831	rBV2	5624	7579	0.25%	0.103%
81	12.317	1837	1842	1852	rBV	207652	274306	8.88%	3.742%
82	12.481	1867	1869	1870	rBV	369	299	0.01%	0.004%
83	12.555	1879	1881	1884	rBV	242	315	0.01%	0.004%
84	13.018	1955	1957	1961	rBV2	168	167	0.01%	0.002%
85	13.152	1976	1979	1980	rBV	219	271	0.01%	0.004%
86	13.384	2013	2017	2018	rBV	252	271	0.01%	0.004%
87	13.542	2040	2043	2044	rBV	245	281	0.01%	0.004%
88	13.591	2050	2051	2053	rBV	232	174	0.01%	0.002%
89	14.024	2120	2122	2124	rBV	267	279	0.01%	0.004%
90	14.176	2145	2147	2151	rBV2	355	403	0.01%	0.005%
91	14.213	2151	2153	2154	rBV	305	198	0.01%	0.003%
92	14.365	2176	2178	2182	rBV2	344	371	0.01%	0.005%
93	14.396	2182	2183	2185	rBV	209	143	0.00%	0.002%
94	14.493	2197	2199	2200	rBV	231	177	0.01%	0.002%
95	14.627	2219	2221	2223	rBV	274	208	0.01%	0.003%
96	14.682	2228	2230	2232	rBV2	262	221	0.01%	0.003%
97	14.847	2255	2257	2260	rVB2	381	418	0.01%	0.006%
98	14.877	2260	2262	2264	rBV	310	282	0.01%	0.004%
99	15.121	2300	2302	2304	rBV2	273	208	0.01%	0.003%
100	15.853	2421	2422	2425	rBV3	321	280	0.01%	0.004%



Sum of corrected areas: 7330688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042723.D
Acq On : 30 Jul 2024 03:49
Operator : JC/MD
Sample : P3388-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

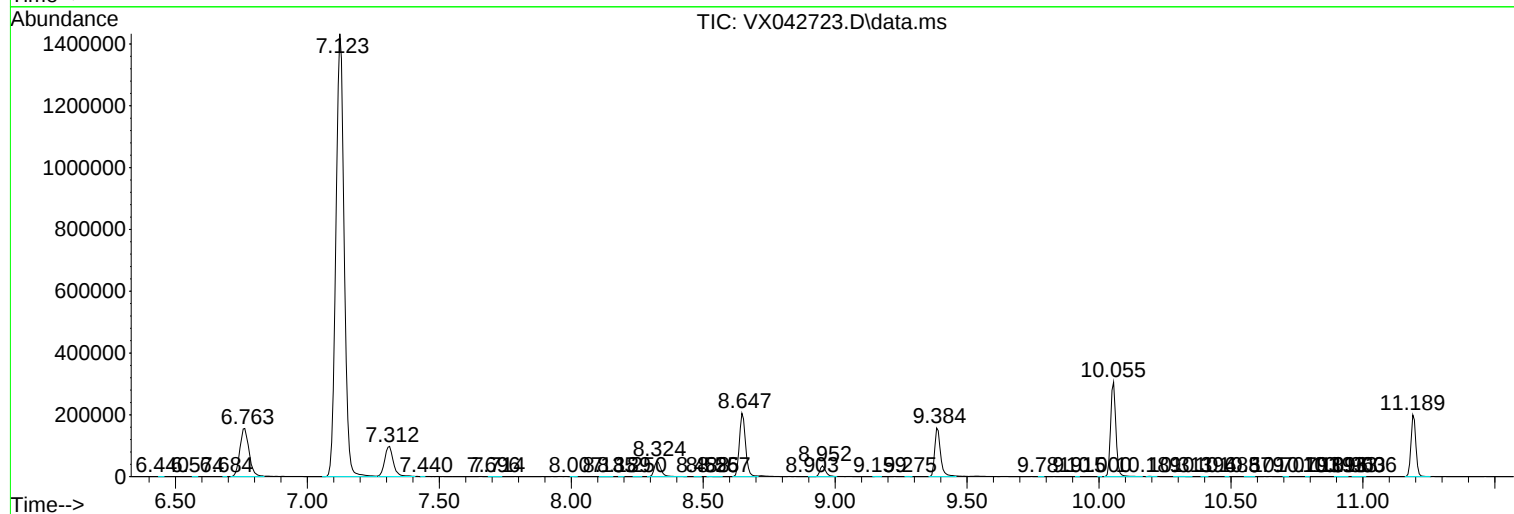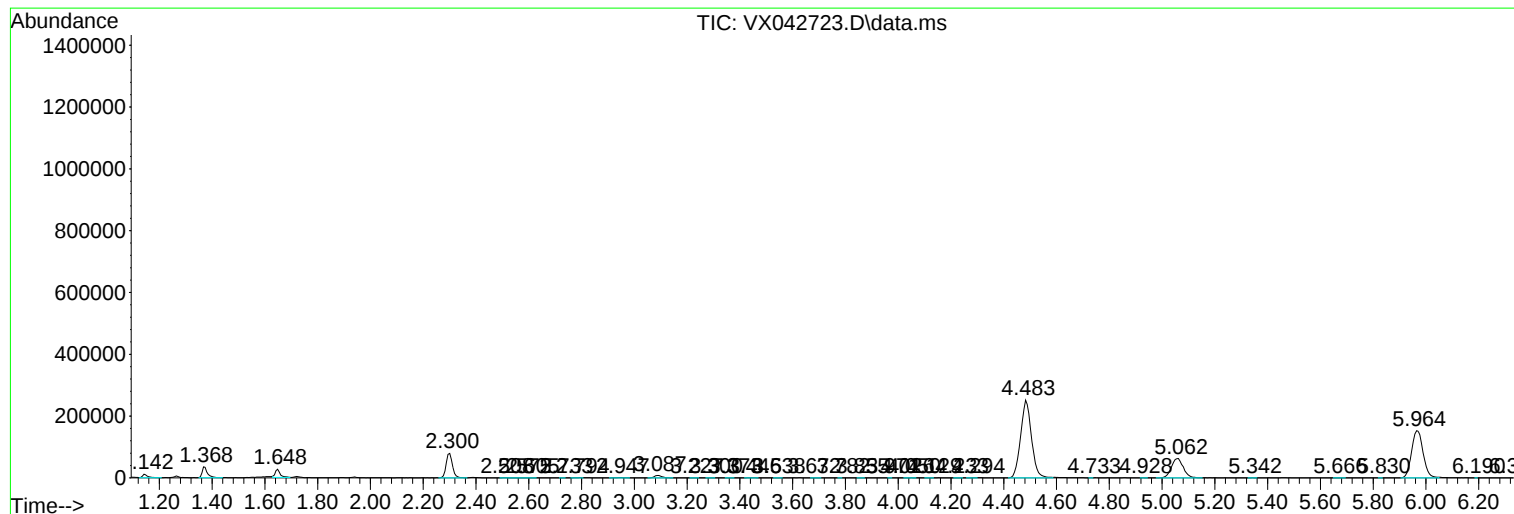

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042723.D
Acq On : 30 Jul 2024 03:49
Operator : JC/MD
Sample : P3388-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042723.D
Acq On : 30 Jul 2024 03:49
Operator : JC/MD
Sample : P3388-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc