
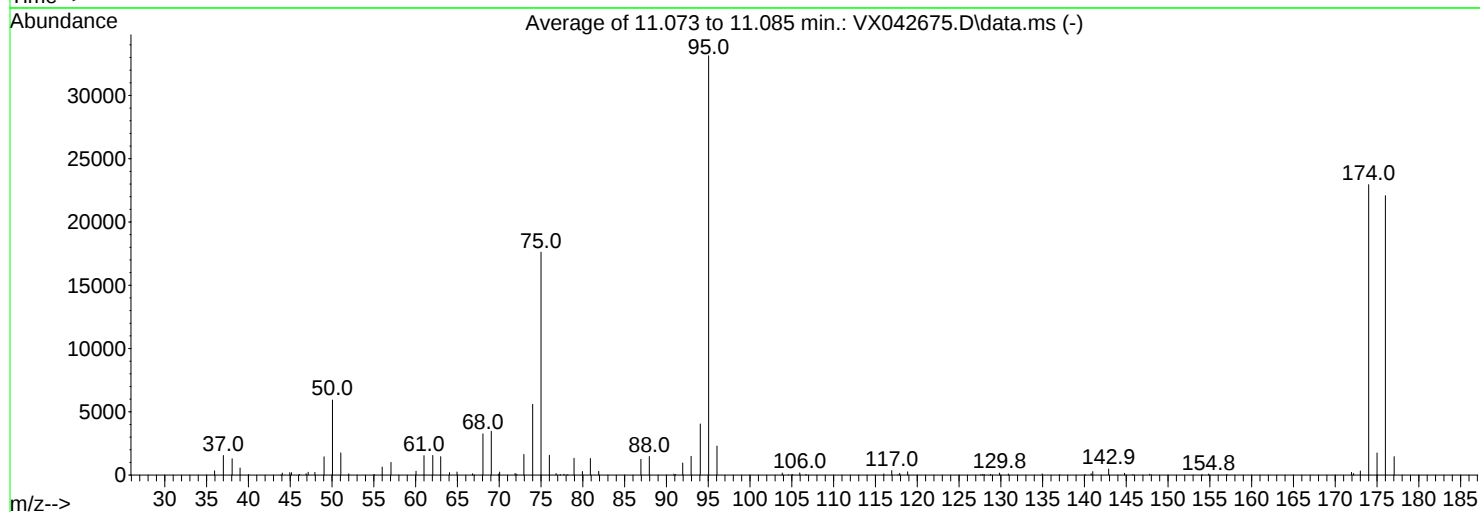


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072924\
Data File : VX042675.D
Acq On : 29 Jul 2024 07:48
Operator : JC/MD
Sample : BFB687
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB687

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM072624WMA.M
Title : VOC Analysis
Last Update : Tue Jul 30 02:11:54 2024

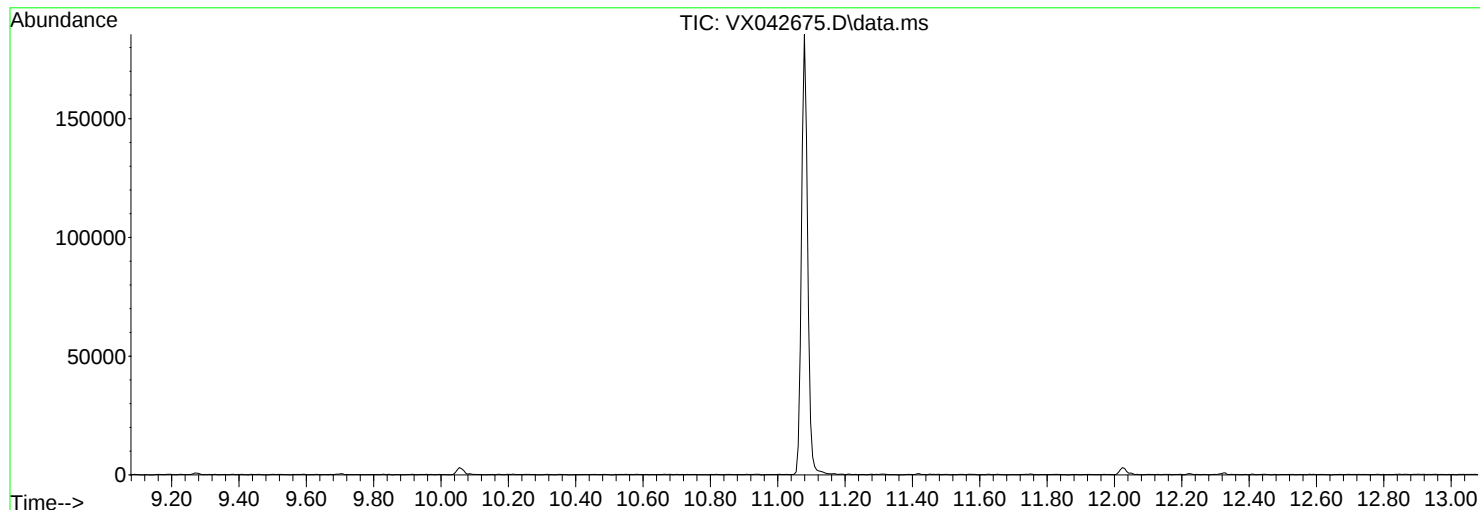

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	5935	PASS
75	95	30	80	53.2	17618	PASS
95	95	100	100	100.0	33139	PASS
96	95	5	9	6.9	2297	PASS
173	174	0.00	2	1.4	324	PASS
174	95	50	120	69.3	22955	PASS
175	174	5	9	7.6	1751	PASS
176	174	95	101	96.2	22083	PASS
177	176	5	9	6.6	1457	PASS

m/z	Abundance
40.00	85.0
43.90	95.0

Instrument :
MSVOA_X
ClientSampleId :
BFB687

m/z	Abundance
36.00	351.0
37.00	1552.0
38.00	1316.0
39.00	504.0
40.00	94.0
43.90	305.0
45.00	356.0
46.10	59.0
47.20	490.0
47.90	226.0
49.10	1326.0
50.10	5698.0
51.00	1773.0
52.00	65.0
55.10	71.0
56.00	511.0
57.00	992.0
60.00	265.0
61.00	1723.0
62.00	1419.0
63.00	1157.0
64.00	213.0
65.00	188.0
66.80	180.0
68.10	3000.0
69.00	3154.0
69.90	234.0
71.90	226.0
72.90	1660.0
74.00	5263.0
75.00	16752.0
76.00	1684.0
76.80	159.0
79.00	1236.0
80.00	234.0
80.90	1209.0
81.90	254.0
87.00	1143.0
87.90	1557.0
90.90	144.0
92.00	839.0
93.00	1264.0
94.00	3542.0
95.00	30288.0
96.10	2156.0
103.80	147.0
105.00	85.0
105.90	197.0
106.70	99.0
116.10	95.0
116.90	347.0
117.70	109.0
118.90	236.0
127.60	78.0
128.70	56.0
129.90	124.0
134.90	95.0
137.00	62.0
140.80	339.0
142.90	445.0
144.80	76.0
147.80	58.0
154.90	82.0
157.10	66.0
172.00	289.0
173.00	239.0
174.00	18272.0
175.00	1460.0
176.00	17152.0
177.00	1159.0

Instrument :
MSVOA_X
ClientSampleId :
BFB687

m/z	Abundance
35.90	320.0
37.00	1887.0
38.00	1357.0
39.00	641.0
40.10	149.0
44.10	234.0
44.90	240.0
45.20	218.0
46.10	107.0
46.90	337.0
47.90	213.0
49.10	1703.0
50.00	7426.0
51.00	1903.0
52.00	137.0
55.00	61.0
56.00	690.0
57.10	1212.0
60.00	274.0
61.00	1614.0
62.10	1811.0
63.00	1834.0
64.00	225.0
65.00	340.0
66.80	137.0
68.00	3723.0
69.10	4339.0
70.10	387.0
72.10	227.0
72.90	1937.0
74.00	6853.0
75.00	20240.0
76.00	1903.0
76.80	111.0
77.30	150.0
77.80	128.0
78.20	131.0
79.00	1612.0
80.00	341.0
80.90	1702.0
81.80	422.0
87.00	1500.0
87.90	1573.0
91.10	149.0
91.90	1154.0
93.00	1948.0
94.10	4720.0
95.10	40032.0
96.10	2693.0
103.90	202.0
105.10	86.0
106.00	172.0
106.70	84.0
115.90	125.0
117.00	466.0
117.90	294.0
118.90	308.0
127.80	141.0
128.80	115.0
129.80	205.0
131.00	135.0
134.90	99.0
141.00	370.0
142.90	650.0
144.80	217.0
145.80	73.0
147.80	148.0
154.10	65.0
154.80	103.0
172.20	362.0
173.00	410.0
174.00	27632.0
175.00	2109.0
176.00	26048.0
177.00	1759.0

Instrument :
MSVOA_X
ClientSampleId :
BFB687

m/z	Abundance
36.00	330.0
37.00	1204.0
38.10	1198.0
39.00	535.0
40.10	98.0
44.00	250.0
45.10	347.0
47.10	188.0
48.00	209.0
49.00	1305.0
50.00	4682.0
51.10	1586.0
52.00	85.0
56.00	696.0
57.00	799.0
60.10	378.0
61.00	1283.0
62.00	1423.0
63.00	1387.0
64.10	160.0
64.90	213.0
67.00	55.0
68.00	3053.0
69.00	2895.0
70.00	332.0
71.90	186.0
73.00	1293.0
74.00	4676.0
75.00	15863.0
76.00	1107.0
76.80	99.0
77.70	90.0
78.80	1140.0
79.80	286.0
80.90	1022.0
82.00	216.0
86.90	1111.0
88.00	1290.0
90.90	100.0
91.90	867.0
92.90	1238.0
94.00	3861.0
95.00	29096.0
96.00	2041.0
103.90	142.0
104.60	69.0
106.00	153.0
115.90	65.0
116.90	258.0
117.90	116.0
118.80	231.0
128.00	137.0
129.90	151.0
130.80	135.0
135.00	76.0
137.10	53.0
140.10	74.0
141.00	467.0
143.00	341.0
144.80	139.0
145.80	66.0
148.00	55.0
154.80	65.0
157.00	66.0
171.90	369.0
173.00	322.0
174.00	22960.0
175.00	1684.0
176.00	23048.0
177.10	1452.0

Instrument :
MSVOA_X
ClientSampleId :
BFB687