

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072925\
 Data File : VX047172.D
 Acq On : 29 Jul 2025 10:19
 Operator : JC/MD
 Sample : VX0729MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0729MBL01

Quant Time: Jul 30 01:12:34 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 22 03:59:51 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	234873	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	435500	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	430801	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	221028	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	176153	60.207	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	120.420%#
35) Dibromofluoromethane	5.391	113	145504	54.112	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	108.220%
50) Toluene-d8	8.647	98	536842	61.649	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	123.300%#
62) 4-Bromofluorobenzene	11.079	95	227628	60.658	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	121.320%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072925\
Data File : VX047172.D
Acq On : 29 Jul 2025 10:19
Operator : JC/MD
Sample : VX0729MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0729MBL01

Quant Time: Jul 30 01:12:34 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 22 03:59:51 2025
Response via : Initial Calibration




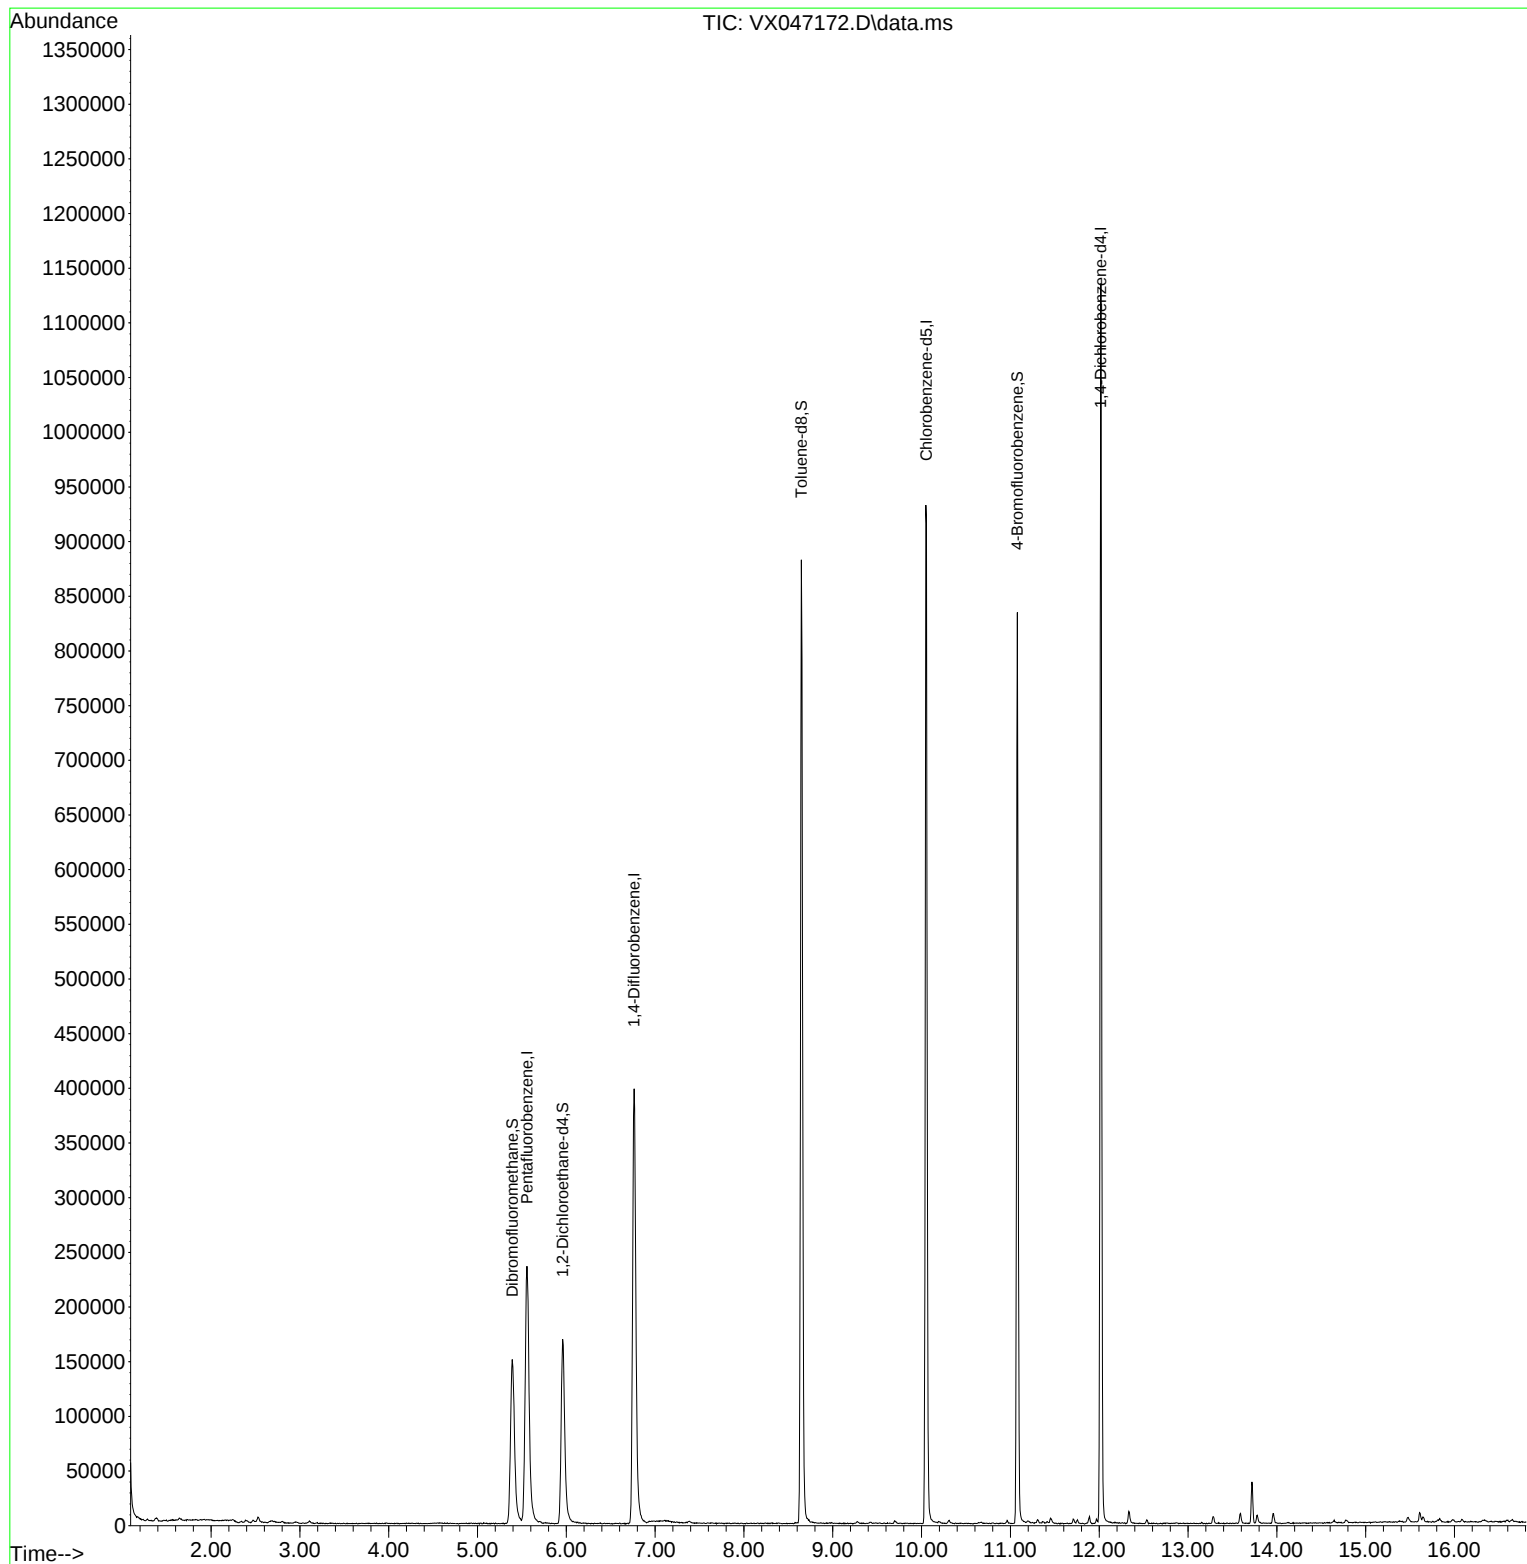


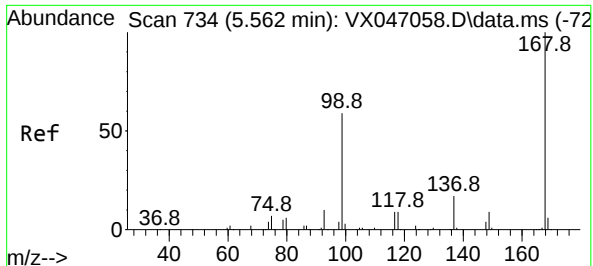

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 712
Delta R.T. -0.006 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19




Instrument :
MSVOA_X
ClientSampleId :
VX0729MBL01


Tgt Ion:168 Resp: 234873
Ion Ratio Lower Upper
168 100
99 61.5 48.0 72.0

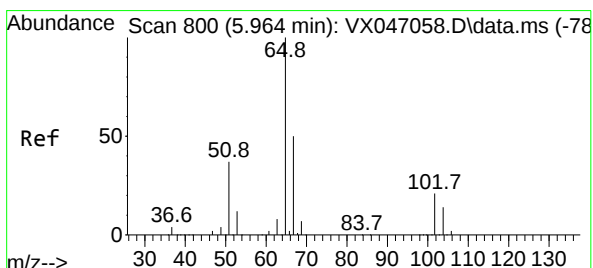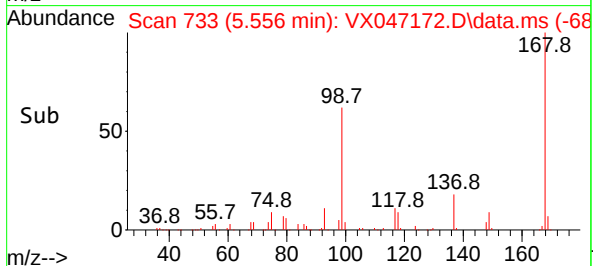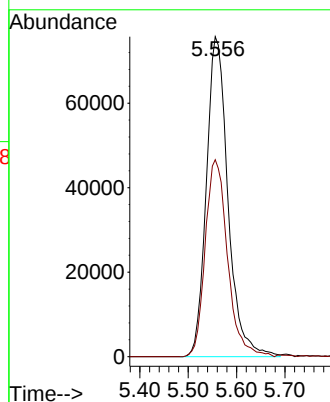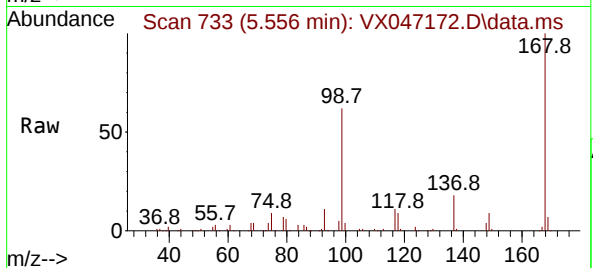

#33
1,2-Dichloroethane-d4
Concen: 60.207 ug/l
RT: 5.958 min Scan# 799
Delta R.T. -0.006 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19

Tgt Ion: 65 Resp: 176153
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.8


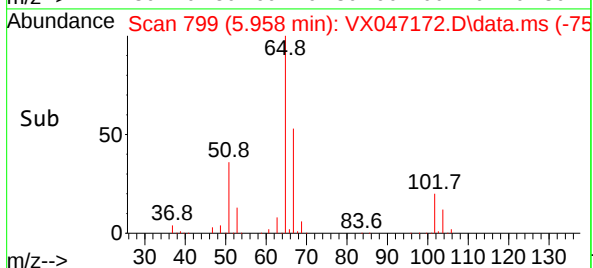
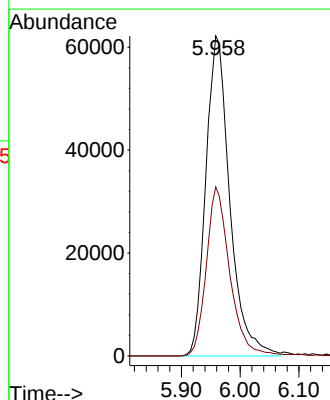
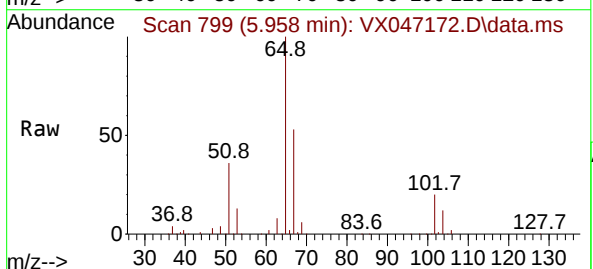


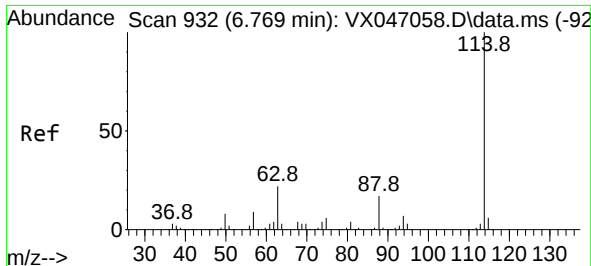

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19




Instrument :
MSVOA_X
ClientSampleId :
VX0729MBL01


Tgt Ion:114 Resp: 435500
Ion Ratio Lower Upper
114 100
63 22.5 0.0 43.2
88 17.8 0.0 33.8

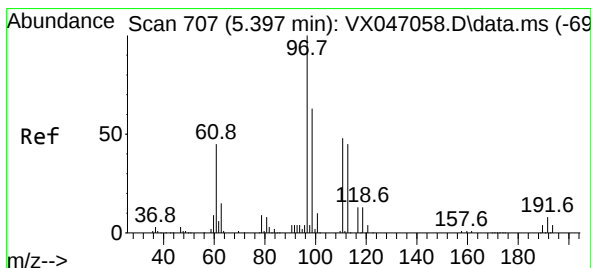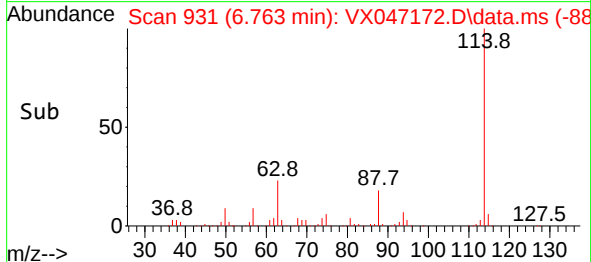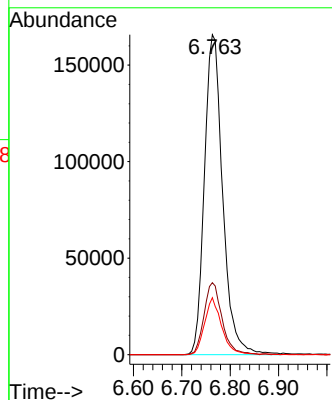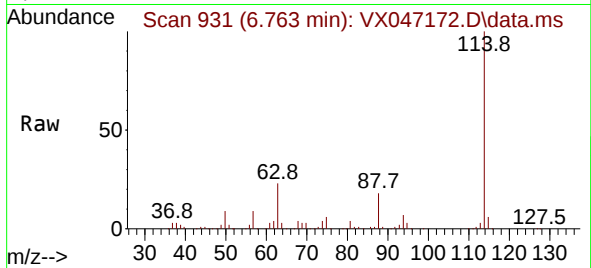

#35
Dibromofluoromethane
Concen: 54.112 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19

Tgt Ion:113 Resp: 145504
Ion Ratio Lower Upper
113 100
111 103.2 82.6 124.0
192 18.2 14.9 22.3


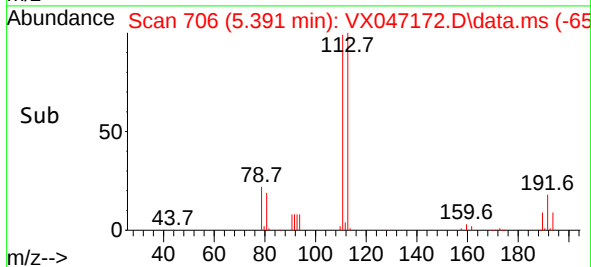
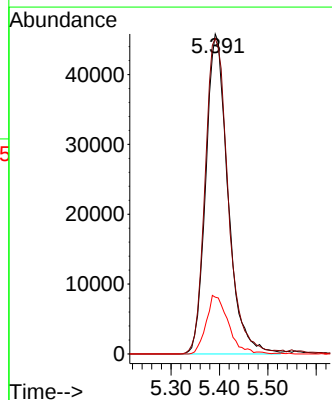
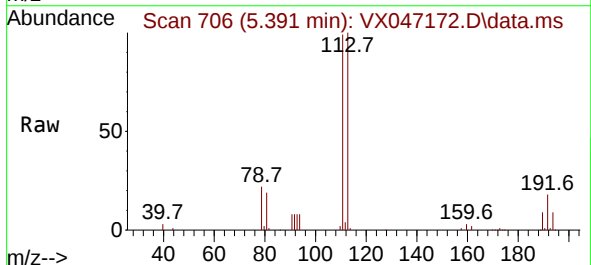


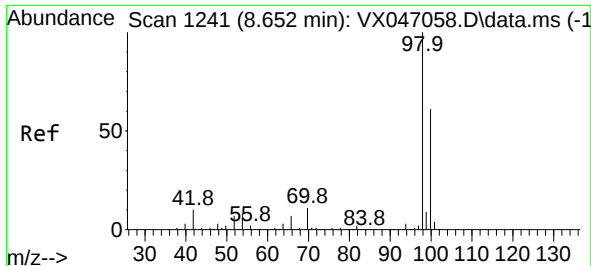

#50
Toluene-d8
Concen: 61.649 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19




Instrument :
MSVOA_X
ClientSampleId :
VX0729MBL01


Tgt Ion: 98 Resp: 536842
Ion Ratio Lower Upper
98 100
100 65.9 53.3 79.9

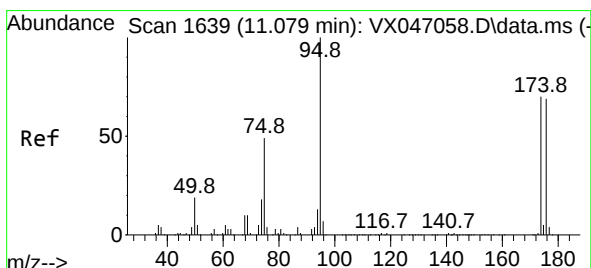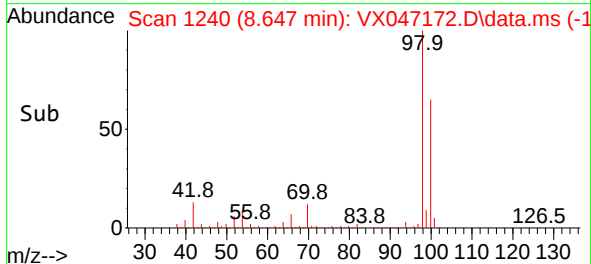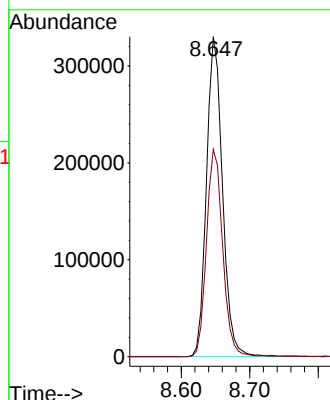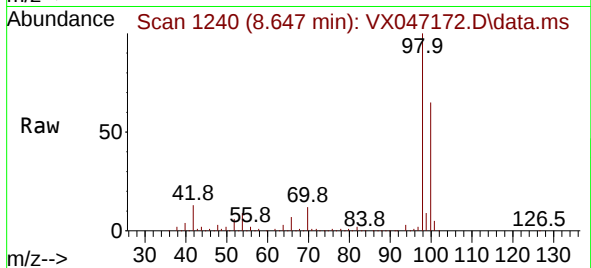

#62
4-Bromofluorobenzene
Concen: 60.658 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19

Tgt Ion: 95 Resp: 227628
Ion Ratio Lower Upper
95 100
174 72.0 0.0 144.6
176 70.3 0.0 139.6


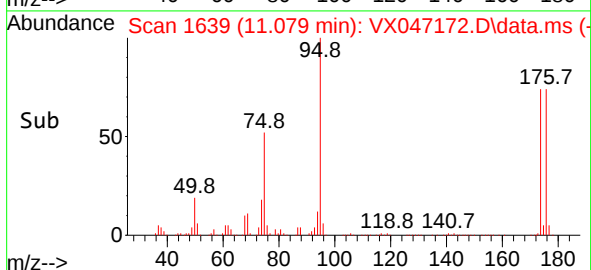
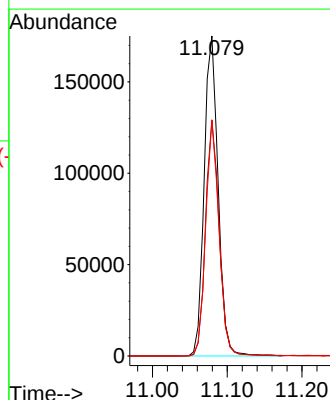
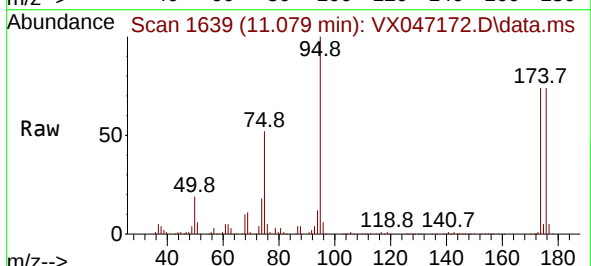


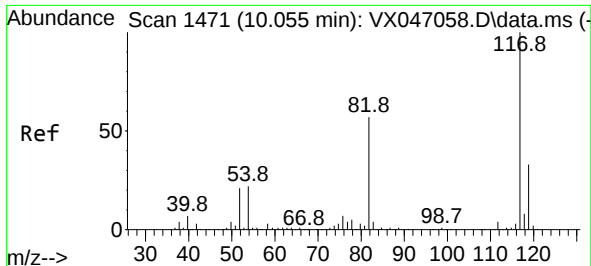

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19

Instrument :
MSVOA_X
ClientSampleId :
VX0729MBL01

Tgt Ion:117 Resp: 430801
Ion Ratio Lower Upper
117 100
82 55.5 45.4 68.2
119 31.1 26.1 39.1

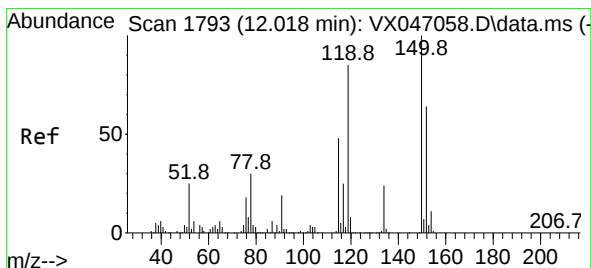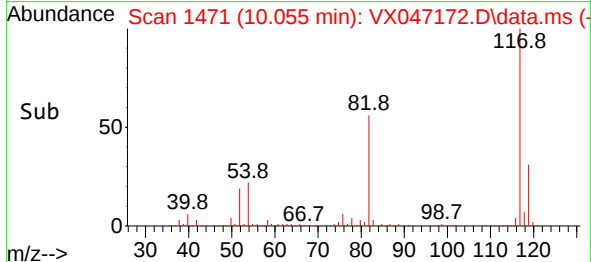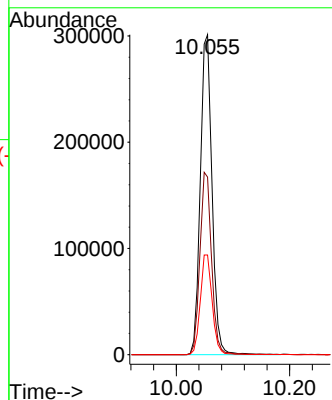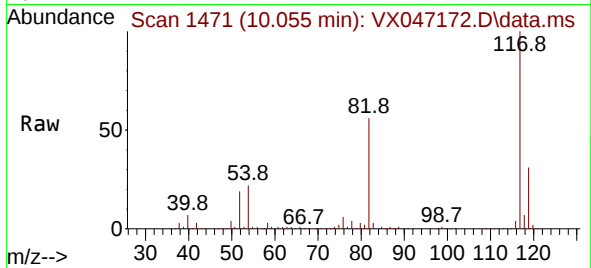

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX047172.D
Acq: 29 Jul 2025 10:19

Tgt Ion:152 Resp: 221028
Ion Ratio Lower Upper
152 100
115 64.1 45.6 136.7
150 160.1 0.0 354.6

