



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072925\
Data File : VX047170.D
Acq On : 29 Jul 2025 08:46
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Title : SW846 8260
Last Update : Tue Jul 22 03:59:51 2025

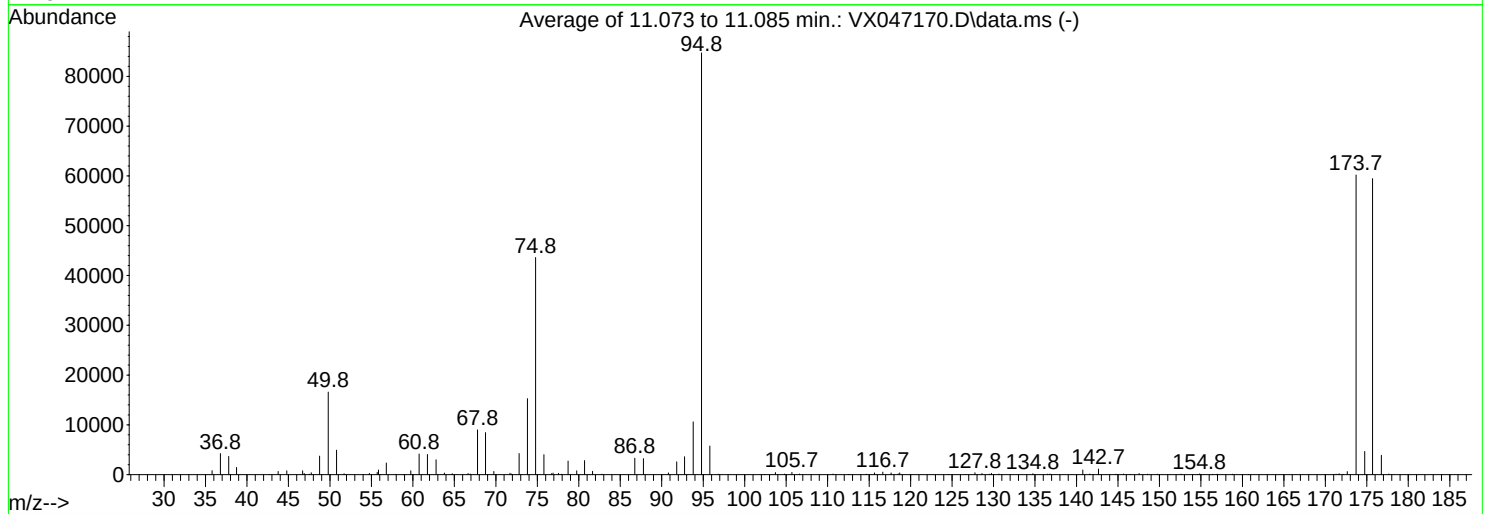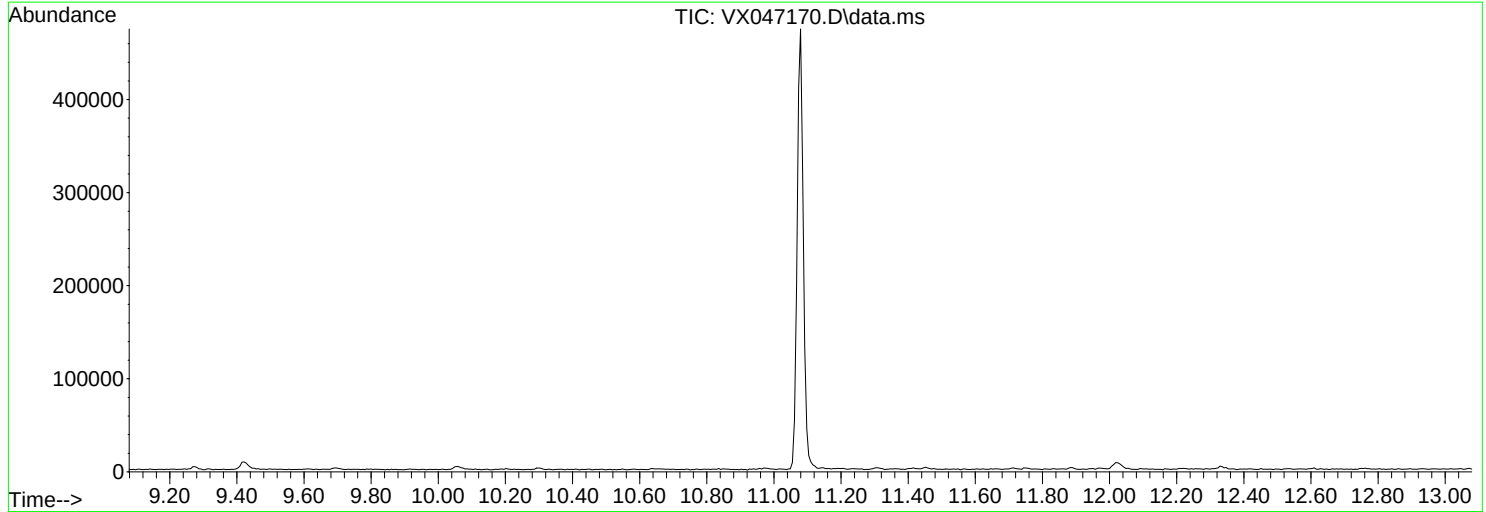

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	16571	PASS
75	95	30	60	51.5	43616	PASS
95	95	100	100	100.0	84717	PASS
96	95	5	9	6.8	5767	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	71.1	60195	PASS
175	174	5	9	7.8	4674	PASS
176	174	95	101	98.8	59464	PASS
177	176	5	9	6.5	3891	PASS