



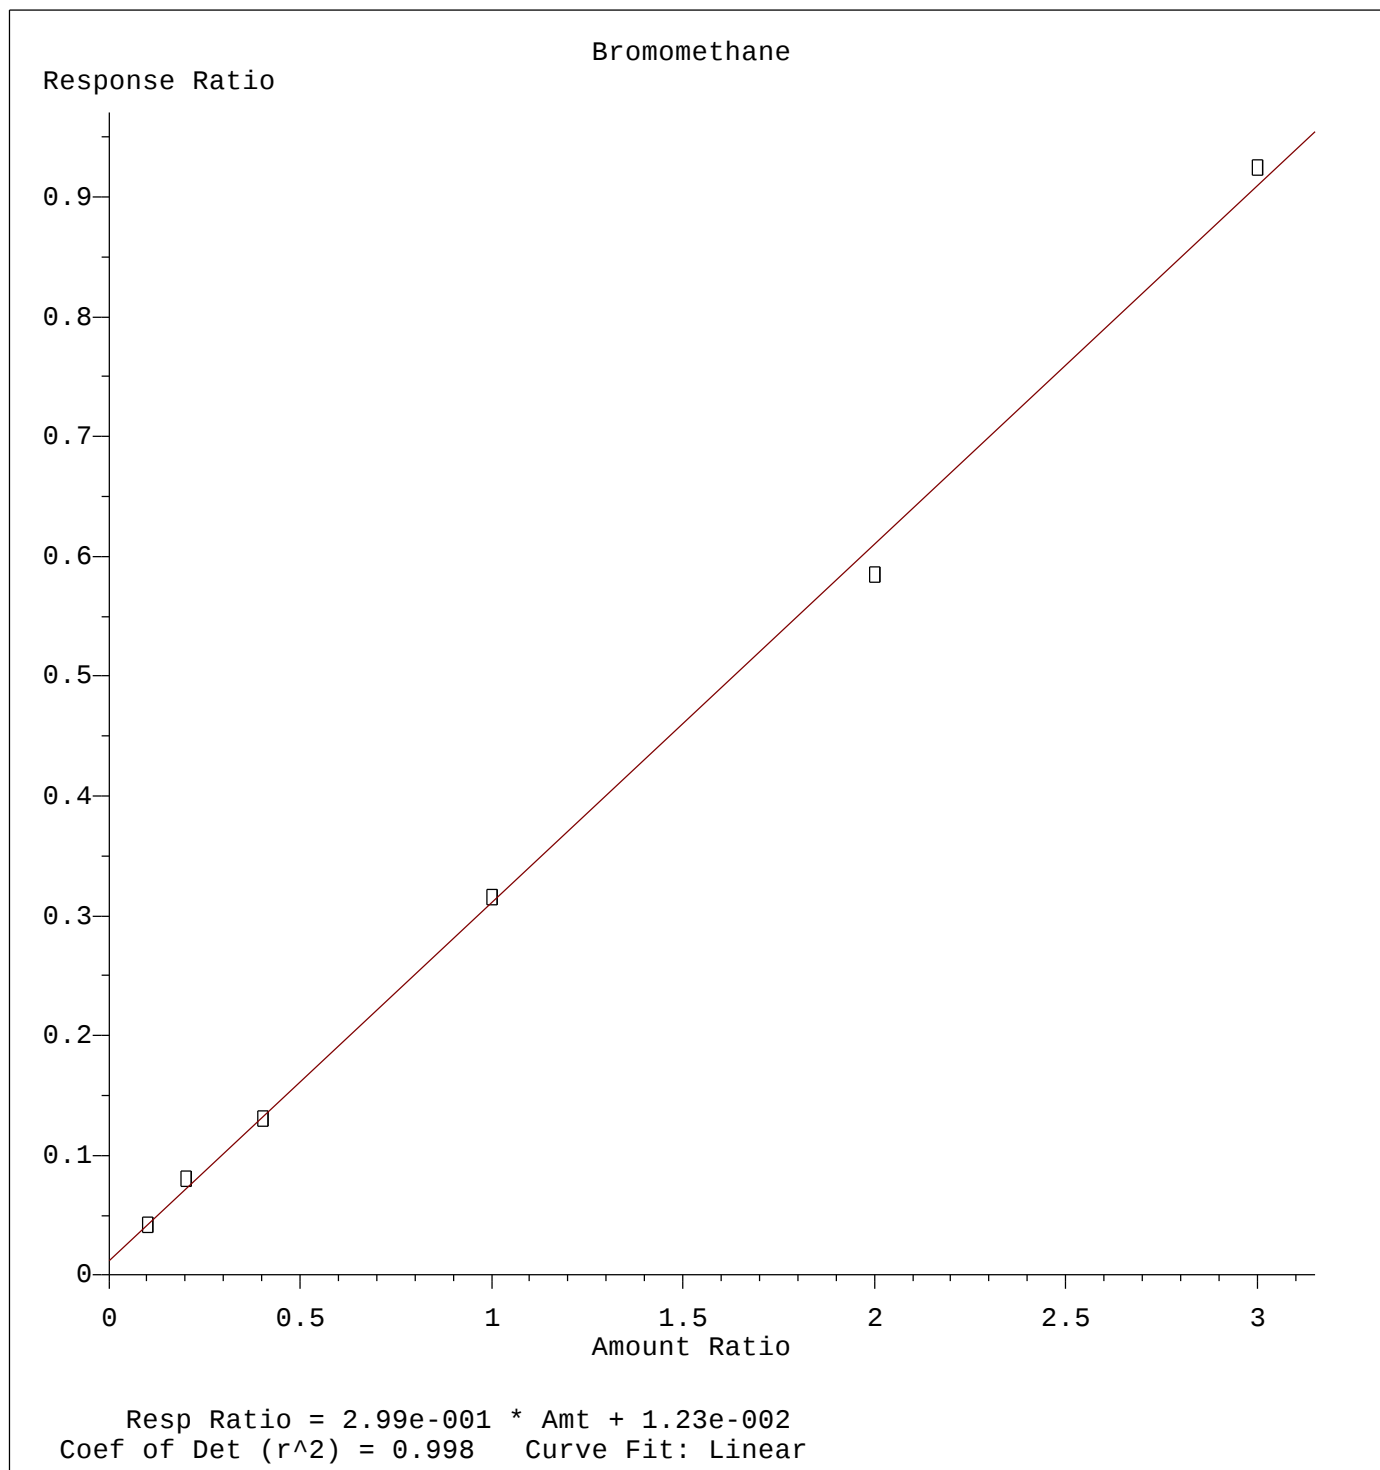

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X073018S.M
Calibration Table Last Updated: Wed Aug 01 16:45:53 2018

Methylene Chloride

Response Ratio

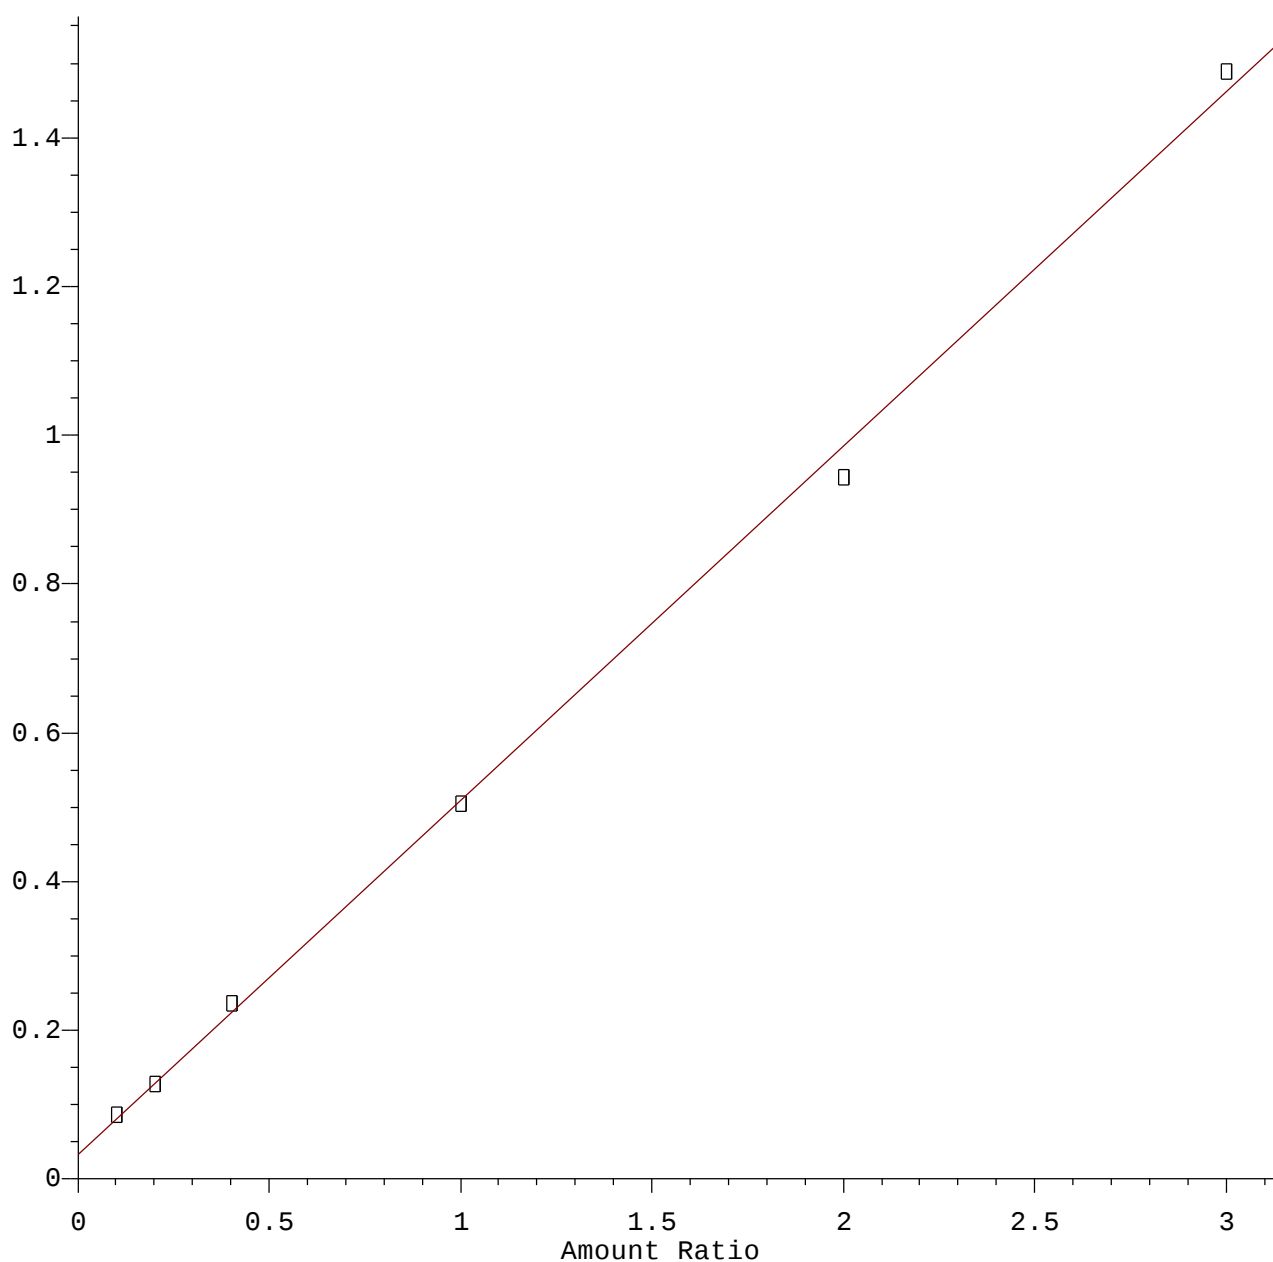


Resp Ratio = $4.76 \times 10^{-1} \times \text{Amt} + 3.24 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X073018S.M
Calibration Table Last Updated: Wed Aug 01 16:45:53 2018

2-Chloroethyl Vinyl ether

Response Ratio

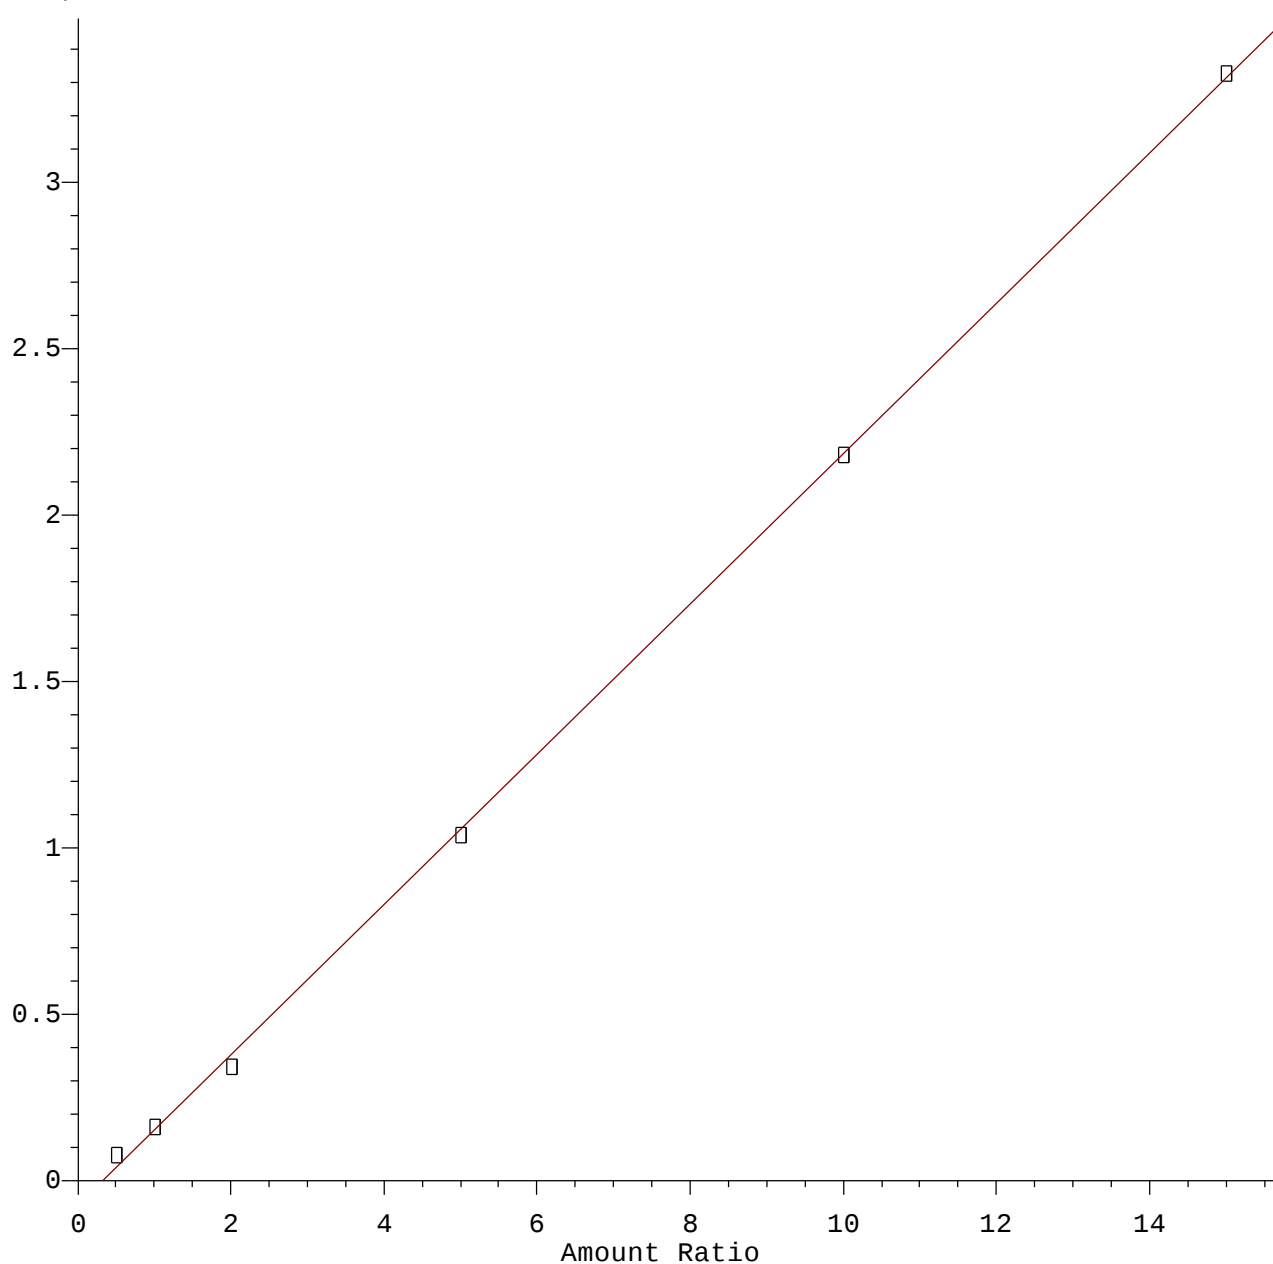

Resp Ratio = $2.26 \times 10^{-1} \times \text{Amt} - 7.29 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X073018S.M
Calibration Table Last Updated: Wed Aug 01 16:45:53 2018