


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX073018\
Data File : VX003724.D
Acq On : 30 Jul 2018 15:25
Operator : JC/SP
Sample : BFB
Misc : 5.00G/5.0mL/MSVOA X/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X073018S.M
Title : SW846 8260
Last Update : Wed Aug 01 16:45:53 2018

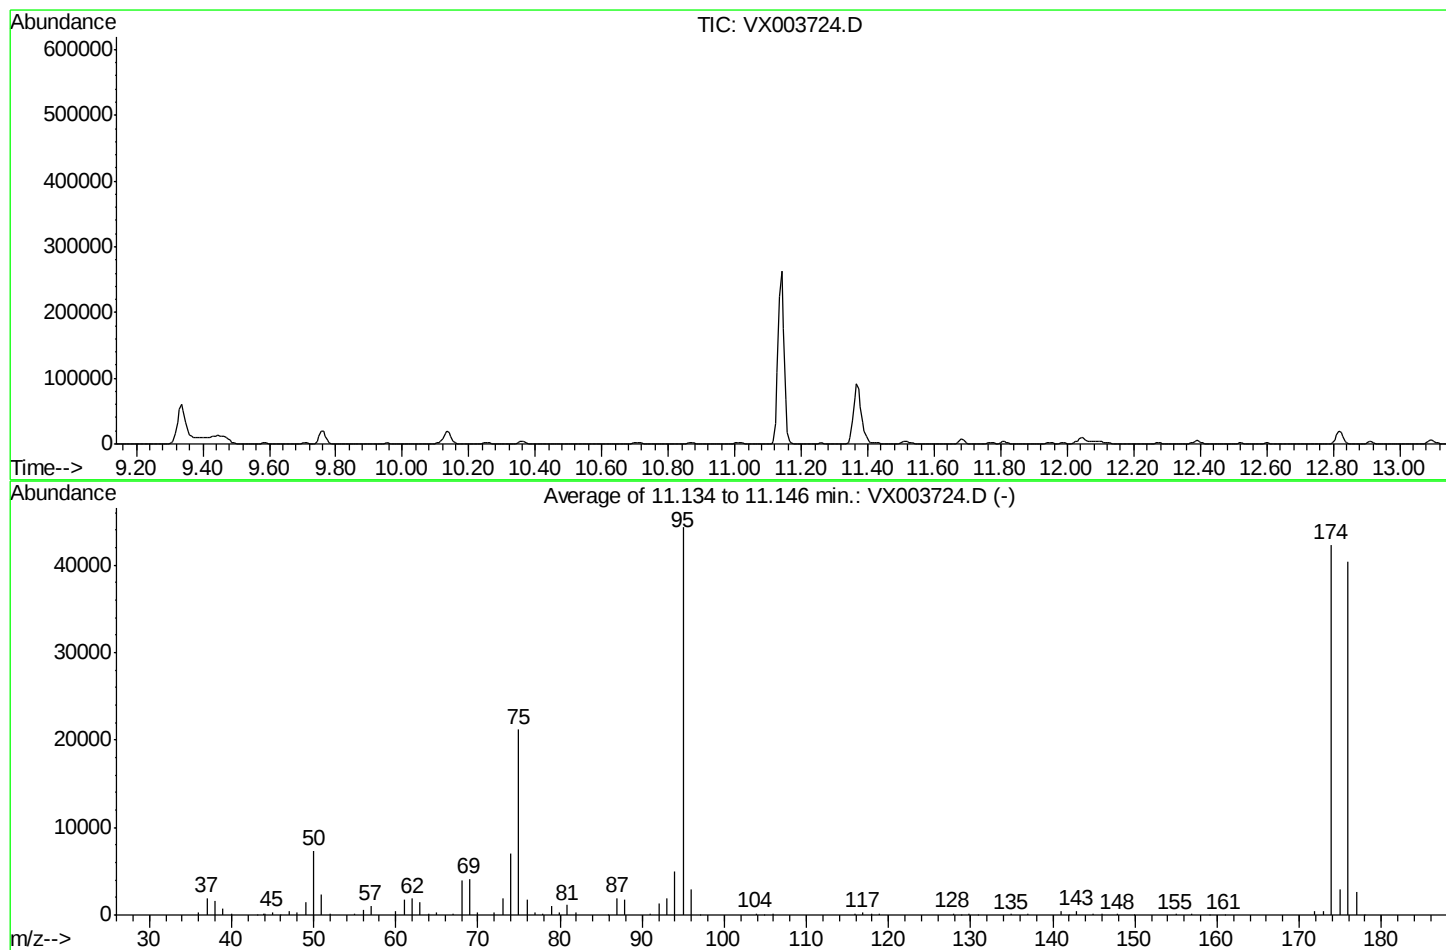

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	7320	PASS
75	95	30	60	47.9	21206	PASS
95	95	100	100	100.0	44304	PASS
96	95	5	9	6.7	2965	PASS
173	174	0.00	2	1.0	422	PASS
174	95	50	100	95.5	42309	PASS
175	174	5	9	6.9	2933	PASS
176	174	95	101	95.3	40328	PASS
177	176	5	9	6.6	2662	PASS