

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\WX073019\
 Data File : VX011204.D
 Acq On : 30 Jul 2019 18:50
 Operator : JC/SP
 Sample : K4026-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0674

Quant Time: Jul 31 08:42:03 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 24 05:39:23 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	213714	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	299602	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	261119	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	114624	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	104823	46.10	ug/l	0.00
Spiked Amount			Recovery	=	92.20%	
35) Dibromofluoromethane	5.50	113	89327	46.97	ug/l	0.00
Spiked Amount			Recovery	=	93.94%	
50) Toluene-d8	8.71	98	350706	49.17	ug/l	0.00
Spiked Amount			Recovery	=	98.34%	
62) 4-Bromofluorobenzene	11.13	95	110381	42.10	ug/l	0.00
Spiked Amount			Recovery	=	84.20%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Dichlorodifluoromethane	1.26	85	44	0.565	ug/l #	43
3) Chloromethane	1.33	50	420	0.214	ug/l	97
4) Vinyl Chloride	1.41	62	12653	6.312	ug/l	97
5) Bromomethane	1.65	94	608	0.538	ug/l #	57
6) Chloroethane	1.71	64	2230	1.751	ug/l #	46
11) Tert butyl alcohol	3.02	59	1657	3.129	ug/l #	92
12) 1,1-Dichloroethene	2.37	96	743	0.390	ug/l #	87
13) Acrolein	2.31	56	147	0.481	ug/l #	55
16) Acetone	2.44	43	1974	1.922	ug/l	88
21) trans-1,2-Dichloroethene	3.17	96	10716	5.305	ug/l	87
27) cis-1,2-Dichloroethene	4.60	96	484492	207.261	ug/l	89
29) Tetrahydrofuran	5.15	42	268	0.287	ug/l #	51
36) 1,1-Dichloropropene	5.66	75	14448	5.871	ug/l #	48
38) Carbon Tetrachloride	5.67	117	20058	7.822	ug/l #	16
40) Benzene	6.15	78	13716	1.819	ug/l	99
44) Trichloroethene	7.22	130	506	0.227	ug/l	84
49) 1,4-Dioxane	7.76	88	20	0.354	ug/l #	28
51) 4-Methyl-2-Pentanone	8.49	43	544	0.203	ug/l	88
60) Dibromochloromethane	9.34	129	38	2.543	ug/l #	11
65) Chlorobenzene	10.13	112	53018	9.886	ug/l	99
76) 1,2,3-Trichloropropane	11.13	75	56230	27.185	ug/l #	35
81) trans-1,4-Dichloro-2-buten	11.13	75	56230	67.371	ug/l #	11
88) 1,4-Dichlorobenzene	12.10	146	936	0.246	ug/l #	10
90) Hexachloroethane	12.75	117	348	0.320	ug/l #	6

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX073019\
Data File : VX011204.D
Acq On : 30 Jul 2019 18:50
Operator : JC/SP
Sample : K4026-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z3-0674

Quant Time: Jul 31 08:42:03 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 24 05:39:23 2019
Response via : Initial Calibration

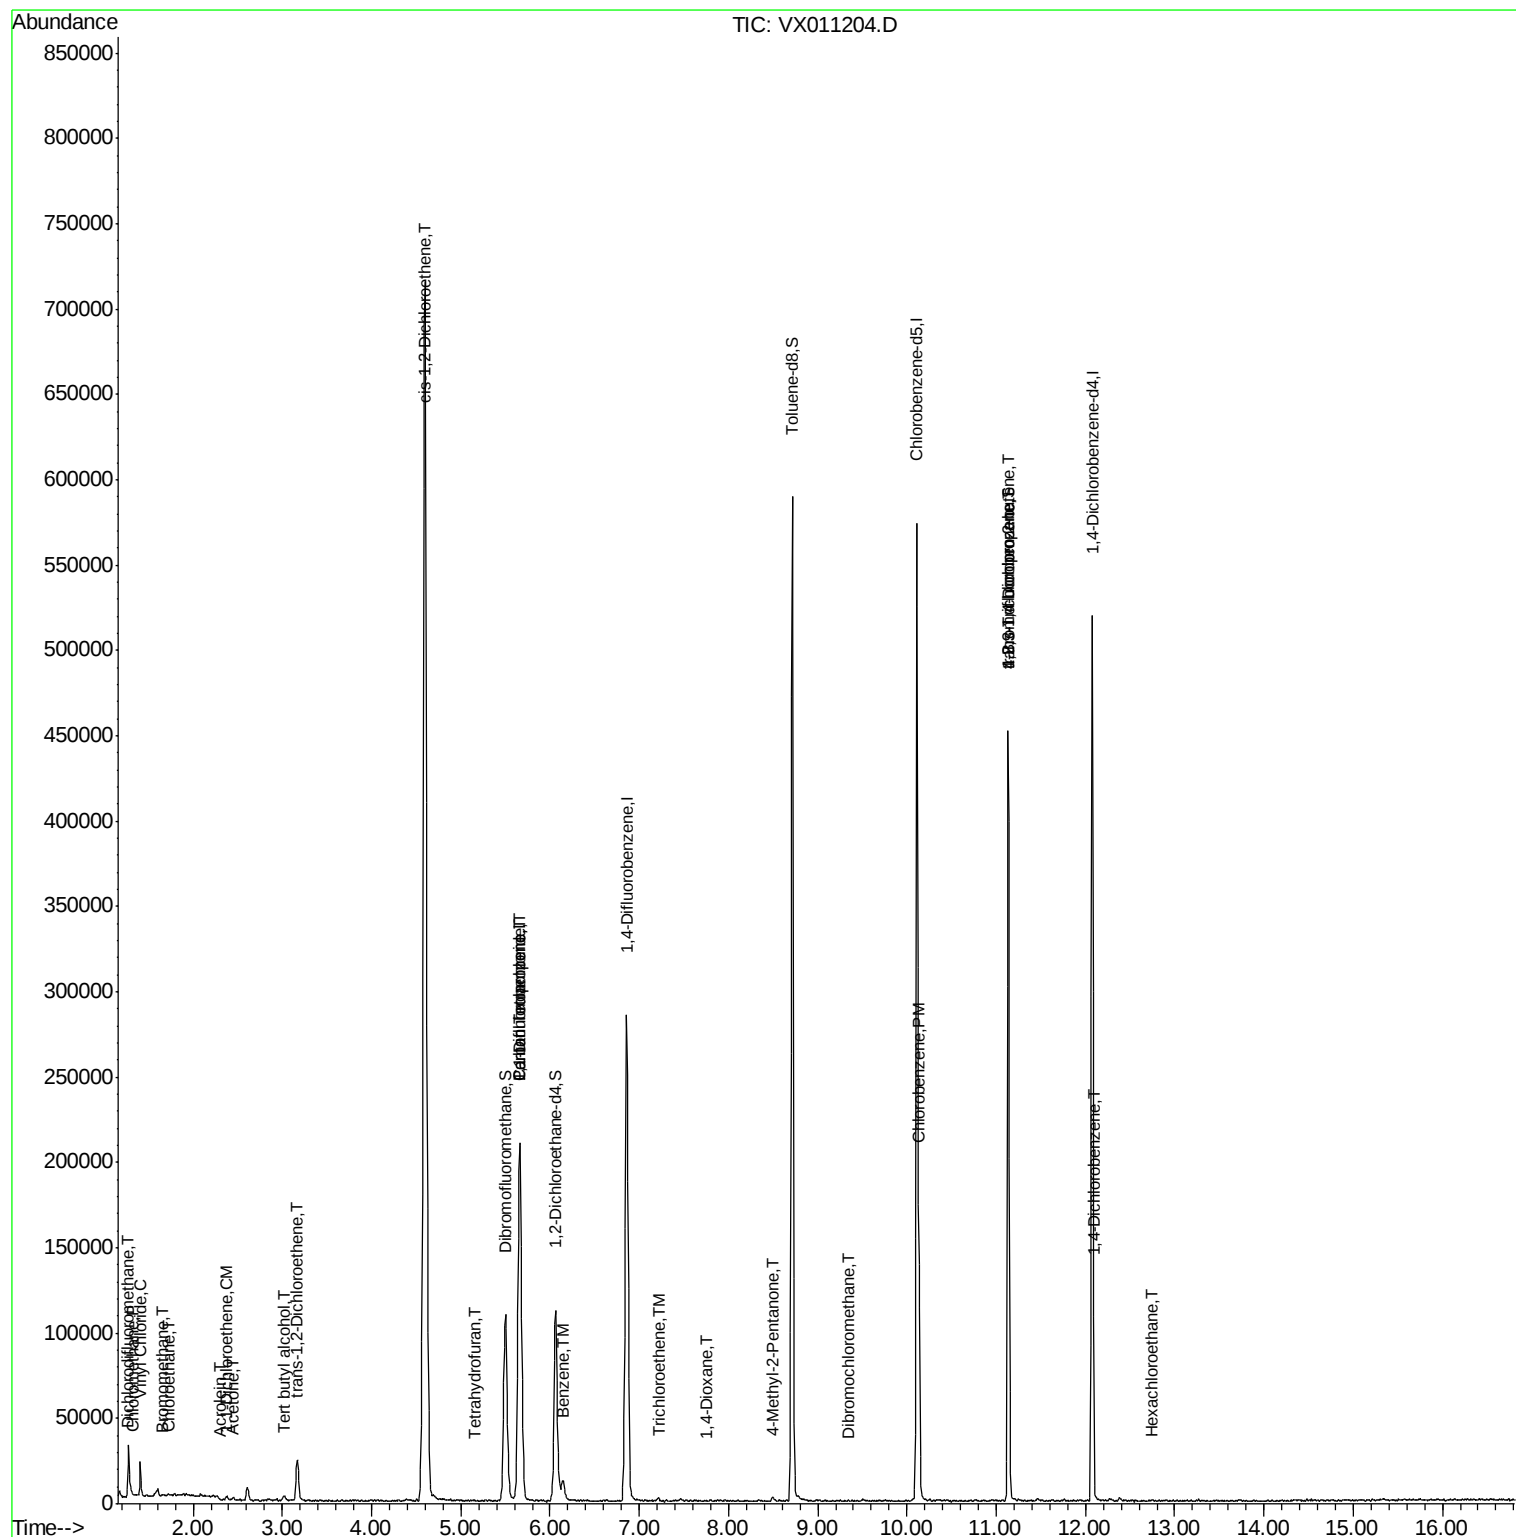



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :


Z3-0674

Tgt Ion:168 Resp: 213714

Ion Ratio Lower Upper

168 100

99 51.5 37.6 56.4

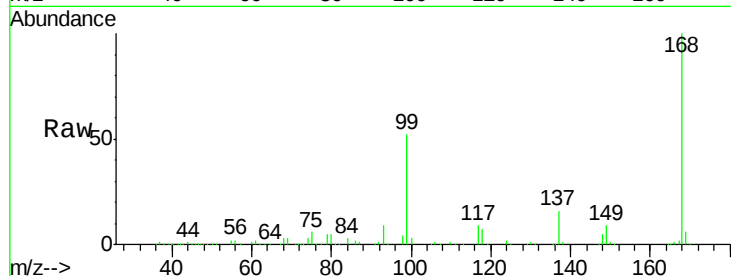

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67

80000



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#2

Dichlorodifluoromethane

Concen: 0.565 ug/l

RT: 1.26 min Scan# 17

Delta R.T. 0.06 min

Lab File: VX011204.D


Acq: 30 Jul 2019 18:50

Tgt Ion: 85 Resp: 44

Ion Ratio Lower Upper

85 100

87 0.0 15.9 47.7#



Abundance Ion 84.90 (84.60 to 85.60): VX0

Ion 86.90 (86.60 to 87.60): VX0

1.26


60


40

20

0

Time--> 1.24 1.26 1.28





#3

Chloromethane

Concen: 0.214 ug/l

RT: 1.33 min Scan# 29

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :


Z3-0674

Tgt Ion: 50 Resp: 420

Ion Ratio Lower Upper




50 100

52 34.6 26.4 39.6

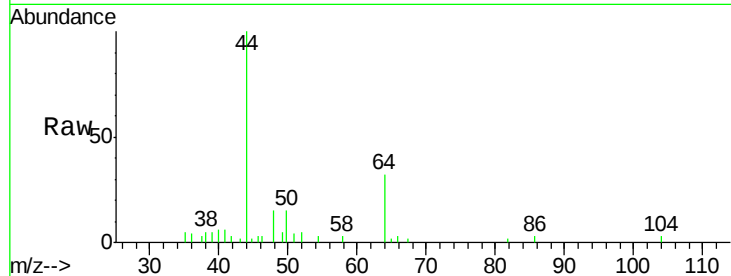

Abundance Ion 49.90 (49.60 to 50.60): VX0

Ion 51.90 (51.60 to 52.60): VX0

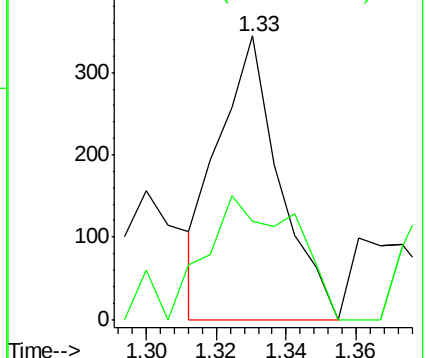

#4

Vinyl Chloride

Concen: 6.312 ug/l

RT: 1.41 min Scan# 42

Delta R.T. -0.00 min

Lab File: VX011204.D


Acq: 30 Jul 2019 18:50

Tgt Ion: 62 Resp: 12653

Ion Ratio Lower Upper



62 100


64 33.6 25.7 38.5



Abundance Ion 61.90 (61.60 to 62.60): VX0

Ion 63.90 (63.60 to 64.60): VX0

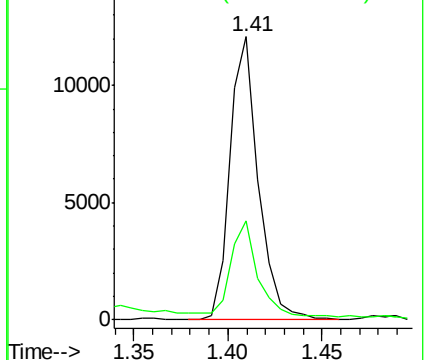



#5

Bromomethane

Concen: 0.538 ug/l

RT: 1.65 min Scan# 81

Delta R.T. 0.01 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :


Z3-0674

Tgt Ion: 94 Resp: 608

Ion Ratio Lower Upper




94 100

96 52.4 75.6 113.4#

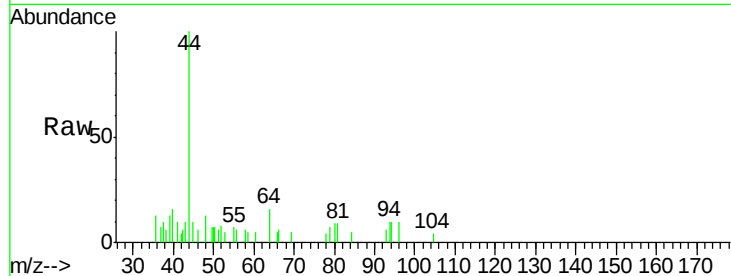

Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

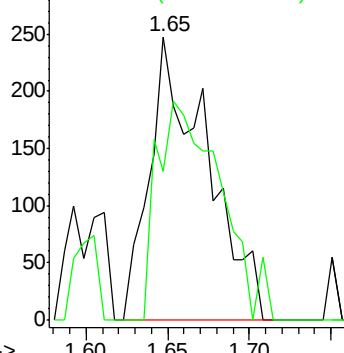

#6

Chloroethane

Concen: 1.751 ug/l

RT: 1.71 min Scan# 92

Delta R.T. -0.01 min

Lab File: VX011204.D


Acq: 30 Jul 2019 18:50

Tgt Ion: 64 Resp: 2230

Ion Ratio Lower Upper



64 100


66 2.9 27.0 40.6#



Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0




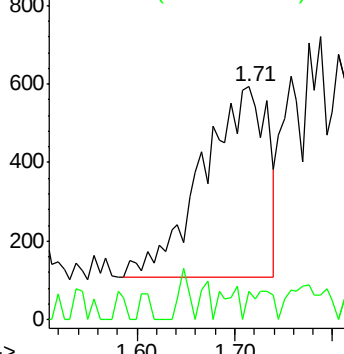




#11
Tert butyl alcohol
Concen: 3.129 ug/l
RT: 3.02 min Scan# 306
Delta R.T. -0.03 min
Lab File: VX011204.D
Acq: 30 Jul 2019 18:50




Instrument :
MSVOA_X
ClientSampleId :
Z3-0674


Tgt Ion: 59 Resp: 1657
Ion Ratio Lower Upper
59 100
57 6.8 7.9 11.9#

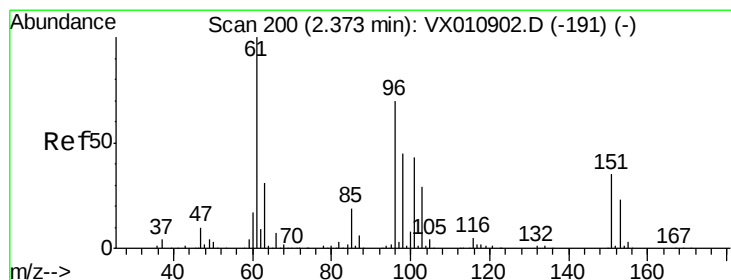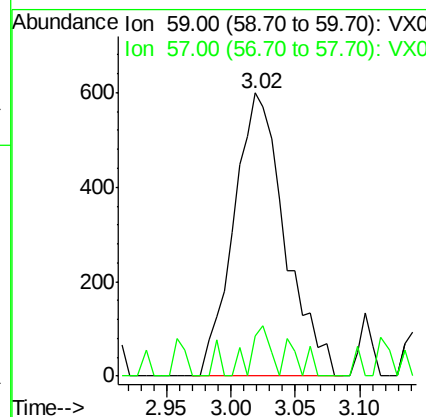

#12
1,1-Dichloroethene
Concen: 0.390 ug/l
RT: 2.37 min Scan# 200
Delta R.T. -0.00 min
Lab File: VX011204.D
Acq: 30 Jul 2019 18:50

Tgt Ion: 96 Resp: 743
Ion Ratio Lower Upper
96 100
61 134.1 115.0 172.4
98 83.7 52.2 78.2#

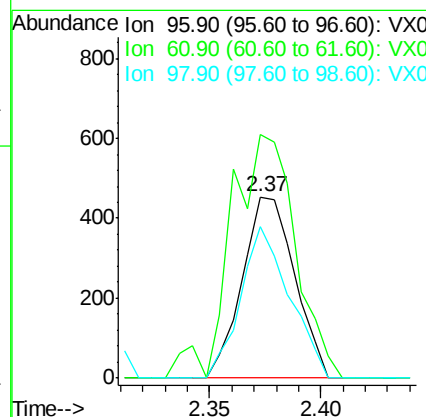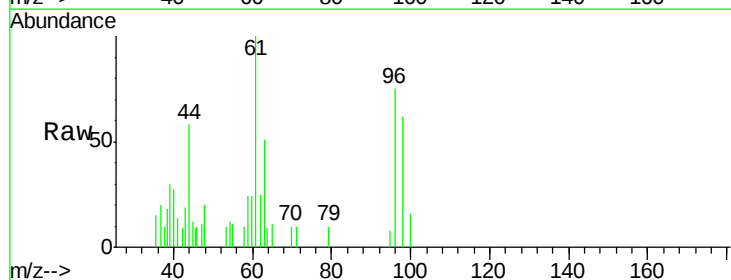



#13

Acrolein

Concen: 0.481 ug/l

RT: 2.31 min Scan# 189

Delta R.T. 0.01 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampled :


Z3-0674

Tgt Ion: 56 Resp: 147

Ion Ratio Lower Upper




56 100

55 32.7 55.9 83.9#

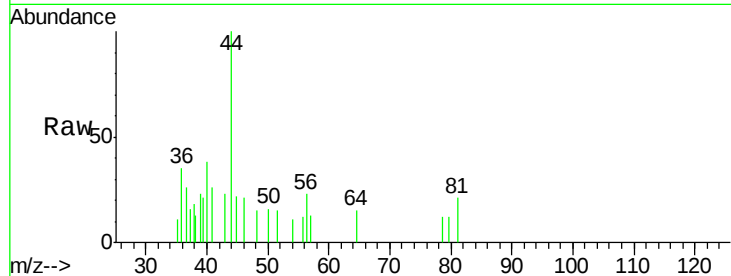

Abundance Ion 56.00 (55.70 to 56.70): VX0

Ion 55.00 (54.70 to 55.70): VX0

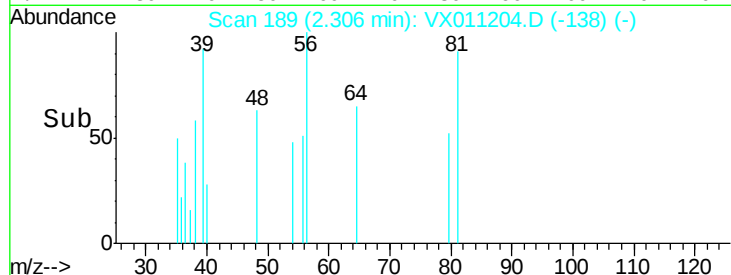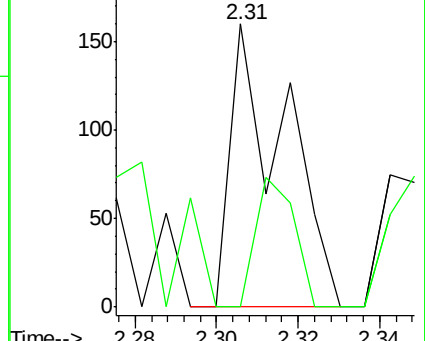

#16

Acetone

Concen: 1.922 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX011204.D


Acq: 30 Jul 2019 18:50

Tgt Ion: 43 Resp: 1974

Ion Ratio Lower Upper



43 100


58 27.9 27.7 41.5



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

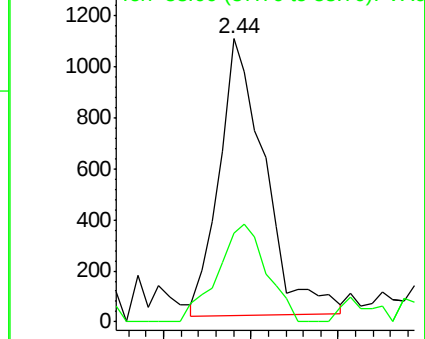



#21

trans-1,2-Dichloroethene

Concen: 5.305 ug/l

RT: 3.17 min Scan# 331

Delta R.T. 0.01 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :

Z3-0674


Tgt Ion: 96 Resp: 10716

Ion Ratio Lower Upper

96 100

61 111.7 104.2 156.2




98 58.9 52.2 78.4



Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

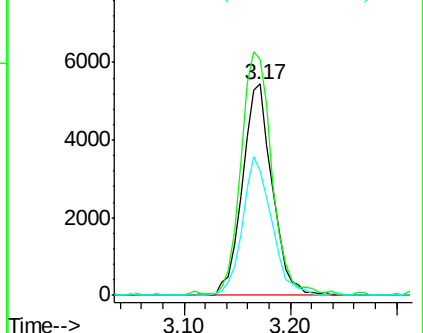

#27

cis-1,2-Dichloroethene

Concen: 207.261 ug/l

RT: 4.60 min Scan# 565

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50


Tgt Ion: 96 Resp: 484492

Ion Ratio Lower Upper

96 100

61 115.1 0.0 269.0



98 64.4 0.0 131.4




Abundance Ion 95.90 (95.60 to 96.60): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 97.90 (97.60 to 98.60): VX0

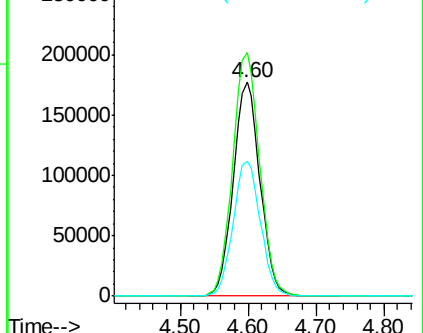



#29

Tetrahydrofuran

Concen: 0.287 ug/l

RT: 5.15 min Scan# 656

Delta R.T. 0.02 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampled :

Z3-0674





Tgt Ion: 42 Resp: 268

Ion Ratio Lower Upper

42 100

72 0.0 39.8 59.8#

71 30.6 37.0 55.4#

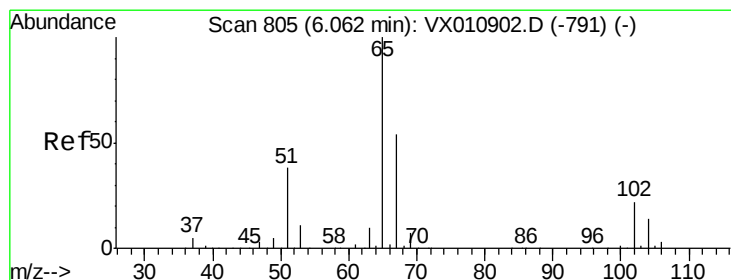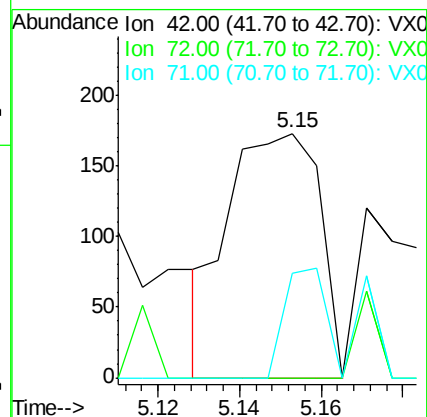

#33

1,2-Dichloroethane-d4

Concen: 46.105 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX011204.D




Acq: 30 Jul 2019 18:50


Tgt Ion: 65 Resp: 104823

Ion Ratio Lower Upper

65 100

67 52.5 0.0 107.8

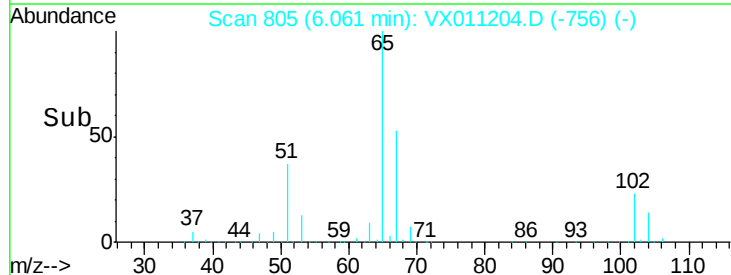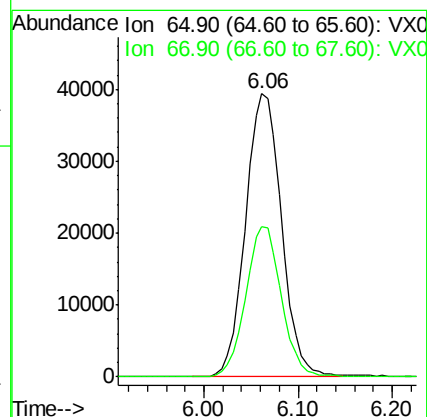

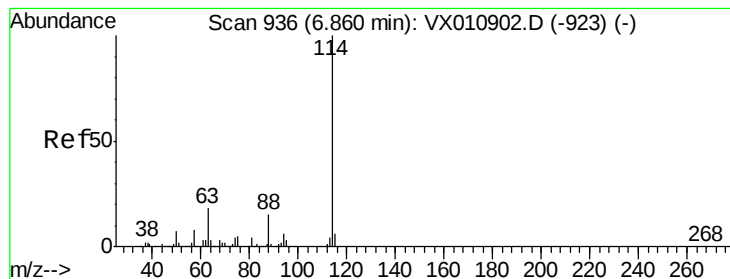

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :

Z3-0674


Tgt Ion:114 Resp: 299602

Ion Ratio Lower Upper

114 100

63 18.3 0.0 35.6




88 14.6 0.0 29.8



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

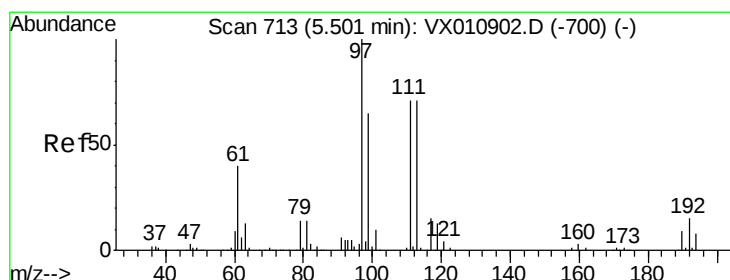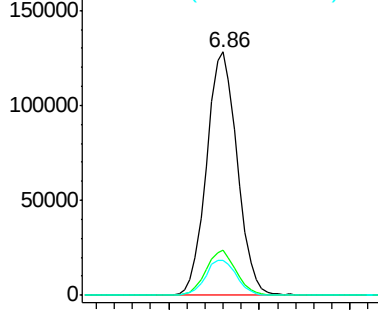

#35

Dibromofluoromethane

Concen: 46.974 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50


Tgt Ion:113 Resp: 89327

Ion Ratio Lower Upper

113 100

111 102.8 82.3 123.5



192 22.2 17.4 26.2




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

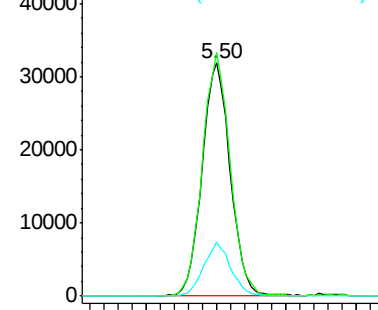

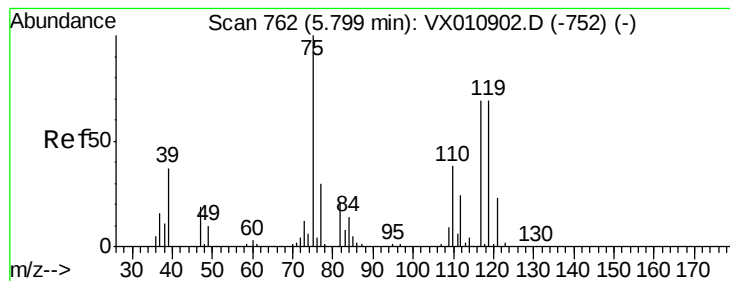

#36

1,1-Dichloropropene

Concen: 5.871 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.14 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :

Z3-0674


Tgt Ion: 75 Resp: 14448

Ion Ratio Lower Upper




75 100

110 10.2 19.9 59.7#

77 0.2 25.0 37.4#



Abundance Ion 74.90 (74.60 to 75.60): VX011204.D (-713) (-)

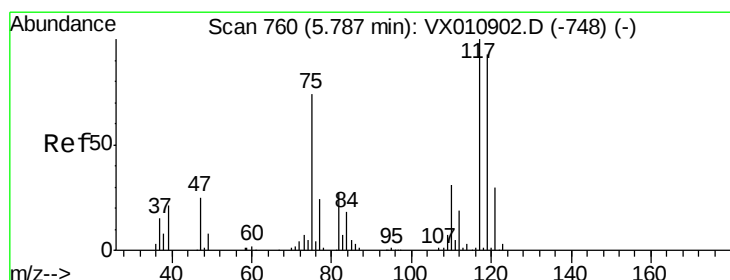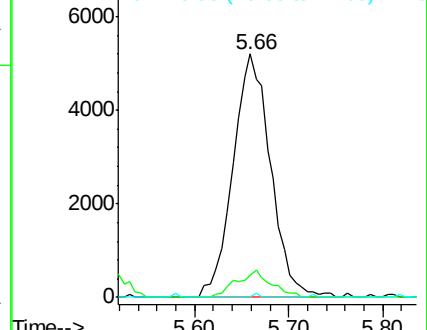

#38

Carbon Tetrachloride

Concen: 7.822 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50


Tgt Ion: 117 Resp: 20058

Ion Ratio Lower Upper



117 100


119 3.6 74.2 111.2#

121 0.0 24.2 36.2#



Abundance Ion 116.80 (116.50 to 117.50): VX011204.D (-711) (-)

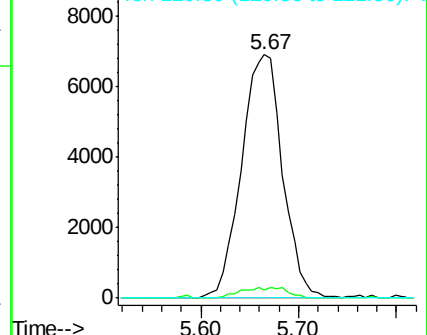

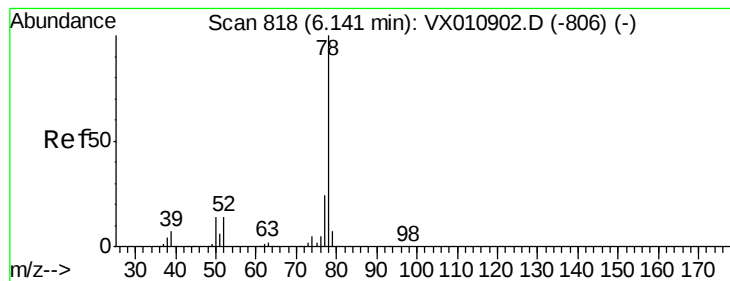

#40

Benzene

Concen: 1.819 ug/l

RT: 6.15 min Scan# 819

Delta R.T. 0.01 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :


Z3-0674

Tgt Ion: 78 Resp: 13716

Ion Ratio Lower Upper




78 100

77 23.5 19.0 28.6



Abundance Ion 78.00 (77.70 to 78.70): VX0

Ion 77.00 (76.70 to 77.70): VX0

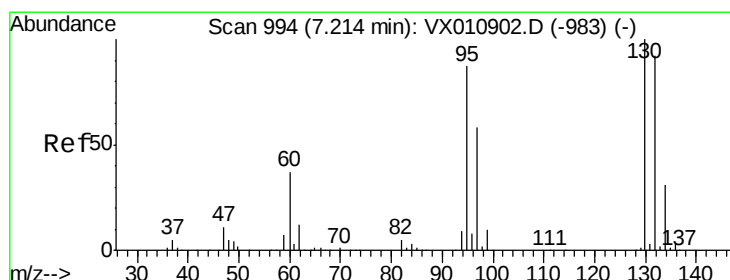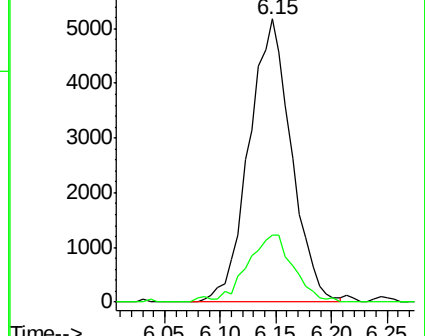

#44

Trichloroethene

Concen: 0.227 ug/l

RT: 7.22 min Scan# 995

Delta R.T. 0.01 min

Lab File: VX011204.D


Acq: 30 Jul 2019 18:50

Tgt Ion: 130 Resp: 506

Ion Ratio Lower Upper



130 100


95 73.0 0.0 174.8

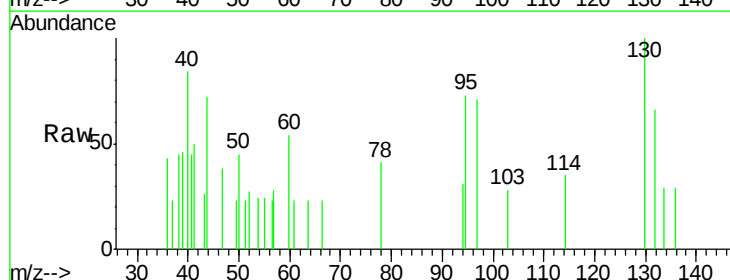

Abundance Ion 129.80 (129.50 to 130.50): V

Ion 94.90 (94.60 to 95.60): VX0

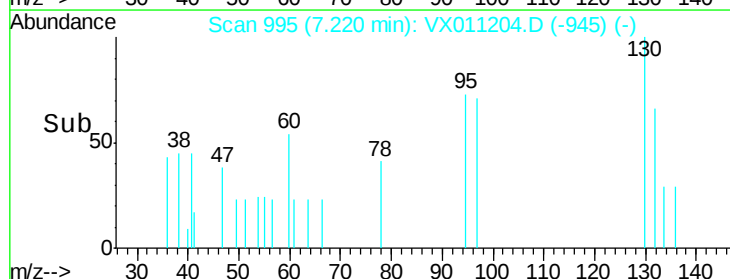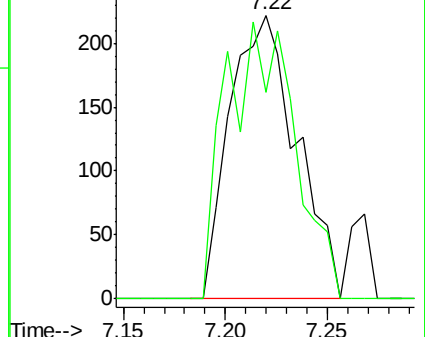







#49
1,4-Dioxane
Concen: 0.354 ug/l
RT: 7.76 min Scan# 1084
Delta R.T. 0.02 min
Lab File: VX011204.D
Acq: 30 Jul 2019 18:50

Instrument :
MSVOA_X
ClientSampleId :
Z3-0674

Tgt Ion: 88 Resp: 20
Ion Ratio Lower Upper
88 100
43 0.0 22.9 34.3#
58 0.0 49.8 74.8#




Abundance Ion 88.00 (87.70 to 88.70): VX0
Ion 43.00 (42.70 to 43.70): VX0
Ion 58.00 (57.70 to 58.70): VX0

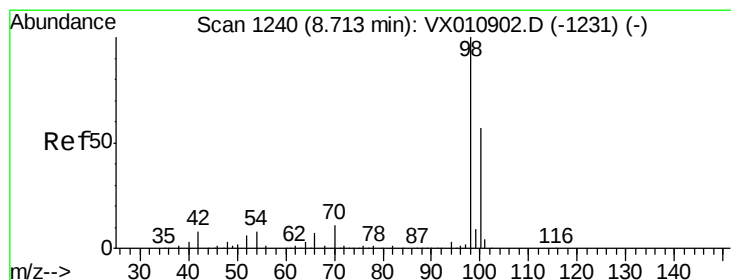
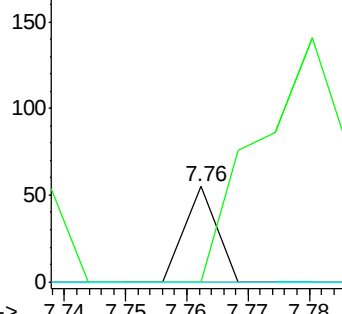



#50
Toluene-d8
Concen: 49.171 ug/l
RT: 8.71 min Scan# 1240
Delta R.T. -0.00 min
Lab File: VX011204.D
Acq: 30 Jul 2019 18:50

Tgt Ion: 98 Resp: 350706
Ion Ratio Lower Upper
98 100
100 63.6 50.6 75.8



Abundance Ion 98.00 (97.70 to 98.70): VX0
Ion 100.00 (99.70 to 100.70): VX0



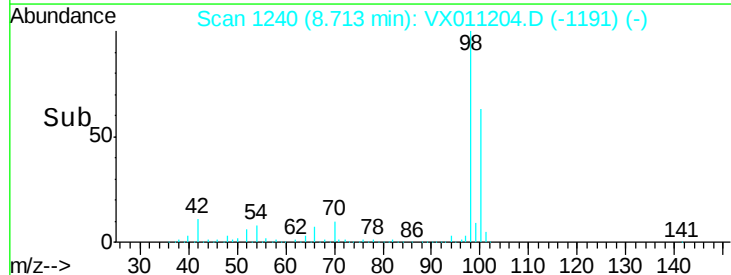
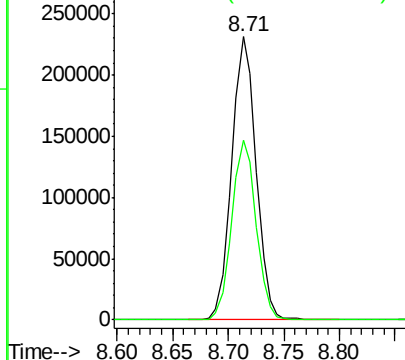


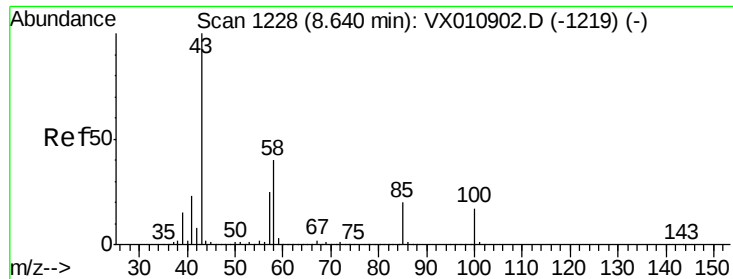

#51
 4-Methyl-2-Pentanone
 Concen: 0.203 ug/l
 RT: 8.49 min Scan# 1203
 Delta R.T. -0.15 min
 Lab File: VX011204.D
 Acq: 30 Jul 2019 18:50




Instrument :
 MSVOA_X
 ClientSampleId :
 Z3-0674


Tgt Ion: 43 Resp: 544
 Ion Ratio Lower Upper
 43 100
 58 32.7 32.2 48.4

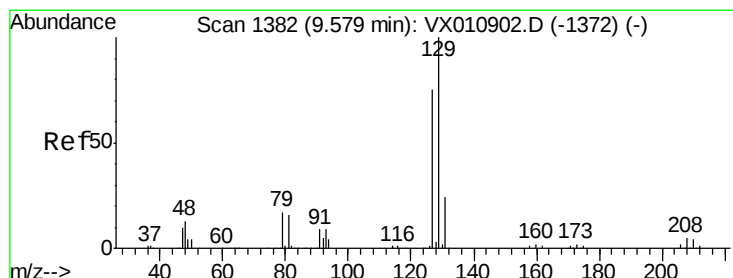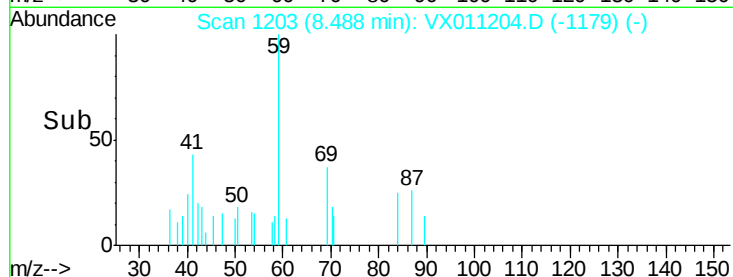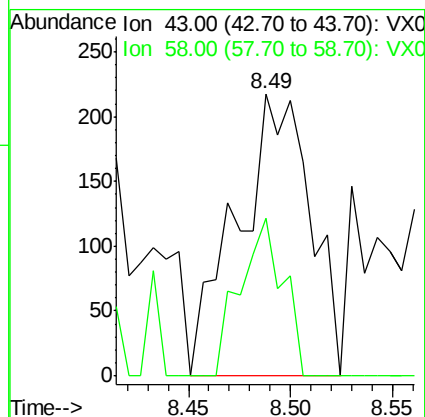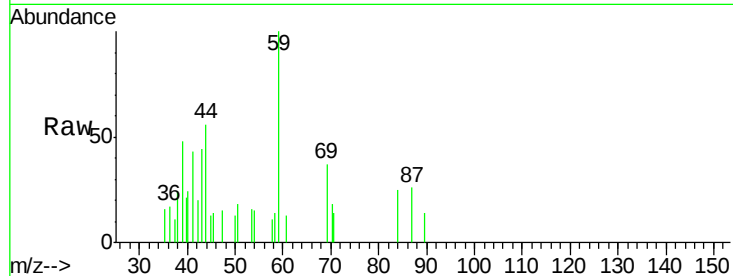

#60
 Dibromochloromethane
 Concen: 2.543 ug/l
 RT: 9.34 min Scan# 1343
 Delta R.T. -0.24 min
 Lab File: VX011204.D
 Acq: 30 Jul 2019 18:50

Tgt Ion: 129 Resp: 38
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.6 115.8#

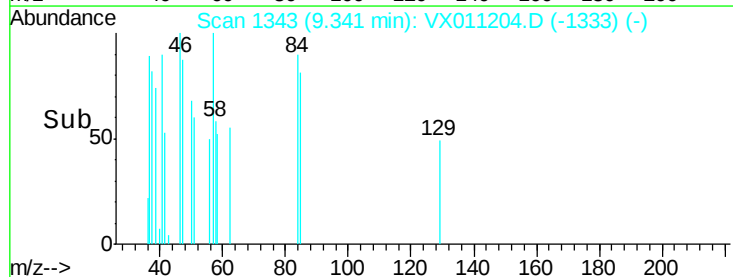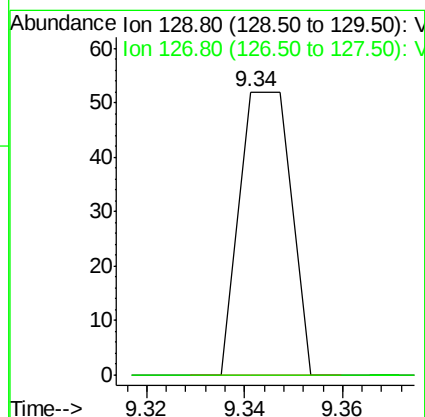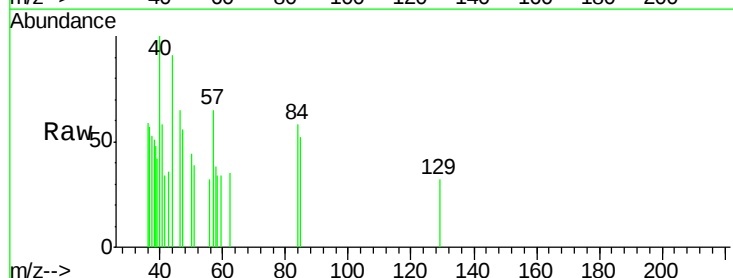



#62

4-Bromofluorobenzene

Concen: 42.104 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :

Z3-0674


Tgt Ion: 95 Resp: 110381

Ion Ratio Lower Upper

95 100

174 92.3 0.0 180.6




176 89.2 0.0 173.8

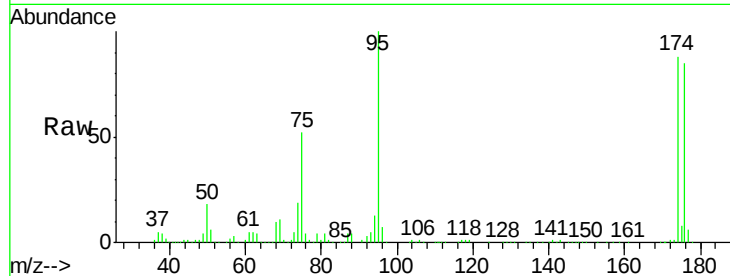

Abundance Ion 94.90 (94.60 to 95.60): VX011204.D (-1588) (-)

Ion 173.80 (173.50 to 174.50): VX011204.D (-1588) (-)

Ion 175.80 (175.50 to 176.50): VX011204.D (-1588) (-)

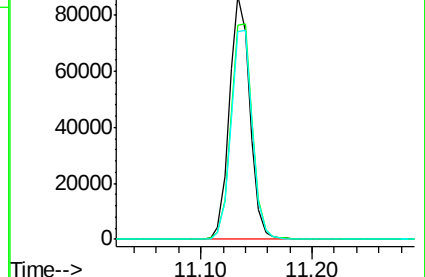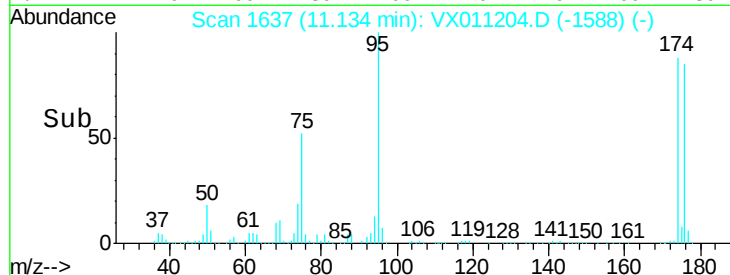

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50


Tgt Ion: 117 Resp: 261119

Ion Ratio Lower Upper

117 100

82 53.1 42.6 63.8



119 33.2 25.9 38.9




Abundance Ion 116.90 (116.60 to 117.60): VX011204.D (-1420) (-)

Ion 82.00 (81.70 to 82.70): VX011204.D (-1420) (-)

Ion 118.90 (118.60 to 119.60): VX011204.D (-1420) (-)

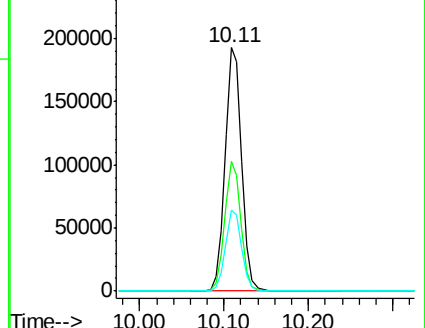



#65

Chlorobenzene

Concen: 9.886 ug/l

RT: 10.13 min Scan# 1473

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampleId :


Z3-0674

Tgt Ion:112 Resp: 53018

Ion Ratio Lower Upper




112 100

114 32.5 26.2 39.4

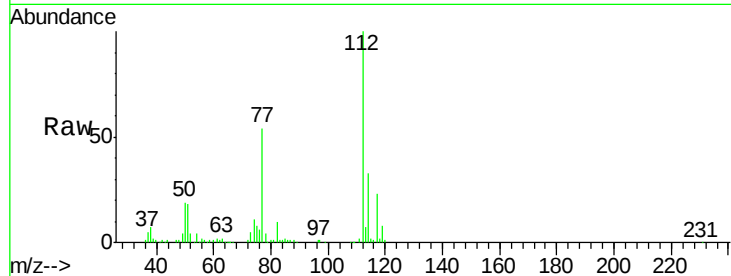

Abundance Ion 111.90 (111.60 to 112.60): V

Ion 113.90 (113.60 to 114.60): V

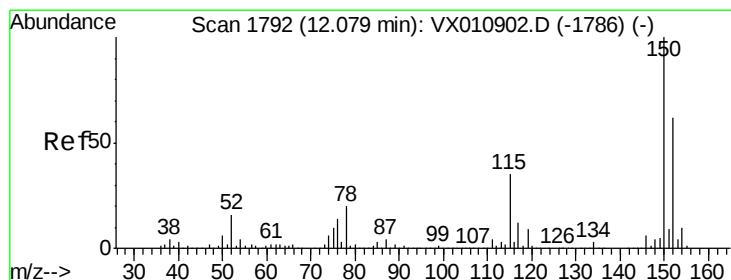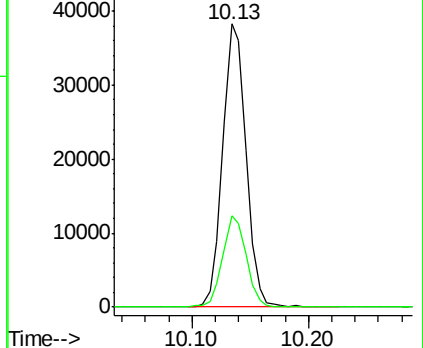

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50


Tgt Ion:152 Resp: 114624

Ion Ratio Lower Upper

152 100

115 55.5 39.7 119.1



150 156.8 0.0 345.6




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V




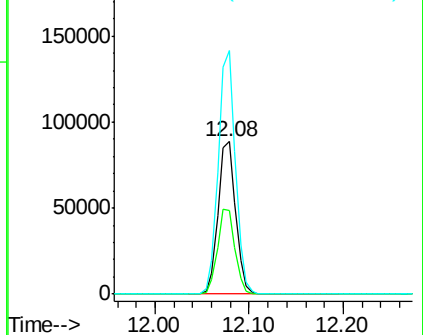




#76
 1,2,3-Trichloropropane
 Concen: 27.185 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.16 min
 Lab File: VX011204.D
 Acq: 30 Jul 2019 18:50




Instrument :
 MSVOA_X
 ClientSampled :
 Z3-0674


Tgt Ion: 75 Resp: 56230
 Ion Ratio Lower Upper
 75 100
 77 1.5 21.3 64.0#

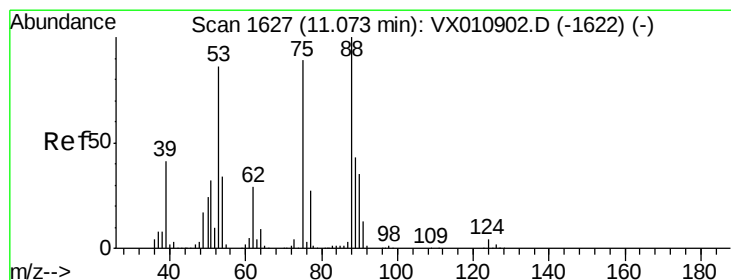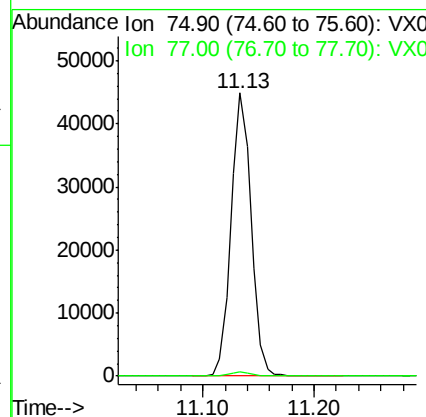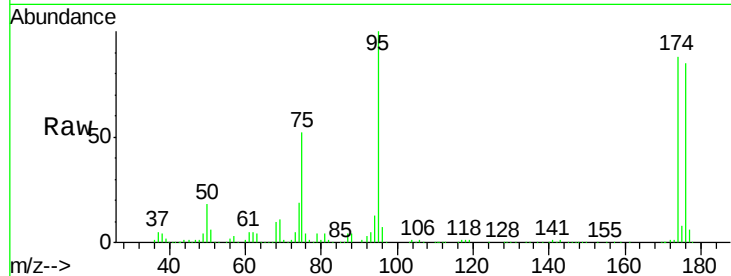

#81
 trans-1,4-Dichloro-2-butene
 Concen: 67.371 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.06 min
 Lab File: VX011204.D
 Acq: 30 Jul 2019 18:50

Tgt Ion: 75 Resp: 56230
 Ion Ratio Lower Upper
 75 100
 53 0.0 76.7 115.1#
 89 0.1 38.5 57.7#

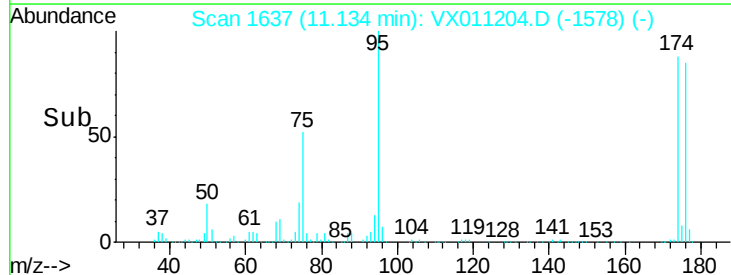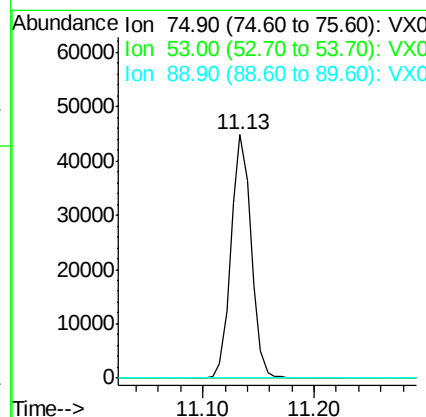



#88

1,4-Dichlorobenzene

Concen: 0.246 ug/l

RT: 12.10 min Scan# 1795

Delta R.T. -0.00 min

Lab File: VX011204.D

Acq: 30 Jul 2019 18:50

Instrument :

MSVOA_X

ClientSampled :

Z3-0674


Tgt Ion:146 Resp: 936

Ion Ratio Lower Upper

146 100

111 0.0 18.6 55.8#




148 145.3 31.6 94.7#

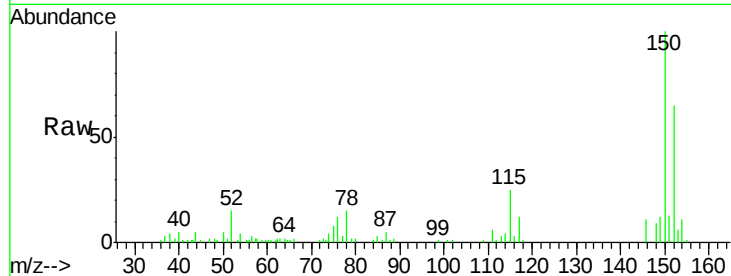

Abundance Ion 145.90 (145.60 to 146.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 147.90 (147.60 to 148.60): V

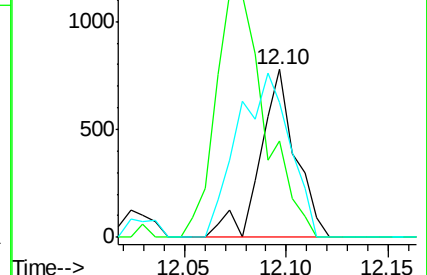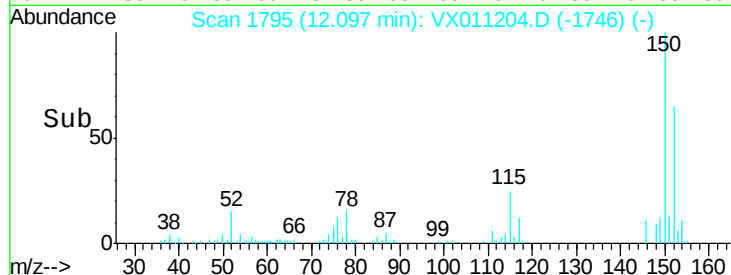

#90

Hexachloroethane

Concen: 0.320 ug/l

RT: 12.75 min Scan# 1902

Delta R.T. 0.16 min

Lab File: VX011204.D


Acq: 30 Jul 2019 18:50

Tgt Ion:117 Resp: 348

Ion Ratio Lower Upper

117 100

201 0.0 43.3 129.8#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

