

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX073019\
 Data File : VX011226.D
 Acq On : 31 Jul 2019 04:11
 Operator : JC/SP
 Sample : PB121803ZHE#06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB121803ZHE#06

Quant Time: Jul 31 09:50:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 24 05:39:23 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	225017	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	326644	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	295694	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	133569	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.06	65	112074	46.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.64%	
35) Dibromofluoromethane	5.50	113	96023	46.31	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.62%	
50) Toluene-d8	8.71	98	388904	50.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.02%	
62) 4-Bromofluorobenzene	11.13	95	126302	44.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	88.38%	
Target Compounds						
16) Acetone	2.45	43	3974	3.676	ug/l	99
20) Methylene Chloride	2.86	84	2442	1.066	ug/l	96
43) Isopropyl Acetate	6.45	43	11109	2.459	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX073019\
Data File : VX011226.D
Acq On : 31 Jul 2019 04:11
Operator : JC/SP
Sample : PB121803ZHE#06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB121803ZHE#06

Quant Time: Jul 31 09:50:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 24 05:39:23 2019
Response via : Initial Calibration

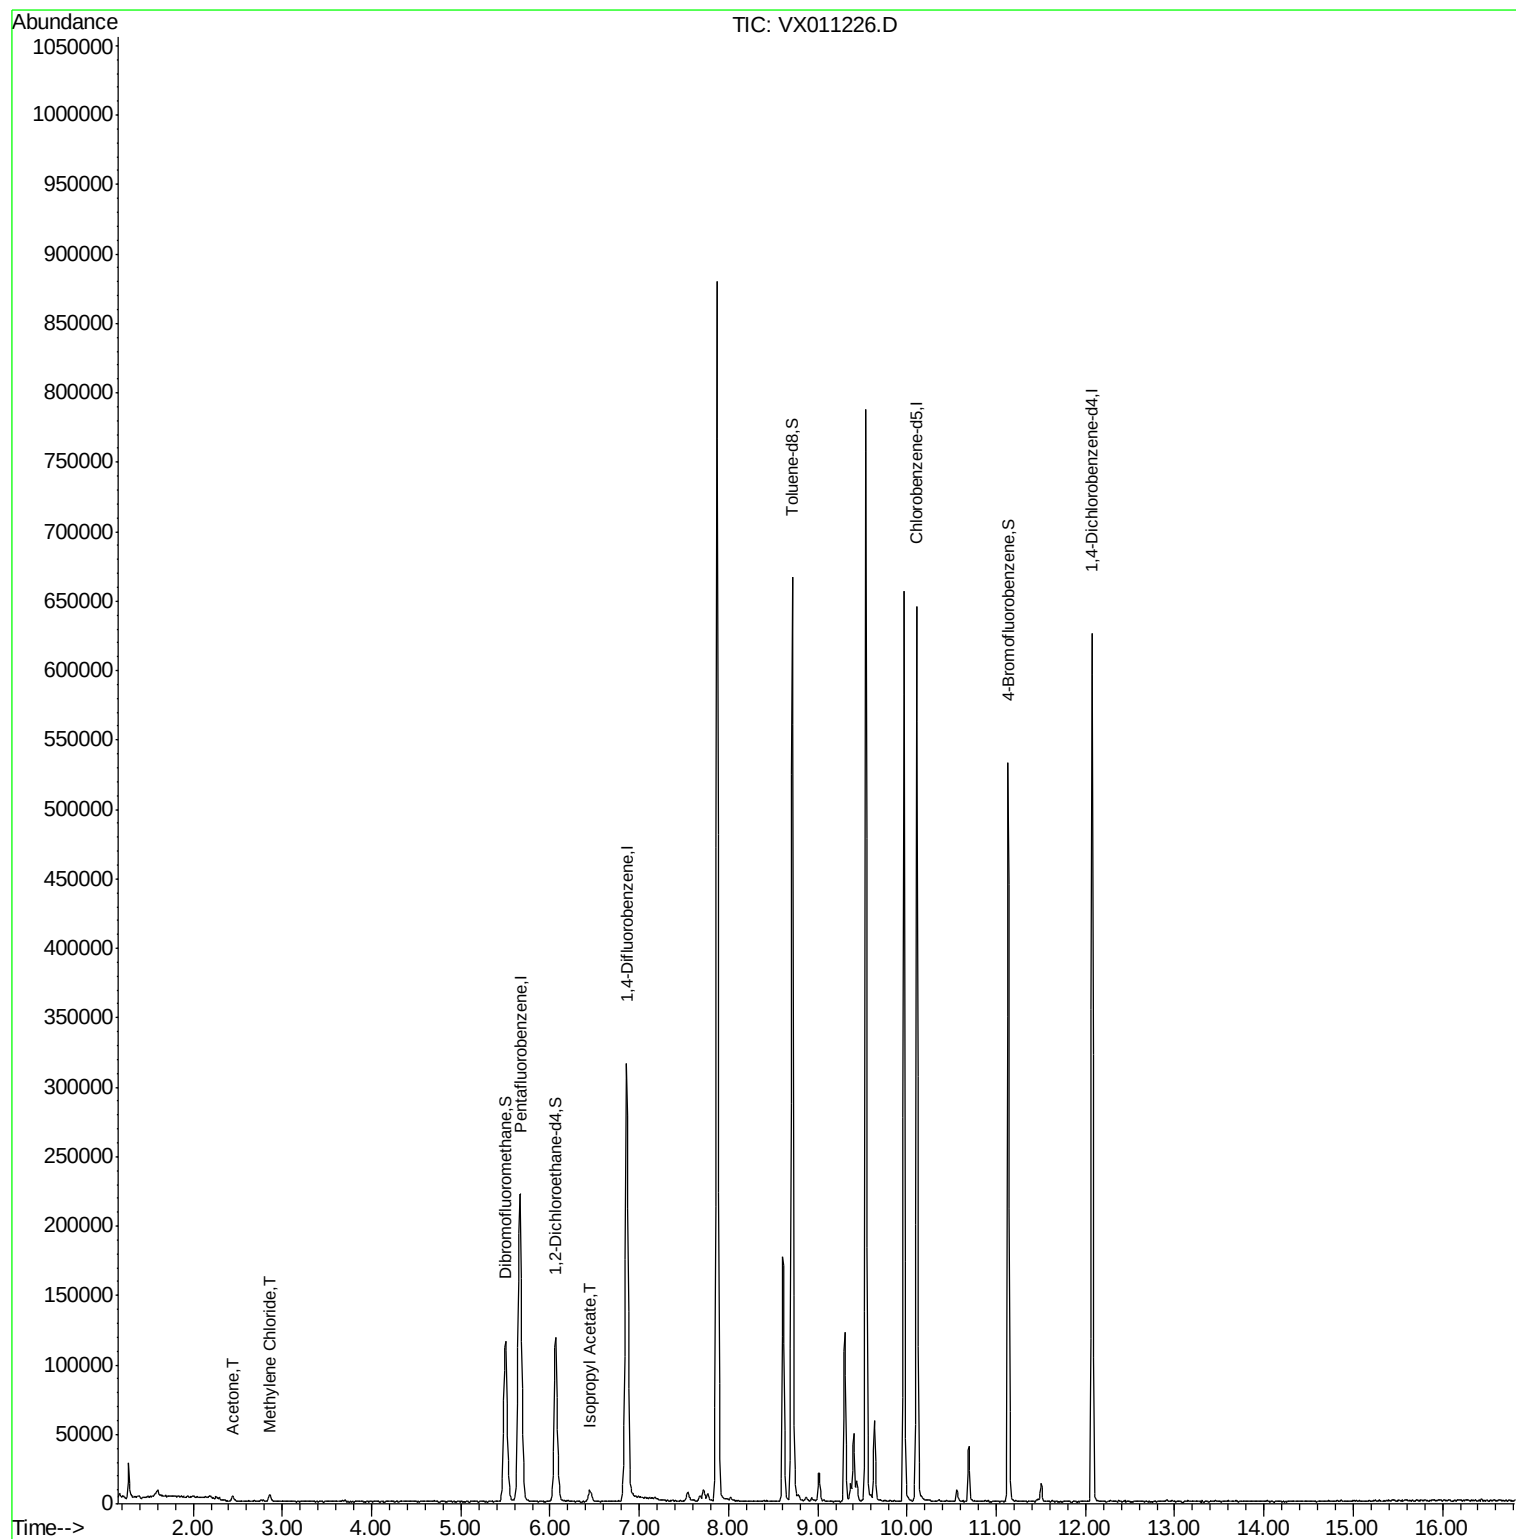

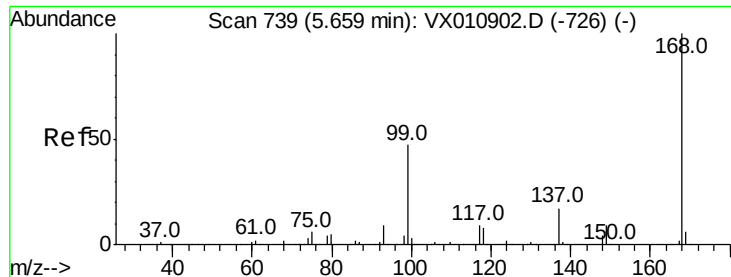

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.01 min

Lab File: VX011226.D

Acq: 31 Jul 2019 04:11

Instrument :

MSVOA_X

ClientSampleId :


PB121803ZHE#06

Tot Ion:168 Resp: 225017

Ion Ratio Lower Upper

168 100

99 50.8 37.6 56.4

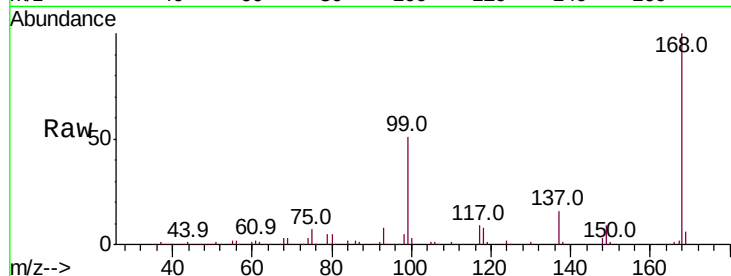

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

80000

60000



40000

20000

0

5.50 5.60 5.70 5.80

5.67

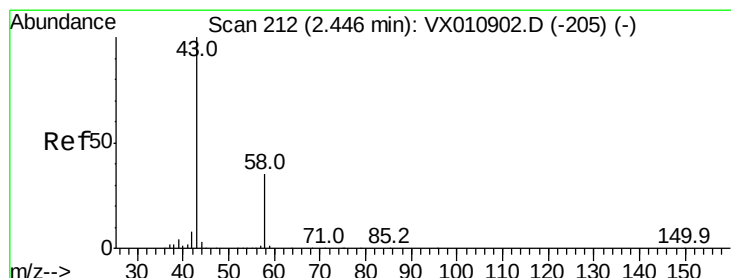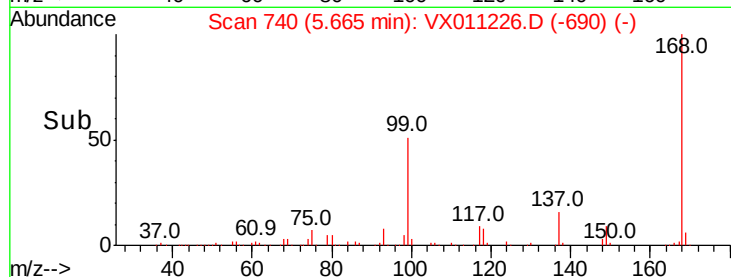

#16

Acetone

Concen: 3.676 ug/l

RT: 2.45 min Scan# 212

Delta R.T. -0.00 min

Lab File: VX011226.D


Acq: 31 Jul 2019 04:11

Tgt Ion: 43 Resp: 3974

Ion Ratio Lower Upper

43 100

58 35.0 27.7 41.5

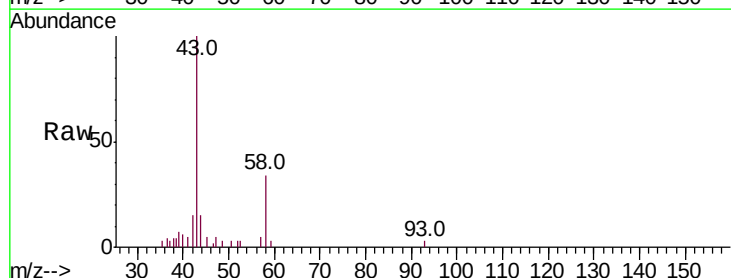

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

2500

2000

1500


1000


500

0

2.35 2.40 2.45 2.50

2.45

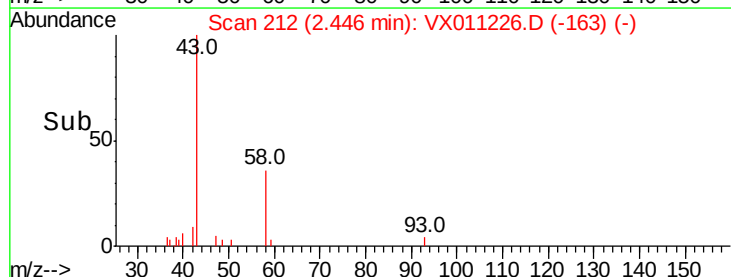

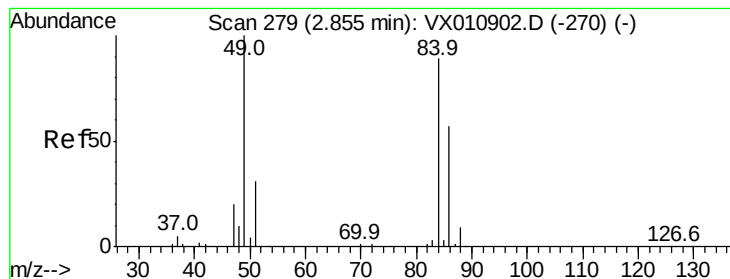

#20

Methylene Chloride

Concen: 1.066 ug/l

RT: 2.86 min Scan# 280

Delta R.T. 0.01 min

Lab File: VX011226.D

Acq: 31 Jul 2019 04:11

Instrument :

MSVOA_X

ClientSampleId :

PB121803ZHE#06

Tot Ion: 84 Resp: 2442


Ion Ratio Lower Upper

84 100

49 111.1 89.9 134.9

51 40.0 27.8 41.6

86 69.8 51.8 77.6



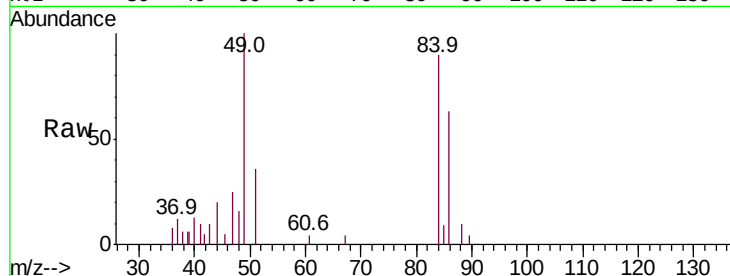


Abundance Ion 83.90 (83.60 to 84.60): VX0

Ion 48.90 (48.60 to 49.60): VX0

Ion 50.90 (50.60 to 51.60): VX0

Ion 85.90 (85.60 to 86.60): VX0

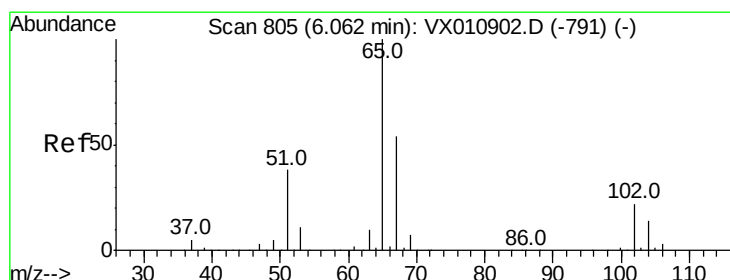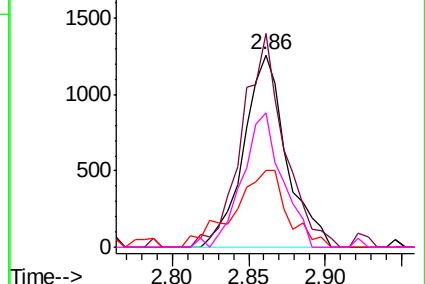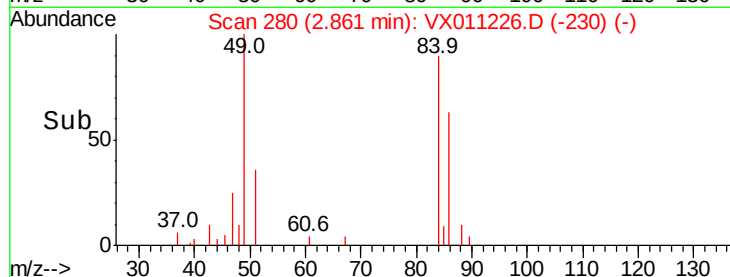

#33

1,2-Dichloroethane-d4

Concen: 46.818 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX011226.D


Acq: 31 Jul 2019 04:11

Tgt Ion: 65 Resp: 112074

Ion Ratio Lower Upper



65 100


67 52.7 0.0 107.8

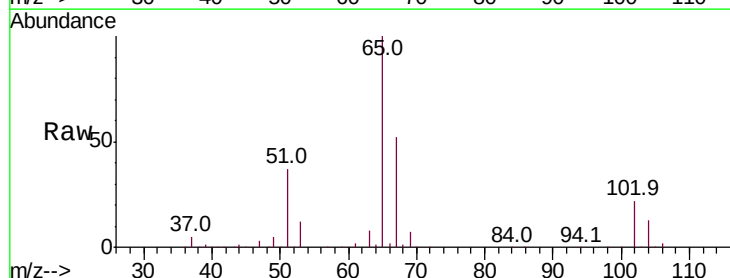

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

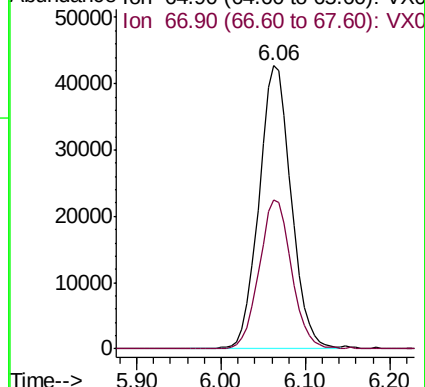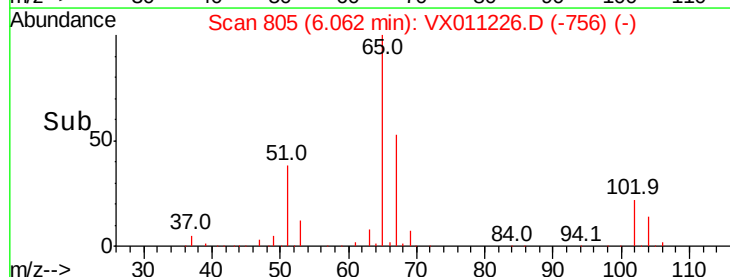

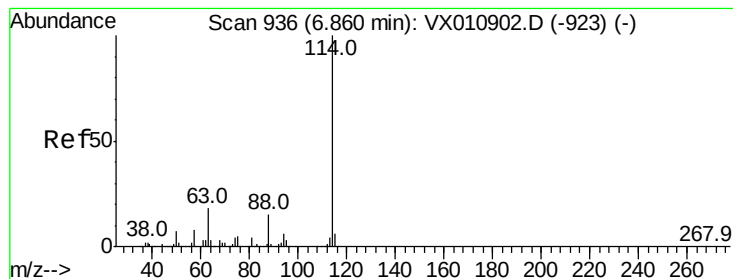

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. -0.00 min

Lab File: VX011226.D

Acq: 31 Jul 2019 04:11

Instrument :

MSVOA_X

ClientSampleId :

PB121803ZHE#06


Tot Ion:114 Resp: 326644

Ion Ratio Lower Upper

114 100

63 18.3 0.0 35.6




88 14.5 0.0 29.8

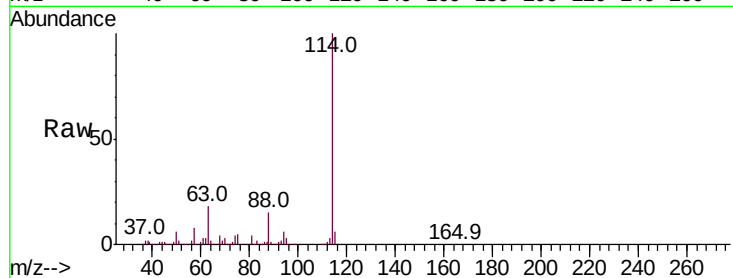

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

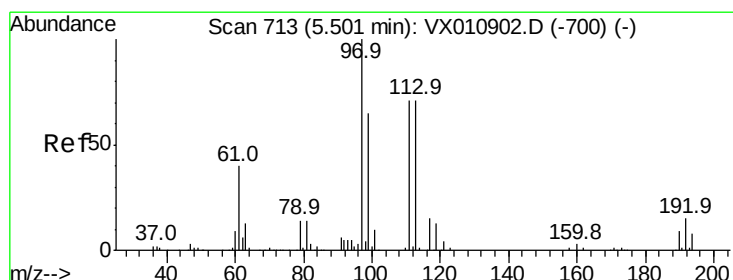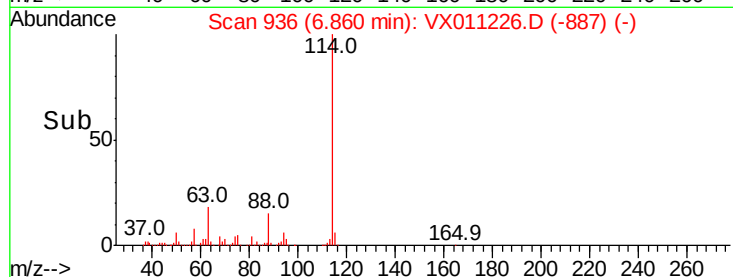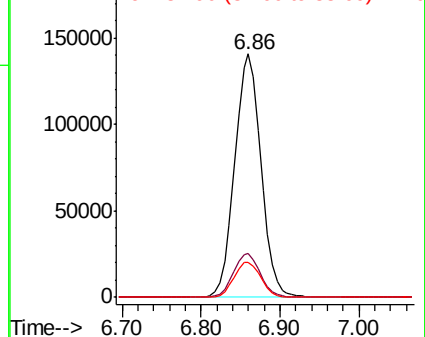

#35

Dibromofluoromethane

Concen: 46.315 ug/l

RT: 5.50 min Scan# 713

Delta R.T. -0.00 min

Lab File: VX011226.D

Acq: 31 Jul 2019 04:11


Tgt Ion:113 Resp: 96023

Ion Ratio Lower Upper

113 100

111 102.3 82.3 123.5



192 21.7 17.4 26.2

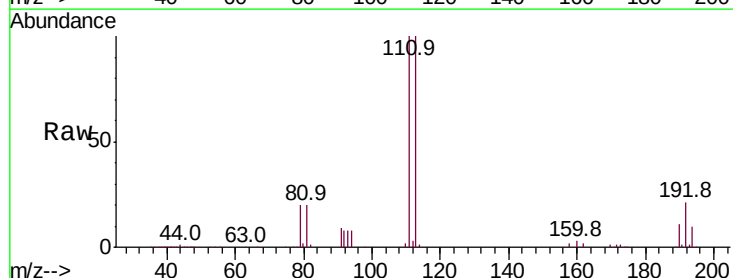


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

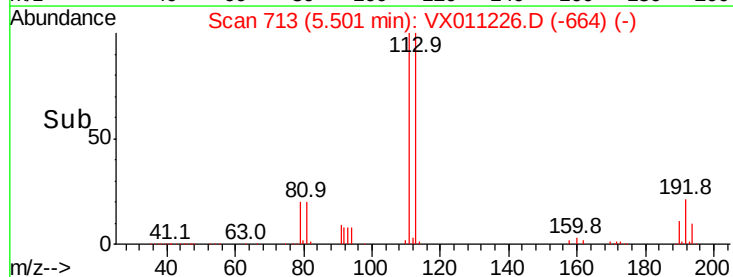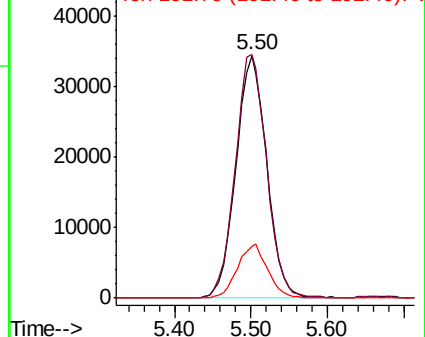

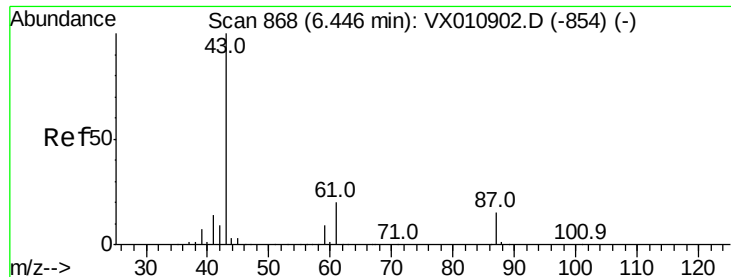

#43

Isopropyl Acetate

Concen: 2.459 ug/l

RT: 6.45 min Scan# 868

Delta R.T. -0.00 min

Lab File: VX011226.D

Acq: 31 Jul 2019 04:11

Instrument :

MSVOA_X

ClientSampleId :

PB121803ZHE#06


Tot Ion: 43 Resp: 11109

Ion Ratio Lower Upper

43 100

61 22.4 17.1 25.7




87 16.6 12.0 18.0

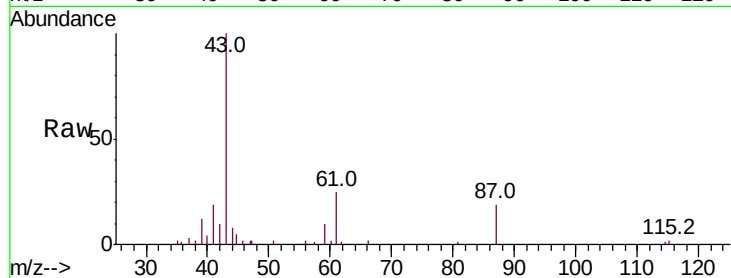

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

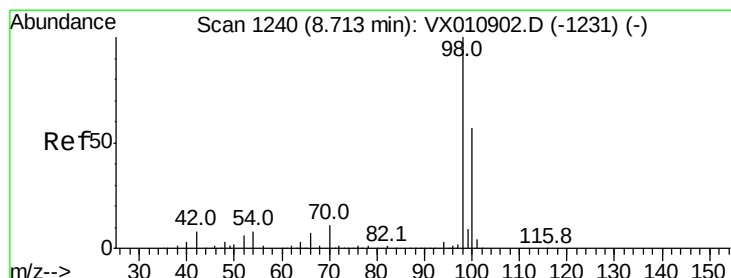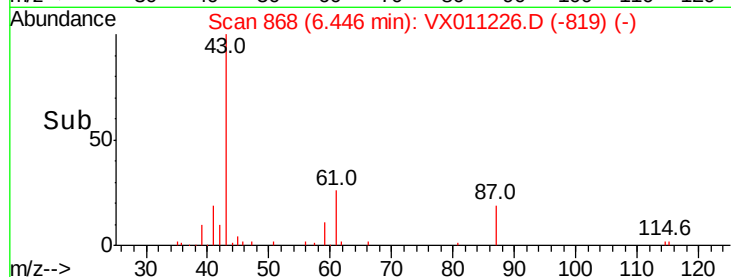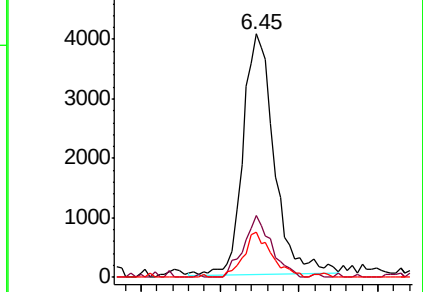

#50

Toluene-d8

Concen: 50.013 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX011226.D


Acq: 31 Jul 2019 04:11

Tgt Ion: 98 Resp: 388904

Ion Ratio Lower Upper



98 100


100 63.6 50.6 75.8

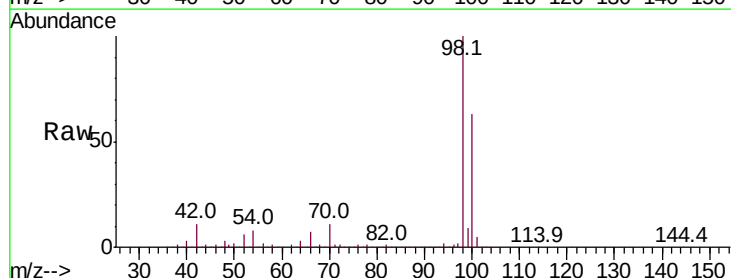

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

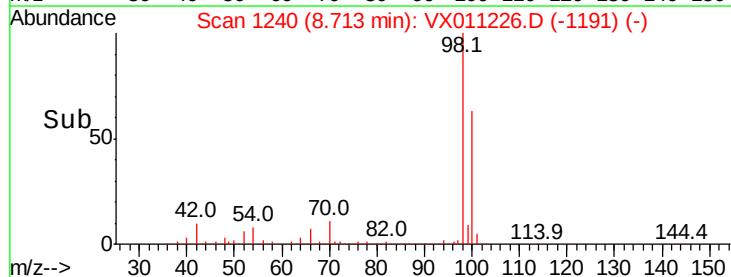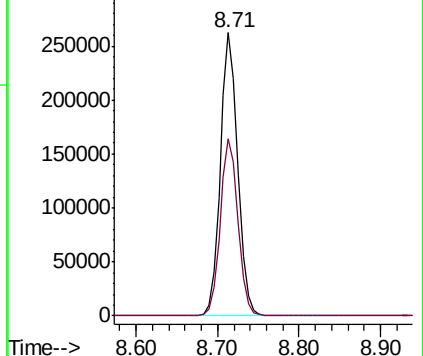

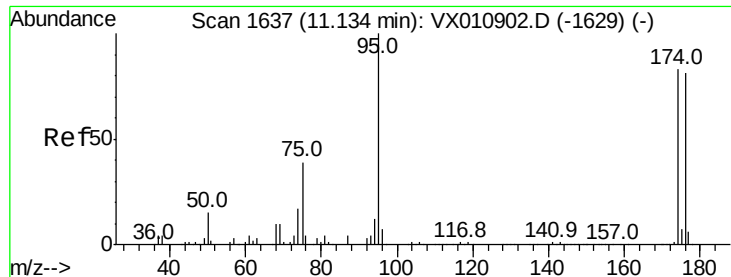

#62

4-Bromofluorobenzene

Concen: 44.188 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.00 min

Lab File: VX011226.D

Acq: 31 Jul 2019 04:11

Instrument :

MSVOA_X

ClientSampleId :

PB121803ZHE#06


Tot Ion: 95 Resp: 126302

Ion Ratio Lower Upper

95 100

174 90.8 0.0 180.6




176 90.0 0.0 173.8

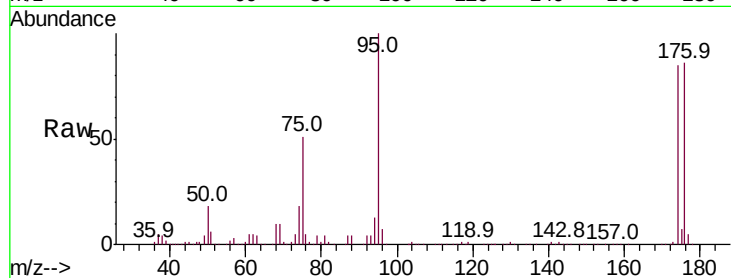

Abundance Ion 94.90 (94.60 to 95.60): VX011226.D (-1588) (-)

Ion 173.80 (173.50 to 174.50): VX011226.D (-1588) (-)

Ion 175.80 (175.50 to 176.50): VX011226.D (-1588) (-)

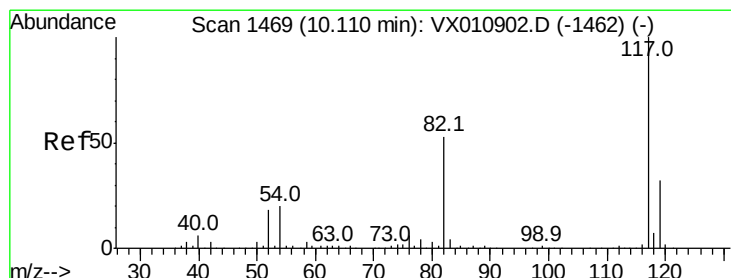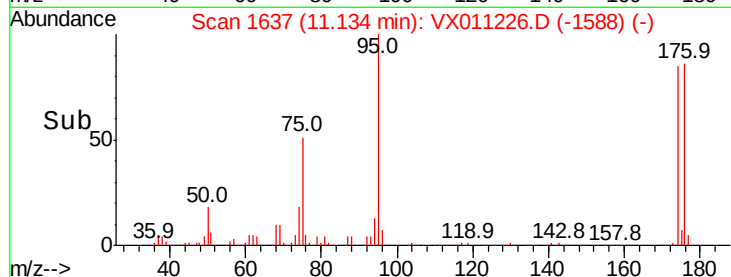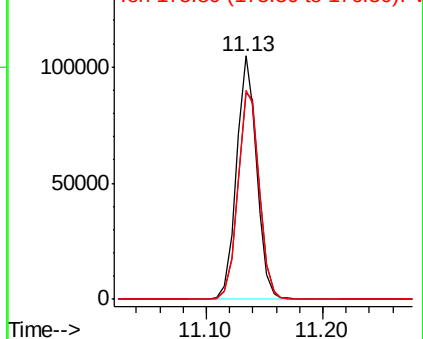

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VX011226.D

Acq: 31 Jul 2019 04:11


Tgt Ion: 117 Resp: 295694

Ion Ratio Lower Upper

117 100

82 53.2 42.6 63.8



119 31.9 25.9 38.9

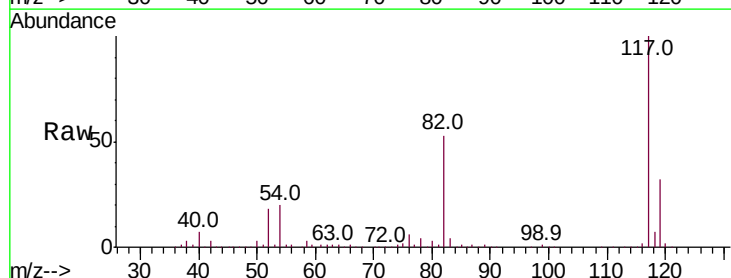


Abundance Ion 116.90 (116.60 to 117.60): VX011226.D (-1420) (-)

Ion 82.00 (81.70 to 82.70): VX011226.D (-1420) (-)

Ion 118.90 (118.60 to 119.60): VX011226.D (-1420) (-)

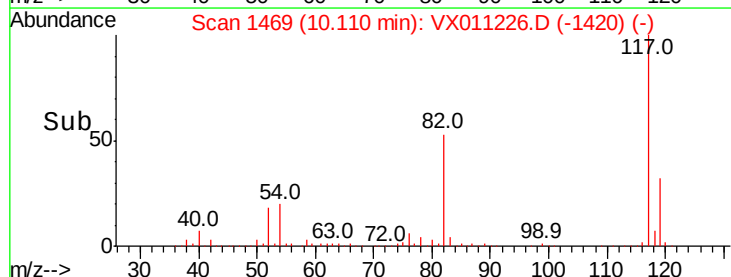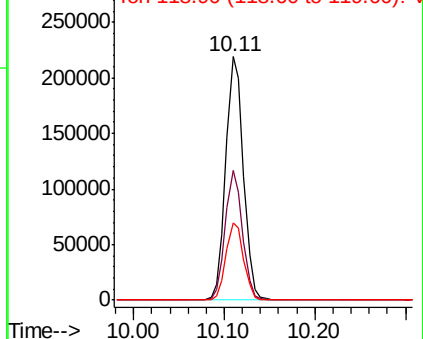


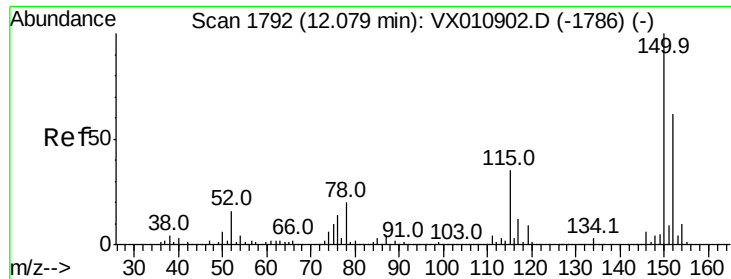

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.08 min Scan# 1792
 Delta R.T. -0.00 min
 Lab File: VX011226.D
 Acq: 31 Jul 2019 04:11

Instrument :
 MSVOA_X
 ClientSampleId :
 PB121803ZHE#06

Tot Ion	Ratio	Lower	Upper
152	100		
115	55.9	39.7	119.1
150	157.8	0.0	345.6

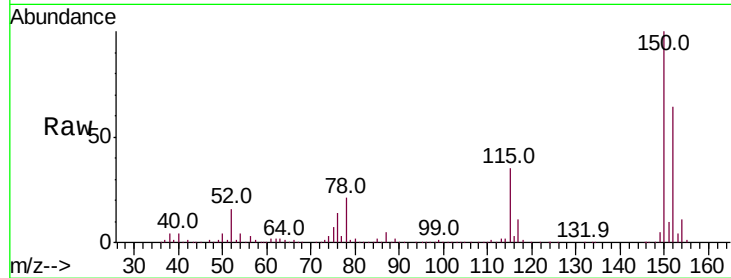

Abundance

Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

