


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX073019\
Data File : VX011214.D
Acq On : 30 Jul 2019 23:07
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Title : SW846 8260
Last Update : Wed Jul 24 05:39:23 2019

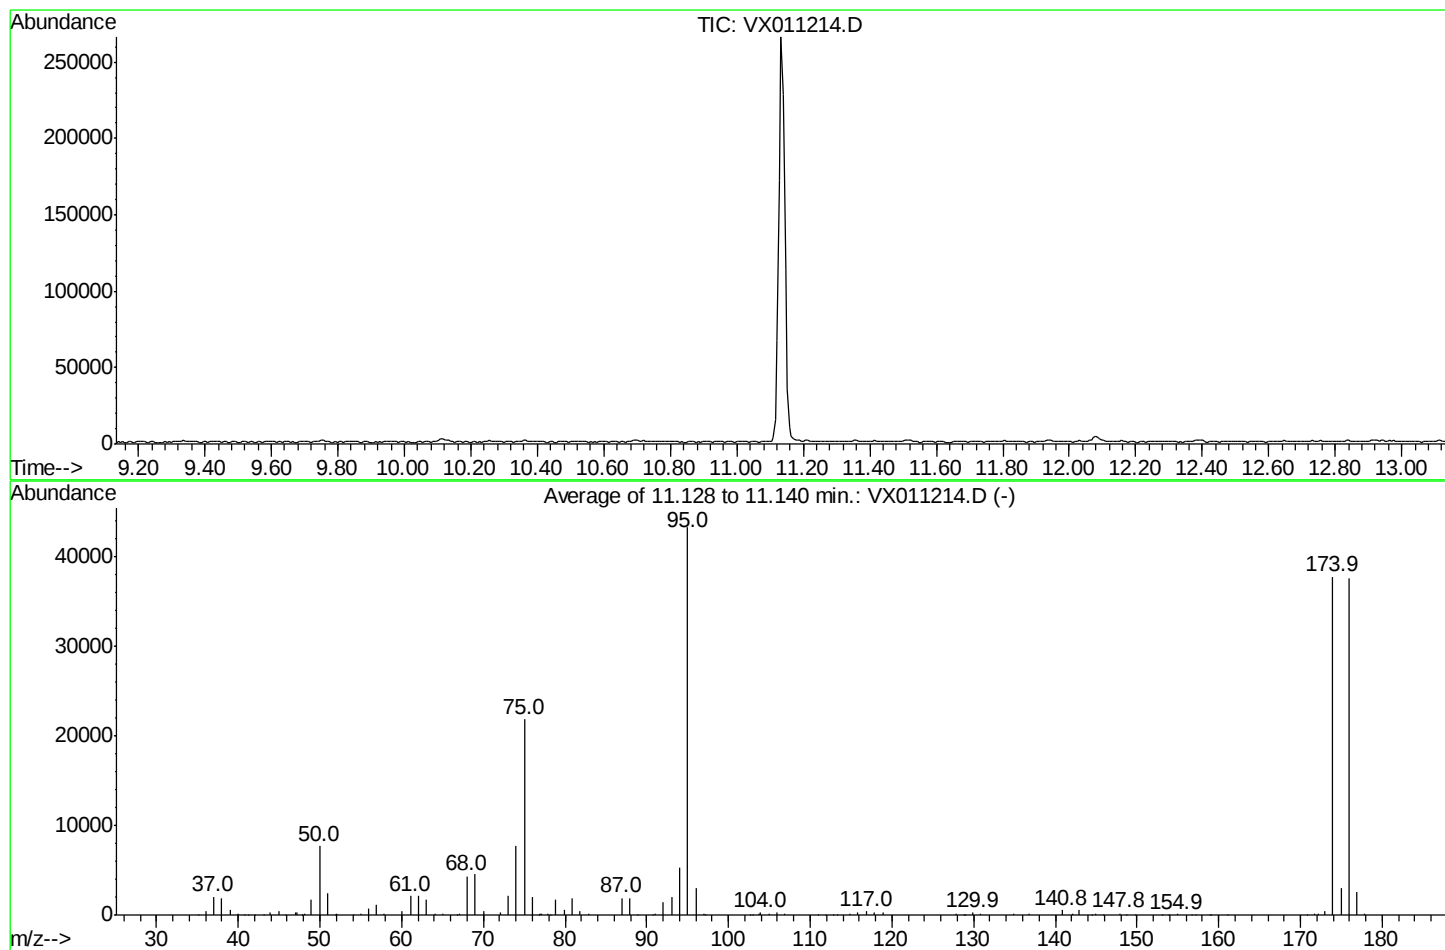

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	7677	PASS
75	95	30	60	50.4	21789	PASS
95	95	100	100	100.0	43205	PASS
96	95	5	9	7.0	3036	PASS
173	174	0.00	2	1.3	487	PASS
174	95	50	100	87.3	37728	PASS
175	174	5	9	7.8	2934	PASS
176	174	95	101	99.3	37477	PASS
177	176	5	9	6.8	2536	PASS