

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042731.D
 Acq On : 30 Jul 2024 11:55
 Operator : JC/MD
 Sample : VX0730MBL02
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 31 03:15:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 31 03:10:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	158586	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	144996	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	58185	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	40779	42.325	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.660%
7) Chloroethane-d5	1.648	69	18500	46.598	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.200%
11) 1,1-Dichloroethene-d2	2.294	65	21358	44.992	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.980%
21) 2-Butanone-d5	4.458	46	59567	83.418	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	83.420%
24) Chloroform-d	5.050	84	90596	42.960	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.920%
26) 1,2-Dichloroethane-d4	5.952	65	61137	44.936	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.880%
32) Benzene-d6	5.970	84	183613	45.628	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.260%
36) 1,2-Dichloropropane-d6	7.306	67	53630	45.030	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.060%
41) Toluene-d8	8.647	98	161574	44.782	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.560%
43) trans-1,3-Dichloroprop...	8.952	79	23145	41.527	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.060%
47) 2-Hexanone-d5	9.384	63	43345	81.401	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	81.400%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	74712	43.569	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	87.140%
66) 1,2-Dichlorobenzene-d4	12.317	152	53919	49.034	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.060%
Target Compounds						
37) 1,2-Dichloropropane	7.306	63	6246	5.416	ug/L	Qvalue # 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042731.D
Acq On : 30 Jul 2024 11:55
Operator : JC/MD
Sample : VX0730MBL02
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 31 03:15:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 03:10:58 2024
Response via : Initial Calibration

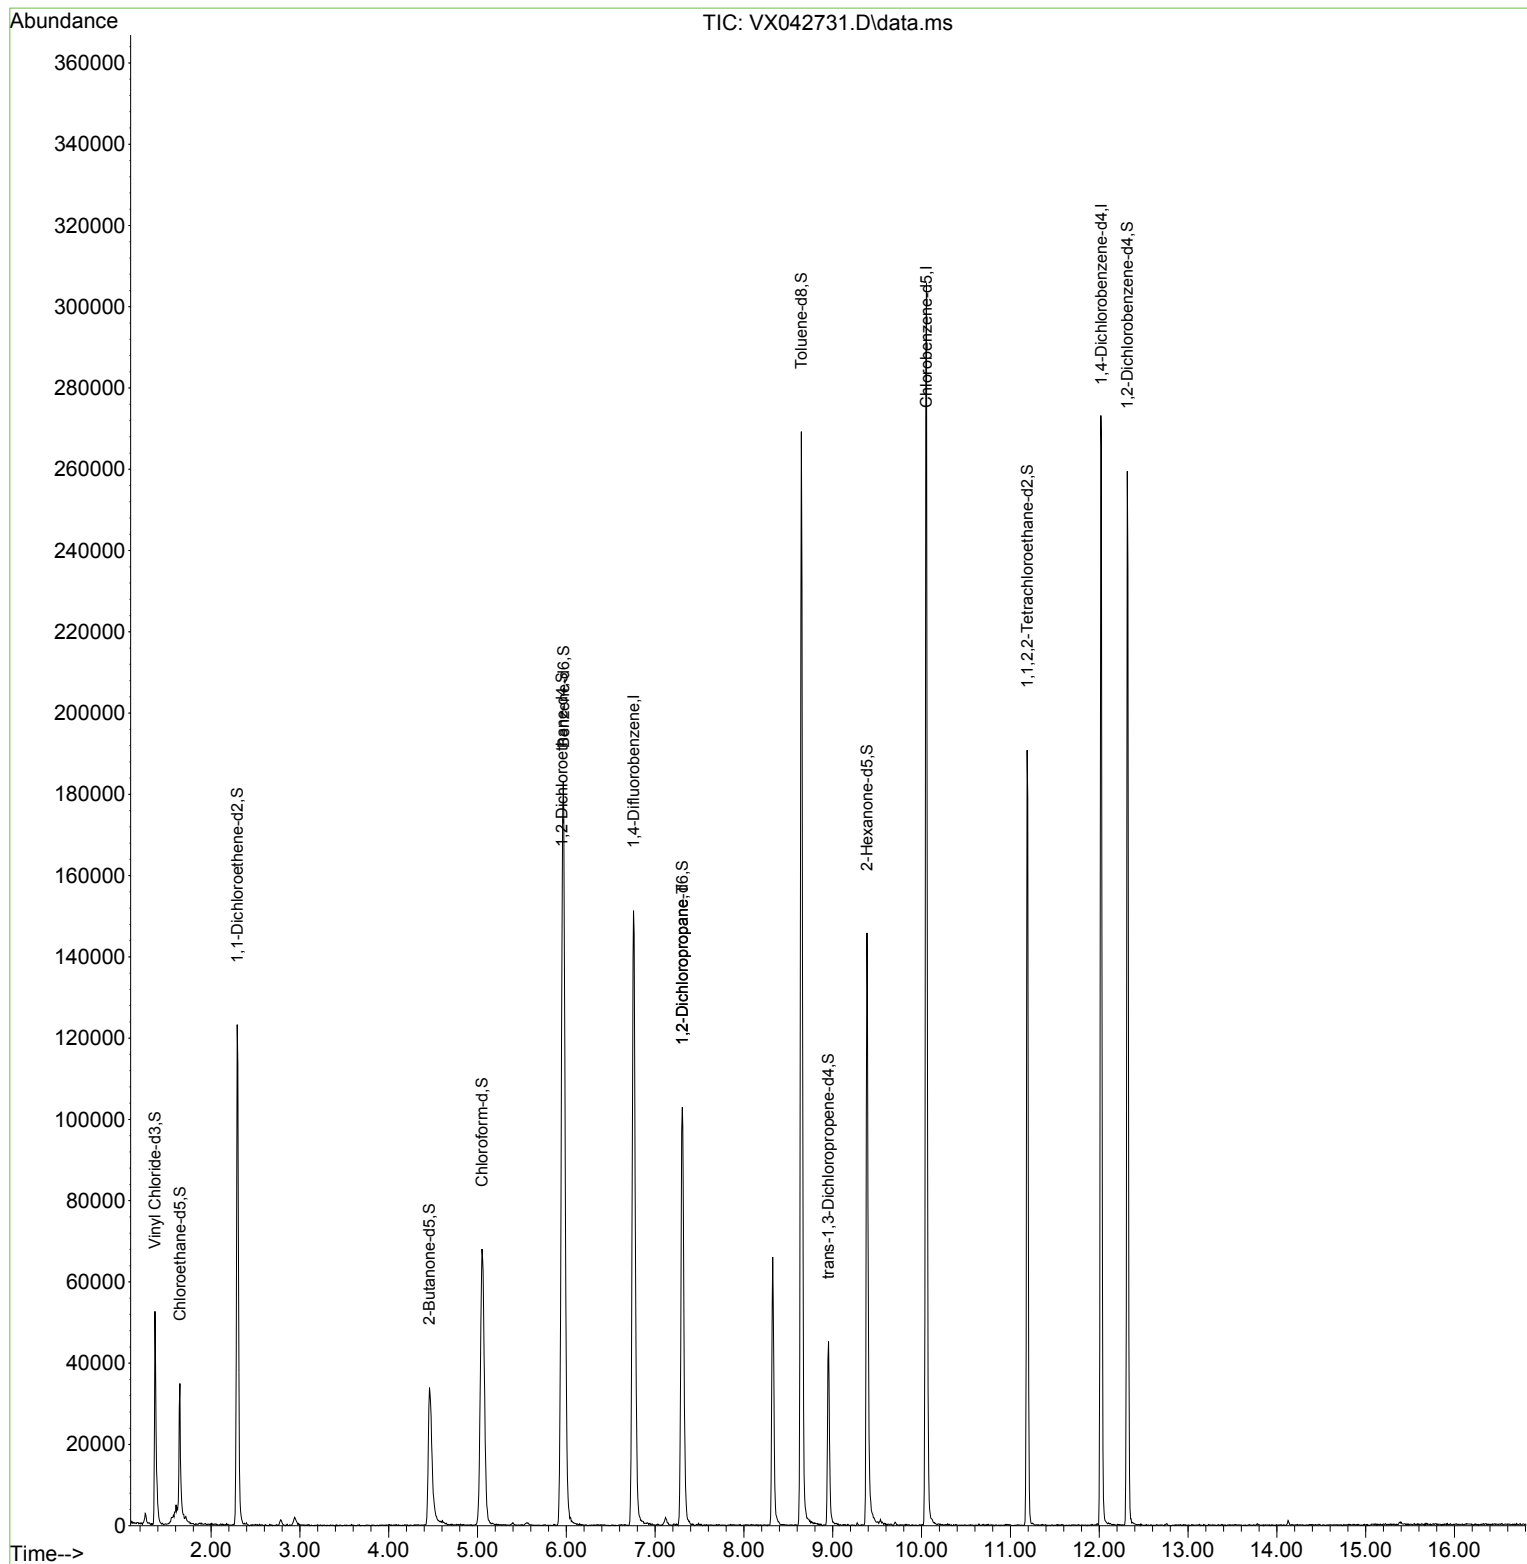

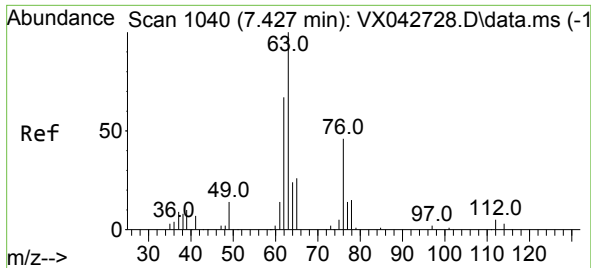

#37
1,2-Dichloropropane
Concen: 5.416 ug/L
RT: 7.306 min Scan# 10
Delta R.T. -0.122 min
Lab File: VX042731.D
Acq: 30 Jul 2024 11:55

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 63 Resp: 6246
Ion Ratio Lower Upper
63 100
112 0.0 3.7 5.5#

