

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042743.D
 Acq On : 30 Jul 2024 16:42
 Operator : JC/MD
 Sample : P3361-01ME 10X
 Misc : 11.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 31 03:18:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 31 03:10:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	132139	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	122395	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	49848	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	36951	46.028	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.060%
7) Chloroethane-d5	1.642	69	16384	49.527	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.060%
11) 1,1-Dichloroethene-d2	2.294	65	17925	45.318	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.640%
21) 2-Butanone-d5	4.471	46	55948	94.031	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.030%
24) Chloroform-d	5.056	84	84014	47.812	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.620%
26) 1,2-Dichloroethane-d4	5.958	65	56392	49.745	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.480%
32) Benzene-d6	5.970	84	167542	49.322	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.640%
36) 1,2-Dichloropropane-d6	7.312	67	49108	48.847	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	97.700%
41) Toluene-d8	8.647	98	145349	47.724	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.440%
43) trans-1,3-Dichloroprop...	8.952	79	20338	43.229	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.460%
47) 2-Hexanone-d5	9.391	63	41068	91.366	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.370%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	69616	48.094	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.180%
66) 1,2-Dichlorobenzene-d4	12.323	152	50250	53.340	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.680%
Target Compounds						
					Qvalue	
34) Trichloroethene	7.123	95	7268	7.263	ug/L	89
61) 1,2,3-Trichloropropane	12.024	75	5922	5.135	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042743.D
Acq On : 30 Jul 2024 16:42
Operator : JC/MD
Sample : P3361-01ME 10X
Misc : 11.91g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :


Quant Time: Jul 31 03:18:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 03:10:58 2024
Response via : Initial Calibration

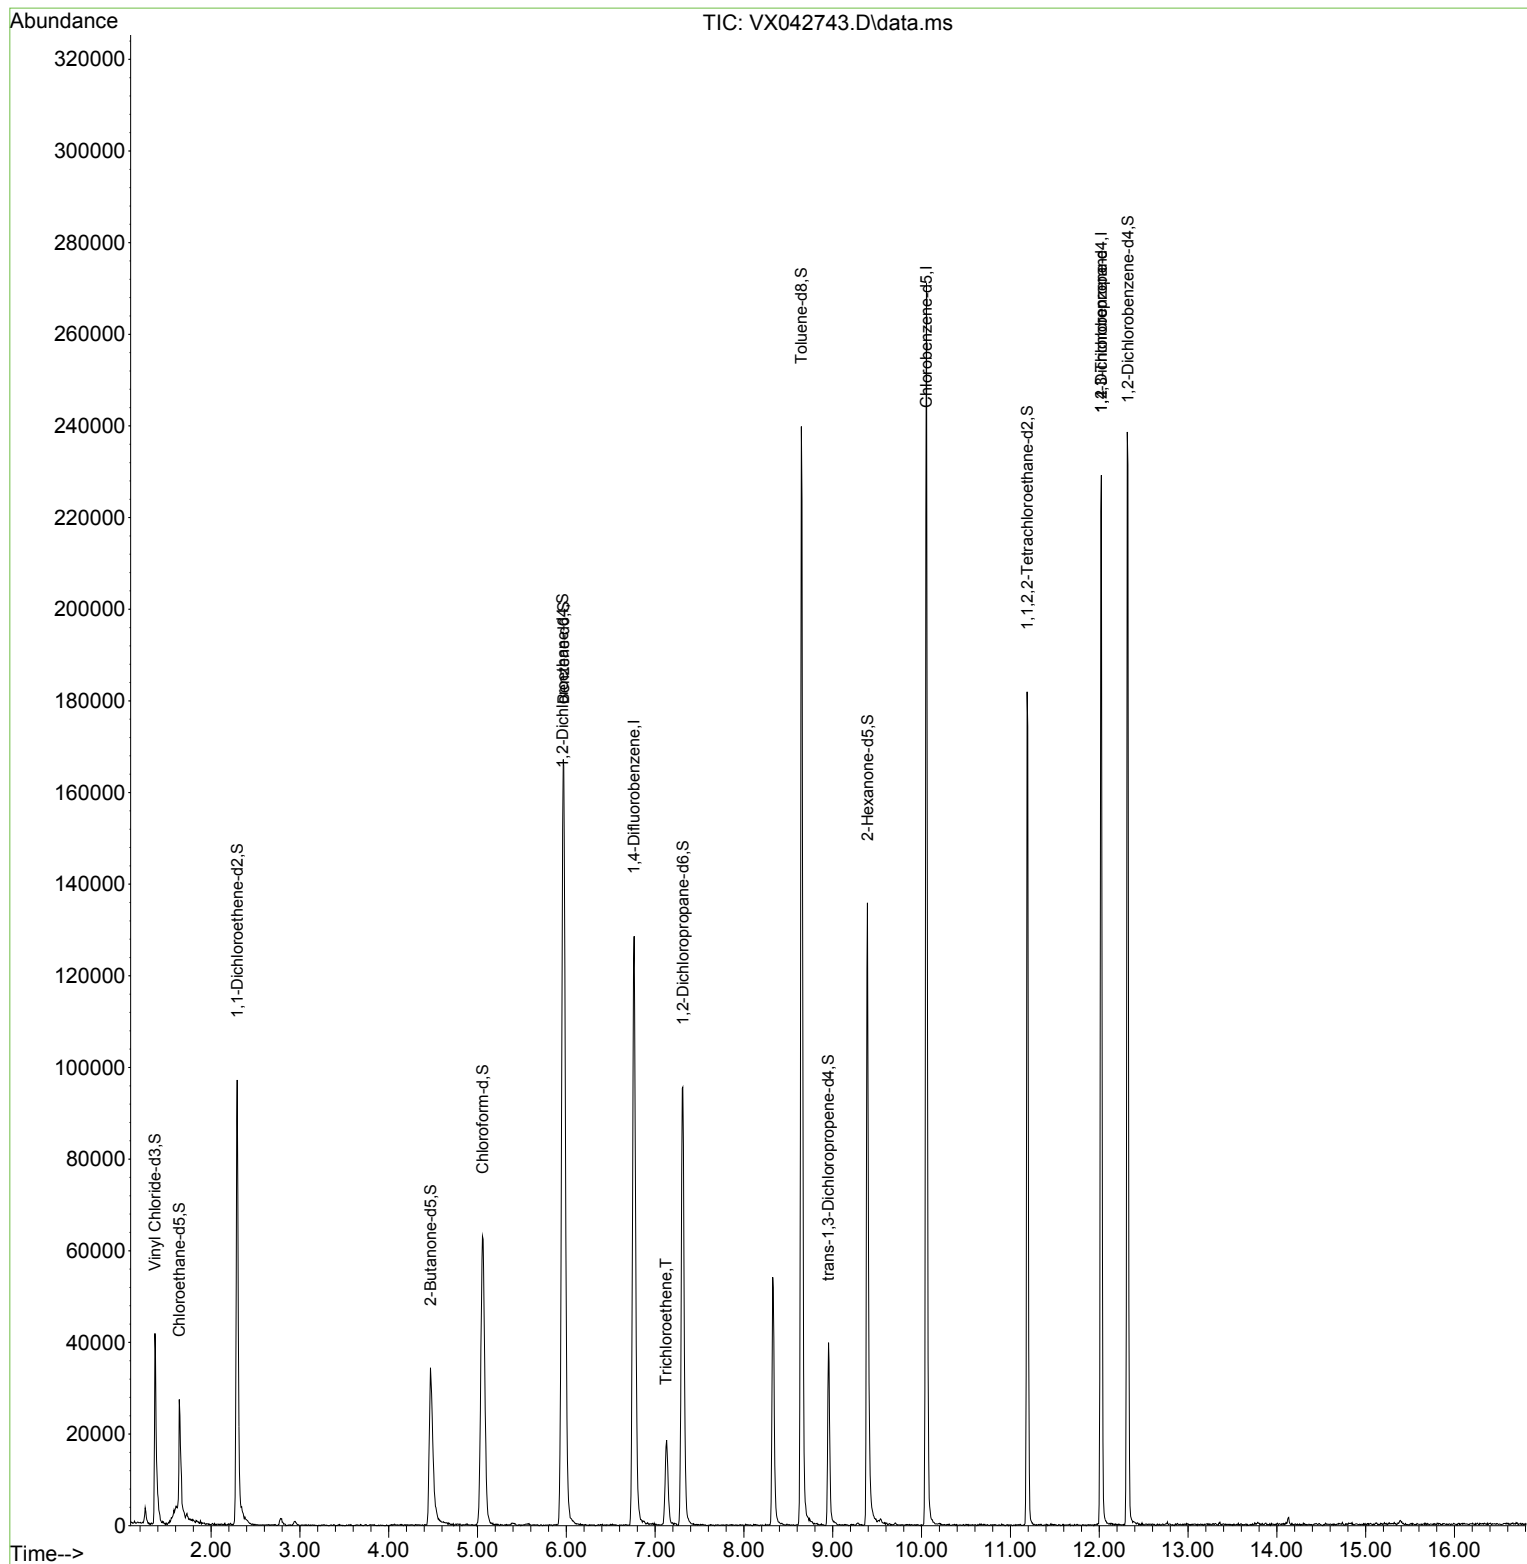

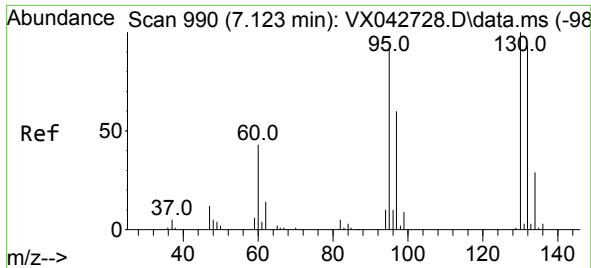




#34
Trichloroethene
Concen: 7.263 ug/L
RT: 7.123 min Scan# 990
Delta R.T. 0.000 min
Lab File: VX042743.D
Acq: 30 Jul 2024 16:42

Instrument :
MSVOA_X
ClientSampleId :

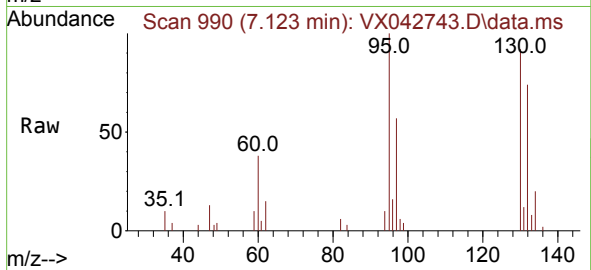

Tgt Ion: 95 Resp: 7268

Ion	Ratio	Lower	Upper
95	100		
97	57.4	46.3	86.1
132	73.8	64.3	119.5
130	91.9	67.0	124.4

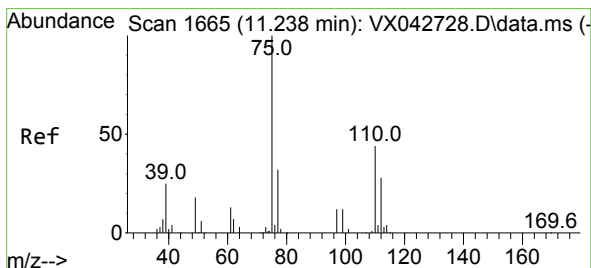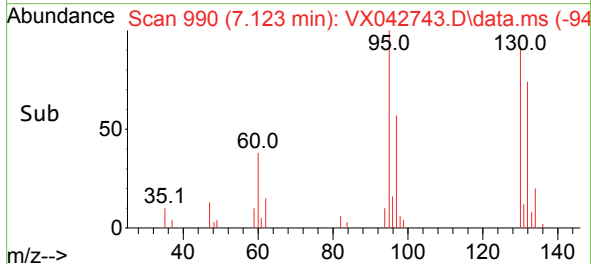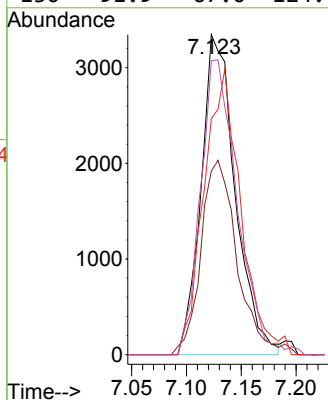

#61
1,2,3-Trichloropropane
Concen: 5.135 ug/L
RT: 12.024 min Scan# 1794
Delta R.T. 0.786 min
Lab File: VX042743.D
Acq: 30 Jul 2024 16:42

Tgt Ion: 75 Resp: 5922

Ion	Ratio	Lower	Upper
75	100		
77	33.7	26.2	39.4
110	3.1	33.0	49.4#

