

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042749.D
 Acq On : 30 Jul 2024 19:02
 Operator : JC/MD
 Sample : P3378-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B06

Quant Time: Jul 31 03:20:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jul 31 03:10:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	138050	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	126398	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	51418	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	33668	40.143	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	80.280%
7) Chloroethane-d5	1.648	69	16031	46.385	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.780%
11) 1,1-Dichloroethene-d2	2.294	65	18775	45.434	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.860%
21) 2-Butanone-d5	4.471	46	56470	90.844	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.840%
24) Chloroform-d	5.062	84	83663	45.574	ug/L	0.01
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.140%
26) 1,2-Dichloroethane-d4	5.958	65	55454	46.823	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.640%
32) Benzene-d6	5.970	84	166235	47.388	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.780%
36) 1,2-Dichloropropane-d6	7.305	67	49403	47.584	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.160%
41) Toluene-d8	8.647	98	145326	46.205	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.400%
43) trans-1,3-Dichloroprop...	8.951	79	20247	41.673	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.340%
47) 2-Hexanone-d5	9.384	63	41499	89.401	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.400%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	70291	47.022	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.040%
66) 1,2-Dichlorobenzene-d4	12.323	152	49470	50.909	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.820%
Target Compounds						
13) Acetone	2.386	43	2281	4.694	ug/L	Qvalue 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042749.D
Acq On : 30 Jul 2024 19:02
Operator : JC/MD
Sample : P3378-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B06

Quant Time: Jul 31 03:20:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Jul 31 03:10:58 2024
Response via : Initial Calibration

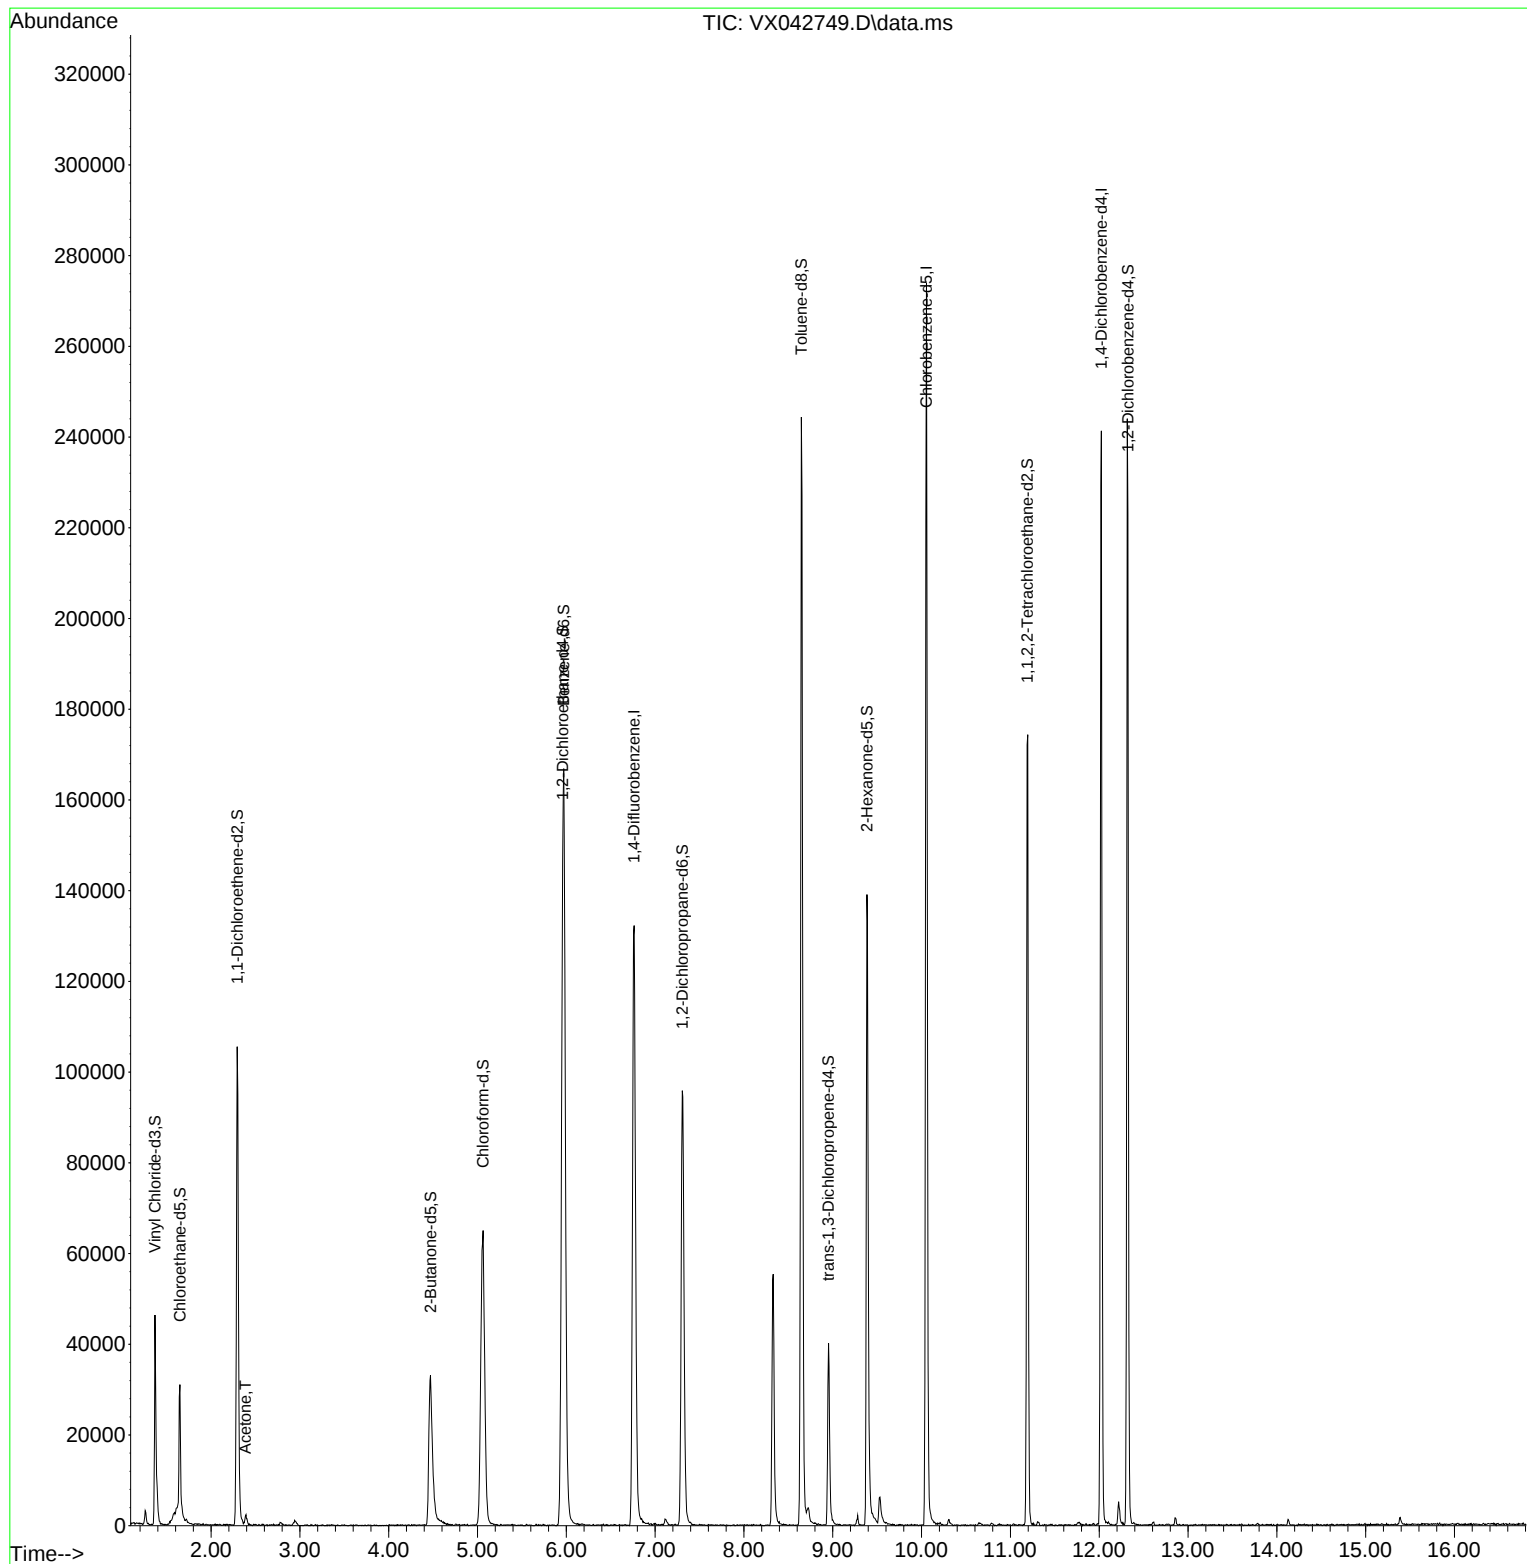

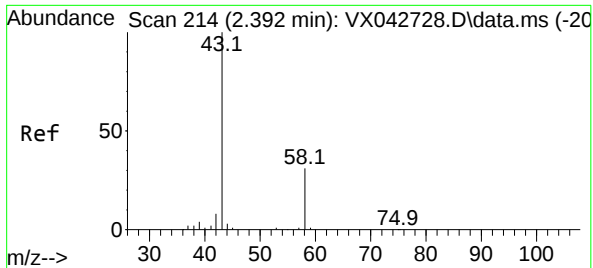

#13
 Acetone
 Concen: 4.694 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VX042749.D
 Acq: 30 Jul 2024 19:02

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B06

Tgt Ion: 43 Resp: 2281
 Ion Ratio Lower Upper
 43 100
 58 21.1 0.0 62.4

