

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042730.D
 Acq On : 30 Jul 2024 11:25
 Operator : JC/MD
 Sample : VX0730WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK709

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.264	24	29	32	rBV4	2870	3857	0.74%	0.100%
2	1.374	43	47	57	rBV	45658	61566	11.77%	1.599%
3	1.648	89	92	101	rVB	30693	38505	7.36%	1.000%
4	2.300	192	199	211	rBV	116614	183477	35.08%	4.767%
5	2.575	242	244	246	rBV	187	210	0.04%	0.005%
6	2.709	263	266	268	rBV2	343	408	0.08%	0.011%
7	2.746	271	272	274	rBV2	290	221	0.04%	0.006%
8	2.794	274	280	287	rVB4	1590	3324	0.64%	0.086%
9	2.947	298	305	312	rBV2	3686	7286	1.39%	0.189%
10	3.032	315	319	320	rBV	303	289	0.06%	0.008%
11	3.099	325	330	331	rBV4	779	1305	0.25%	0.034%
12	3.282	353	360	362	rBV	139	306	0.06%	0.008%
13	3.367	371	374	375	rVB	219	202	0.04%	0.005%
14	3.392	375	378	383	rBV	213	373	0.07%	0.010%
15	3.508	394	397	398	rBV	206	193	0.04%	0.005%
16	3.605	409	413	415	rBV	352	379	0.07%	0.010%
17	3.678	422	425	427	rBB	159	165	0.03%	0.004%
18	3.697	427	428	431	rBV	146	160	0.03%	0.004%
19	3.721	431	432	435	rVV	215	114	0.02%	0.003%
20	3.800	443	445	448	rBV2	219	267	0.05%	0.007%
21	3.898	457	461	464	rBV	124	217	0.04%	0.006%
22	3.922	464	465	468	rVB2	143	133	0.03%	0.003%
23	3.965	471	472	474	rBB2	209	135	0.03%	0.004%
24	3.989	474	476	478	rBB	223	208	0.04%	0.005%
25	4.020	478	481	482	rBV	333	305	0.06%	0.008%
26	4.123	496	498	499	rVB	184	121	0.02%	0.003%
27	4.142	499	501	504	rVB	171	121	0.02%	0.003%
28	4.325	528	531	533	rBV	191	263	0.05%	0.007%
29	4.410	543	545	547	rBV	254	238	0.05%	0.006%
30	4.465	547	554	571	rBV2	33653	102115	19.53%	2.653%
31	4.794	605	608	610	rBV2	418	379	0.07%	0.010%
32	5.056	640	651	669	rBV2	67796	207311	39.64%	5.386%
33	5.282	687	688	691	rBV	260	161	0.03%	0.004%
34	5.349	697	699	700	rBV	180	122	0.02%	0.003%
35	5.550	731	732	734	rBV2	600	532	0.10%	0.014%
36	5.654	746	749	750	rBV	482	411	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042730.D
 Acq On : 30 Jul 2024 11:25
 Operator : JC/MD
 Sample : VX0730WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK709

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.739	762	763	764	rBV	170	102	0.02%	0.003%
38	5.806	771	774	776	rBV	217	226	0.04%	0.006%
39	5.873	784	785	790	rBV	201	282	0.05%	0.007%
40	5.971	790	801	820	rBV3	175165	522988	100.00%	13.587%
41	6.288	849	853	854	rBV2	174	151	0.03%	0.004%
42	6.464	879	882	884	rBB	206	192	0.04%	0.005%
43	6.495	884	887	889	rBB	233	218	0.04%	0.006%
44	6.531	889	893	894	rBV	164	246	0.05%	0.006%
45	6.696	919	920	922	rBV	267	233	0.04%	0.006%
46	6.757	922	930	947	rVV	141500	343429	65.67%	8.922%
47	7.068	978	981	983	rVB2	297	331	0.06%	0.009%
48	7.129	985	991	997	rVB6	2198	5719	1.09%	0.149%
49	7.208	1002	1004	1007	rVV	257	174	0.03%	0.005%
50	7.306	1012	1020	1031	rBV	101899	225826	43.18%	5.867%
51	7.897	1115	1117	1118	rBV2	122	118	0.02%	0.003%
52	8.001	1132	1134	1135	rBV	183	164	0.03%	0.004%
53	8.110	1150	1152	1153	rBV	162	110	0.02%	0.003%
54	8.245	1171	1174	1177	rBV	226	236	0.05%	0.006%
55	8.324	1182	1187	1201	rVV	65589	109008	20.84%	2.832%
56	8.525	1218	1220	1223	rBV2	245	318	0.06%	0.008%
57	8.647	1234	1240	1250	rBV	260501	408577	78.12%	10.615%
58	8.952	1285	1290	1302	rBV	44855	71542	13.68%	1.859%
59	9.104	1314	1315	1318	rBV	305	269	0.05%	0.007%
60	9.275	1340	1343	1348	rVB4	1194	1860	0.36%	0.048%
61	9.385	1356	1361	1374	rBV	139593	218603	41.80%	5.679%
62	9.964	1454	1456	1458	rVB	277	218	0.04%	0.006%
63	9.982	1458	1459	1462	rBV	288	333	0.06%	0.009%
64	10.055	1465	1471	1487	rVV	288404	399358	76.36%	10.375%
65	10.427	1529	1532	1535	rBV	215	249	0.05%	0.006%
66	10.561	1552	1554	1557	rVB	190	207	0.04%	0.005%
67	10.604	1557	1561	1564	rBV2	223	283	0.05%	0.007%
68	10.647	1564	1568	1570	rBV3	1733	2538	0.49%	0.066%
69	10.921	1611	1613	1617	rVV2	159	177	0.03%	0.005%
70	10.964	1617	1620	1626	rVB3	1910	2282	0.44%	0.059%
71	11.104	1641	1643	1646	rBV2	248	292	0.06%	0.008%
72	11.189	1652	1657	1669	rBV	194036	249820	47.77%	6.490%
73	11.293	1673	1674	1677	rBB	203	202	0.04%	0.005%
74	11.329	1678	1680	1681	rBV	241	154	0.03%	0.004%
75	11.427	1694	1696	1698	rBV	138	135	0.03%	0.004%
76	11.457	1698	1701	1705	rVV2	1224	1514	0.29%	0.039%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042730.D
 Acq On : 30 Jul 2024 11:25
 Operator : JC/MD
 Sample : VX0730WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK709

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.622	1726	1728	1730	rVB	241	180	0.03%	0.005%
78	11.646	1730	1732	1736	rBB	222	284	0.05%	0.007%
79	11.701	1740	1741	1743	rBV	129	108	0.02%	0.003%
80	11.756	1747	1750	1754	rBV4	1536	2225	0.43%	0.058%
81	11.884	1770	1771	1772	rBV4	246	141	0.03%	0.004%
82	11.969	1782	1785	1788	rVV4	1551	1984	0.38%	0.052%
83	12.018	1788	1793	1804	rVB	252817	329677	63.04%	8.565%
84	12.317	1837	1842	1857	rVB	245241	323475	61.85%	8.404%
85	12.567	1880	1883	1884	rBV	224	268	0.05%	0.007%
86	12.707	1903	1906	1909	rVV2	198	227	0.04%	0.006%
87	12.847	1928	1929	1932	rBV2	247	217	0.04%	0.006%
88	12.981	1950	1951	1954	rVB	250	191	0.04%	0.005%
89	13.018	1954	1957	1959	rBV	313	382	0.07%	0.010%
90	13.055	1961	1963	1964	rBV	208	201	0.04%	0.005%
91	13.305	2002	2004	2007	rVB	369	315	0.06%	0.008%
92	13.500	2035	2036	2038	rBV	219	199	0.04%	0.005%
93	13.591	2048	2051	2058	rVB4	1034	1312	0.25%	0.034%
94	13.670	2063	2064	2065	rBV	225	124	0.02%	0.003%
95	13.725	2072	2073	2076	rBV	231	198	0.04%	0.005%
96	13.780	2079	2082	2090	rVB4	1273	1981	0.38%	0.051%
97	13.841	2090	2092	2093	rBV	231	167	0.03%	0.004%
98	14.189	2146	2149	2153	rBV2	358	536	0.10%	0.014%
99	14.500	2198	2200	2201	rBV	276	262	0.05%	0.007%
100	16.103	2461	2463	2465	rBV	378	415	0.08%	0.011%




Sum of corrected areas: 3849132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042730.D
Acq On : 30 Jul 2024 11:25
Operator : JC/MD
Sample : VX0730WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK709

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

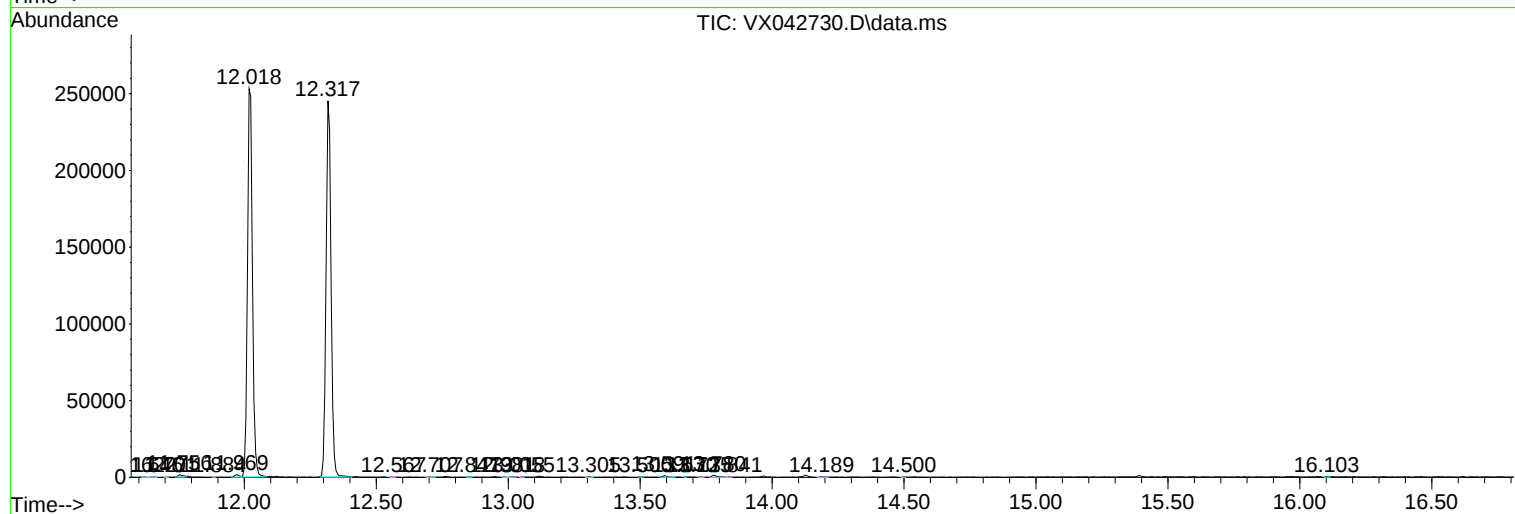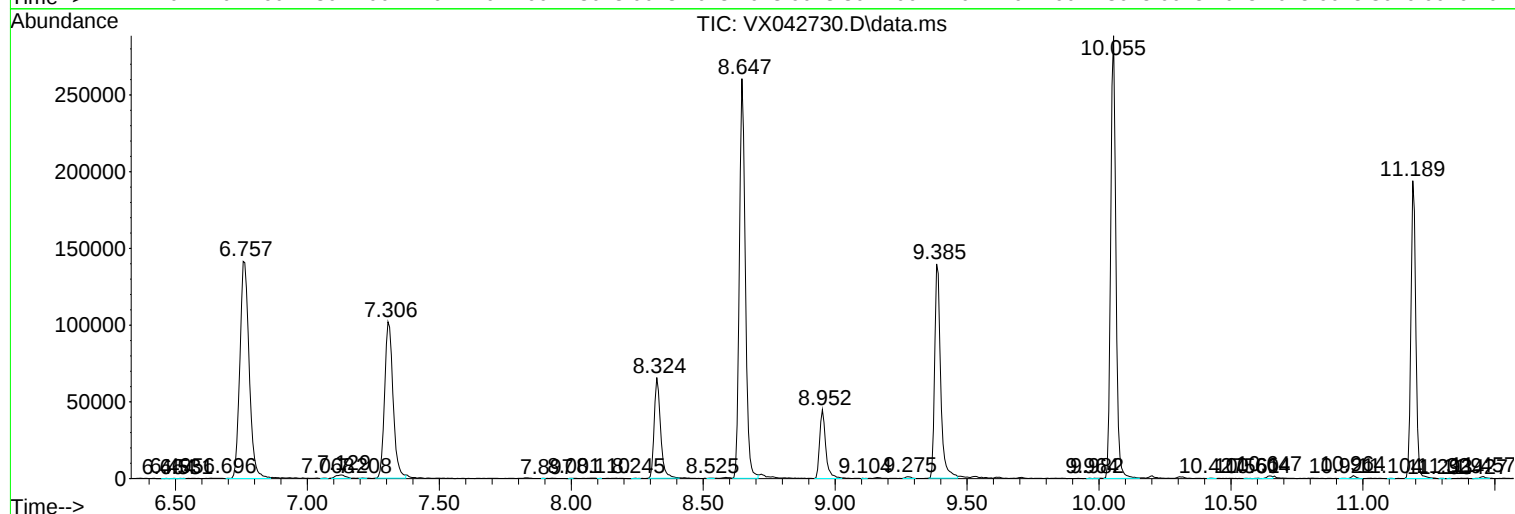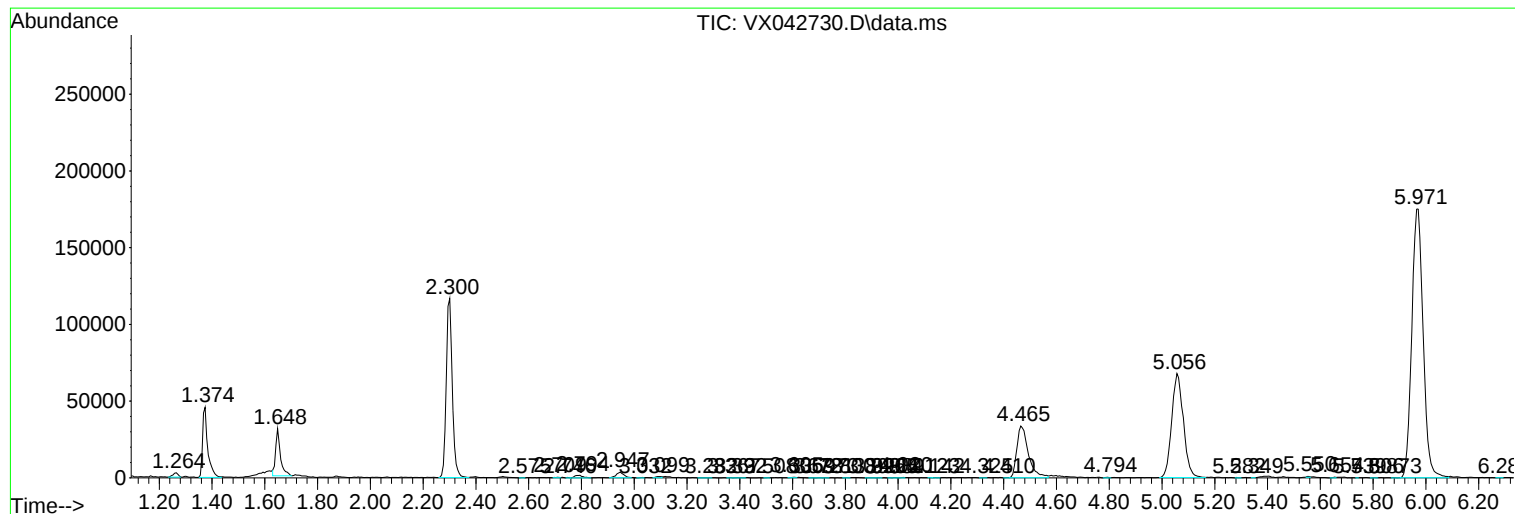

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042730.D
Acq On : 30 Jul 2024 11:25
Operator : JC/MD
Sample : VX0730WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK709

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042730.D
Acq On : 30 Jul 2024 11:25
Operator : JC/MD
Sample : VX0730WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK709

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc