

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042735.D
 Acq On : 30 Jul 2024 13:35
 Operator : JC/MD
 Sample : P3398-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	14	rVB	2447	2614	0.44%	0.060%
2	1.264	26	29	32	rVB3	2767	3307	0.55%	0.076%
3	1.368	43	46	57	rBV	57674	75193	12.57%	1.734%
4	1.648	88	92	100	rVB	31558	42901	7.17%	0.989%
5	2.093	164	165	167	rBV	443	239	0.04%	0.006%
6	2.294	192	198	210	rBV	129952	212532	35.53%	4.900%
7	2.392	210	214	220	rVB2	1655	3255	0.54%	0.075%
8	2.495	230	231	236	rVB2	202	247	0.04%	0.006%
9	2.569	241	243	249	rVB3	582	876	0.15%	0.020%
10	2.672	259	260	263	rBV	216	263	0.04%	0.006%
11	2.788	275	279	284	rBV3	1212	2000	0.33%	0.046%
12	2.873	290	293	295	rBV	279	349	0.06%	0.008%
13	2.940	298	304	311	rVV3	3345	7219	1.21%	0.166%
14	3.361	370	373	376	rBV	231	273	0.05%	0.006%
15	4.135	498	500	505	rVB2	310	284	0.05%	0.007%
16	4.471	546	555	570	rBV2	40190	120879	20.21%	2.787%
17	4.904	623	626	629	rBV2	375	574	0.10%	0.013%
18	5.056	637	651	664	rBV	81341	241515	40.38%	5.568%
19	5.397	705	707	709	rVV2	380	368	0.06%	0.008%
20	5.458	712	717	718	rBV	218	297	0.05%	0.007%
21	5.562	731	734	740	rBV3	342	739	0.12%	0.017%
22	5.964	789	800	820	rVV3	200111	598096	100.00%	13.789%
23	6.178	833	835	840	rVB2	299	368	0.06%	0.008%
24	6.251	846	847	852	rBV2	162	238	0.04%	0.005%
25	6.318	857	858	862	rVB2	332	389	0.07%	0.009%
26	6.385	867	869	875	rVB2	235	407	0.07%	0.009%
27	6.763	920	931	948	rBV	146667	359802	60.16%	8.295%
28	6.909	954	955	960	rBV2	330	488	0.08%	0.011%
29	7.117	985	989	990	rBV3	1521	1695	0.28%	0.039%
30	7.306	1012	1020	1038	rBV	116129	261579	43.74%	6.031%
31	7.482	1047	1049	1052	rBV3	416	419	0.07%	0.010%
32	7.598	1063	1068	1073	rBV2	683	1451	0.24%	0.033%
33	7.708	1084	1086	1090	rVB2	299	361	0.06%	0.008%
34	7.751	1090	1093	1095	rBV	257	377	0.06%	0.009%
35	7.836	1102	1107	1109	rBV2	558	989	0.17%	0.023%
36	7.982	1126	1131	1132	rBV2	285	345	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042735.D
 Acq On : 30 Jul 2024 13:35
 Operator : JC/MD
 Sample : P3398-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	8.324	1181	1187	1200	rBV	72423	125246	20.94%	2.888%
38	8.415	1200	1202	1205	rVV	697	658	0.11%	0.015%
39	8.458	1207	1209	1211	rVV	399	311	0.05%	0.007%
40	8.494	1214	1215	1217	rBV	378	289	0.05%	0.007%
41	8.598	1227	1232	1233	rBV	410	476	0.08%	0.011%
42	8.647	1234	1240	1249	rBV	293484	462529	77.33%	10.664%
43	8.848	1271	1273	1276	rVB3	288	263	0.04%	0.006%
44	8.952	1284	1290	1303	rBV	53488	81861	13.69%	1.887%
45	9.275	1339	1343	1347	rBV3	2837	3844	0.64%	0.089%
46	9.384	1356	1361	1376	rBV	161598	255250	42.68%	5.885%
47	9.573	1391	1392	1395	rVB2	647	365	0.06%	0.008%
48	9.610	1396	1398	1404	rVB4	649	963	0.16%	0.022%
49	9.671	1406	1408	1410	rBV	251	239	0.04%	0.006%
50	9.951	1451	1454	1456	rVB	213	263	0.04%	0.006%
51	10.055	1465	1471	1486	rBV	292304	408623	68.32%	9.421%
52	10.159	1486	1488	1492	rBV5	733	879	0.15%	0.020%
53	10.275	1503	1507	1508	rBV	318	385	0.06%	0.009%
54	10.305	1508	1512	1519	rVB2	2617	4513	0.75%	0.104%
55	10.360	1519	1521	1524	rVB2	313	352	0.06%	0.008%
56	10.396	1524	1527	1530	rBV2	308	493	0.08%	0.011%
57	10.659	1564	1570	1578	rVV4	4714	8841	1.48%	0.204%
58	10.799	1591	1593	1596	rBV3	584	470	0.08%	0.011%
59	10.866	1603	1604	1608	rVB	241	251	0.04%	0.006%
60	10.970	1617	1621	1625	rVB3	232	340	0.06%	0.008%
61	11.189	1652	1657	1663	rBV	205839	273622	45.75%	6.308%
62	11.280	1669	1672	1673	rBV2	343	438	0.07%	0.010%
63	11.451	1698	1700	1701	rBV	482	275	0.05%	0.006%
64	11.628	1725	1729	1732	rVB2	280	420	0.07%	0.010%
65	11.756	1747	1750	1752	rVB2	640	532	0.09%	0.012%
66	11.805	1755	1758	1761	rBV2	229	338	0.06%	0.008%
67	11.933	1775	1779	1782	rVB	399	556	0.09%	0.013%
68	11.969	1782	1785	1788	rBV2	3378	4096	0.68%	0.094%
69	12.024	1789	1794	1804	rVB	262502	344815	57.65%	7.950%
70	12.183	1818	1820	1822	rBV	332	297	0.05%	0.007%
71	12.219	1824	1826	1830	rVV2	891	996	0.17%	0.023%
72	12.317	1836	1842	1851	rBV	276978	370325	61.92%	8.538%
73	12.384	1851	1853	1855	rVB3	479	297	0.05%	0.007%
74	12.664	1895	1899	1902	rBV2	274	492	0.08%	0.011%
75	12.762	1912	1915	1916	rBV	239	246	0.04%	0.006%
76	12.866	1925	1932	1937	rBV3	668	1168	0.20%	0.027%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042735.D
 Acq On : 30 Jul 2024 13:35
 Operator : JC/MD
 Sample : P3398-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	12.957	1940	1947	1948	rVB	418	680	0.11%	0.016%
78	12.994	1948	1953	1955	rBV	193	329	0.06%	0.008%
79	13.030	1958	1959	1961	rBV	320	243	0.04%	0.006%
80	13.335	2006	2009	2012	rVV	270	311	0.05%	0.007%
81	13.384	2012	2017	2019	rVB2	222	323	0.05%	0.007%
82	13.445	2024	2027	2029	rBV	260	303	0.05%	0.007%
83	13.573	2045	2048	2049	rBV	254	293	0.05%	0.007%
84	13.591	2049	2051	2058	rVV3	1637	1750	0.29%	0.040%
85	13.725	2069	2073	2077	rBV4	3667	4056	0.68%	0.094%
86	13.780	2077	2082	2091	rVB2	14486	19914	3.33%	0.459%
87	14.073	2126	2130	2131	rBV2	265	280	0.05%	0.006%
88	14.127	2135	2139	2143	rVV	1727	2305	0.39%	0.053%
89	14.164	2143	2145	2149	rVB	270	245	0.04%	0.006%
90	14.225	2153	2155	2158	rVB2	219	257	0.04%	0.006%
91	14.615	2216	2219	2221	rBV2	276	360	0.06%	0.008%
92	14.688	2227	2231	2234	rVB2	314	395	0.07%	0.009%
93	15.127	2301	2303	2304	rBV2	314	269	0.04%	0.006%
94	15.396	2338	2347	2352	rBV4	1730	3592	0.60%	0.083%
95	15.609	2380	2382	2384	rVB	460	293	0.05%	0.007%
96	15.792	2410	2412	2416	rVB2	285	335	0.06%	0.008%
97	16.133	2465	2468	2469	rBV3	368	405	0.07%	0.009%
98	16.158	2471	2472	2474	rBV	289	267	0.04%	0.006%
99	16.523	2530	2532	2533	rBV	345	276	0.05%	0.006%
100	16.566	2536	2539	2540	rBV2	371	345	0.06%	0.008%




Sum of corrected areas: 4337371

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042735.D
Acq On : 30 Jul 2024 13:35
Operator : JC/MD
Sample : P3398-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

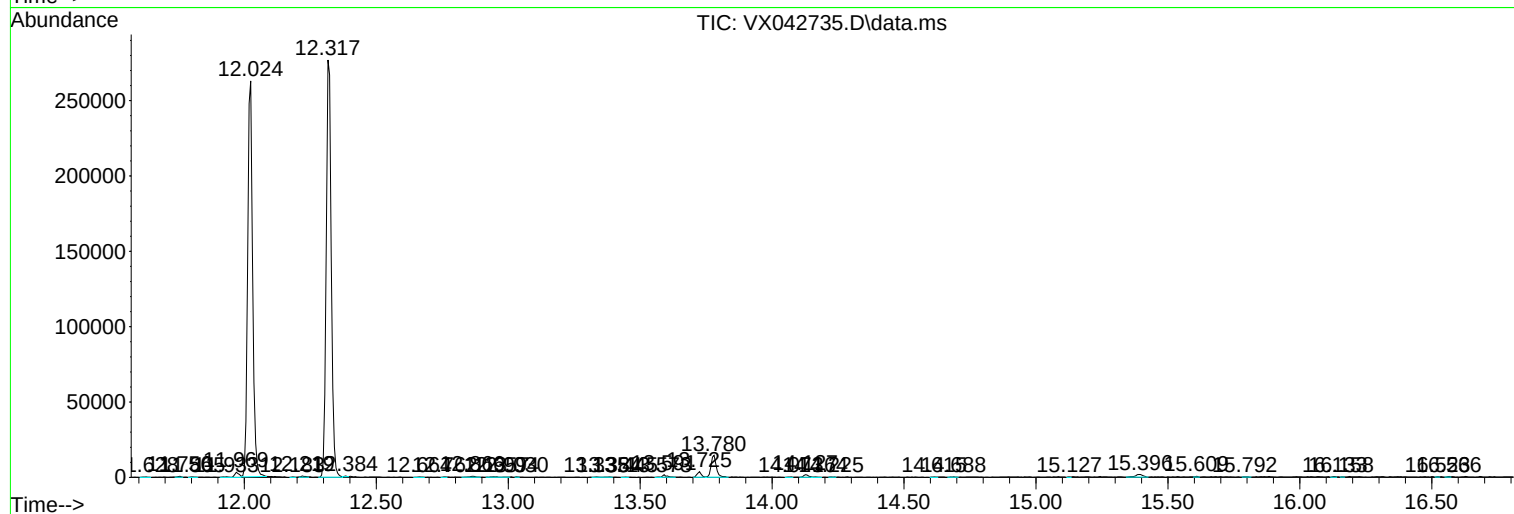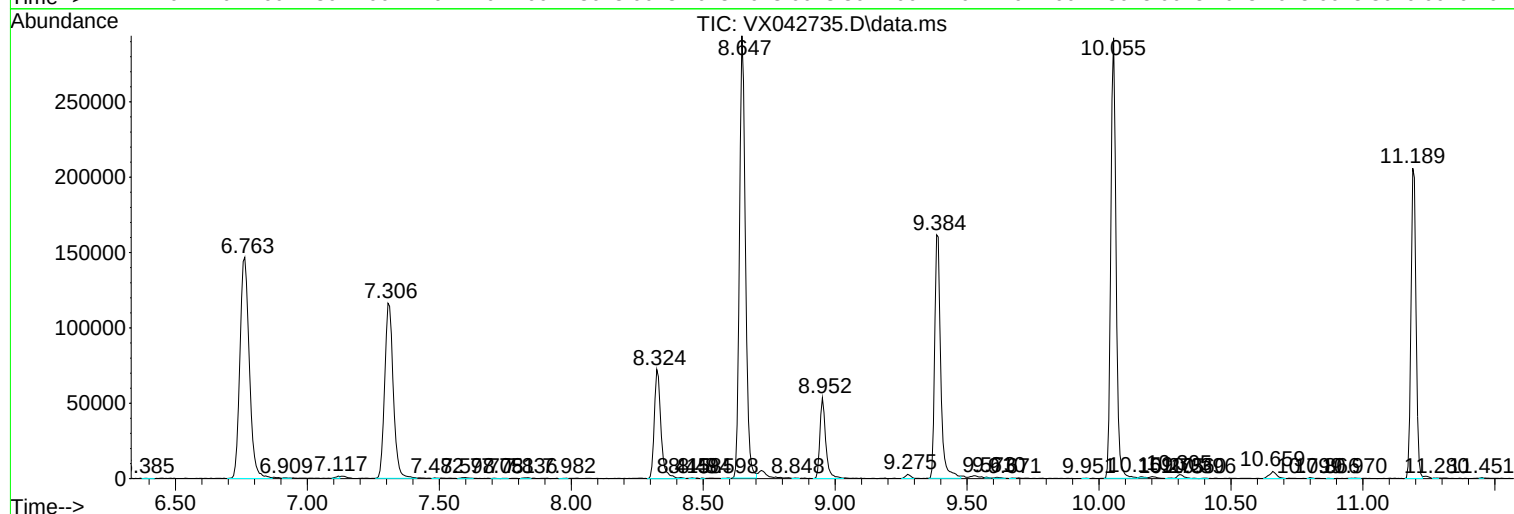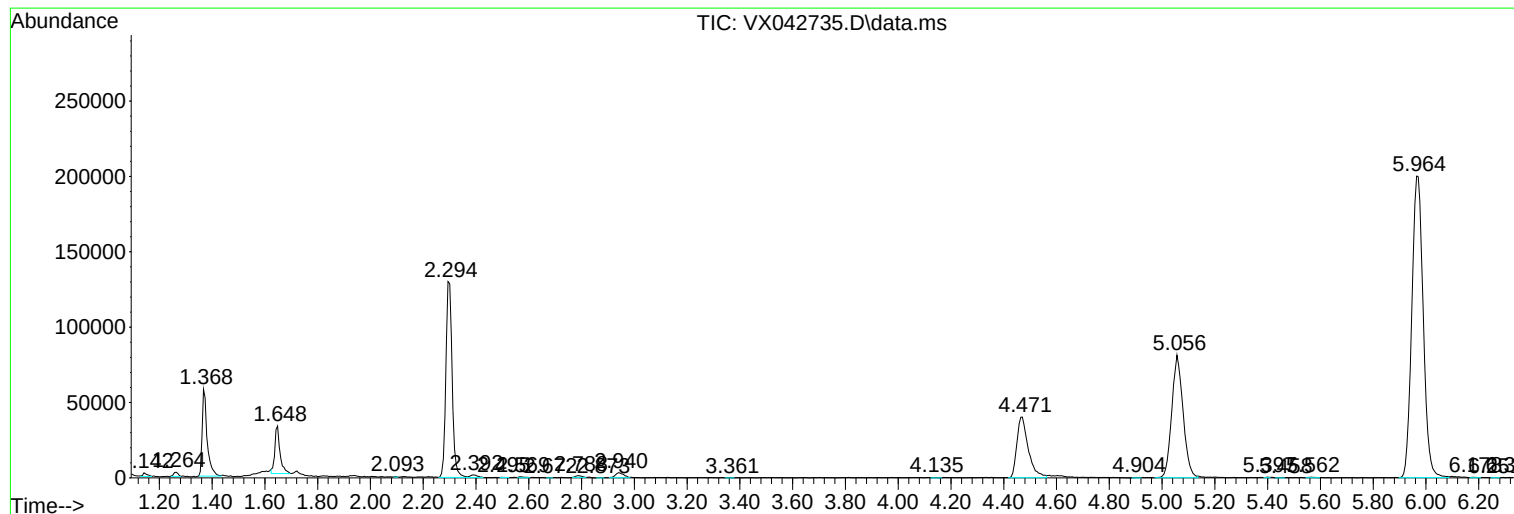

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042735.D
Acq On : 30 Jul 2024 13:35
Operator : JC/MD
Sample : P3398-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08K3










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1H-Indene, 1-methylene- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.780	2.89 ug/L	19914	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1H-Indene, 1-methylene-			128	C10H8	002471-84-3	91
2	Naphthalene			128	C10H8	000091-20-3	91
3	Naphthalene			128	C10H8	000091-20-3	91
4	Naphthalene			128	C10H8	000091-20-3	91
5	Azulene			128	C10H8	000275-51-4	90

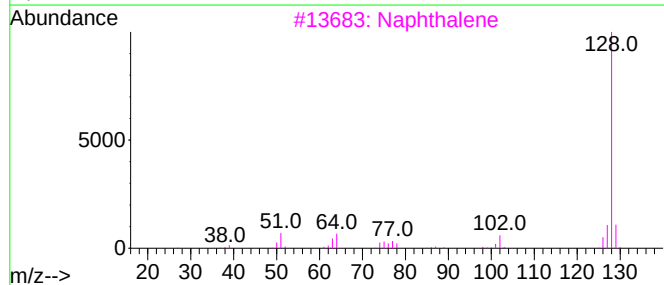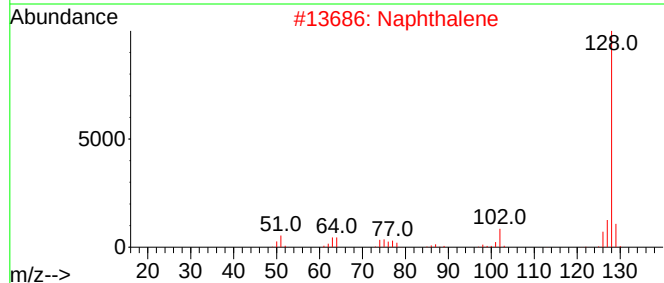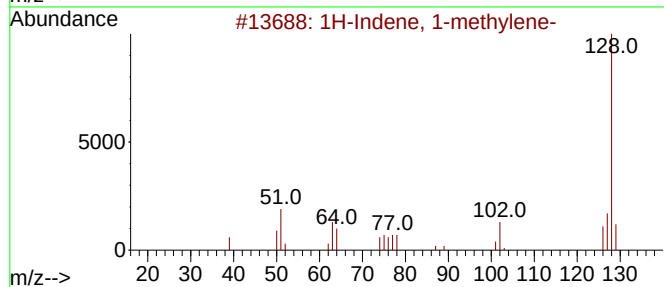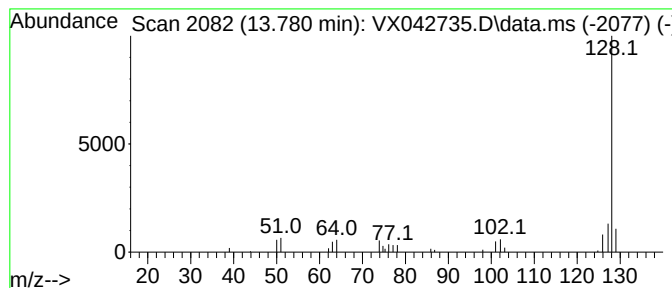

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042735.D
Acq On : 30 Jul 2024 13:35
Operator : JC/MD
Sample : P3398-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 1-me...	13.780	2.9	ug/L	19914	3	12.024	344815	50.0