

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042738.D
 Acq On : 30 Jul 2024 14:45
 Operator : JC/MD
 Sample : P3388-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042738.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	53757	67599	12.43%	1.713%
2	1.648	89	92	101	rVB	31388	38583	7.09%	0.978%
3	2.294	192	198	211	rBV	118785	192214	35.34%	4.870%
4	2.477	226	228	230	rBV	191	165	0.03%	0.004%
5	2.697	262	264	265	rBV	193	158	0.03%	0.004%
6	2.794	274	280	286	rBV5	1661	3467	0.64%	0.088%
7	2.880	293	294	296	rBV	129	80	0.01%	0.002%
8	2.941	298	304	313	rVV3	2083	4915	0.90%	0.125%
9	3.136	332	336	338	rBV2	373	463	0.09%	0.012%
10	3.160	338	340	341	rVB	157	88	0.02%	0.002%
11	3.337	368	369	373	rBB	91	85	0.02%	0.002%
12	3.373	374	375	377	rBV	268	239	0.04%	0.006%
13	3.447	385	387	390	rBV2	247	228	0.04%	0.006%
14	3.501	394	396	397	rBV	270	108	0.02%	0.003%
15	3.562	404	406	407	rBV	132	74	0.01%	0.002%
16	3.684	424	426	427	rBV	149	120	0.02%	0.003%
17	3.727	432	433	436	rVB	160	115	0.02%	0.003%
18	3.751	436	437	439	rBB	68	25	0.00%	0.001%
19	3.776	440	441	442	rBV	85	58	0.01%	0.001%
20	3.855	452	454	456	rVB	284	162	0.03%	0.004%
21	3.873	456	457	460	rBV	212	119	0.02%	0.003%
22	4.142	500	501	502	rBV	310	125	0.02%	0.003%
23	4.202	509	511	514	rBB	177	218	0.04%	0.006%
24	4.465	545	554	571	rBV	36330	107977	19.85%	2.736%
25	4.922	626	629	631	rVB	308	382	0.07%	0.010%
26	4.946	631	633	635	rBV2	348	328	0.06%	0.008%
27	5.056	639	651	666	rBV2	69832	222184	40.85%	5.629%
28	5.282	686	688	691	rBV	204	208	0.04%	0.005%
29	5.312	691	693	695	rVB	202	163	0.03%	0.004%
30	5.343	695	698	699	rBV	161	125	0.02%	0.003%
31	5.391	705	706	710	rBV	334	362	0.07%	0.009%
32	5.422	710	711	713	rVB	266	127	0.02%	0.003%
33	5.483	718	721	723	rBV	137	165	0.03%	0.004%
34	5.635	741	746	749	rBV2	265	536	0.10%	0.014%
35	5.970	789	801	819	rBV4	183392	543851	100.00%	13.779%
36	6.391	868	870	872	rVB	200	137	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042738.D
 Acq On : 30 Jul 2024 14:45
 Operator : JC/MD
 Sample : P3388-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.763	922	931	947	rBV	137943	340770	62.66%	8.633%
38	7.056	978	979	980	rBV	251	131	0.02%	0.003%
39	7.171	996	998	999	rBV	172	145	0.03%	0.004%
40	7.306	1012	1020	1035	rBV	105252	237454	43.66%	6.016%
41	7.635	1071	1074	1075	rBV	157	155	0.03%	0.004%
42	7.751	1090	1093	1094	rBV	248	285	0.05%	0.007%
43	7.805	1100	1102	1107	rBB	163	183	0.03%	0.005%
44	8.232	1171	1172	1175	rVB	235	153	0.03%	0.004%
45	8.269	1175	1178	1181	rBV	285	326	0.06%	0.008%
46	8.324	1181	1187	1197	rBV	64600	110708	20.36%	2.805%
47	8.647	1234	1240	1250	rBV	268950	427262	78.56%	10.825%
48	8.952	1285	1290	1300	rBV	48292	72615	13.35%	1.840%
49	9.153	1322	1323	1327	rVB	464	493	0.09%	0.012%
50	9.202	1328	1331	1333	rBV	214	254	0.05%	0.006%
51	9.281	1340	1344	1348	rBV2	975	1527	0.28%	0.039%
52	9.384	1356	1361	1383	rBV	144576	231019	42.48%	5.853%
53	9.738	1417	1419	1420	rBV	335	198	0.04%	0.005%
54	9.842	1434	1436	1437	rBV	213	168	0.03%	0.004%
55	9.854	1437	1438	1440	rVV	236	145	0.03%	0.004%
56	9.988	1458	1460	1462	rBV2	231	285	0.05%	0.007%
57	10.055	1465	1471	1487	rVV	281113	390271	71.76%	9.888%
58	10.232	1499	1500	1502	rBV	249	224	0.04%	0.006%
59	10.317	1509	1514	1520	rBV3	1139	1666	0.31%	0.042%
60	10.396	1523	1527	1528	rBV	214	251	0.05%	0.006%
61	10.579	1556	1557	1560	rBV	257	218	0.04%	0.006%
62	10.659	1565	1570	1571	rBV2	946	1272	0.23%	0.032%
63	10.781	1588	1590	1595	rBV	147	185	0.03%	0.005%
64	10.915	1609	1612	1614	rBV	256	281	0.05%	0.007%
65	10.945	1614	1617	1619	rBV2	159	201	0.04%	0.005%
66	11.073	1637	1638	1640	rVB	257	114	0.02%	0.003%
67	11.098	1640	1642	1643	rBV	306	218	0.04%	0.006%
68	11.189	1652	1657	1671	rVB	197727	261204	48.03%	6.618%
69	11.317	1676	1678	1681	rBV	147	104	0.02%	0.003%
70	11.457	1698	1701	1703	rBV2	379	327	0.06%	0.008%
71	11.543	1712	1715	1716	rBV	229	213	0.04%	0.005%
72	11.573	1719	1720	1724	rVB2	361	341	0.06%	0.009%
73	11.622	1724	1728	1730	rBV2	291	445	0.08%	0.011%
74	11.677	1735	1737	1739	rVV	225	153	0.03%	0.004%
75	11.695	1739	1740	1742	rVV	216	150	0.03%	0.004%
76	11.762	1745	1751	1753	rBV3	454	754	0.14%	0.019%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042738.D
 Acq On : 30 Jul 2024 14:45
 Operator : JC/MD
 Sample : P3388-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.975	1783	1786	1788	rBV2	1056	1220	0.22%	0.031%
78	12.018	1788	1793	1804	rVV	247842	328916	60.48%	8.333%
79	12.189	1817	1821	1824	rBV2	390	598	0.11%	0.015%
80	12.317	1837	1842	1851	rBV	253617	338579	62.26%	8.578%
81	12.475	1866	1868	1869	rBV	172	98	0.02%	0.002%
82	12.597	1887	1888	1890	rBV	136	91	0.02%	0.002%
83	12.616	1890	1891	1893	rVB	184	102	0.02%	0.003%
84	12.640	1893	1895	1896	rBV	290	208	0.04%	0.005%
85	12.664	1898	1899	1900	rVV	154	59	0.01%	0.001%
86	12.823	1923	1925	1926	rBV	193	165	0.03%	0.004%
87	12.841	1926	1928	1931	rVV	164	209	0.04%	0.005%
88	12.908	1936	1939	1941	rBV	251	200	0.04%	0.005%
89	13.042	1960	1961	1964	rBV	139	142	0.03%	0.004%
90	13.152	1977	1979	1982	rBV2	225	232	0.04%	0.006%
91	13.378	2012	2016	2017	rBV	193	168	0.03%	0.004%
92	13.628	2056	2057	2060	rBV	210	211	0.04%	0.005%
93	13.670	2060	2064	2065	rVB	168	137	0.03%	0.003%
94	13.725	2070	2073	2075	rVB2	529	451	0.08%	0.011%
95	13.780	2078	2082	2088	rBV	3217	4593	0.84%	0.116%
96	13.884	2097	2099	2100	rVB	237	114	0.02%	0.003%
97	13.926	2104	2106	2108	rBV	142	119	0.02%	0.003%
98	14.128	2136	2139	2144	rVB2	904	1275	0.23%	0.032%
99	14.182	2147	2148	2152	rBV3	265	243	0.04%	0.006%
100	14.585	2213	2214	2215	rBV3	253	147	0.03%	0.004%

Sum of corrected areas: 3947098




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042738.D
Acq On : 30 Jul 2024 14:45
Operator : JC/MD
Sample : P3388-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

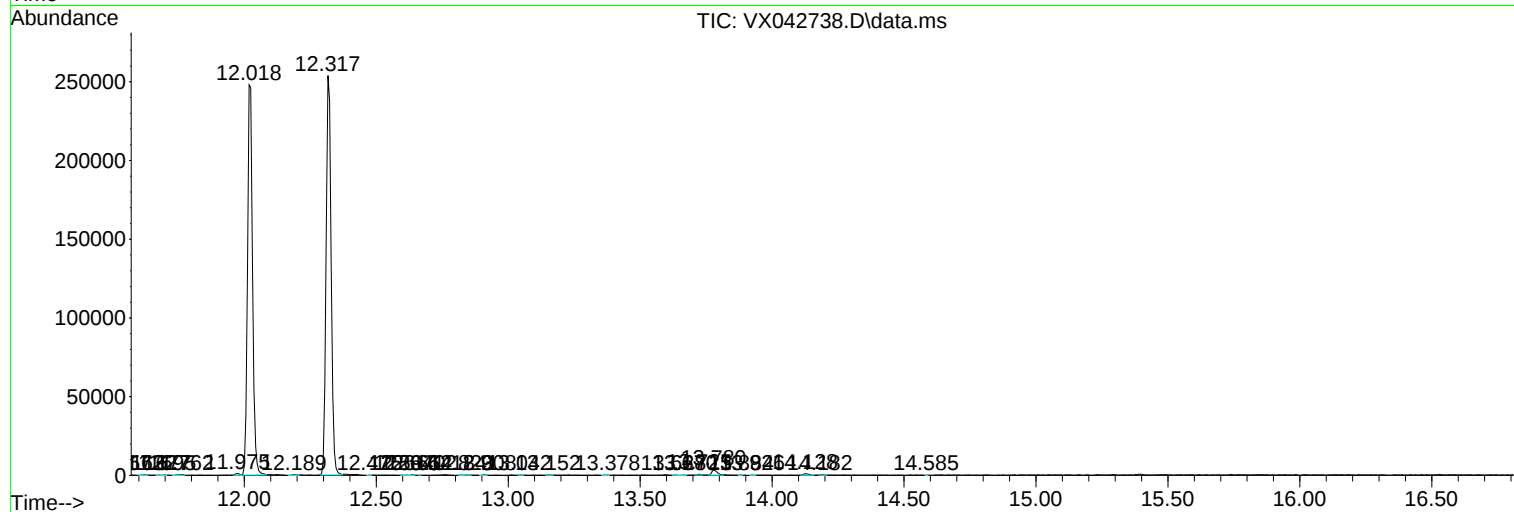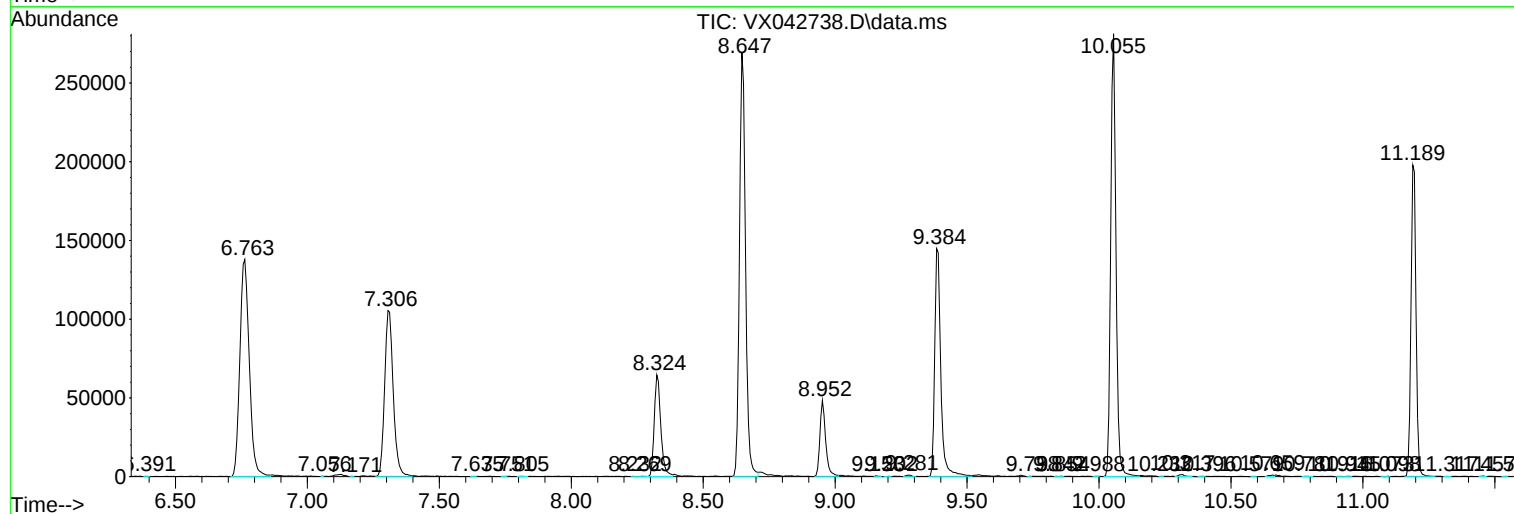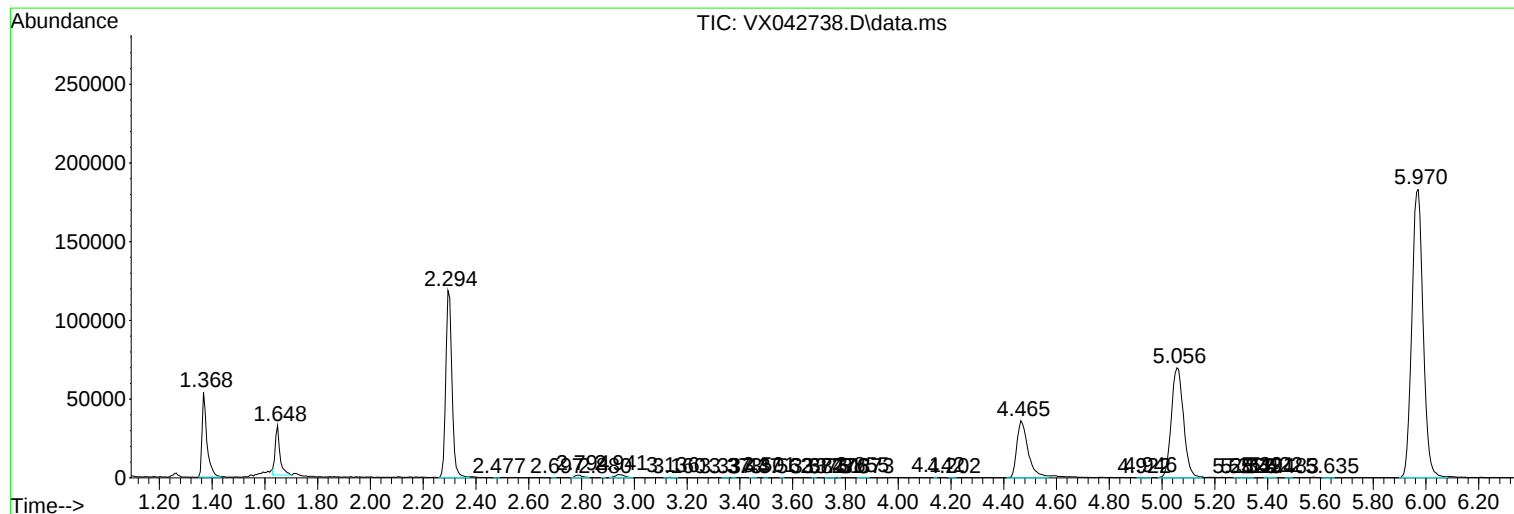

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042738.D
Acq On : 30 Jul 2024 14:45
Operator : JC/MD
Sample : P3388-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042738.D
Acq On : 30 Jul 2024 14:45
Operator : JC/MD
Sample : P3388-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
