

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042739.D
 Acq On : 30 Jul 2024 15:09
 Operator : JC/MD
 Sample : P3335-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M

Title : VOC Analysis

Signal : TIC: VX042739.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	57	rVB	54322	65195	11.97%	1.646%
2	1.642	89	91	100	rVB	27781	40822	7.49%	1.030%
3	2.038	155	156	160	rBV	267	349	0.06%	0.009%
4	2.227	185	187	192	rBV2	386	343	0.06%	0.009%
5	2.294	192	198	209	rBV	115891	190670	35.00%	4.813%
6	2.782	273	278	289	rVV3	4289	8778	1.61%	0.222%
7	2.886	293	295	298	rVB	195	173	0.03%	0.004%
8	2.947	298	305	307	rBV2	808	1435	0.26%	0.036%
9	3.166	338	341	343	rBV	146	182	0.03%	0.005%
10	3.227	348	351	352	rBV	213	220	0.04%	0.006%
11	3.404	377	380	381	rBV2	237	264	0.05%	0.007%
12	3.562	401	406	407	rBV	190	225	0.04%	0.006%
13	3.599	411	412	415	rBV	186	142	0.03%	0.004%
14	3.629	415	417	420	rVB	216	166	0.03%	0.004%
15	3.684	425	426	428	rVB	228	137	0.03%	0.003%
16	3.703	428	429	432	rBB	176	170	0.03%	0.004%
17	3.782	440	442	443	rBV	223	144	0.03%	0.004%
18	3.934	463	467	469	rBV2	276	346	0.06%	0.009%
19	4.056	481	487	490	rBV2	255	535	0.10%	0.014%
20	4.239	515	517	522	rVB	240	360	0.07%	0.009%
21	4.306	523	528	530	rBB	143	231	0.04%	0.006%
22	4.337	530	533	535	rBV	181	194	0.04%	0.005%
23	4.471	545	555	573	rBV	35926	106301	19.51%	2.683%
24	4.952	629	634	635	rBV2	228	350	0.06%	0.009%
25	5.056	640	651	667	rVV	70990	219587	40.31%	5.543%
26	5.367	701	702	703	rBV	447	233	0.04%	0.006%
27	5.544	727	731	732	rBV2	453	486	0.09%	0.012%
28	5.861	781	783	785	rBB	196	191	0.04%	0.005%
29	5.885	785	787	788	rBV	226	162	0.03%	0.004%
30	5.964	790	800	814	rBV3	186385	544733	100.00%	13.751%
31	6.275	847	851	853	rBV2	229	341	0.06%	0.009%
32	6.348	861	863	867	rBV2	164	185	0.03%	0.005%
33	6.416	872	874	876	rVB	284	148	0.03%	0.004%
34	6.470	880	883	885	rBV	187	149	0.03%	0.004%
35	6.495	885	887	892	rBV	191	260	0.05%	0.007%
36	6.531	892	893	896	rBV	161	143	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042739.D
 Acq On : 30 Jul 2024 15:09
 Operator : JC/MD
 Sample : P3335-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.690	917	919	920	rBV	174	147	0.03%	0.004%
38	6.763	922	931	945	rVV	148895	354232	65.03%	8.942%
39	7.062	978	980	982	rBV	216	255	0.05%	0.006%
40	7.208	1003	1004	1007	rBV	256	252	0.05%	0.006%
41	7.312	1012	1021	1037	rBV	105939	242836	44.58%	6.130%
42	7.464	1043	1046	1048	rBV2	203	297	0.05%	0.007%
43	7.623	1069	1072	1075	rBB	202	274	0.05%	0.007%
44	7.653	1075	1077	1079	rBV2	240	282	0.05%	0.007%
45	7.745	1087	1092	1093	rBV2	273	434	0.08%	0.011%
46	7.824	1103	1105	1106	rBV2	158	151	0.03%	0.004%
47	7.866	1111	1112	1114	rBV	201	164	0.03%	0.004%
48	7.952	1124	1126	1129	rBB2	193	213	0.04%	0.005%
49	7.995	1129	1133	1135	rBV2	218	360	0.07%	0.009%
50	8.037	1138	1140	1143	rBB	288	289	0.05%	0.007%
51	8.226	1169	1171	1173	rVB	274	201	0.04%	0.005%
52	8.244	1173	1174	1178	rBV2	225	331	0.06%	0.008%
53	8.324	1182	1187	1201	rVV	65362	110911	20.36%	2.800%
54	8.494	1214	1215	1218	rBV	168	207	0.04%	0.005%
55	8.561	1225	1226	1228	rBV	308	229	0.04%	0.006%
56	8.647	1234	1240	1257	rBV	274170	432806	79.45%	10.925%
57	8.952	1285	1290	1302	rBV	47393	71321	13.09%	1.800%
58	9.385	1356	1361	1381	rBV	146628	230848	42.38%	5.827%
59	9.848	1434	1437	1441	rBV	347	473	0.09%	0.012%
60	10.055	1466	1471	1482	rBV	293746	403732	74.12%	10.191%
61	10.269	1503	1506	1508	rBV	214	246	0.05%	0.006%
62	10.384	1523	1525	1526	rBV	260	152	0.03%	0.004%
63	10.622	1561	1564	1565	rBV	250	223	0.04%	0.006%
64	10.726	1579	1581	1583	rBV	317	283	0.05%	0.007%
65	10.805	1593	1594	1597	rVB	234	147	0.03%	0.004%
66	10.848	1599	1601	1602	rVB	256	137	0.03%	0.003%
67	10.872	1602	1605	1609	rVB	217	342	0.06%	0.009%
68	10.909	1610	1611	1613	rBV	269	218	0.04%	0.006%
69	11.043	1629	1633	1635	rBV2	206	223	0.04%	0.006%
70	11.140	1646	1649	1652	rVB2	191	211	0.04%	0.005%
71	11.189	1652	1657	1666	rBV	188260	253252	46.49%	6.393%
72	11.439	1696	1698	1700	rVB	237	212	0.04%	0.005%
73	11.457	1700	1701	1703	rBV	356	241	0.04%	0.006%
74	11.561	1716	1718	1719	rVB	199	143	0.03%	0.004%
75	11.610	1723	1726	1727	rBV	195	228	0.04%	0.006%
76	11.768	1751	1752	1755	rVB	308	271	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042739.D
 Acq On : 30 Jul 2024 15:09
 Operator : JC/MD
 Sample : P3335-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20K3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.854	1763	1766	1772	rBV	342	550	0.10%	0.014%
78	11.908	1772	1775	1776	rBV	181	166	0.03%	0.004%
79	11.976	1783	1786	1789	rBV3	332	485	0.09%	0.012%
80	12.024	1789	1794	1805	rVV	257164	331149	60.79%	8.359%
81	12.134	1810	1812	1815	rVB	380	275	0.05%	0.007%
82	12.171	1816	1818	1820	rVB	264	176	0.03%	0.004%
83	12.238	1827	1829	1833	rBV	272	375	0.07%	0.009%
84	12.323	1837	1843	1856	rVV	249204	331634	60.88%	8.371%
85	12.482	1866	1869	1870	rBV	242	236	0.04%	0.006%
86	12.835	1924	1927	1929	rBV	242	253	0.05%	0.006%
87	12.853	1929	1930	1933	rVB	186	154	0.03%	0.004%
88	12.939	1942	1944	1947	rBV	199	174	0.03%	0.004%
89	12.988	1949	1952	1955	rBV	349	368	0.07%	0.009%
90	13.116	1971	1973	1978	rBV2	238	328	0.06%	0.008%
91	13.353	2010	2012	2013	rBV	231	200	0.04%	0.005%
92	13.841	2091	2092	2094	rBV	175	175	0.03%	0.004%
93	14.067	2125	2129	2131	rBV	349	355	0.07%	0.009%
94	14.182	2145	2148	2149	rBV	283	258	0.05%	0.007%
95	14.335	2172	2173	2176	rVB	315	218	0.04%	0.006%
96	14.926	2269	2270	2273	rBV	548	526	0.10%	0.013%
97	15.487	2360	2362	2365	rBV	476	537	0.10%	0.014%
98	15.603	2380	2381	2383	rBV	388	365	0.07%	0.009%
99	15.816	2415	2416	2417	rBV	374	222	0.04%	0.006%
100	16.261	2488	2489	2490	rBV	365	198	0.04%	0.005%

Sum of corrected areas: 3961501




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042739.D
Acq On : 30 Jul 2024 15:09
Operator : JC/MD
Sample : P3335-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

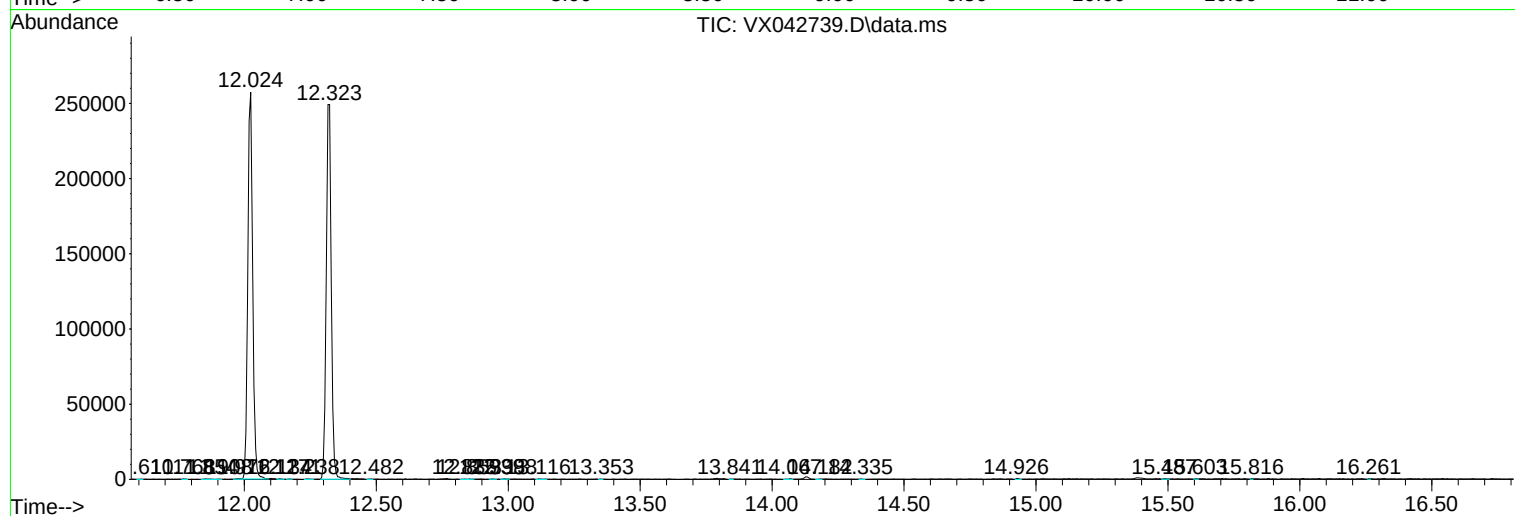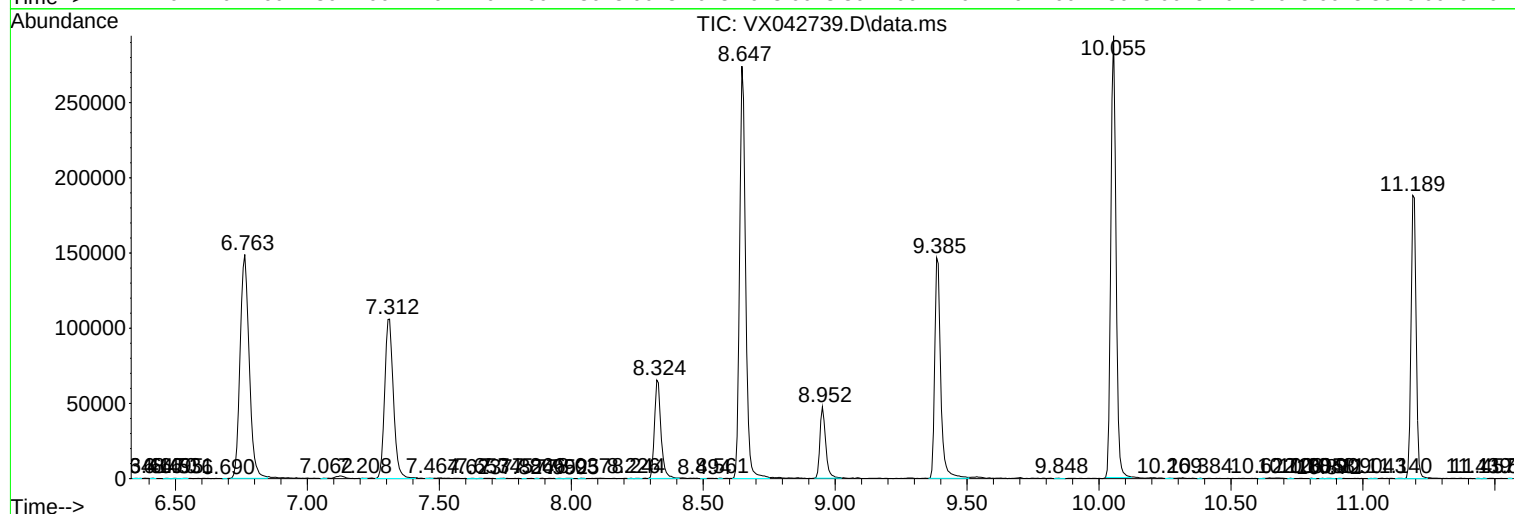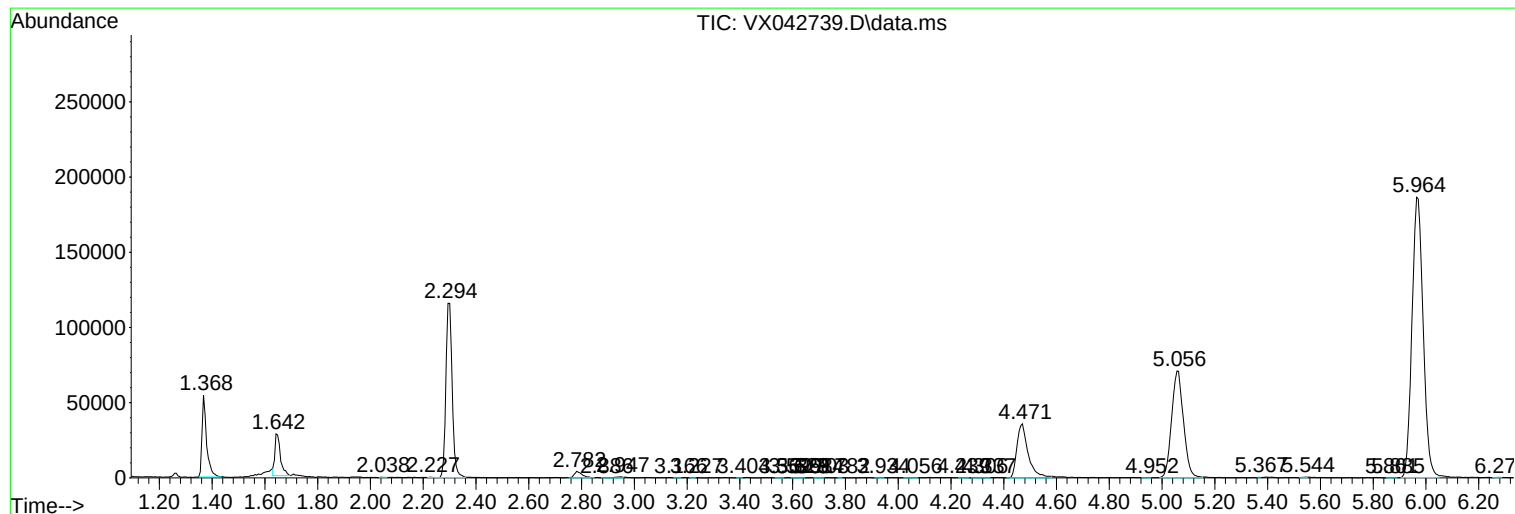

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042739.D
Acq On : 30 Jul 2024 15:09
Operator : JC/MD
Sample : P3335-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042739.D
Acq On : 30 Jul 2024 15:09
Operator : JC/MD
Sample : P3335-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20K3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------