

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042748.D
 Acq On : 30 Jul 2024 18:39
 Operator : JC/MD
 Sample : P3378-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	26	28	33	rVB3	2859	3361	0.69%	0.092%
2	1.368	43	46	59	rVB	43314	54711	11.22%	1.495%
3	1.520	70	71	73	rBV2	581	434	0.09%	0.012%
4	1.648	89	92	100	rVB	28564	35142	7.21%	0.960%
5	2.294	192	198	209	rBV	104926	169156	34.70%	4.622%
6	2.471	224	227	229	rBV	340	267	0.05%	0.007%
7	2.508	229	233	239	rVV2	500	665	0.14%	0.018%
8	2.654	254	257	262	rBV	291	391	0.08%	0.011%
9	2.703	262	265	270	rVV2	279	470	0.10%	0.013%
10	2.782	275	278	279	rBV	991	925	0.19%	0.025%
11	2.910	297	299	300	rBV	223	214	0.04%	0.006%
12	2.947	300	305	311	rVV3	1273	2781	0.57%	0.076%
13	3.087	324	328	329	rBV3	507	462	0.09%	0.013%
14	3.221	347	350	352	rBV	173	213	0.04%	0.006%
15	3.270	355	358	359	rVB	254	231	0.05%	0.006%
16	3.599	410	412	415	rBV	276	328	0.07%	0.009%
17	3.794	442	444	447	rBB	148	188	0.04%	0.005%
18	3.849	450	453	455	rBV	129	172	0.04%	0.005%
19	3.922	463	465	469	rBV2	201	303	0.06%	0.008%
20	4.123	493	498	500	rBB	174	249	0.05%	0.007%
21	4.154	500	503	504	rBV	165	165	0.03%	0.005%
22	4.215	510	513	514	rBV	203	180	0.04%	0.005%
23	4.282	522	524	529	rVB	281	356	0.07%	0.010%
24	4.367	532	538	540	rBB	291	331	0.07%	0.009%
25	4.471	547	555	572	rBV	33788	100411	20.60%	2.744%
26	5.062	640	652	667	rBV2	65688	198840	40.79%	5.433%
27	5.251	679	683	685	rBV2	156	167	0.03%	0.005%
28	5.379	702	704	705	rBV2	354	295	0.06%	0.008%
29	5.464	715	718	719	rBV2	445	541	0.11%	0.015%
30	5.647	745	748	749	rBV	212	246	0.05%	0.007%
31	5.678	749	753	756	rVB2	257	409	0.08%	0.011%
32	5.769	766	768	773	rVV	250	203	0.04%	0.006%
33	5.970	790	801	818	rBV2	166956	487457	100.00%	13.319%
34	6.519	888	891	893	rBV	254	312	0.06%	0.009%
35	6.574	899	900	903	rBV	236	228	0.05%	0.006%
36	6.672	915	916	920	rVB	178	189	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042748.D
 Acq On : 30 Jul 2024 18:39
 Operator : JC/MD
 Sample : P3378-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	6.763	923	931	943	rVV	134469	320550	65.76%	8.758%
38	7.050	975	978	980	rBV	323	247	0.05%	0.007%
39	7.074	980	982	983	rBV	200	166	0.03%	0.005%
40	7.214	1003	1005	1007	rBV	322	178	0.04%	0.005%
41	7.312	1012	1021	1037	rBV	94749	215801	44.27%	5.896%
42	7.488	1048	1050	1055	rBV3	451	528	0.11%	0.014%
43	7.684	1081	1082	1084	rBV3	242	165	0.03%	0.005%
44	7.830	1102	1106	1109	rBV	328	549	0.11%	0.015%
45	7.860	1109	1111	1113	rVB	287	204	0.04%	0.006%
46	7.934	1119	1123	1125	rBB	263	288	0.06%	0.008%
47	7.958	1125	1127	1131	rBV	235	283	0.06%	0.008%
48	8.019	1135	1137	1140	rBV	161	177	0.04%	0.005%
49	8.208	1166	1168	1172	rBB	245	316	0.06%	0.009%
50	8.238	1172	1173	1176	rBV	143	168	0.03%	0.005%
51	8.324	1182	1187	1198	rBV	57021	95829	19.66%	2.618%
52	8.580	1227	1229	1234	rBV5	625	814	0.17%	0.022%
53	8.647	1234	1240	1249	rBV	246246	388140	79.63%	10.605%
54	8.952	1285	1290	1302	rBV	41019	62688	12.86%	1.713%
55	9.116	1315	1317	1319	rBV	191	180	0.04%	0.005%
56	9.153	1321	1323	1324	rVV	374	250	0.05%	0.007%
57	9.189	1328	1329	1331	rBV	246	199	0.04%	0.005%
58	9.275	1337	1343	1348	rBV5	1607	2273	0.47%	0.062%
59	9.384	1356	1361	1379	rVV	141916	219482	45.03%	5.997%
60	9.531	1381	1385	1393	rVB3	6178	11391	2.34%	0.311%
61	9.927	1449	1450	1452	rBV	200	176	0.04%	0.005%
62	10.055	1465	1471	1487	rBV	279280	380169	77.99%	10.387%
63	10.348	1518	1519	1521	rVB	373	213	0.04%	0.006%
64	10.366	1521	1522	1524	rBV	195	188	0.04%	0.005%
65	10.433	1530	1533	1535	rBV	235	258	0.05%	0.007%
66	10.488	1540	1542	1544	rBB	207	174	0.04%	0.005%
67	10.549	1550	1552	1553	rBV	271	219	0.04%	0.006%
68	10.646	1565	1568	1573	rBV4	1437	2117	0.43%	0.058%
69	10.963	1618	1620	1623	rVB	1003	986	0.20%	0.027%
70	11.024	1628	1630	1635	rVB2	362	487	0.10%	0.013%
71	11.189	1652	1657	1667	rBV	177254	239523	49.14%	6.545%
72	11.451	1697	1700	1707	rVB3	1026	1548	0.32%	0.042%
73	11.628	1727	1729	1730	rBV3	242	169	0.03%	0.005%
74	11.665	1733	1735	1736	rBV3	234	190	0.04%	0.005%
75	11.756	1747	1750	1759	rBV5	1371	2653	0.54%	0.072%
76	11.847	1762	1765	1768	rBB	408	403	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042748.D
 Acq On : 30 Jul 2024 18:39
 Operator : JC/MD
 Sample : P3378-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 C0B05

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.878	1768	1770	1771	rBV	220	186	0.04%	0.005%
78	12.024	1788	1794	1801	rBV	246457	322143	66.09%	8.802%
79	12.219	1822	1826	1829	rBV2	4685	5539	1.14%	0.151%
80	12.317	1837	1842	1854	rVB	250101	310657	63.73%	8.488%
81	12.603	1886	1889	1891	rBV	597	525	0.11%	0.014%
82	12.731	1909	1910	1912	rBV	268	208	0.04%	0.006%
83	12.859	1924	1931	1935	rBV3	1657	2356	0.48%	0.064%
84	13.000	1950	1954	1955	rBV	280	327	0.07%	0.009%
85	13.116	1970	1973	1976	rVB	589	630	0.13%	0.017%
86	13.292	2000	2002	2005	rBV	163	195	0.04%	0.005%
87	13.408	2018	2021	2022	rBV2	231	266	0.05%	0.007%
88	13.445	2026	2027	2030	rVB	278	230	0.05%	0.006%
89	13.481	2030	2033	2036	rBV	242	351	0.07%	0.010%
90	13.554	2044	2045	2048	rBV	151	168	0.03%	0.005%
91	13.774	2080	2081	2087	rVB2	778	962	0.20%	0.026%
92	14.030	2120	2123	2125	rBV2	231	346	0.07%	0.009%
93	14.219	2152	2154	2155	rBV2	240	197	0.04%	0.005%
94	14.274	2159	2163	2166	rVB	283	451	0.09%	0.012%
95	14.310	2167	2169	2172	rBV	195	225	0.05%	0.006%
96	14.530	2200	2205	2206	rBV2	243	311	0.06%	0.008%
97	14.634	2220	2222	2227	rBV	412	571	0.12%	0.016%
98	16.078	2454	2459	2462	rBV2	394	917	0.19%	0.025%
99	16.523	2529	2532	2535	rBV	380	550	0.11%	0.015%
100	16.773	2572	2573	2574	rBV	365	239	0.05%	0.007%

Sum of corrected areas: 3659882




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042748.D
Acq On : 30 Jul 2024 18:39
Operator : JC/MD
Sample : P3378-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

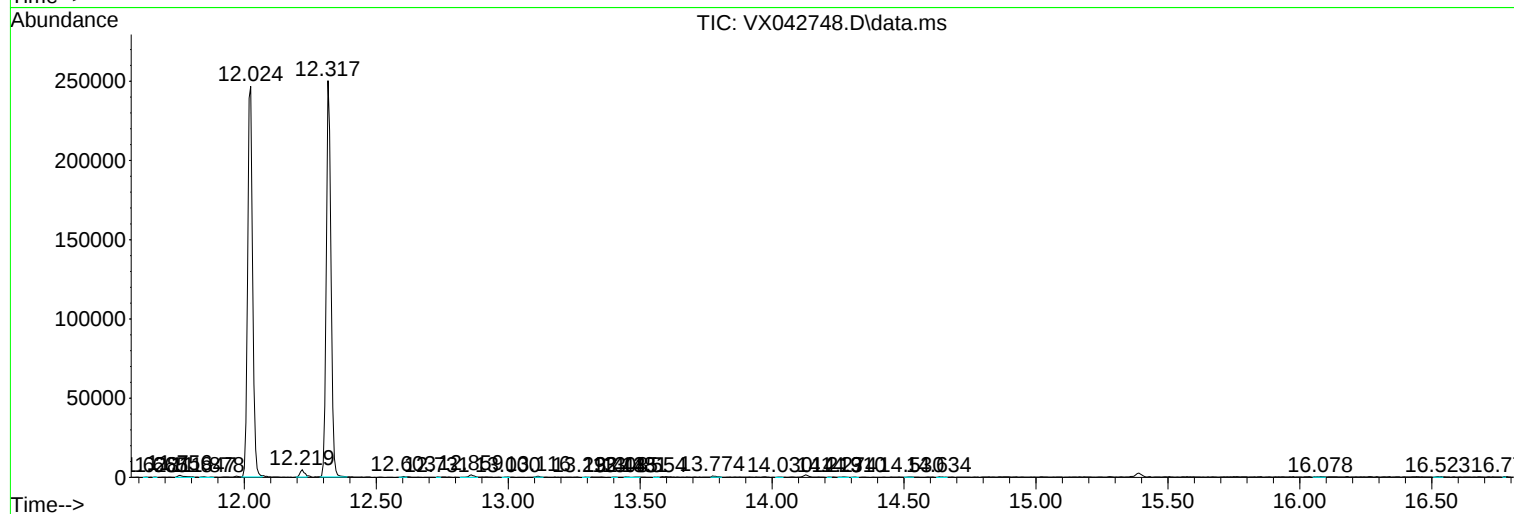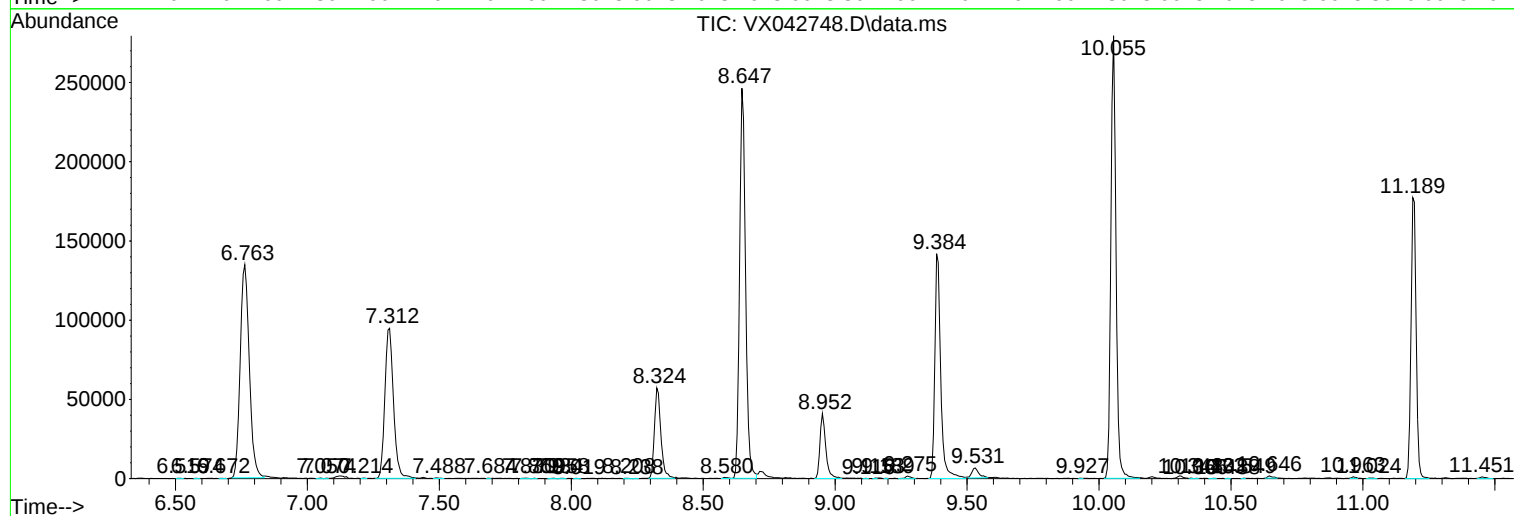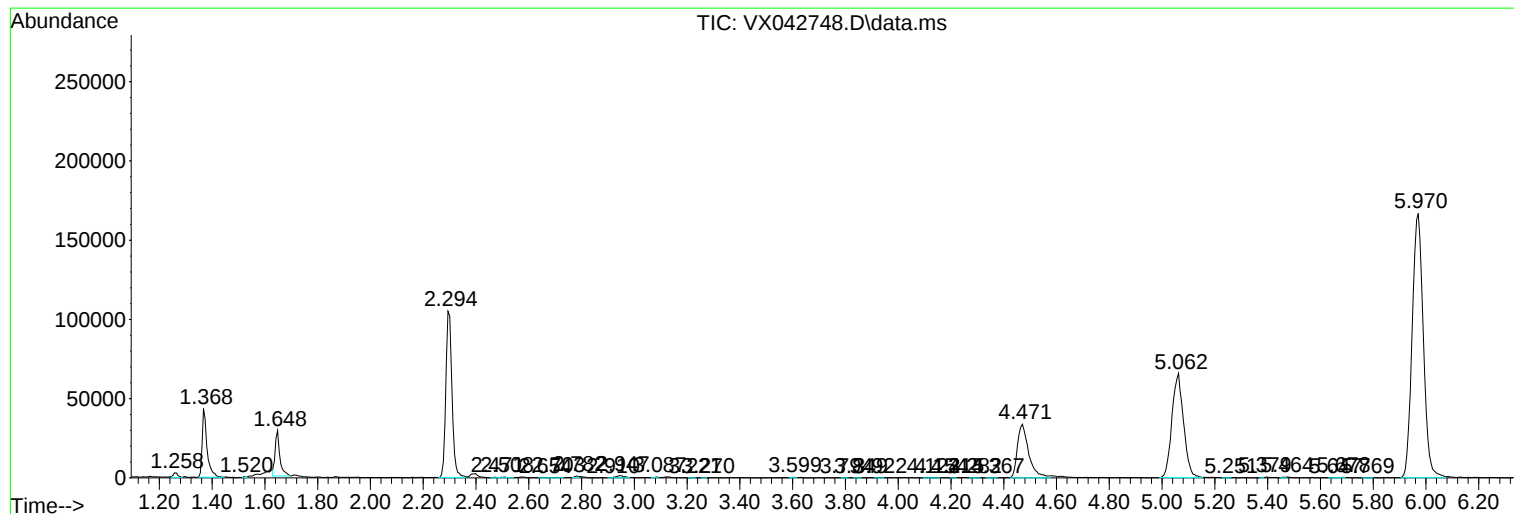

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042748.D
Acq On : 30 Jul 2024 18:39
Operator : JC/MD
Sample : P3378-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042748.D
Acq On : 30 Jul 2024 18:39
Operator : JC/MD
Sample : P3378-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
C0B05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc