

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042752.D
 Acq On : 30 Jul 2024 20:12
 Operator : JC/MD
 Sample : P3389-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	22	rVB	4090	5255	1.07%	0.145%
2	1.245	23	26	28	rBV	5026	6648	1.35%	0.184%
3	1.367	43	46	58	rVB	45359	58529	11.87%	1.618%
4	1.648	89	92	101	rVB	27757	34674	7.03%	0.958%
5	1.831	118	122	124	rBV	432	466	0.09%	0.013%
6	2.300	193	199	209	rBV	104302	166885	33.85%	4.613%
7	2.568	237	243	249	rBV3	1213	2310	0.47%	0.064%
8	2.660	255	258	259	rBV	273	227	0.05%	0.006%
9	2.788	274	279	280	rBV2	806	901	0.18%	0.025%
10	2.952	297	306	311	rBV2	1578	3659	0.74%	0.101%
11	3.038	318	320	323	rBV2	212	260	0.05%	0.007%
12	3.099	328	330	331	rVV	179	181	0.04%	0.005%
13	3.251	353	355	356	rVB	281	138	0.03%	0.004%
14	3.269	356	358	362	rBB	242	244	0.05%	0.007%
15	3.324	365	367	369	rVB	211	145	0.03%	0.004%
16	3.355	369	372	374	rBB	211	223	0.05%	0.006%
17	3.373	374	375	378	rBV	231	185	0.04%	0.005%
18	3.464	389	390	394	rBB	230	210	0.04%	0.006%
19	3.714	428	431	433	rBB	172	170	0.03%	0.005%
20	3.897	455	461	462	rBV	180	252	0.05%	0.007%
21	3.934	464	467	468	rBV	219	198	0.04%	0.005%
22	3.983	473	475	477	rBV	122	152	0.03%	0.004%
23	4.226	512	515	517	rBV	220	293	0.06%	0.008%
24	4.397	541	543	545	rBB	185	156	0.03%	0.004%
25	4.470	545	555	570	rBV	34698	103072	20.91%	2.849%
26	4.714	593	595	598	rBV	284	320	0.06%	0.009%
27	4.787	605	607	609	rBV	264	266	0.05%	0.007%
28	4.806	609	610	613	rBV	180	187	0.04%	0.005%
29	4.873	619	621	622	rBV	176	172	0.03%	0.005%
30	5.056	639	651	667	rBV2	62329	197983	40.16%	5.473%
31	5.348	697	699	703	rBV	218	241	0.05%	0.007%
32	5.476	715	720	723	rBV	386	532	0.11%	0.015%
33	5.586	734	738	741	rBV2	111	140	0.03%	0.004%
34	5.623	743	744	748	rVB2	243	224	0.05%	0.006%
35	5.671	748	752	754	rBV2	212	299	0.06%	0.008%
36	5.744	761	764	767	rBV2	153	216	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042752.D
 Acq On : 30 Jul 2024 20:12
 Operator : JC/MD
 Sample : P3389-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	5.970	789	801	815	rBV2	169794	493017	100.00%	13.628%
38	6.464	880	882	885	rVB	198	138	0.03%	0.004%
39	6.494	885	887	890	rVB	227	192	0.04%	0.005%
40	6.519	890	891	893	rBV	282	167	0.03%	0.005%
41	6.616	905	907	911	rBV	205	253	0.05%	0.007%
42	6.763	922	931	952	rBV	133878	329719	66.88%	9.114%
43	7.006	970	971	975	rVB2	437	446	0.09%	0.012%
44	7.043	975	977	979	rBB	223	158	0.03%	0.004%
45	7.128	985	991	1001	rVB4	4355	10358	2.10%	0.286%
46	7.208	1002	1004	1005	rBV	311	183	0.04%	0.005%
47	7.311	1012	1021	1034	rBV	94241	215426	43.70%	5.955%
48	7.482	1048	1049	1052	rVB	344	213	0.04%	0.006%
49	7.659	1075	1078	1083	rBV	178	300	0.06%	0.008%
50	7.732	1088	1090	1095	rVB	242	341	0.07%	0.009%
51	7.781	1096	1098	1099	rBV	261	187	0.04%	0.005%
52	7.878	1112	1114	1115	rBV	219	208	0.04%	0.006%
53	7.939	1122	1124	1125	rBV	205	171	0.03%	0.005%
54	8.025	1136	1138	1139	rBV	222	195	0.04%	0.005%
55	8.128	1153	1155	1158	rBV	215	220	0.04%	0.006%
56	8.207	1165	1168	1169	rVB	185	154	0.03%	0.004%
57	8.323	1182	1187	1201	rBV	52773	95105	19.29%	2.629%
58	8.482	1212	1213	1215	rBV	210	192	0.04%	0.005%
59	8.518	1217	1219	1220	rBV	236	222	0.05%	0.006%
60	8.646	1234	1240	1250	rBV	238073	384453	77.98%	10.627%
61	8.951	1285	1290	1301	rBV	38955	61571	12.49%	1.702%
62	9.238	1336	1337	1340	rBV	193	207	0.04%	0.006%
63	9.280	1340	1344	1347	rVB2	1215	1649	0.33%	0.046%
64	9.329	1350	1352	1354	rBV	244	282	0.06%	0.008%
65	9.384	1356	1361	1371	rBV	141930	215813	43.77%	5.965%
66	9.768	1421	1424	1426	rBV	126	152	0.03%	0.004%
67	9.793	1426	1428	1431	rVV	187	210	0.04%	0.006%
68	10.055	1466	1471	1487	rVB	268259	374169	75.89%	10.343%
69	10.201	1492	1495	1497	rBV	646	596	0.12%	0.016%
70	10.311	1509	1513	1517	rBV2	929	1019	0.21%	0.028%
71	10.591	1557	1559	1561	rBV2	343	284	0.06%	0.008%
72	10.640	1564	1567	1570	rBV	339	525	0.11%	0.015%
73	10.683	1573	1574	1577	rBV	223	252	0.05%	0.007%
74	11.073	1637	1638	1641	rBV	184	216	0.04%	0.006%
75	11.195	1652	1658	1670	rVB	178189	242114	49.11%	6.692%
76	11.317	1674	1678	1681	rVB2	484	748	0.15%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
 Data File : VX042752.D
 Acq On : 30 Jul 2024 20:12
 Operator : JC/MD
 Sample : P3389-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20T7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	11.347	1682	1683	1686	rBV	164	140	0.03%	0.004%
78	11.420	1693	1695	1697	rBV	224	198	0.04%	0.005%
79	11.798	1755	1757	1758	rBV	267	189	0.04%	0.005%
80	12.024	1789	1794	1806	rVB	236799	295730	59.98%	8.174%
81	12.225	1823	1827	1831	rBV4	2070	2795	0.57%	0.077%
82	12.316	1837	1842	1852	rBV	220563	295091	59.85%	8.157%
83	12.451	1861	1864	1868	rBV2	283	307	0.06%	0.008%
84	12.481	1868	1869	1871	rBV	173	155	0.03%	0.004%
85	12.548	1876	1880	1882	rBV2	227	334	0.07%	0.009%
86	12.701	1903	1905	1906	rBV	302	210	0.04%	0.006%
87	13.103	1968	1971	1974	rBV	208	255	0.05%	0.007%
88	13.200	1986	1987	1989	rBV	217	173	0.04%	0.005%
89	13.487	2031	2034	2035	rVB	189	169	0.03%	0.005%
90	13.511	2035	2038	2042	rBV2	243	467	0.09%	0.013%
91	13.706	2068	2070	2071	rBV	258	171	0.03%	0.005%
92	13.834	2089	2091	2092	rBV	266	218	0.04%	0.006%
93	14.011	2119	2120	2122	rBV	356	317	0.06%	0.009%
94	14.127	2133	2139	2146	rBB3	871	1650	0.33%	0.046%
95	14.194	2146	2150	2152	rBV	263	391	0.08%	0.011%
96	14.292	2163	2166	2168	rBV	254	227	0.05%	0.006%
97	14.481	2194	2197	2198	rBV	363	247	0.05%	0.007%
98	15.432	2351	2353	2354	rBV	304	158	0.03%	0.004%
99	15.633	2384	2386	2387	rBV	345	165	0.03%	0.005%
100	16.127	2466	2467	2468	rBV	265	154	0.03%	0.004%


Sum of corrected areas: 3617749

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042752.D
Acq On : 30 Jul 2024 20:12
Operator : JC/MD
Sample : P3389-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

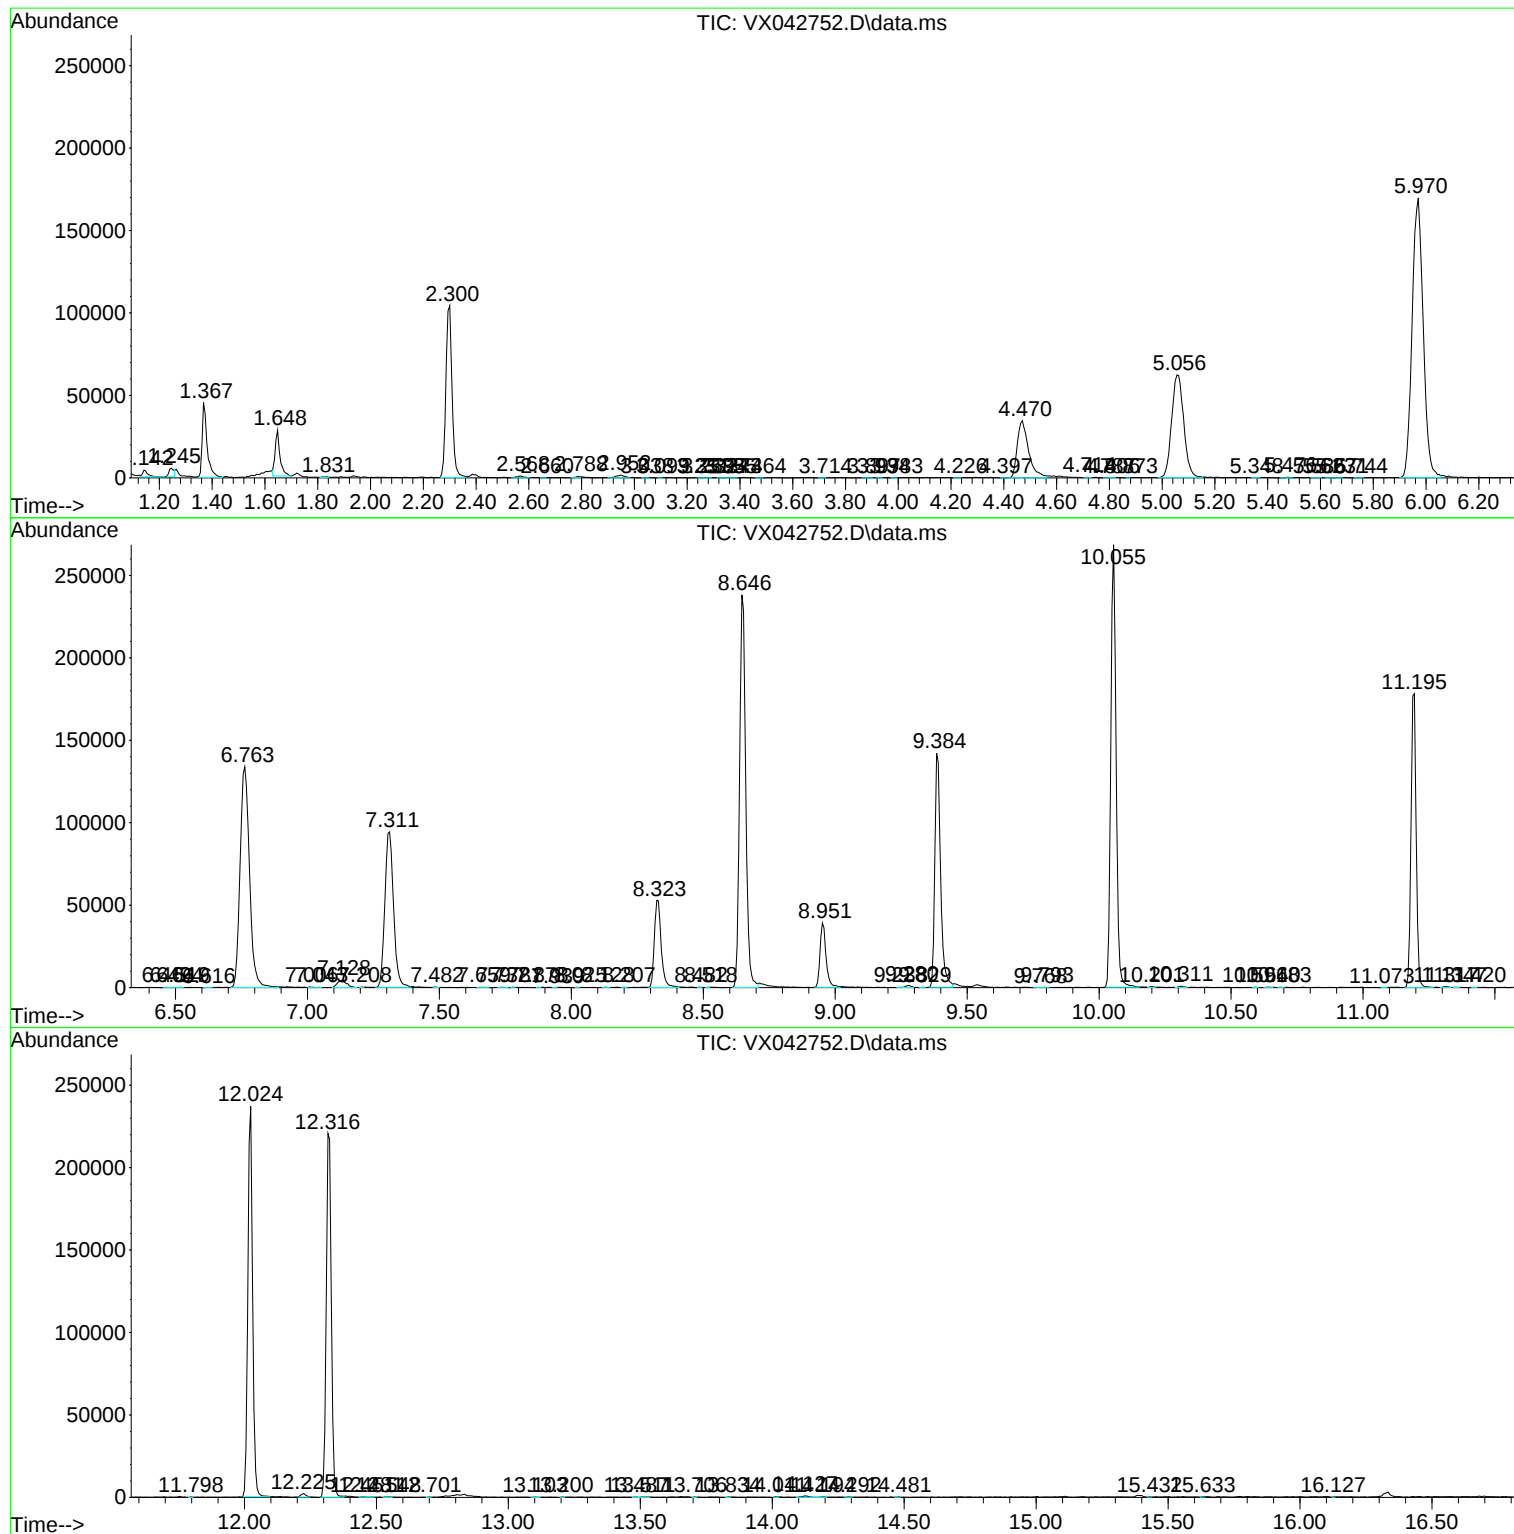

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042752.D
Acq On : 30 Jul 2024 20:12
Operator : JC/MD
Sample : P3389-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042752.D
Acq On : 30 Jul 2024 20:12
Operator : JC/MD
Sample : P3389-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20T7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc