


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073024\
Data File : VX042727.D
Acq On : 30 Jul 2024 10:01
Operator : JC/MD
Sample : BFB688
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB688

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM072624WMA.M
Title : VOC Analysis
Last Update : Wed Jul 31 03:10:58 2024

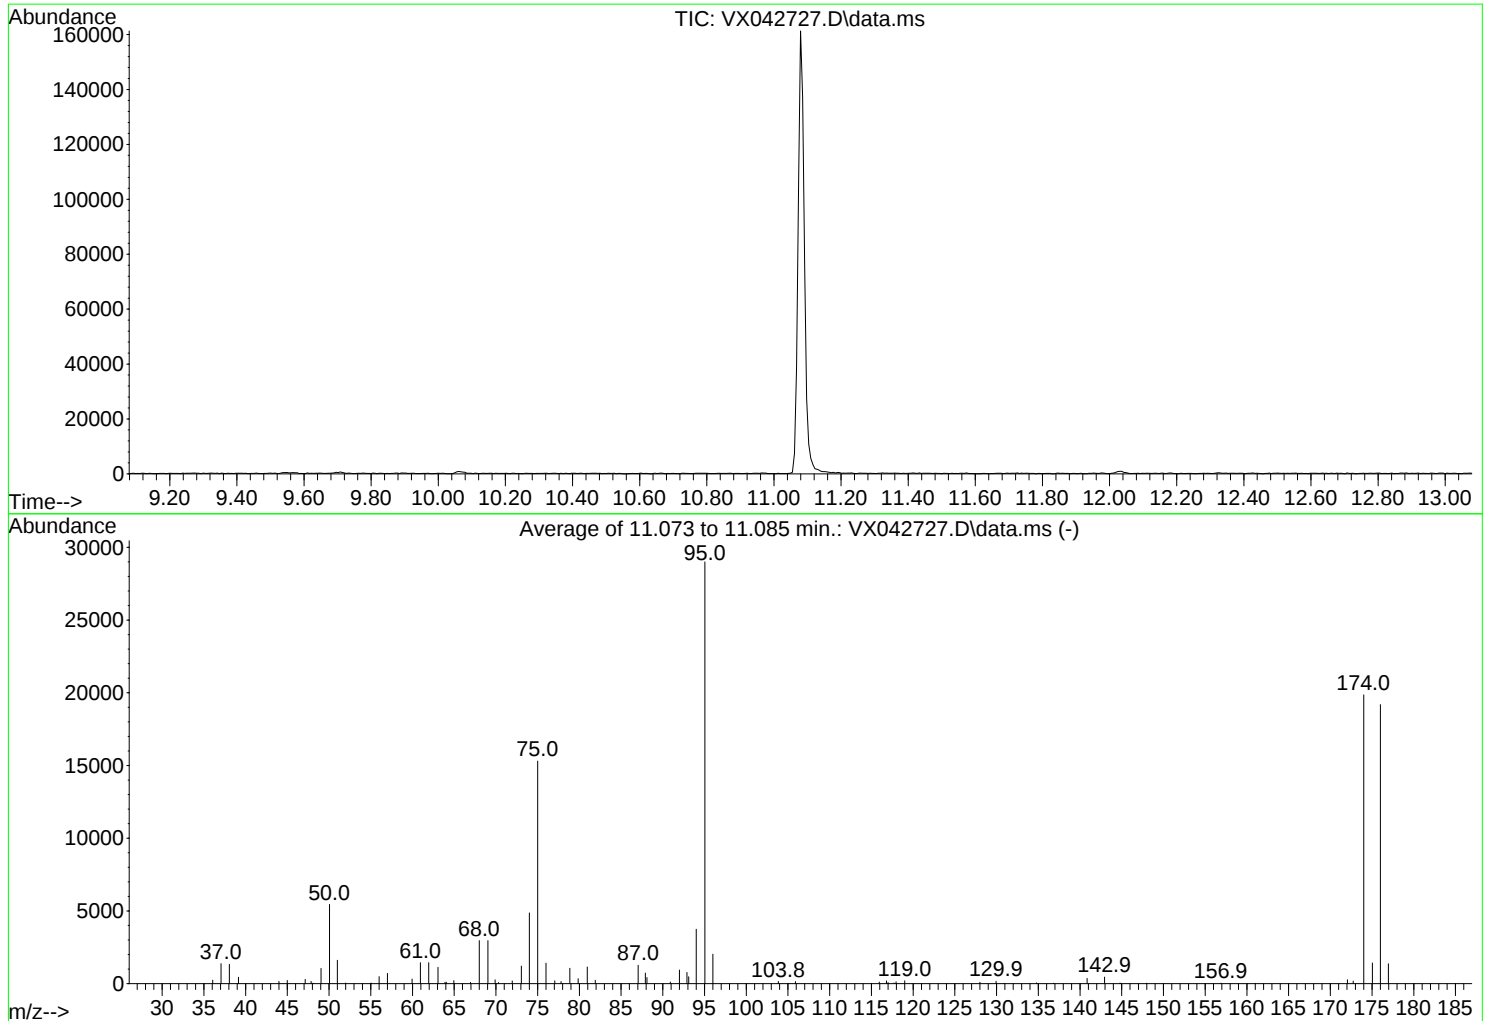

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.8	5443	PASS
75	95	30	80	52.8	15304	PASS
95	95	100	100	100.0	29003	PASS
96	95	5	9	7.0	2024	PASS
173	174	0.00	2	0.9	181	PASS
174	95	50	120	68.5	19857	PASS
175	174	5	9	7.2	1424	PASS
176	174	95	101	96.6	19186	PASS
177	176	5	9	7.1	1360	PASS

m/z	Abundance
36.10	230.0
37.10	1360.0
38.00	1305.0
39.00	379.0
44.00	202.0
44.90	122.0
47.20	270.0
47.90	181.0
49.10	913.0
50.10	5047.0
51.00	1521.0
55.10	55.0
56.00	429.0
56.90	695.0
59.90	282.0
61.00	1234.0
61.90	1224.0
63.10	1054.0
63.90	151.0
65.00	155.0
66.90	93.0
68.00	2696.0
69.10	2799.0
69.90	274.0
71.90	177.0
73.10	1132.0
74.00	4865.0
75.00	14729.0
76.00	1446.0
77.00	165.0
77.80	58.0
78.80	979.0
79.90	309.0
81.00	1038.0
82.00	273.0
87.00	1230.0
87.90	1039.0
90.90	103.0
92.00	1143.0
93.10	1422.0
94.00	3594.0
95.00	29152.0
96.00	1652.0
103.90	123.0
105.10	59.0
106.00	85.0
115.00	70.0
116.00	175.0
117.00	229.0
117.90	184.0
119.00	129.0
128.00	184.0
129.90	155.0
130.90	65.0
140.90	394.0
143.00	294.0
156.90	98.0
172.10	209.0
174.00	21992.0
175.00	1813.0
176.00	22160.0
177.00	1456.0

Instrument :
MSVOA_X
ClientSampleId :
BFB688

m/z	Abundance
36.00	319.0
37.00	1741.0
38.00	1361.0
39.20	507.0
44.00	327.0
45.00	292.0
47.00	306.0
47.80	293.0
49.00	1382.0
50.00	6277.0
51.00	1923.0
52.00	129.0
55.00	64.0
55.90	472.0
57.10	782.0
59.90	351.0
60.90	1781.0
62.00	1827.0
63.10	1394.0
64.00	138.0
65.00	300.0
66.90	106.0
68.00	3702.0
69.00	3482.0
69.90	294.0
72.00	180.0
73.00	1266.0
74.00	5945.0
75.00	18888.0
76.00	1430.0
77.00	308.0
77.80	217.0
78.90	1390.0
79.80	400.0
81.00	1406.0
81.80	211.0
87.00	1444.0
88.10	1260.0
90.90	167.0
92.00	899.0
92.90	1455.0
94.00	4704.0
95.10	34528.0
96.00	2385.0
103.80	168.0
105.80	220.0
115.90	159.0
116.80	334.0
118.00	213.0
119.00	245.0
128.00	107.0
130.00	177.0
134.80	88.0
136.80	84.0
140.80	463.0
142.90	727.0
144.80	66.0
148.00	104.0
161.00	52.0
172.00	337.0
172.70	353.0
174.00	23808.0
175.00	1588.0
176.00	22416.0
176.90	1557.0

Instrument :
MSVOA_X
ClientSampleId :
BFB688

m/z	Abundance
36.10	167.0
37.10	1033.0
38.10	1343.0
39.20	441.0
40.20	62.0
44.10	252.0
45.10	241.0
47.20	322.0
48.10	109.0
49.10	827.0
50.00	5006.0
51.00	1372.0
56.10	561.0
57.00	649.0
60.10	326.0
61.00	1324.0
62.00	1277.0
63.00	926.0
63.90	156.0
64.10	152.0
64.90	182.0
67.00	59.0
68.00	2466.0
69.00	2613.0
69.90	223.0
70.30	239.0
72.00	208.0
73.10	1249.0
74.00	3767.0
75.00	12294.0
76.00	1340.0
77.20	134.0
77.80	142.0
78.90	796.0
79.90	303.0
80.90	975.0
81.90	208.0
87.10	1126.0
87.90	1126.0
90.90	74.0
92.00	767.0
92.90	856.0
94.00	2912.0
95.00	23328.0
96.00	2034.0
103.80	160.0
106.00	112.0
116.80	225.0
117.70	117.0
119.00	209.0
130.00	170.0
134.80	69.0
140.90	241.0
143.00	319.0
144.80	58.0
172.10	237.0
172.80	191.0
174.00	13771.0
175.10	871.0
176.00	12981.0
177.00	1067.0

Instrument :
MSVOA_X
ClientSampleId :
BFB688

m/z	Abundance
40.10	103.0
44.00	101.0

Instrument :
MSVOA_X
ClientSampleId :
BFB688