


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX073118\
Data File : VX003765.D
Acq On : 31 Jul 2018 22:27
Operator : JC/SP
Sample : BFB
Misc : 5.00G/5.0mL/MSVOA X/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X073018S.M
Title : SW846 8260
Last Update : Tue Jul 31 11:17:41 2018

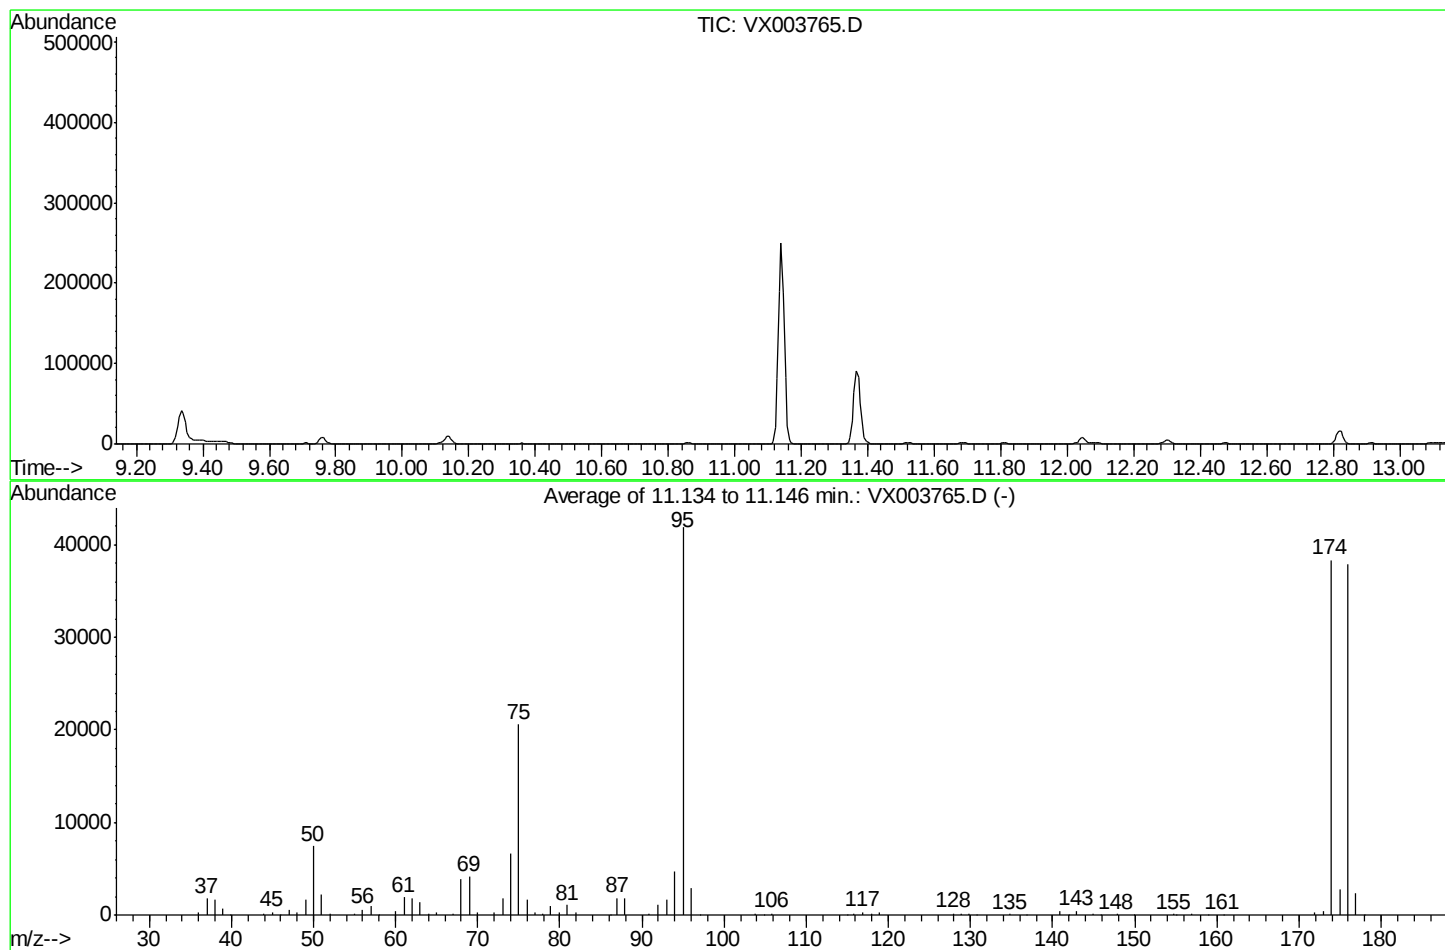

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1723

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	7441	PASS
75	95	30	60	49.1	20584	PASS
95	95	100	100	100.0	41904	PASS
96	95	5	9	6.8	2858	PASS
173	174	0.00	2	0.9	360	PASS
174	95	50	100	91.5	38362	PASS
175	174	5	9	7.3	2792	PASS
176	174	95	101	98.9	37952	PASS
177	176	5	9	6.3	2385	PASS