


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX073119\
Data File : VX011241.D
Acq On : 31 Jul 2019 13:31
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X071619W.M
Title : SW846 8260
Last Update : Wed Jul 24 05:39:23 2019

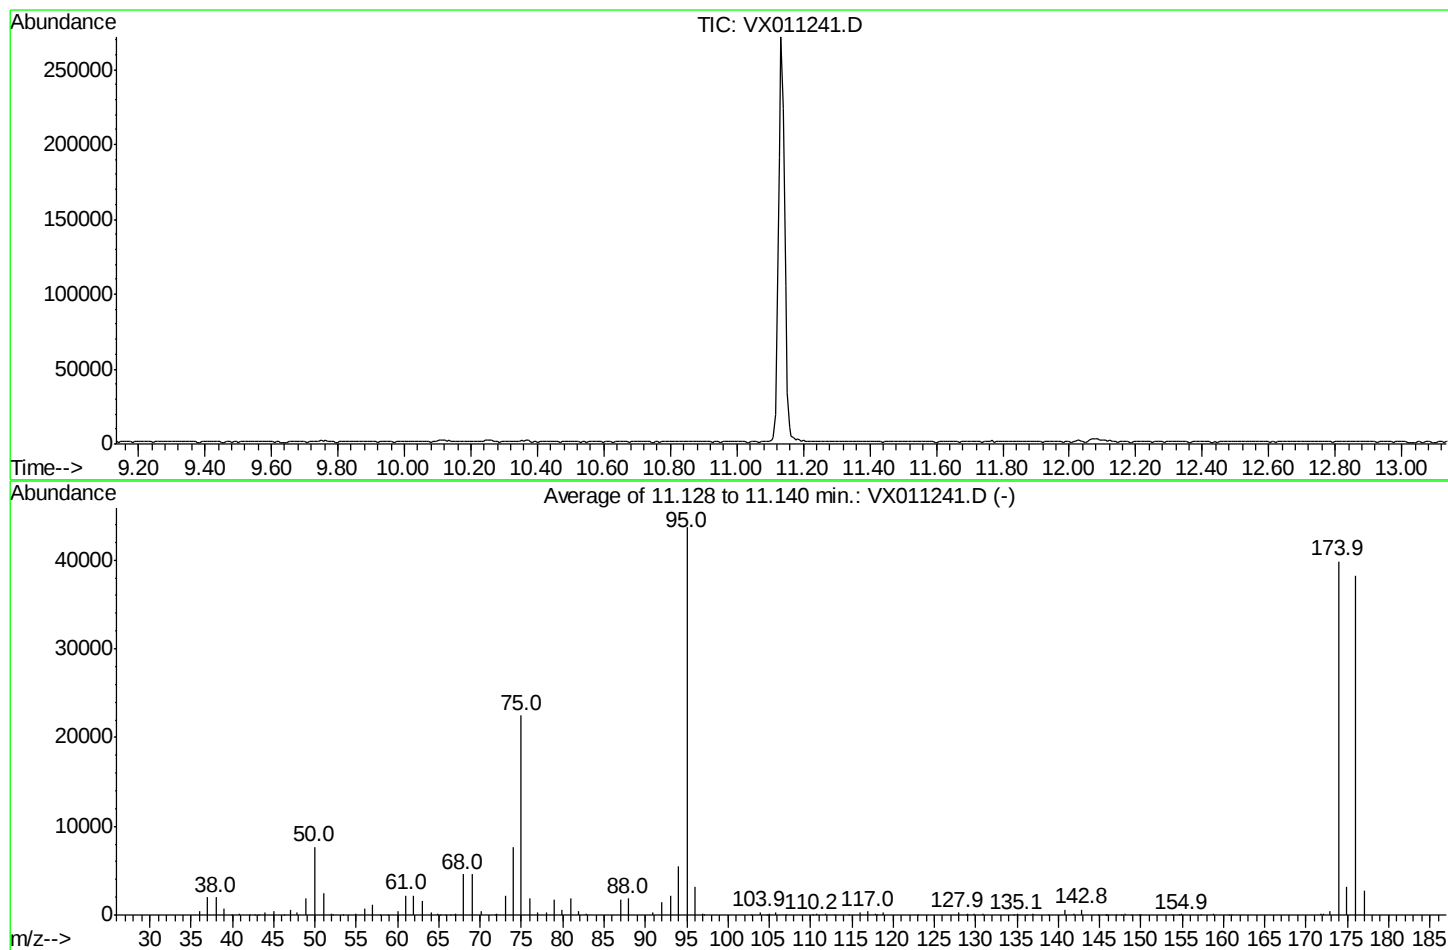

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	7722	PASS
75	95	30	60	51.5	22496	PASS
95	95	100	100	100.0	43690	PASS
96	95	5	9	7.2	3139	PASS
173	174	0.00	2	1.2	490	PASS
174	95	50	100	91.3	39888	PASS
175	174	5	9	8.0	3191	PASS
176	174	95	101	96.0	38301	PASS
177	176	5	9	7.0	2693	PASS