

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX073120\
 Data File : VX017696.D
 Acq On : 31 Jul 2020 13:13
 Operator : JC/SP
 Sample : L3530-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
ClientSampleId :
 STORAGE-BLANK-WATER-REF-6

Quant Time: Aug 01 03:29:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	487406	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	817810	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	868407	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	469729	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	329754	52.67	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	105.34%	
35) Dibromofluoromethane	5.47	113	277258	50.69	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	101.38%	
50) Toluene-d8	8.70	98	1016733	51.53	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	103.06%	
62) 4-Bromofluorobenzene	11.12	95	438752	55.56	ug/l	0.00
Spiked Amount				50.000		
			Recovery	=	111.12%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX073120\
 Data File : VX017696.D
 Acq On : 31 Jul 2020 13:13
 Operator : JC/SP
 Sample : L3530-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
ClientSampled :
 STORAGE-BLANK-WATER-REF-6

Quant Time: Aug 01 03:29:54 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration




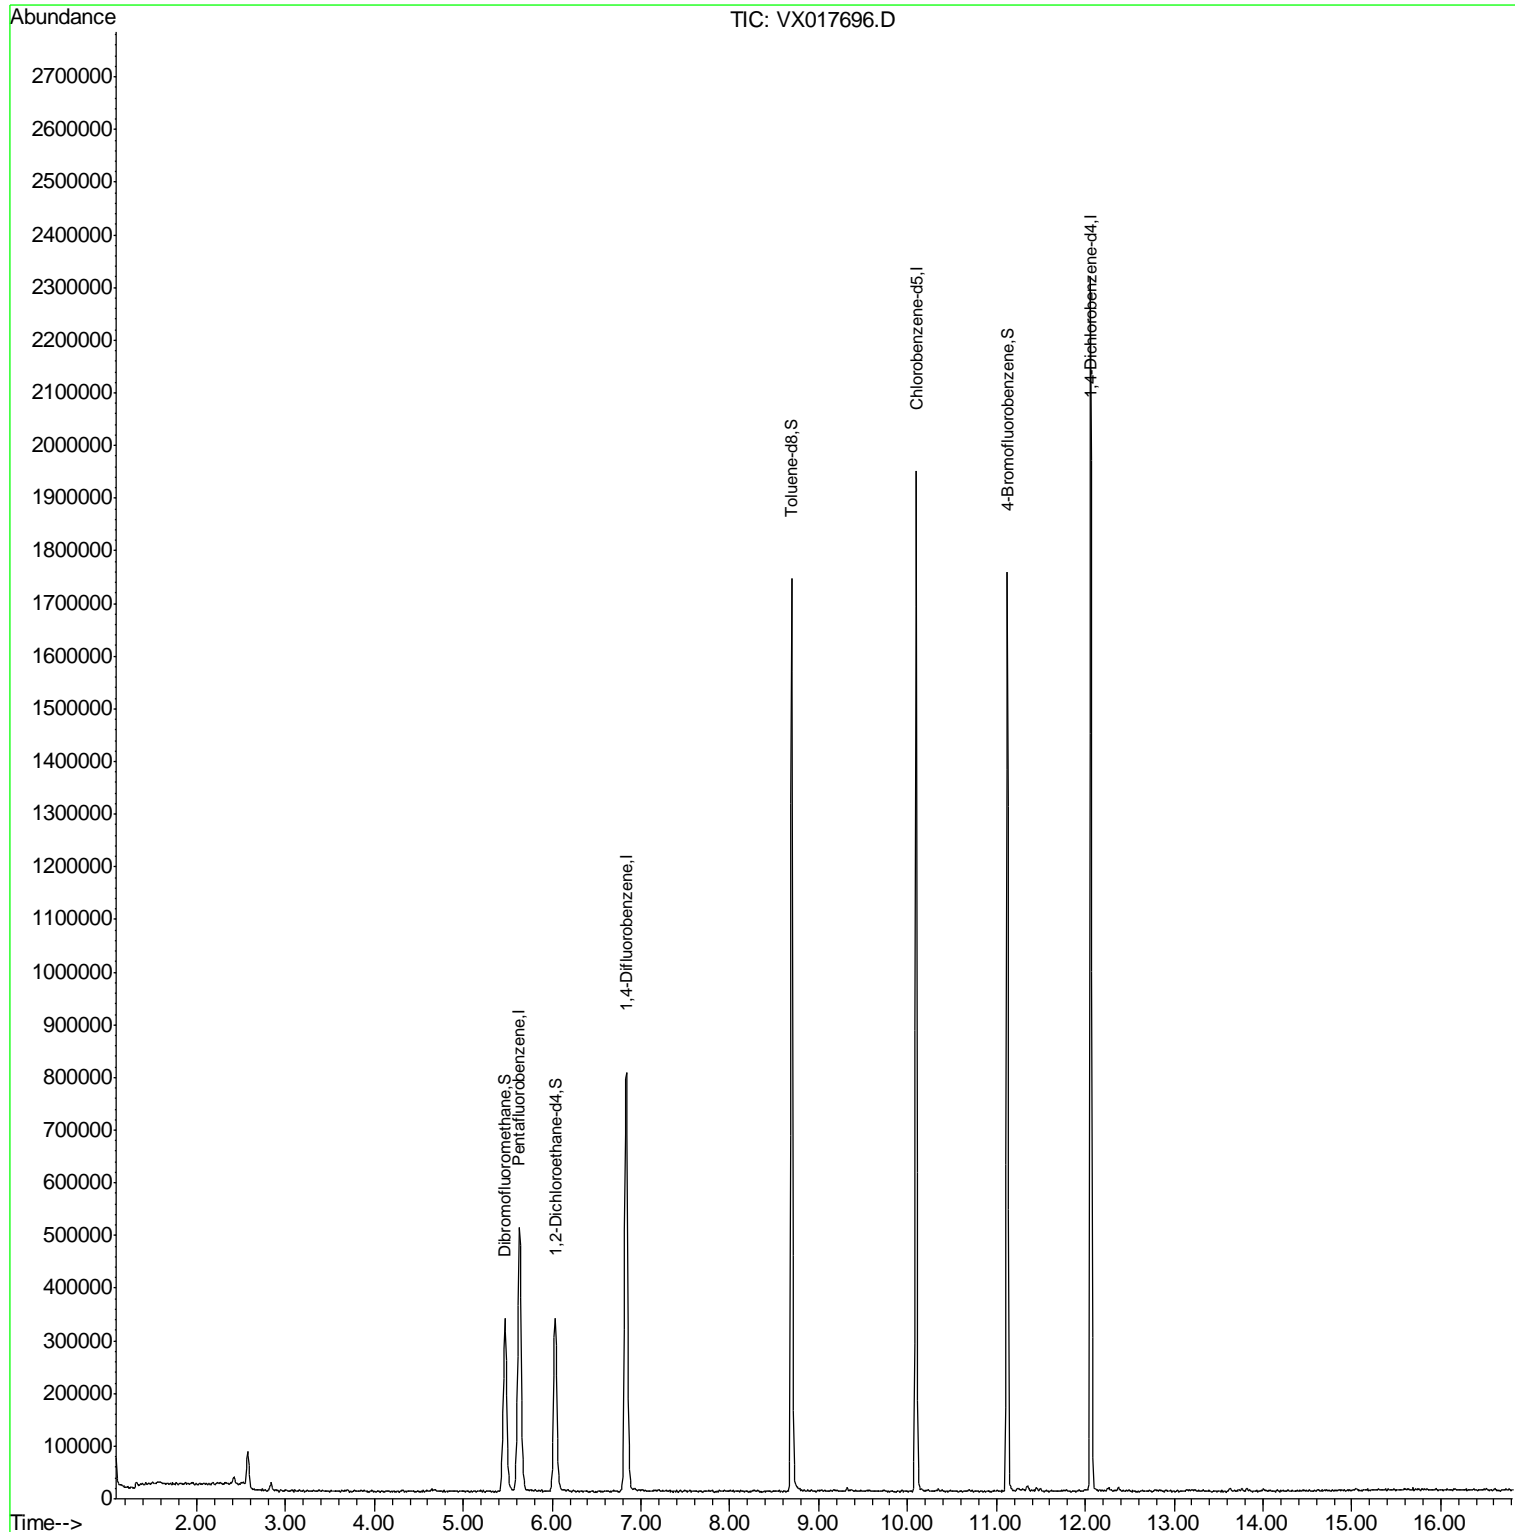


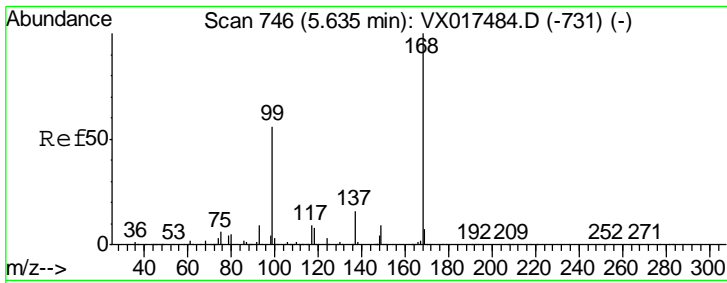

#1
 Pentafluorobenzene
 Concen: 50.000 ug/l
 RT: 5.63 min Scan# 745
 Delta R.T. -0.01 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13




Instrument :
 MSVOA_X
ClientSampled :
 STORAGE-BLANK-WATER-REF-6


Tgt Ion	Resp	Lower	Upper
168	487406		
99	57.0	43.4	65.2

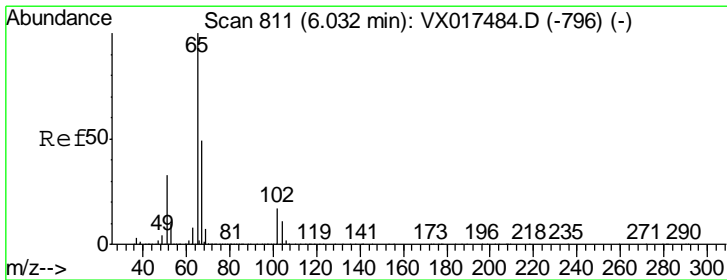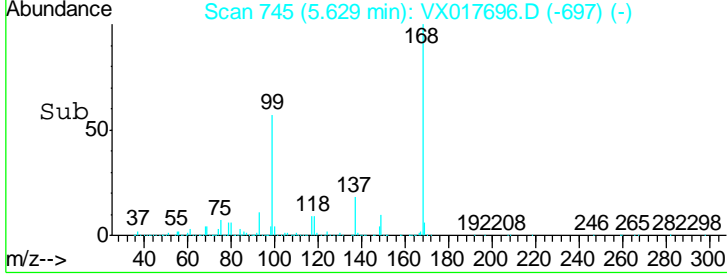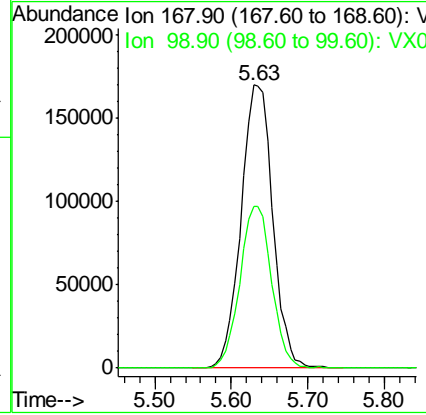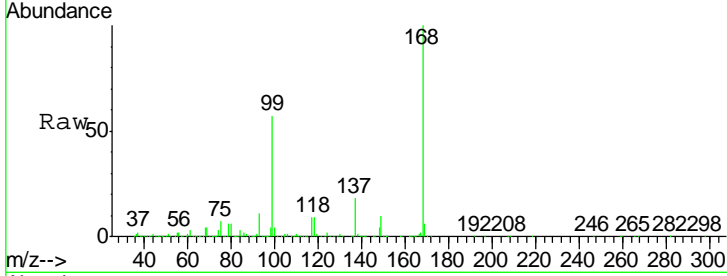

#33
 1,2-Dichloroethane-d4
 Concen: 52.668 ug/l
 RT: 6.03 min Scan# 811
 Delta R.T. -0.00 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13

Tgt Ion	Resp	Lower	Upper
65	329754		
67	51.8	0.0	102.8


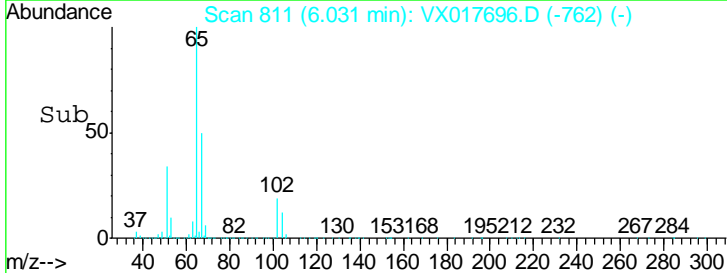
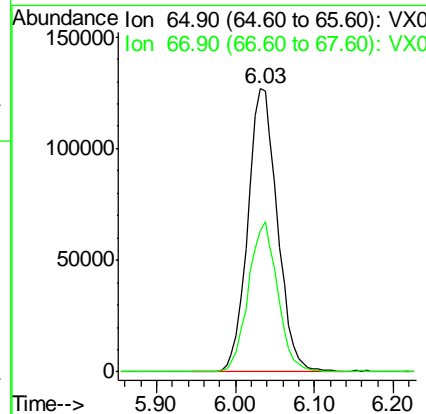
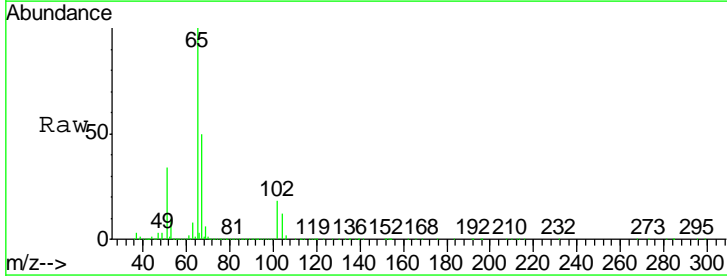


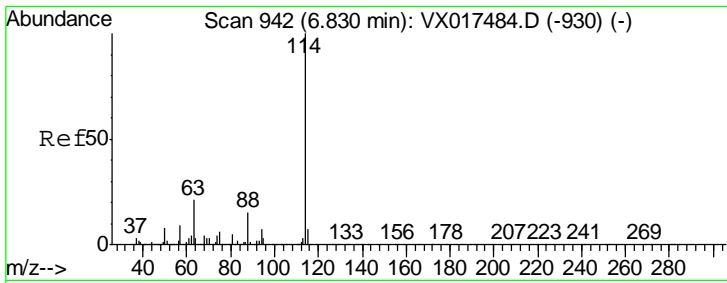

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.84 min Scan# 943
 Delta R.T. 0.01 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13




Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-6


Tgt Ion	Resp	Lower	Upper
114	817810		
63	20.1	0.0	40.6
88	15.3	0.0	33.4

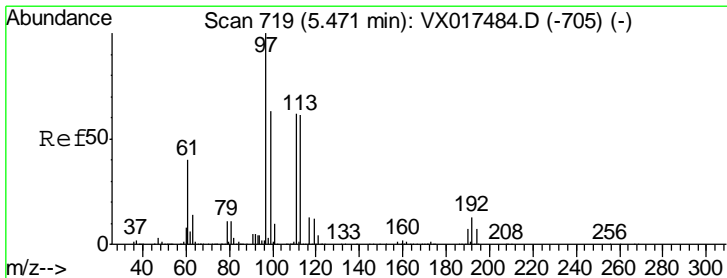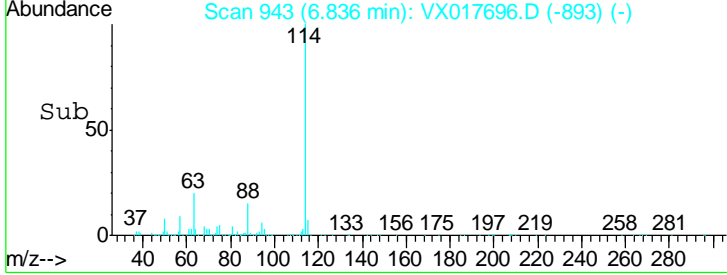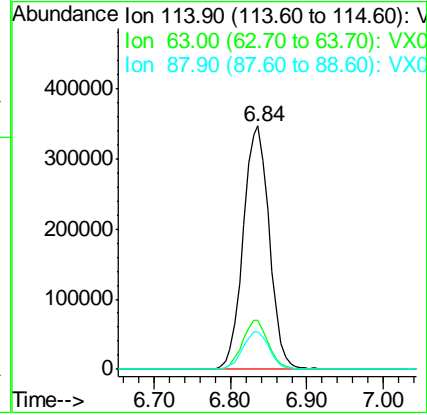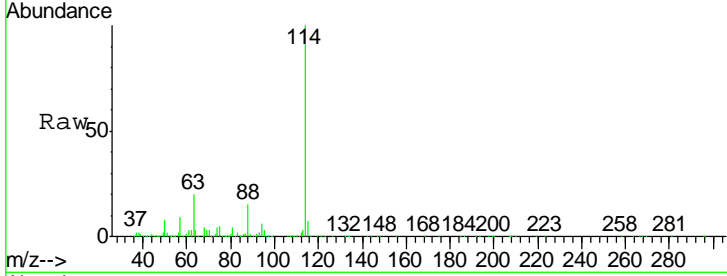

#35
 Dibromofluoromethane
 Concen: 50.691 ug/l
 RT: 5.47 min Scan# 719
 Delta R.T. -0.00 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13

Tgt Ion	Resp	Lower	Upper
113	277258		
111	102.4	80.7	121.1
192	20.5	16.9	25.3


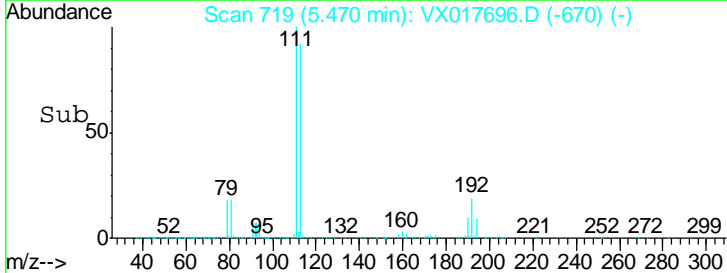
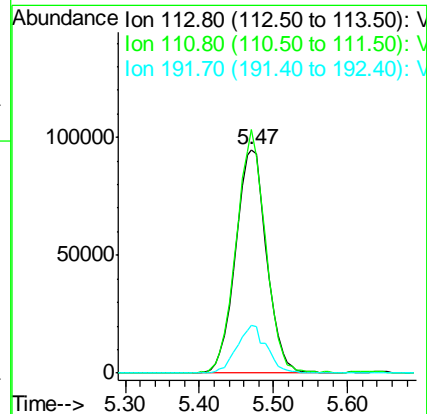
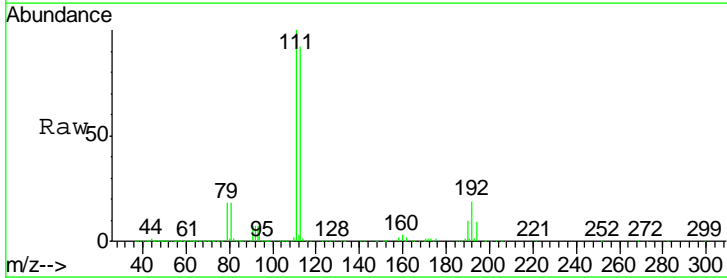


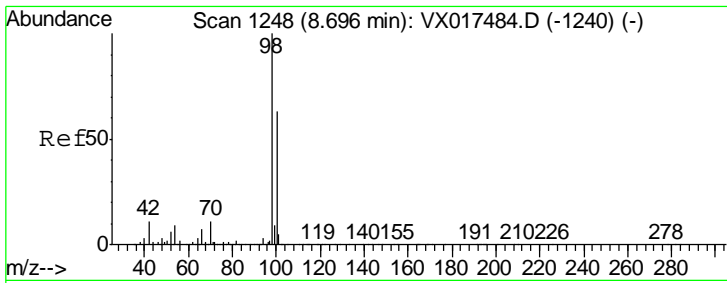

#50
 Toluene-d8
 Concen: 51.529 ug/l
 RT: 8.70 min Scan# 1248
 Delta R.T. -0.00 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13




Instrument :
 MSVOA_X
ClientSampleId :
 STORAGE-BLANK-WATER-REF-6


Tgt Ion: 98 Resp: 1016733
 Ion Ratio Lower Upper
 98 100
 100 64.1 52.3 78.5

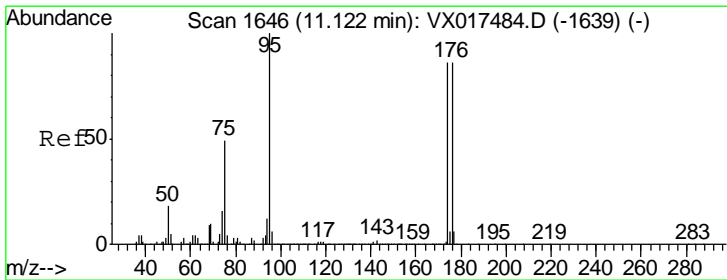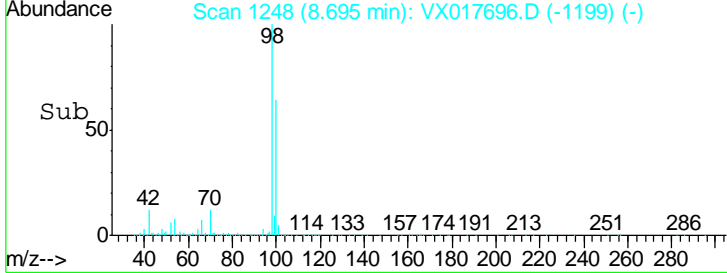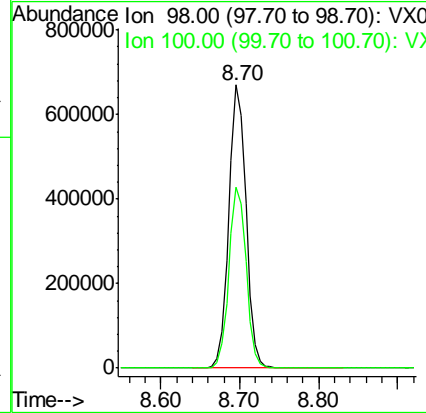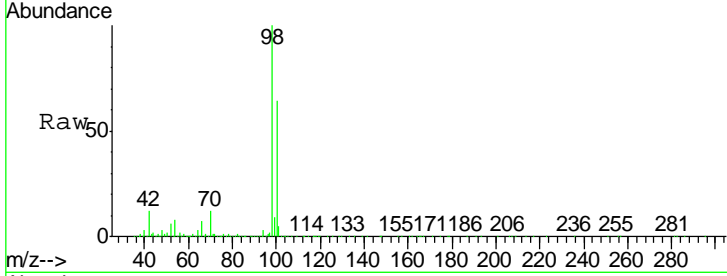

#62
 4-Bromofluorobenzene
 Concen: 55.563 ug/l
 RT: 11.12 min Scan# 1646
 Delta R.T. -0.00 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13

Tgt Ion: 95 Resp: 438752
 Ion Ratio Lower Upper
 95 100
 174 86.9 0.0 169.0
 176 81.0 0.0 161.0


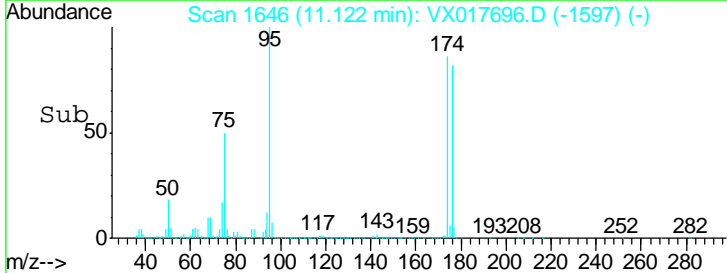
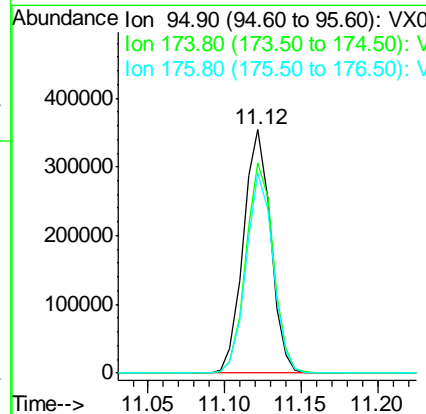
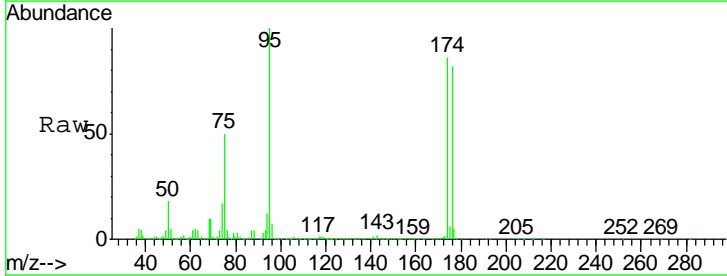


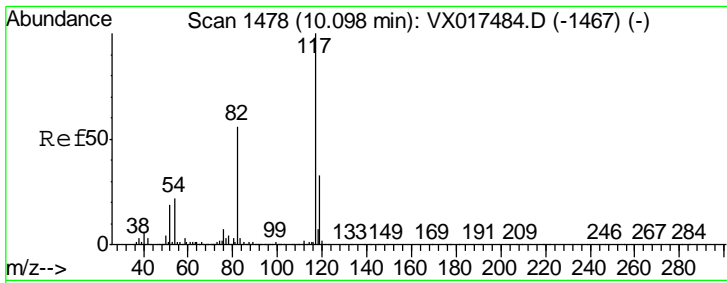

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 10.10 min Scan# 1478
 Delta R.T. -0.00 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13

Instrument :
 MSVOA_X
 ClientSampled :
 STORAGE-BLANK-WATER-REF-6

Tgt Ion	Resp	Lower	Upper
117	100		
82	52.7	44.0	66.0
119	31.8	25.4	38.0

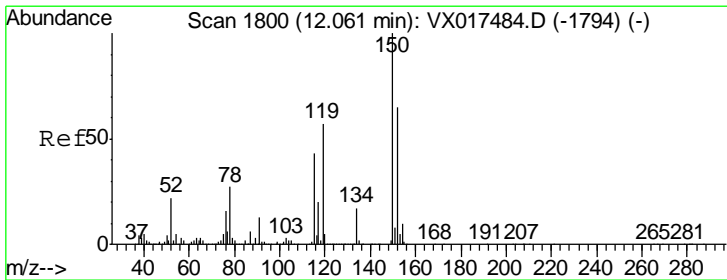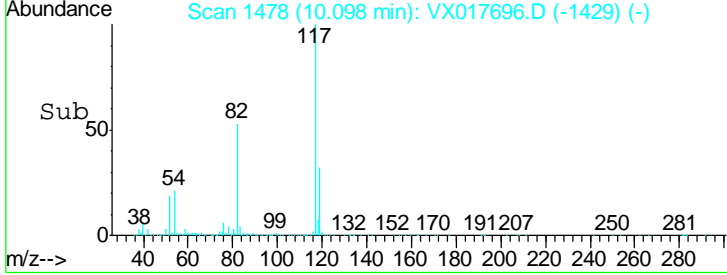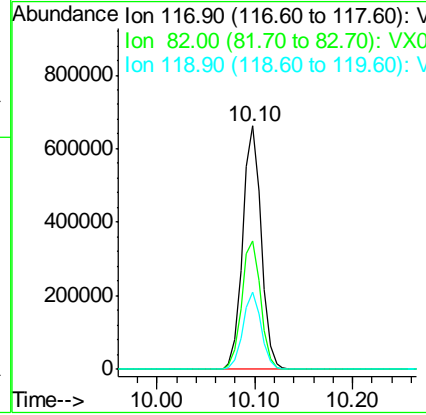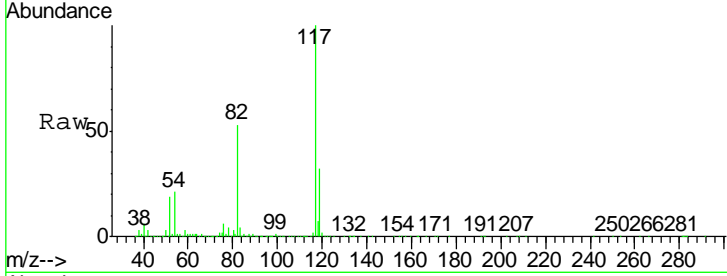

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.06 min Scan# 1800
 Delta R.T. -0.00 min
 Lab File: VX017696.D
 Acq: 31 Jul 2020 13:13

Tgt Ion	Resp	Lower	Upper
152	100		
115	58.7	65.5	196.6#
150	154.9	0.0	412.6

