

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX073120\
 Data File : VX017699.D
 Acq On : 31 Jul 2020 14:21
 Operator : JC/SP
 Sample : L3530-04
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANA

Quant Time: Aug 01 03:38:47 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 24 05:48:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	479111	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.84	114	811730	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	875175	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	477430	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.04	65	330747	53.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.48%	
35) Dibromofluoromethane	5.47	113	277739	51.16	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.32%	
50) Toluene-d8	8.70	98	1004208	51.28	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.56%	
62) 4-Bromofluorobenzene	11.12	95	436698	55.72	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.44%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX073120\
Data File : VX017699.D
Acq On : 31 Jul 2020 14:21
Operator : JC/SP
Sample : L3530-04
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Quant Time: Aug 01 03:38:47 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 24 05:48:09 2020
Response via : Initial Calibration

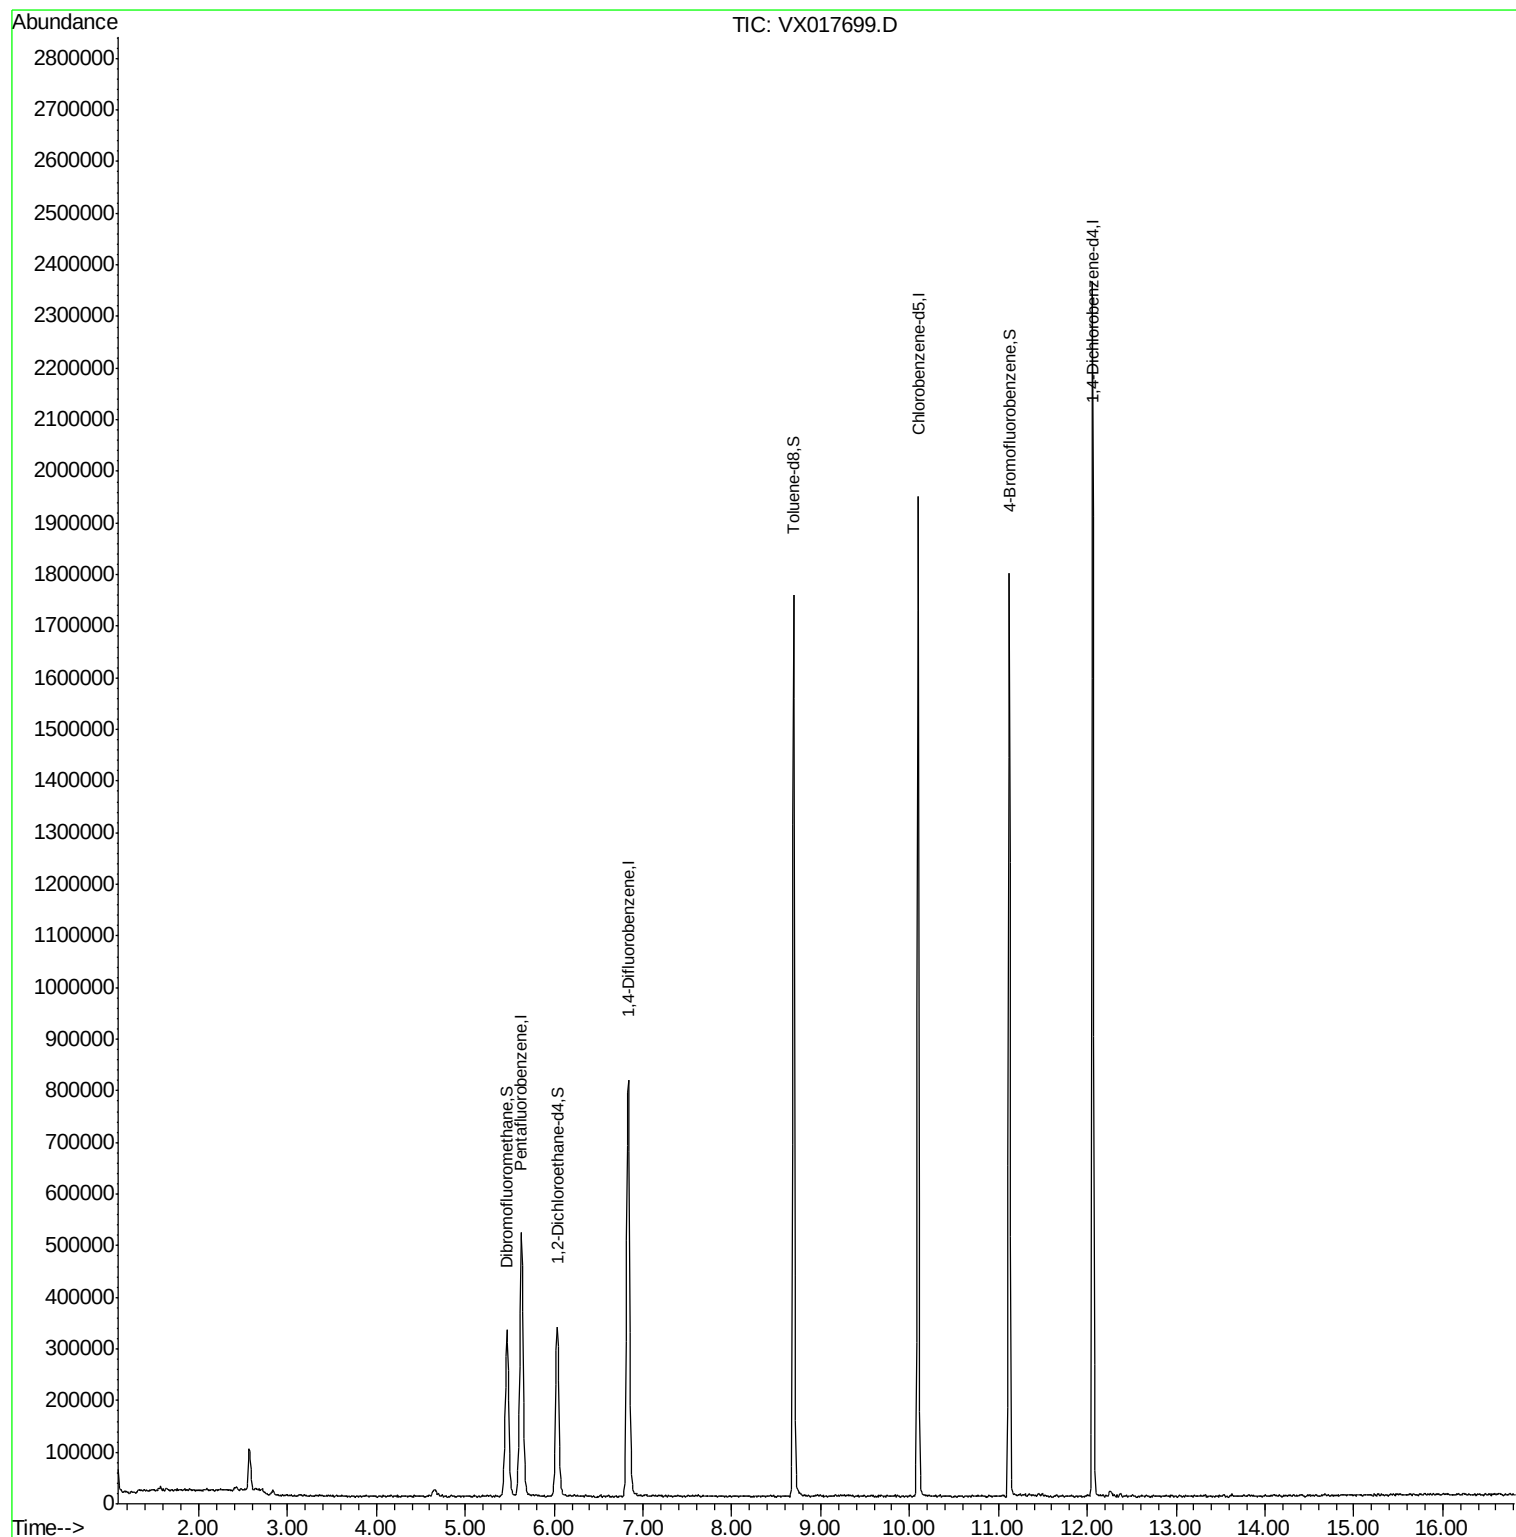

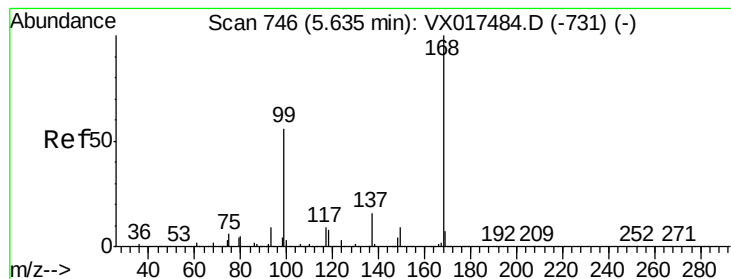

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.01 min

Lab File: VX017699.D

Acq: 31 Jul 2020 14:21

Instrument :

MSVOA_X

ClientSampleId :


STORAGE-BLANK-SAMPLE-MANA

Tot Ion:168 Resp: 479111

Ion Ratio Lower Upper

168 100

99 55.3 43.4 65.2

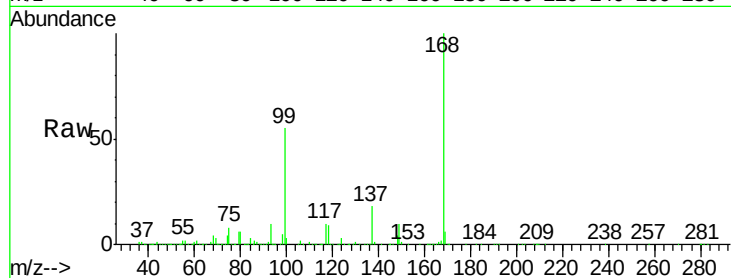

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

200000



150000

100000

50000

0

Time-->

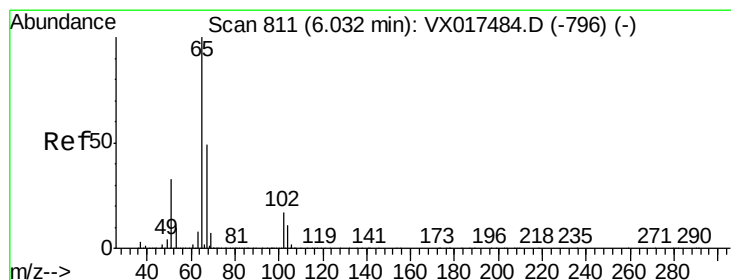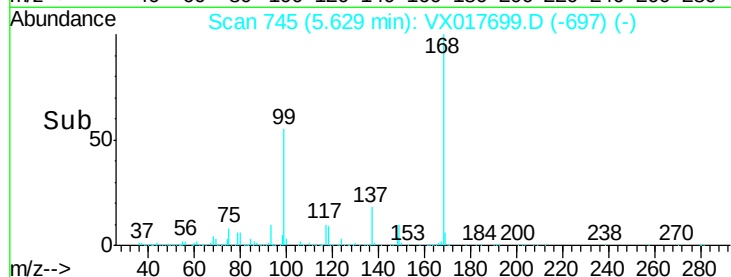

#33

1,2-Dichloroethane-d4

Concen: 53.742 ug/l

RT: 6.04 min Scan# 812

Delta R.T. 0.01 min

Lab File: VX017699.D


Acq: 31 Jul 2020 14:21

Tgt Ion: 65 Resp: 330747

Ion Ratio Lower Upper

65 100

67 51.1 0.0 102.8

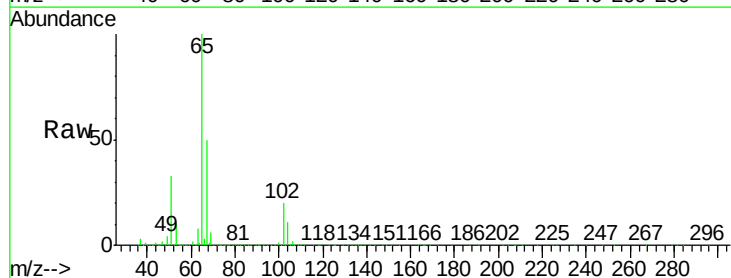

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.04


150000


100000

50000

0

Time-->

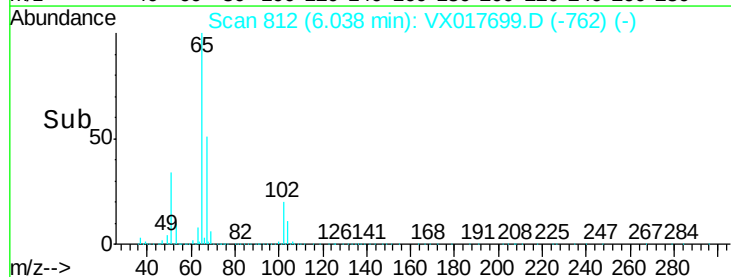

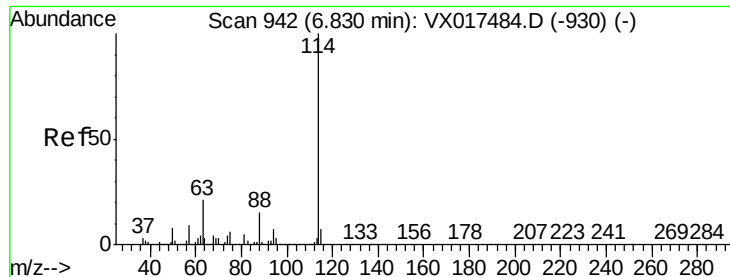

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.84 min Scan# 943

Delta R.T. 0.01 min

Lab File: VX017699.D

Acq: 31 Jul 2020 14:21

Instrument :

MSVOA_X

ClientSampleId :

STORAGE-BLANK-SAMPLE-MANA


Tot Ion:114 Resp: 811730

Ion Ratio Lower Upper

114 100

63 19.6 0.0 40.6




88 15.5 0.0 33.4

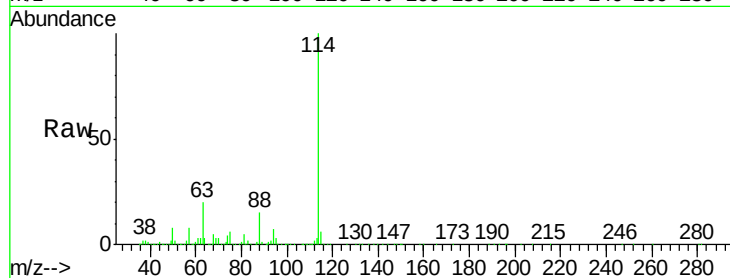

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

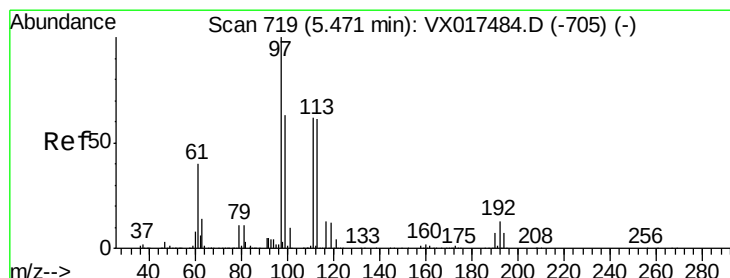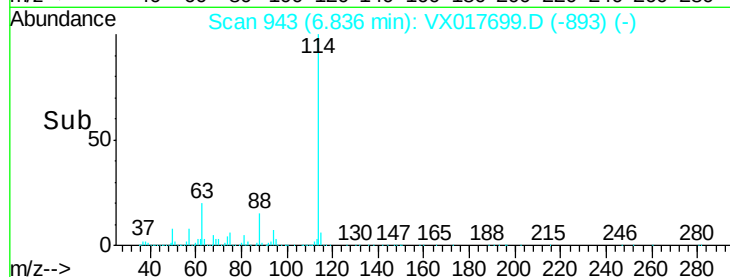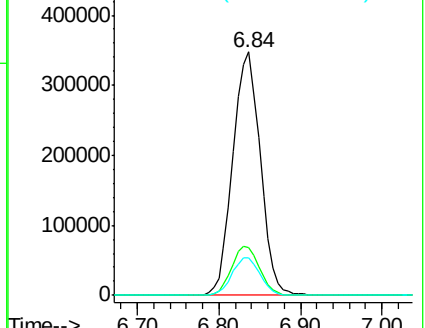

#35

Dibromofluoromethane

Concen: 51.159 ug/l

RT: 5.47 min Scan# 719

Delta R.T. -0.00 min

Lab File: VX017699.D

Acq: 31 Jul 2020 14:21


Tgt Ion:113 Resp: 277739

Ion Ratio Lower Upper

113 100

111 101.5 80.7 121.1



192 20.0 16.9 25.3

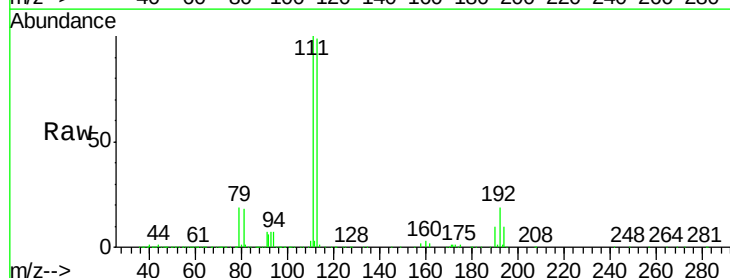


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



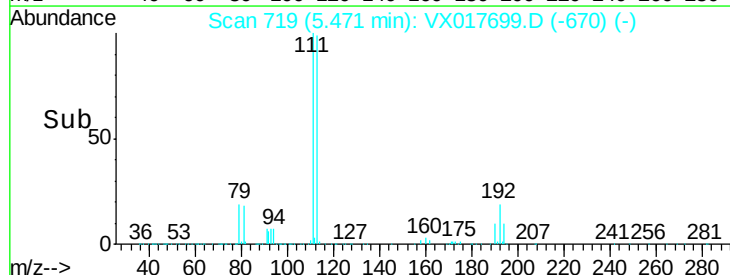
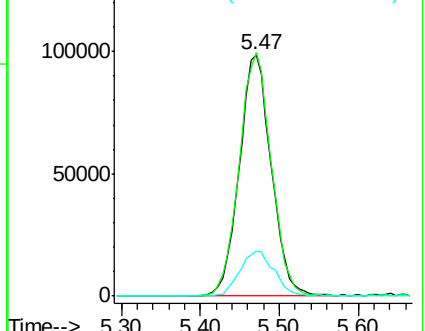


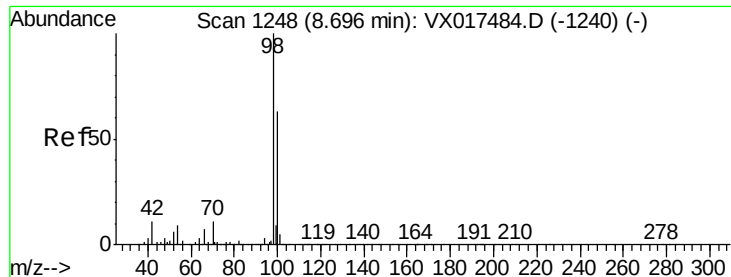

#50
Toluene-d8
Concen: 51.275 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX017699.D
Acq: 31 Jul 2020 14:21




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA


Tot Ion: 98 Resp: 1004208
Ion Ratio Lower Upper
98 100
100 64.1 52.3 78.5

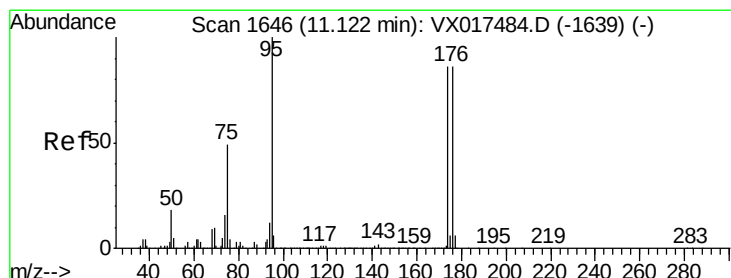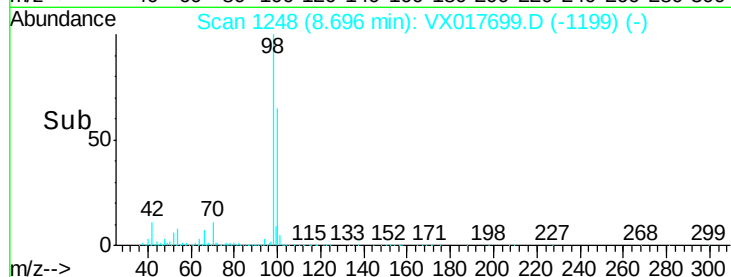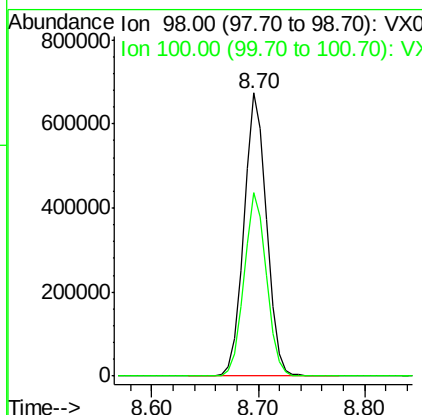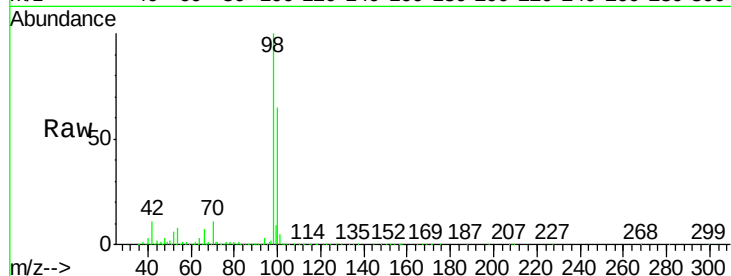

#62
4-Bromofluorobenzene
Concen: 55.717 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017699.D
Acq: 31 Jul 2020 14:21

Tgt Ion: 95 Resp: 436698
Ion Ratio Lower Upper
95 100
174 85.8 0.0 169.0
176 83.0 0.0 161.0


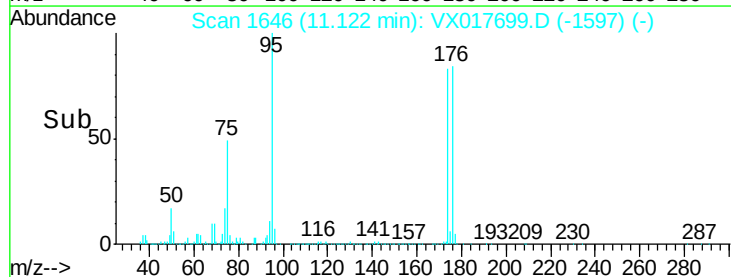
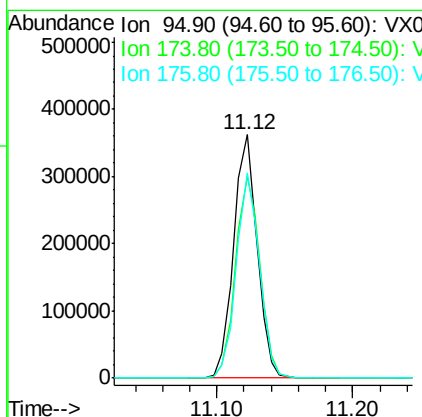
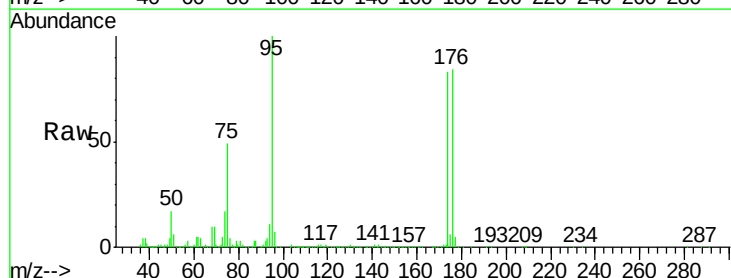


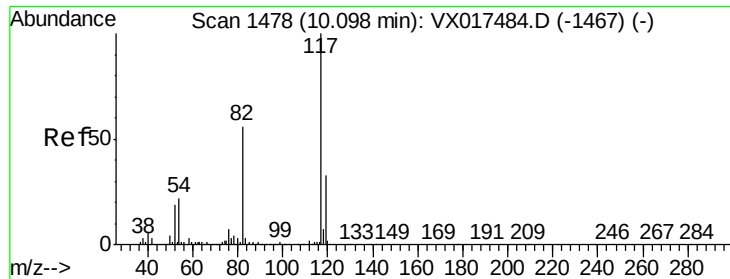

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017699.D
Acq: 31 Jul 2020 14:21

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANA

Tot Ion	Ratio	Lower	Upper
117	100		
82	54.4	44.0	66.0
119	32.7	25.4	38.0

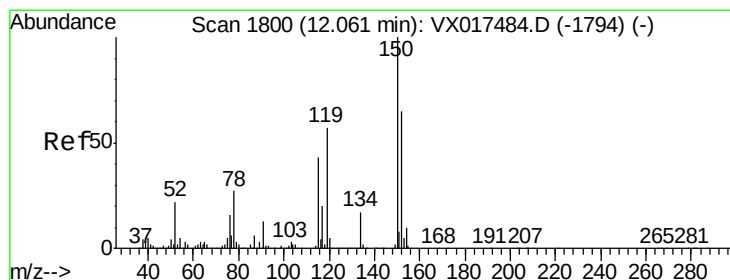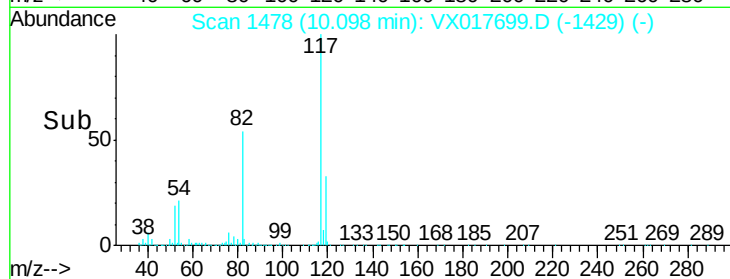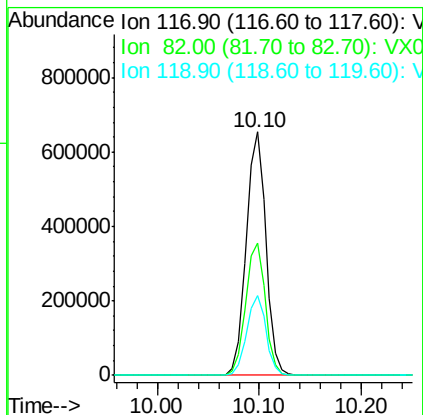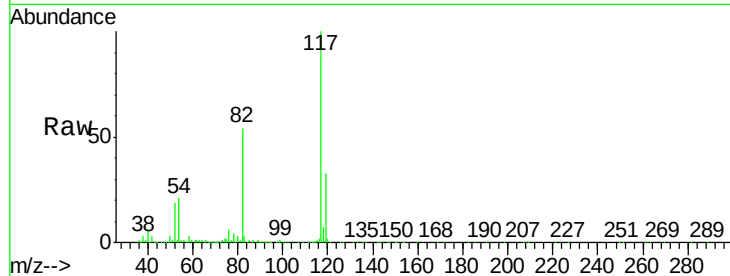

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX017699.D
Acq: 31 Jul 2020 14:21

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.5	65.5	196.6#
150	155.6	0.0	412.6

