


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX073120\
 Data File : VX017688.D
 Acq On : 31 Jul 2020 08:42
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Title : SW846 8260
 Last Update : Fri Jul 24 05:48:09 2020

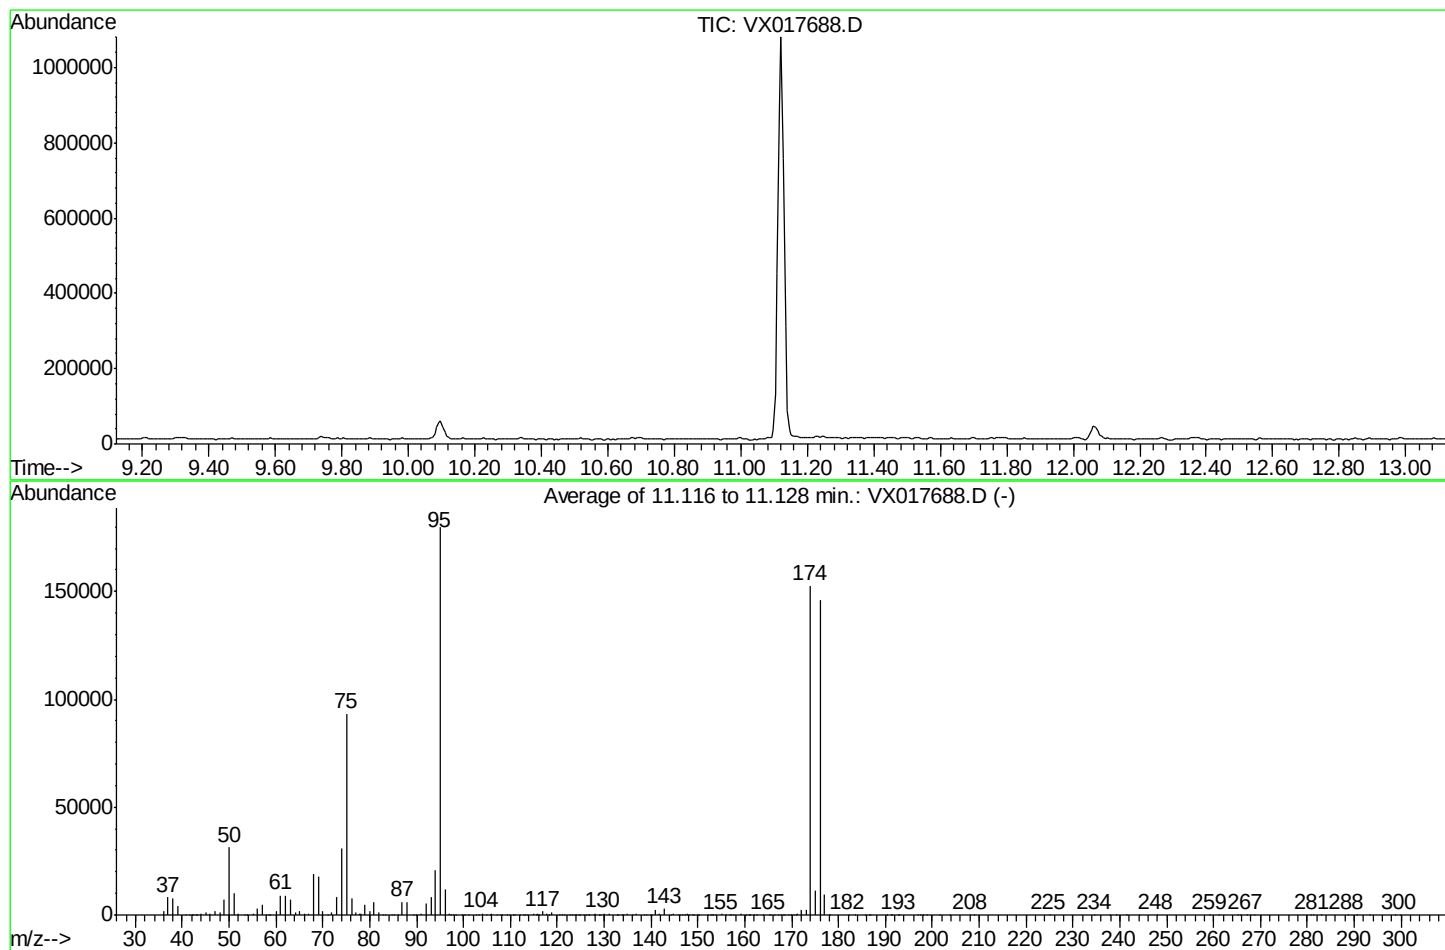

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	31311	PASS
75	95	30	60	51.9	93316	PASS
95	95	100	100	100.0	179776	PASS
96	95	5	9	6.8	12154	PASS
173	174	0.00	2	1.6	2409	PASS
174	95	50	100	85.0	152816	PASS
175	174	5	9	7.2	11046	PASS
176	174	95	101	95.7	146290	PASS
177	176	5	9	6.7	9735	PASS