


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX073120\
 Data File : VX017714.D
 Acq On : 31 Jul 2020 20:49
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
 Title : SW846 8260
 Last Update : Fri Jul 24 05:48:09 2020

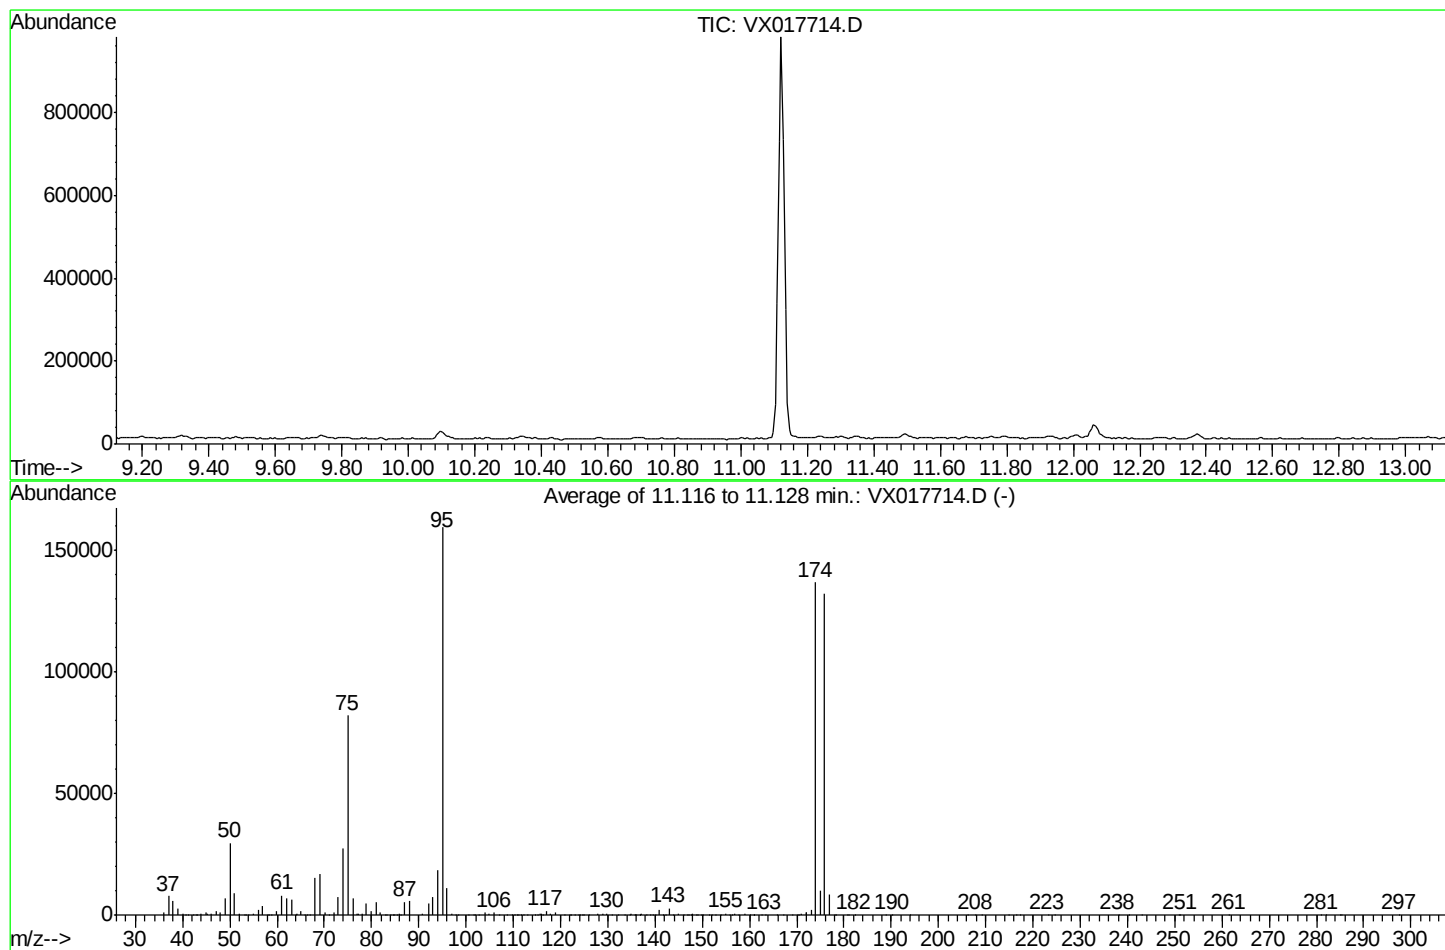

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	29789	PASS
75	95	30	60	51.4	82016	PASS
95	95	100	100	100.0	159646	PASS
96	95	5	9	7.0	11151	PASS
173	174	0.00	2	1.6	2257	PASS
174	95	50	100	85.8	136986	PASS
175	174	5	9	7.5	10255	PASS
176	174	95	101	96.6	132349	PASS
177	176	5	9	6.5	8633	PASS