

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073123\
 Data File : VX036718.D
 Acq On : 31 Jul 2023 14:23
 Operator : JC/MD
 Sample : 03808-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1711

Quant Time: Aug 01 04:36:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	145807	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	263200	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	242099	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	111680	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	97434	45.162	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	90.320%		
35) Dibromofluoromethane	5.385	113	83714	46.274	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	92.540%		
50) Toluene-d8	8.653	98	318032	49.573	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	99.140%		
62) 4-Bromofluorobenzene	11.079	95	118928	49.135	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.260%		
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.946	59	1183	2.316	ug/l #	78
13) Acrolein	2.221	56	60	0.206	ug/l #	1
16) Acetone	2.380	43	15128	16.898	ug/l	99
17) Carbon Disulfide	2.514	76	1184	0.263	ug/l #	75
20) Methylene Chloride	2.788	84	416	0.209	ug/l #	81
25) 2-Butanone	4.568	43	12035	8.286	ug/l	98
31) Cyclohexane	5.550	56	3369	1.128	ug/l #	1
36) 1,1-Dichloropropene	5.550	75	11920	4.421	ug/l #	51
37) Ethyl Acetate	4.568	43	12035	3.943	ug/l #	69
38) Carbon Tetrachloride	5.556	117	15472	5.397	ug/l #	15
51) 4-Methyl-2-Pentanone	8.580	43	5391	1.854	ug/l	99
52) Toluene	8.726	92	4794984	975.448	ug/l	92
53) t-1,3-Dichloropropene	8.726	75	63369	18.633	ug/l #	1
67) Ethyl Benzene	10.195	91	39243	4.025	ug/l	99
68) m/p-Xylenes	10.299	106	49928	13.726	ug/l	100
69) o-Xylene	10.640	106	16924	4.661	ug/l	98
70) Styrene	10.652	104	1883	0.314	ug/l #	1
76) 1,2,3-Trichloropropane	11.079	75	62152	23.660	ug/l #	38
78) n-propylbenzene	11.305	91	2583	0.242	ug/l	99
79) 2-Chlorotoluene	11.378	91	1509	0.233	ug/l #	42
80) 1,3,5-Trimethylbenzene	11.451	105	5475	0.708	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	62152	53.628	ug/l #	5
83) tert-Butylbenzene	11.756	119	1531	0.202	ug/l #	50
84) 1,2,4-Trimethylbenzene	11.750	105	19950	2.580	ug/l	79
85) sec-Butylbenzene	11.890	105	2461	0.260	ug/l	96
86) p-Isopropyltoluene	11.969	119	1936	0.248	ug/l	90
89) n-Butylbenzene	12.323	91	5513	0.790	ug/l #	16
90) Hexachloroethane	12.555	117	1328	0.840	ug/l #	17
92) 1,2-Dibromo-3-Chloropr...	12.920	75	232	0.320	ug/l #	9
95) Naphthalene	13.774	128	9850	1.220	ug/l #	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073123\
Data File : VX036718.D
Acq On : 31 Jul 2023 14:23
Operator : JC/MD
Sample : 03808-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1711

Quant Time: Aug 01 04:36:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration

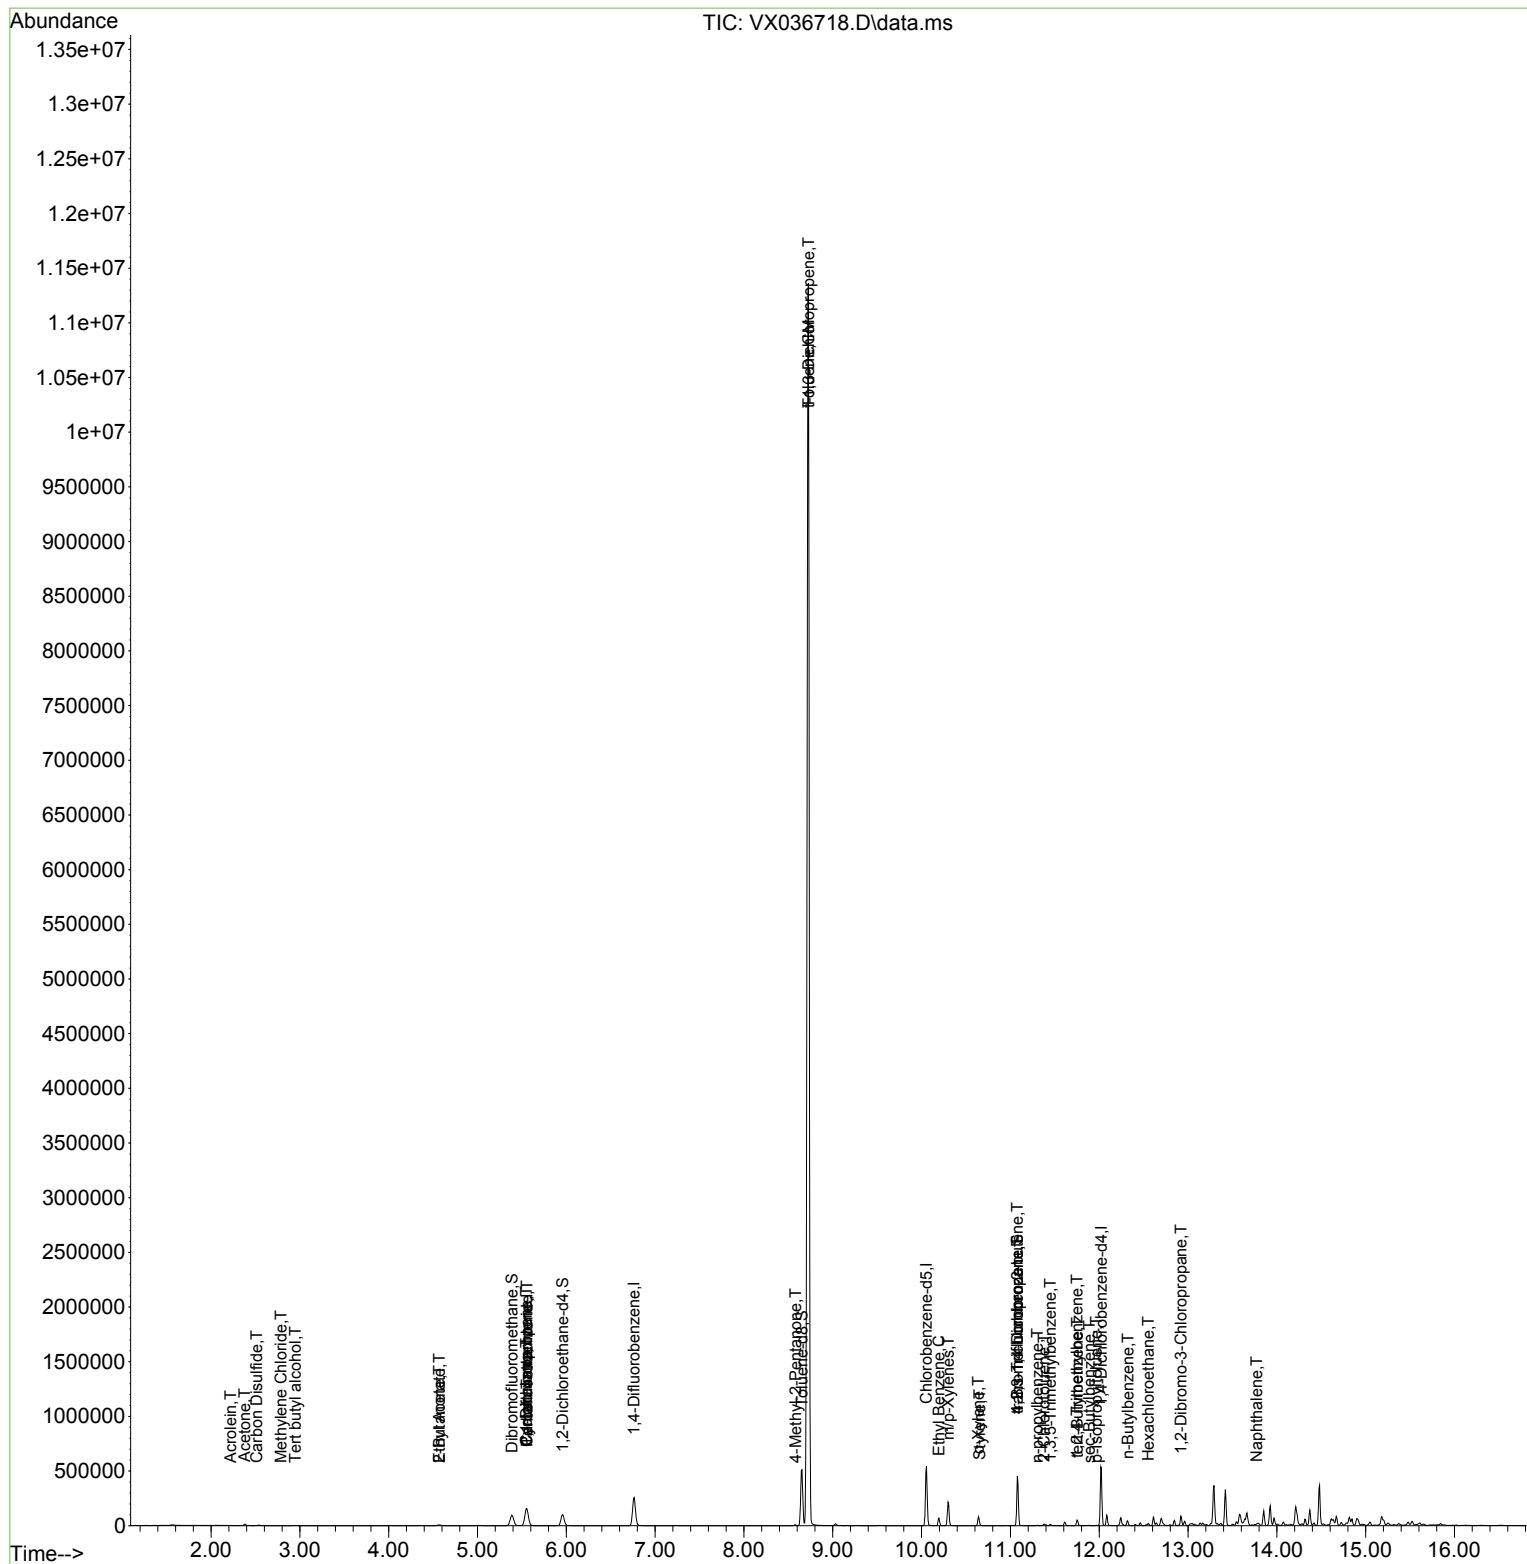

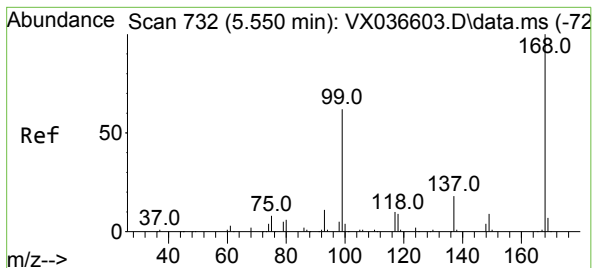

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.556 min Scan# 711

Delta R.T. 0.006 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23

Instrument :

MSVOA_X

ClientSampleId :





1711

Tgt Ion:168 Resp: 145807

Ion Ratio Lower Upper

168 100

99 60.8 56.6 85.0

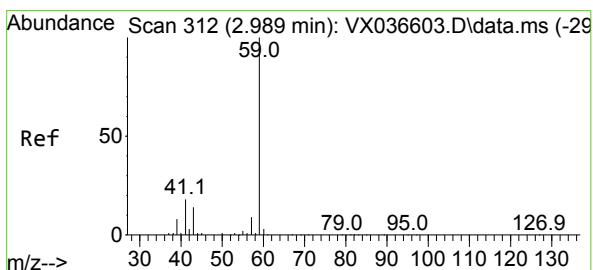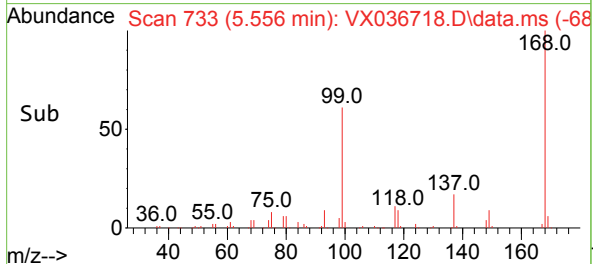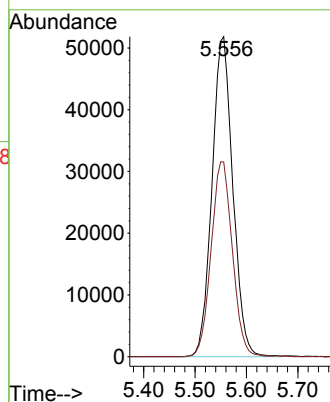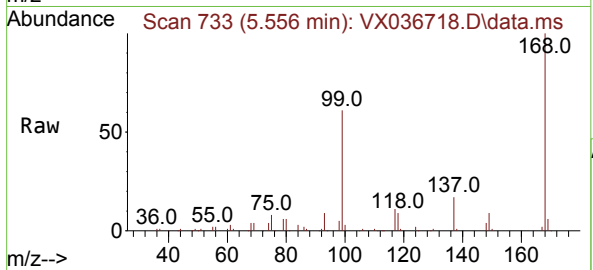

#11

Tert butyl alcohol

Concen: 2.316 ug/l

RT: 2.946 min Scan# 305

Delta R.T. -0.043 min

Lab File: VX036718.D




Acq: 31 Jul 2023 14:23


Tgt Ion: 59 Resp: 1183

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#


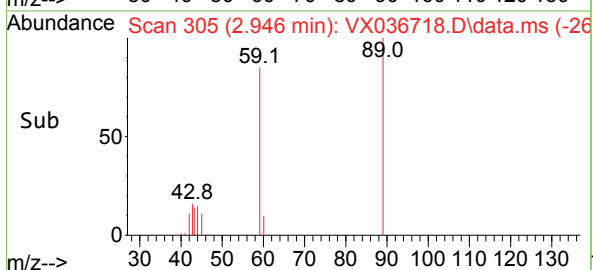

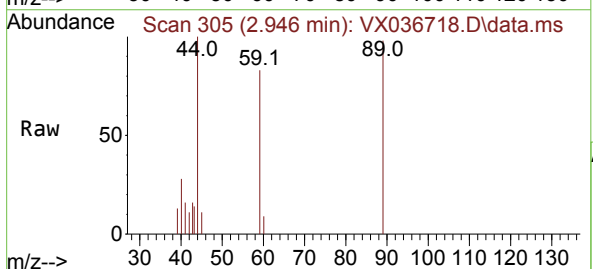


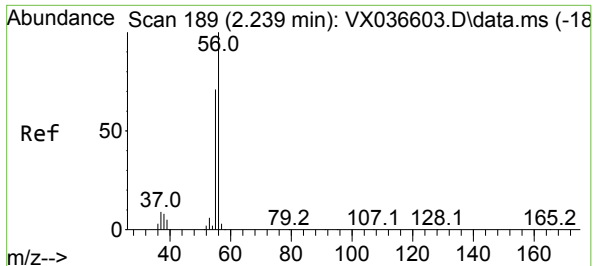

#13
Acrolein
Concen: 0.206 ug/l
RT: 2.221 min Scan# 11
Delta R.T. -0.018 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument :
MSVOA_X
ClientSampleId :
1711


Tgt Ion: 56 Resp: 60
Ion Ratio Lower Upper
56 100
55 160.0 57.1 85.7#

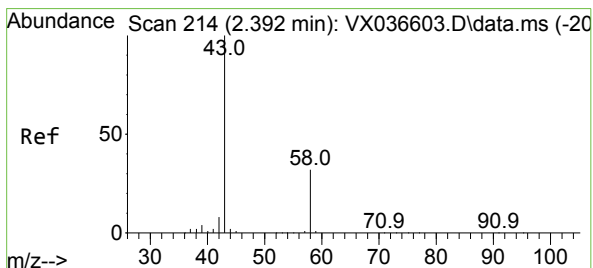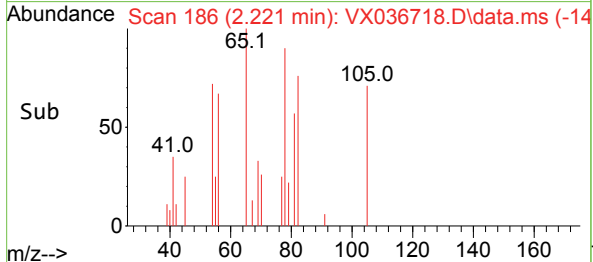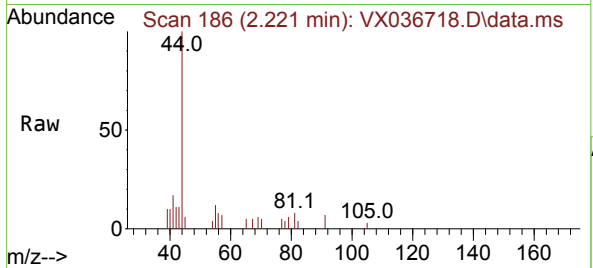

#16
Acetone
Concen: 16.898 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.012 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion: 43 Resp: 15128
Ion Ratio Lower Upper
43 100
58 28.0 21.9 32.9

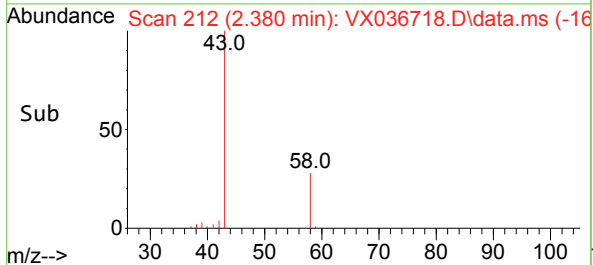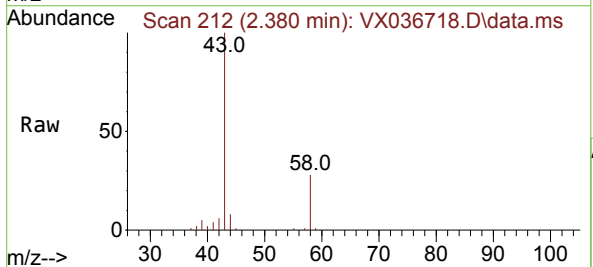



#17

Carbon Disulfide

Concen: 0.263 ug/l

RT: 2.514 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23

Instrument :

MSVOA_X

ClientSampleId :





1711

Tgt Ion: 76 Resp: 1184

Ion Ratio Lower Upper

76 100

78 17.7 7.0 10.6#

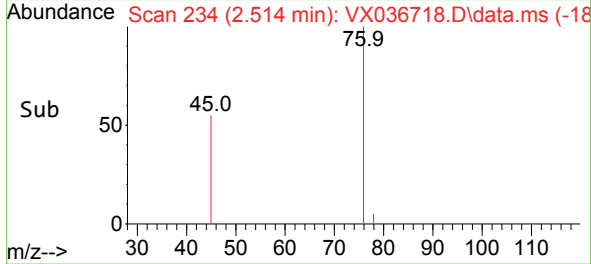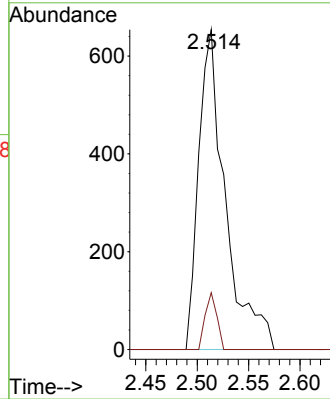

#20

Methylene Chloride

Concen: 0.209 ug/l

RT: 2.788 min Scan# 279

Delta R.T. -0.000 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23

Tgt Ion: 84 Resp: 416




Ion Ratio Lower Upper


84 100

49 113.8 103.6 155.4

51 19.6 33.8 50.6#

86 48.1 49.4 74.0#


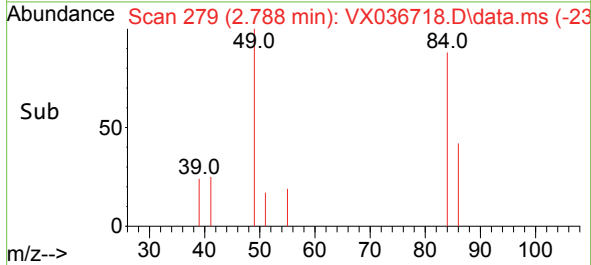
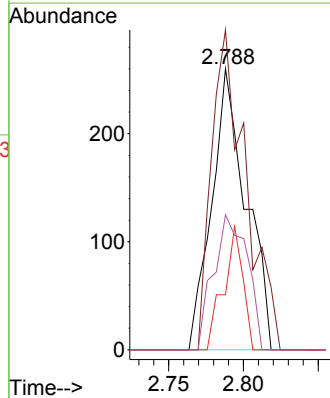





#25
2-Butanone
Concen: 8.286 ug/l
RT: 4.568 min Scan# 511
Delta R.T. 0.006 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument :
MSVOA_X
ClientSampleId :
1711


Tgt Ion: 43 Resp: 12035
Ion Ratio Lower Upper
43 100
72 25.2 19.4 29.2

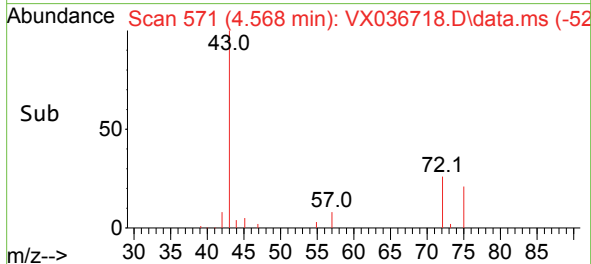

#31
Cyclohexane
Concen: 1.128 ug/l
RT: 5.550 min Scan# 732
Delta R.T. 0.079 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion: 56 Resp: 3369
Ion Ratio Lower Upper
56 100
69 168.0 23.4 35.2#
84 140.9 65.9 98.9#









#33
 1,2-Dichloroethane-d4
 Concen: 45.162 ug/l
 RT: 5.958 min Scan# 798
 Delta R.T. 0.006 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23




Instrument :
 MSVOA_X
 ClientSampleId :
 1711


Tgt Ion: 65 Resp: 97434
 Ion Ratio Lower Upper
 65 100
 67 52.3 0.0 100.2

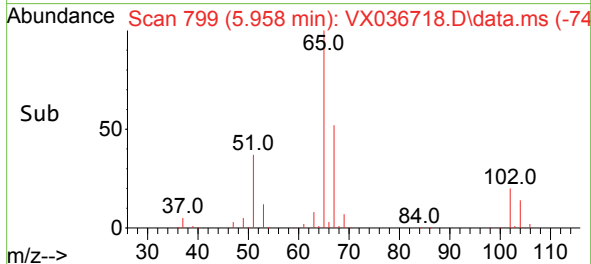

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.000 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23

Tgt Ion: 114 Resp: 263200
 Ion Ratio Lower Upper
 114 100
 63 20.4 0.0 45.0
 88 16.0 0.0 36.6



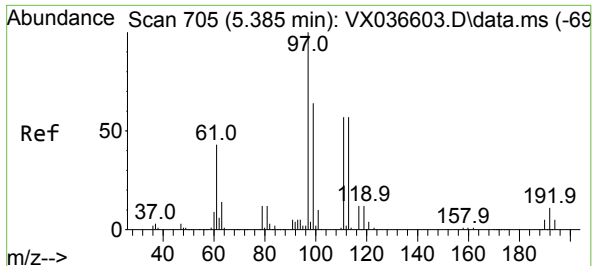

#35

Dibromofluoromethane

Concen: 46.274 ug/l

RT: 5.385 min Scan# 705

Delta R.T. -0.000 min

Lab File: VX036718.D


Acq: 31 Jul 2023 14:23

Instrument :

MSVOA_X

ClientSampleId :

1711

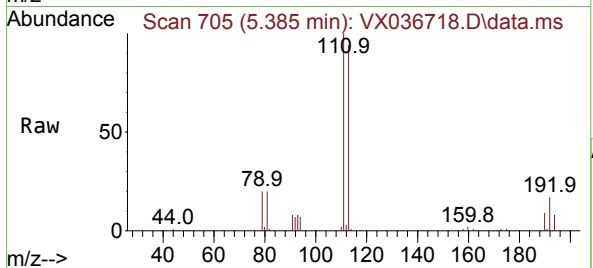




Tgt Ion:113 Resp: 83714

Ion Ratio Lower Upper

113 100

111 102.7 82.9 124.3

192 18.1 13.3 19.9

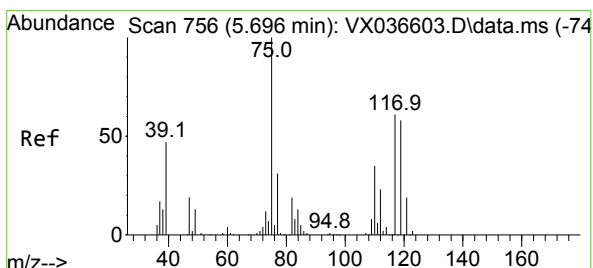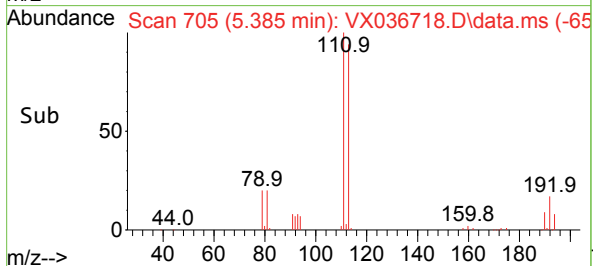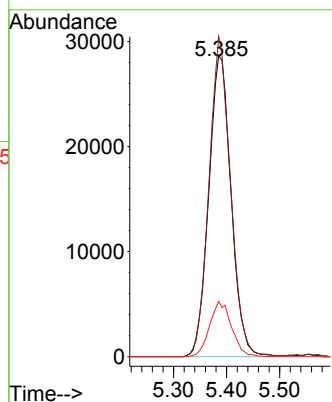

#36

1,1-Dichloropropene

Concen: 4.421 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.146 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23




Tgt Ion: 75 Resp: 11920


Ion Ratio Lower Upper

75 100

110 10.0 17.0 50.9#

77 0.0 24.7 37.1#


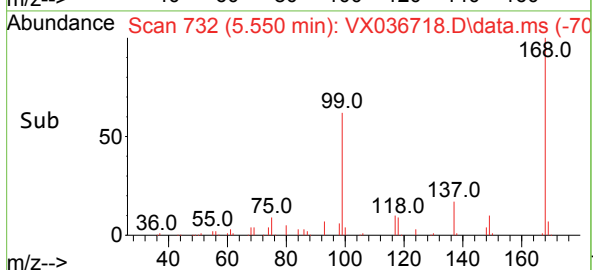

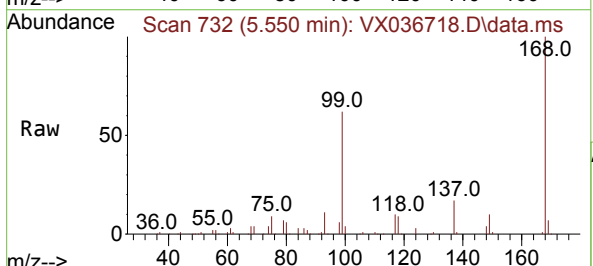




#37
Ethyl Acetate
Concen: 3.943 ug/l
RT: 4.568 min Scan# 511
Delta R.T. -0.146 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument :
MSVOA_X
ClientSampleId :
1711


Tgt Ion: 43 Resp: 12035
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.3 12.5#

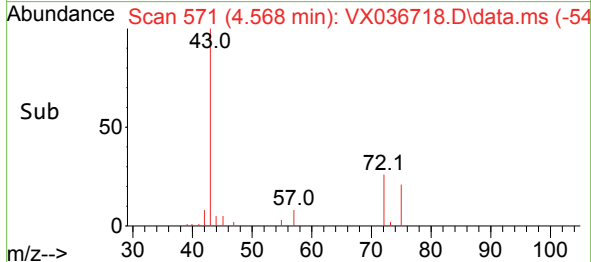

#38
Carbon Tetrachloride
Concen: 5.397 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.122 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion: 117 Resp: 15472
Ion Ratio Lower Upper
117 100
119 5.4 78.2 117.2#
121 0.0 24.4 36.6#



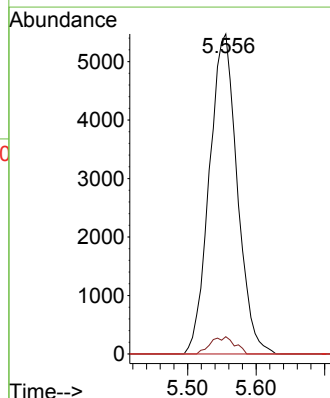



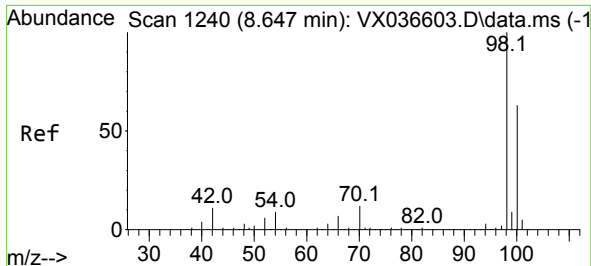

#50
Toluene-d8
Concen: 49.573 ug/l
RT: 8.653 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument :
MSVOA_X
ClientSampleId :
1711


Tgt Ion: 98 Resp: 318032
Ion Ratio Lower Upper
98 100
100 65.7 53.1 79.7

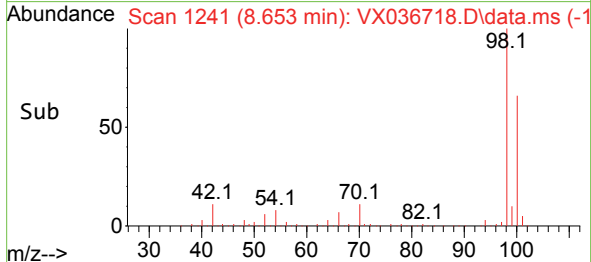

#51
4-Methyl-2-Pentanone
Concen: 1.854 ug/l
RT: 8.580 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion: 43 Resp: 5391
Ion Ratio Lower Upper
43 100
58 38.6 30.4 45.6

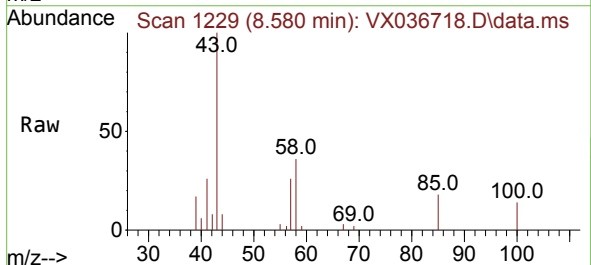



#52

Toluene

Concen: 975.448 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. 0.006 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23

Instrument :

MSVOA_X

ClientSampleId :





1711

Tgt Ion: 92 Resp: 4794984

Ion Ratio Lower Upper

92 100

91 156.2 134.2 201.2

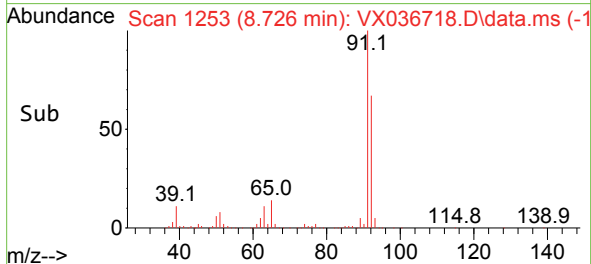

#53

t-1,3-Dichloropropene

Concen: 18.633 ug/l

RT: 8.726 min Scan# 1253

Delta R.T. -0.250 min

Lab File: VX036718.D




Acq: 31 Jul 2023 14:23


Tgt Ion: 75 Resp: 63369

Ion Ratio Lower Upper

75 100

77 162.1 25.7 38.5#









#62
4-Bromofluorobenzene
Concen: 49.135 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument :
MSVOA_X
ClientSampleId :
1711


Tgt Ion: 95 Resp: 118928
Ion Ratio Lower Upper
95 100
174 74.3 0.0 135.6
176 70.8 0.0 131.0

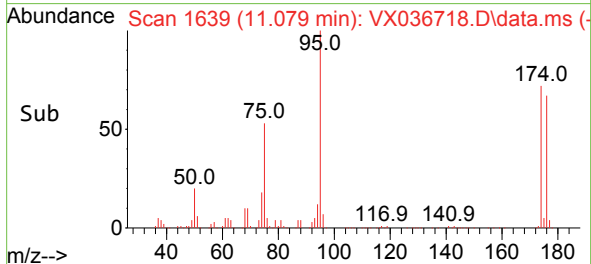

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion: 117 Resp: 242099
Ion Ratio Lower Upper
117 100
82 56.7 46.2 69.4
119 33.0 25.5 38.3

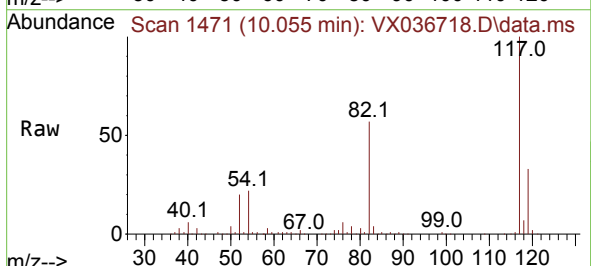



#67

Ethyl Benzene

Concen: 4.025 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. -0.000 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23

Instrument :

MSVOA_X

ClientSampleId :





1711

Tgt Ion: 91 Resp: 39243

Ion Ratio Lower Upper

91 100

106 31.6 24.9 37.3

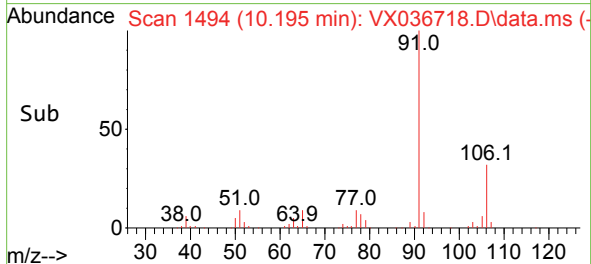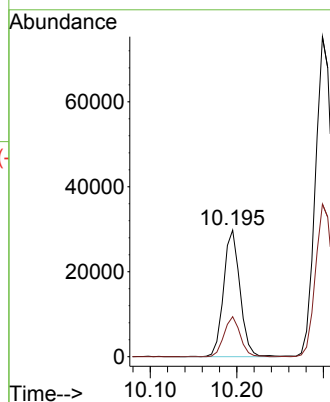

#68

m/p-Xylenes

Concen: 13.726 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX036718.D




Acq: 31 Jul 2023 14:23


Tgt Ion: 106 Resp: 49928

Ion Ratio Lower Upper

106 100

91 206.3 165.5 248.3




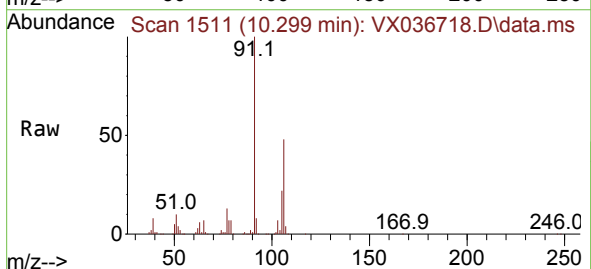




#69
o-Xylene
Concen: 4.661 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument : MSVOA_X
ClientSampleId : 1711


Tgt Ion:106 Resp: 16924
Ion Ratio Lower Upper
106 100
91 220.5 108.9 326.8

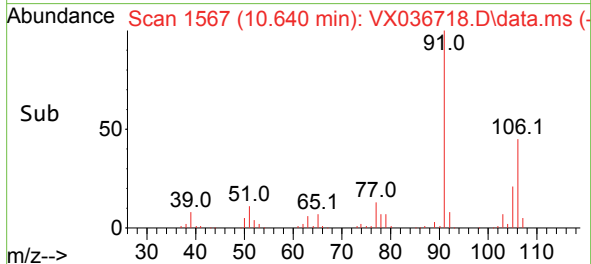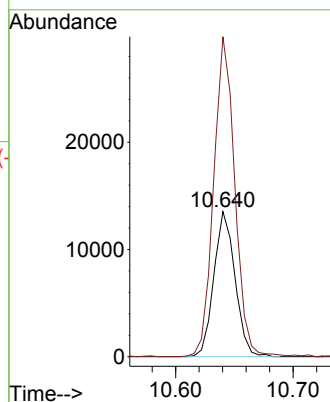

#70
Styrene
Concen: 0.314 ug/l
RT: 10.652 min Scan# 1569
Delta R.T. -0.000 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion:104 Resp: 1883
Ion Ratio Lower Upper
104 100
78 164.1 43.6 65.4#
103 154.0 43.6 65.4#









#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1711
 Delta R.T. -0.000 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23




Instrument :
 MSVOA_X
 ClientSampleId :
 1711


Tgt Ion:152 Resp: 111680
 Ion Ratio Lower Upper
 152 100
 115 61.6 43.3 129.9
 150 154.6 0.0 345.0

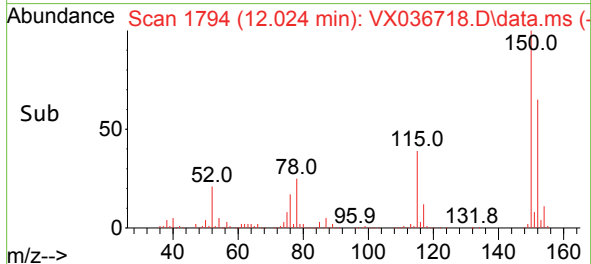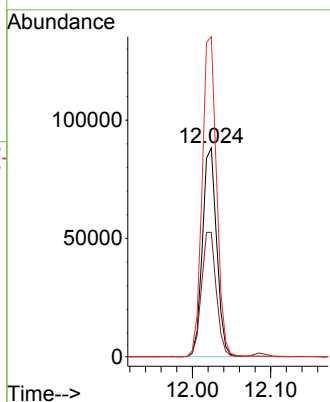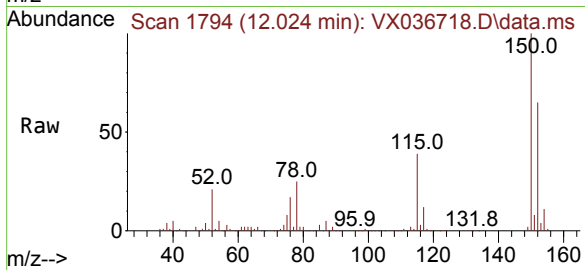

#76
 1,2,3-Trichloropropane
 Concen: 23.660 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23

Tgt Ion: 75 Resp: 62152
 Ion Ratio Lower Upper
 75 100
 77 1.1 19.1 57.5#




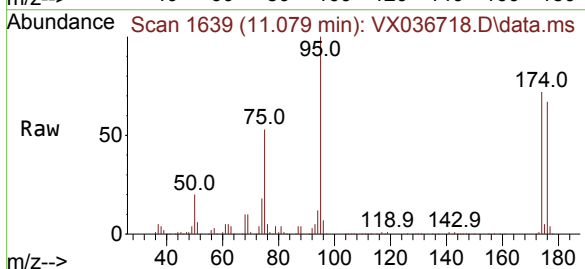


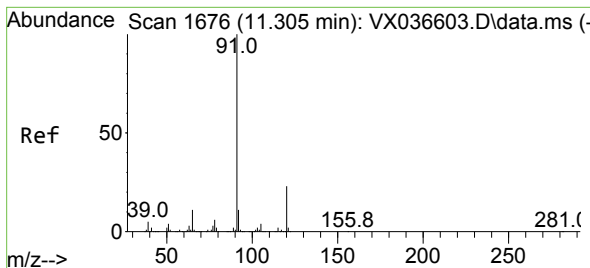

#78
n-propylbenzene
Concen: 0.242 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument :
MSVOA_X
ClientSampleId :
1711


Tgt Ion: 91 Resp: 2583
Ion Ratio Lower Upper
91 100
120 22.6 11.5 34.4

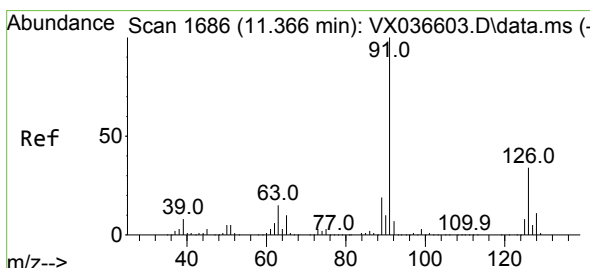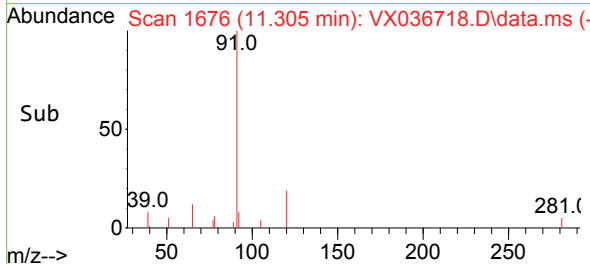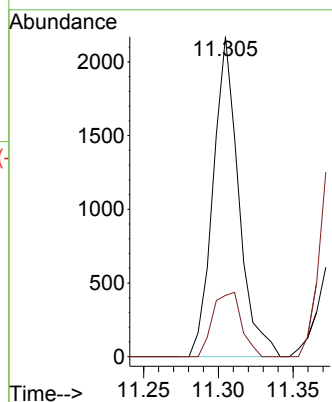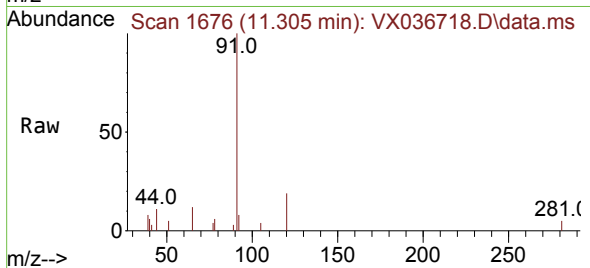

#79
2-Chlorotoluene
Concen: 0.233 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion: 91 Resp: 1509
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

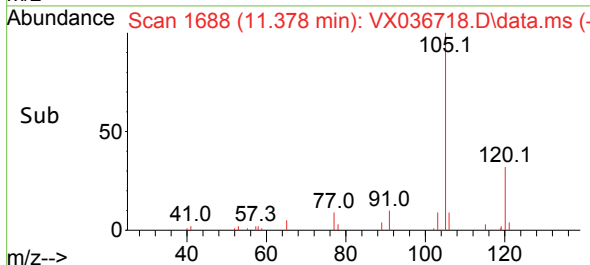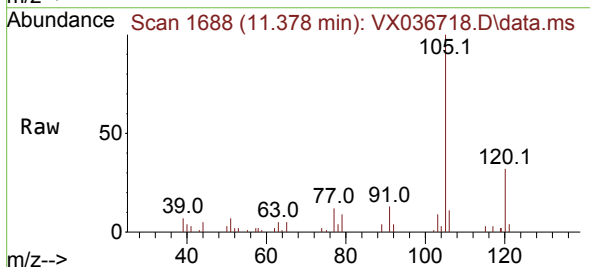



#80

1,3,5-Trimethylbenzene

Concen: 0.708 ug/l

RT: 11.451 min Scan# 1711

Delta R.T. -0.000 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23

Instrument :

MSVOA_X

ClientSampleId :





1711

Tgt Ion:105 Resp: 5475

Ion Ratio Lower Upper

105 100

120 46.3 24.1 72.3

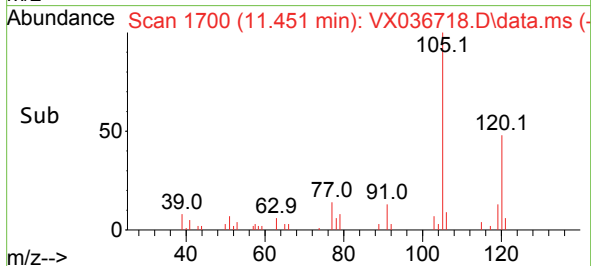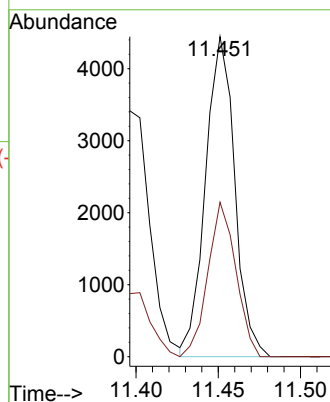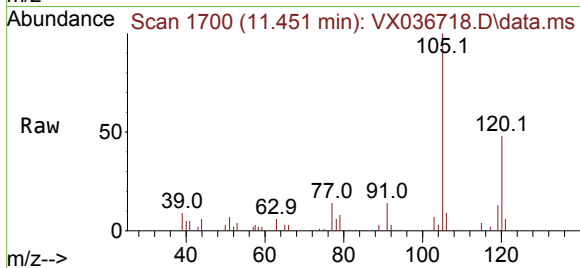

#81

trans-1,4-Dichloro-2-butene

Concen: 53.628 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23




Tgt Ion: 75 Resp: 62152


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#

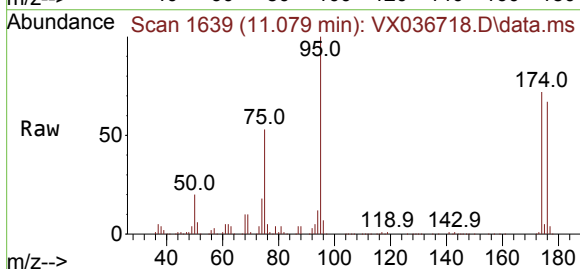



#83

tert-Butylbenzene

Concen: 0.202 ug/l

RT: 11.756 min Scan# 1711

Delta R.T. 0.043 min

Lab File: VX036718.D

Acq: 31 Jul 2023 14:23

Instrument :

MSVOA_X

ClientSampleId :

1711





Tgt Ion:119 Resp: 1531

Ion Ratio Lower Upper

119 100

91 101.2 31.2 93.6#

134 0.0 11.7 35.0#

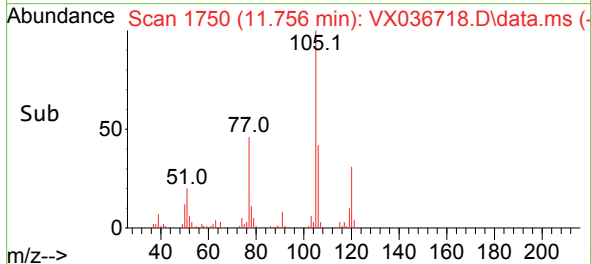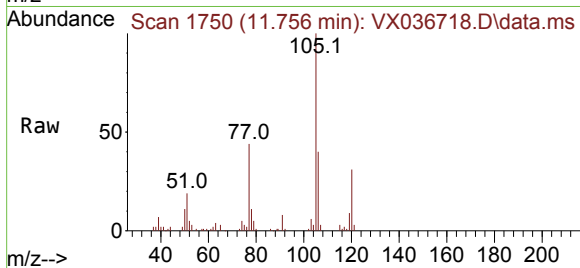

#84

1,2,4-Trimethylbenzene

Concen: 2.580 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX036718.D




Acq: 31 Jul 2023 14:23


Tgt Ion:105 Resp: 19950

Ion Ratio Lower Upper

105 100

120 28.8 21.2 63.6




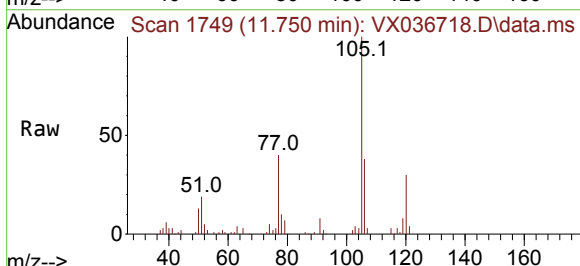




#85
 sec-Butylbenzene
 Concen: 0.260 ug/l
 RT: 11.890 min Scan# 1711
 Delta R.T. -0.000 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23




Instrument :
 MSVOA_X
 ClientSampleId :
 1711


Tgt Ion:105 Resp: 2461
 Ion Ratio Lower Upper
 105 100
 134 21.4 9.8 29.4

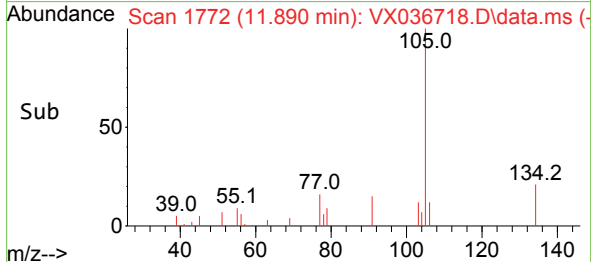

#86
 p-Isopropyltoluene
 Concen: 0.248 ug/l
 RT: 11.969 min Scan# 1785
 Delta R.T. -0.037 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23

Tgt Ion:119 Resp: 1936
 Ion Ratio Lower Upper
 119 100
 134 34.5 12.8 38.3
 91 27.5 13.1 39.3




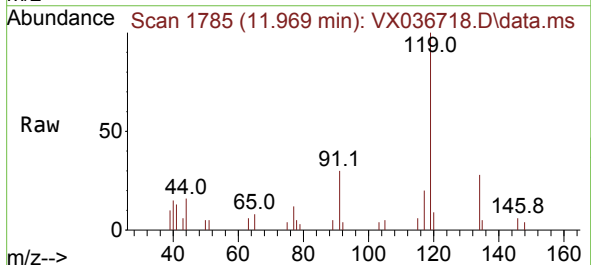


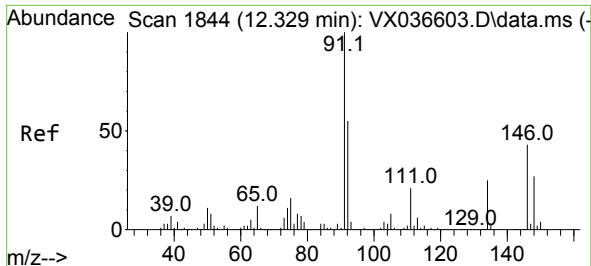

#89
n-Butylbenzene
Concen: 0.790 ug/l
RT: 12.323 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23




Instrument :
MSVOA_X
ClientSampleId :
1711


Tgt Ion: 91 Resp: 5513
Ion Ratio Lower Upper
91 100
92 23.4 27.4 82.0#
134 111.4 12.6 37.8#

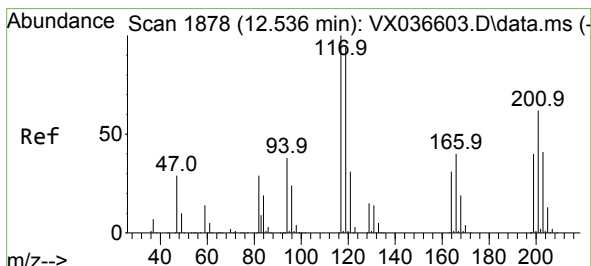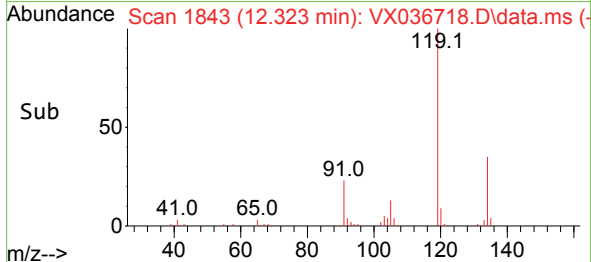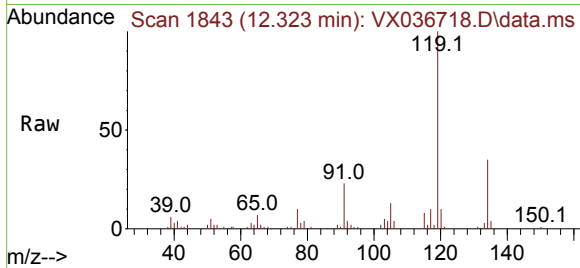

#90
Hexachloroethane
Concen: 0.840 ug/l
RT: 12.555 min Scan# 1881
Delta R.T. 0.018 min
Lab File: VX036718.D
Acq: 31 Jul 2023 14:23

Tgt Ion: 117 Resp: 1328
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

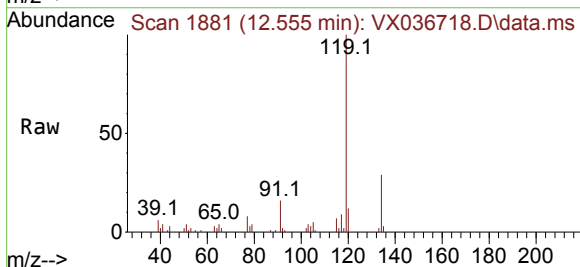




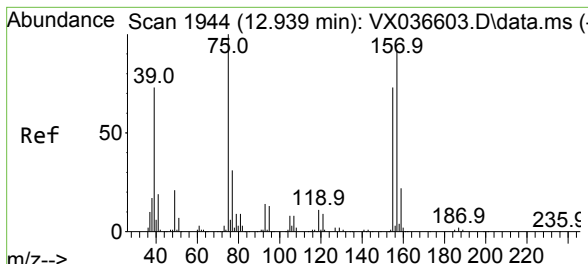


#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.320 ug/l
 RT: 12.920 min Scan# 1941
 Delta R.T. -0.018 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23

Instrument :
 MSVOA_X
 ClientSampleId :
 1711

Tgt Ion: 75 Resp: 232

Ion	Ratio	Lower	Upper
75	100		
155	0.0	36.1	108.5#
157	0.0	44.9	134.7#

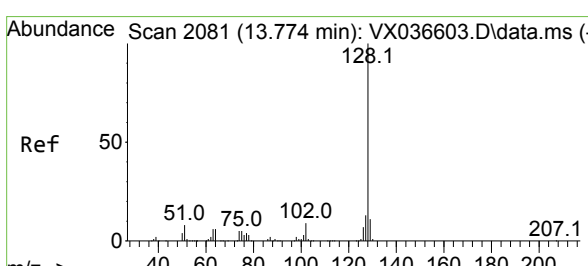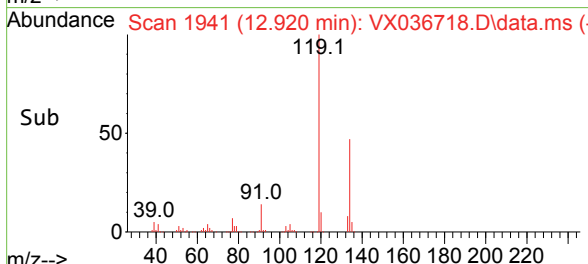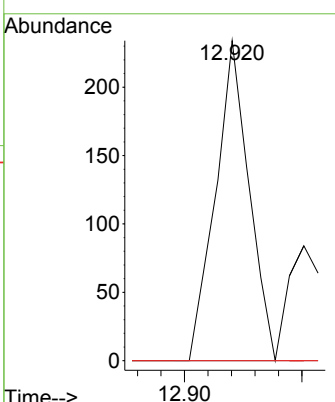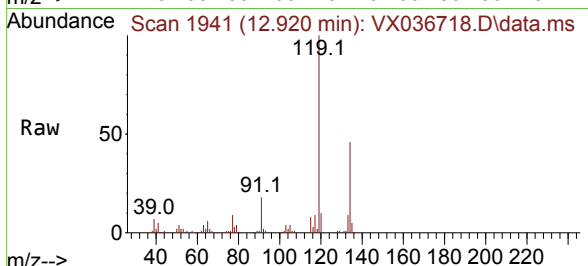

#95
 Naphthalene
 Concen: 1.220 ug/l
 RT: 13.774 min Scan# 2081
 Delta R.T. -0.000 min
 Lab File: VX036718.D
 Acq: 31 Jul 2023 14:23

Tgt Ion: 128 Resp: 9850

Ion	Ratio	Lower	Upper
128	100		
127	15.8	10.3	15.5#
129	23.2	8.8	13.2#

