

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073123\
 Data File : VX036733.D
 Acq On : 31 Jul 2023 20:23
 Operator : JC/MD
 Sample : 03850-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-073123

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	6	10	20	rBV	43862	67428	9.42%	1.724%
2	1.569	72	79	86	rBV8	3973	11419	1.60%	0.292%
3	2.532	230	237	247	rVB	3588	7529	1.05%	0.192%
4	5.099	646	658	669	rBV3	10520	31952	4.47%	0.817%
5	5.391	694	706	720	rBV2	81062	240601	33.62%	6.151%
6	5.556	722	733	748	rVB	134473	381075	53.25%	9.742%
7	5.958	789	799	813	rBV	87389	235341	32.89%	6.016%
8	6.763	921	931	945	rBV	221266	527386	73.70%	13.483%
9	8.647	1234	1240	1248	rBV	455897	715598	100.00%	18.294%
10	8.720	1248	1252	1261	rVB2	4031	7401	1.03%	0.189%
11	10.055	1465	1471	1485	rBV	468948	633418	88.52%	16.193%
12	10.799	1589	1593	1598	rBV	6317	8433	1.18%	0.216%
13	11.079	1634	1639	1651	rBV	372947	472462	66.02%	12.078%
14	12.018	1788	1793	1805	rBV	441137	571578	79.87%	14.612%




Sum of corrected areas: 3911621

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073123\
Data File : VX036733.D
Acq On : 31 Jul 2023 20:23
Operator : JC/MD
Sample : 03850-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-073123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

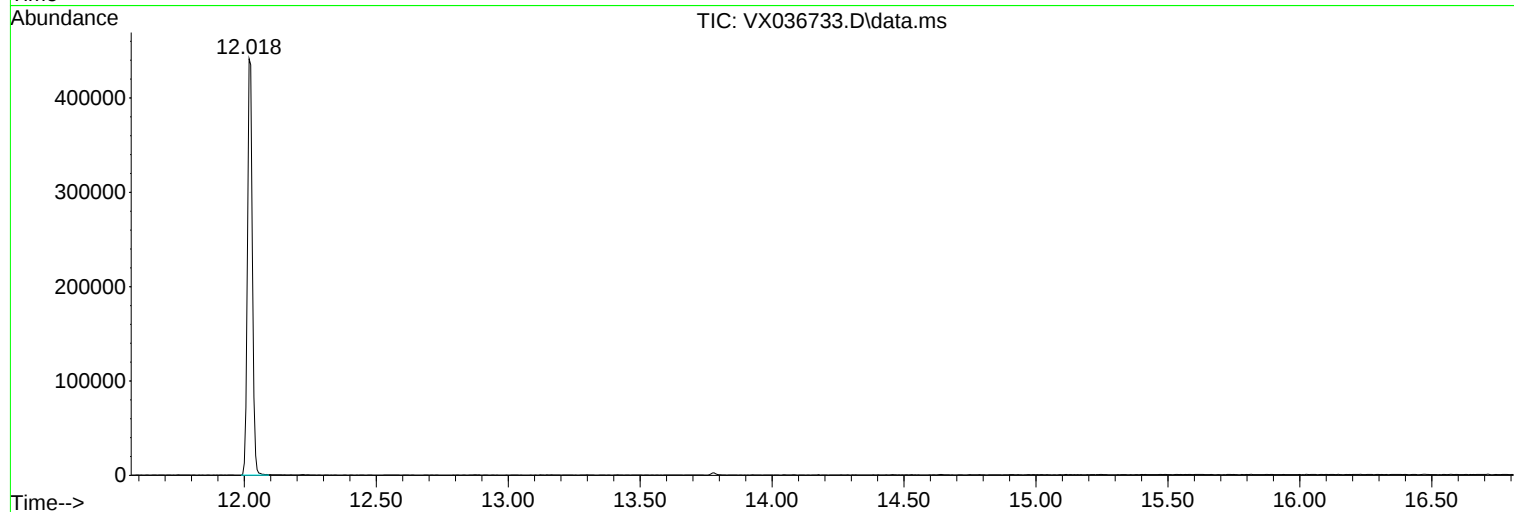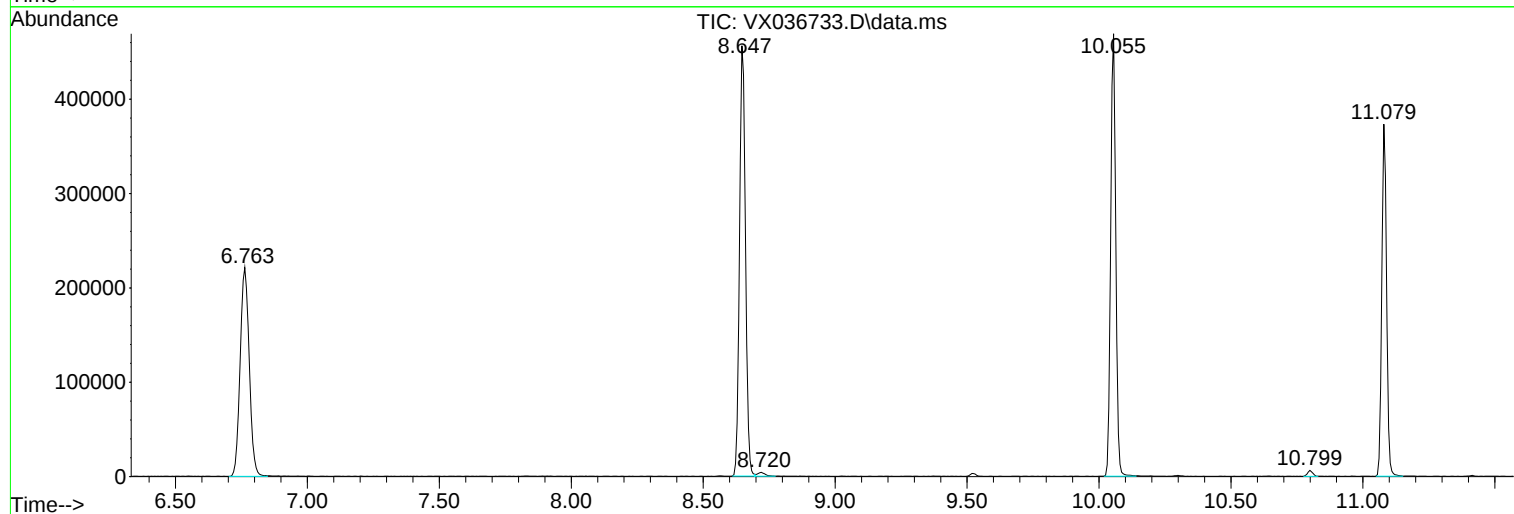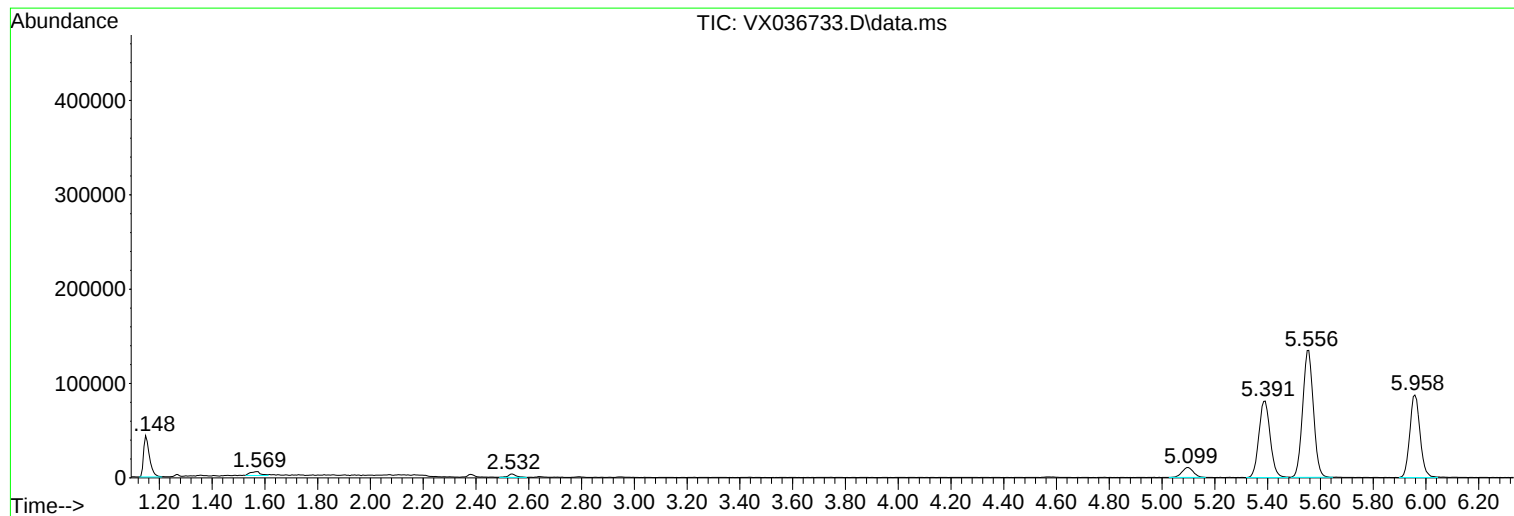

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073123\
Data File : VX036733.D
Acq On : 31 Jul 2023 20:23
Operator : JC/MD
Sample : 03850-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-073123










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethane, 1,1-difluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.148	8.85 ug/l	67428	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethane, 1,1-difluoro-	66	C2H4F2	000075-37-6	91
2			Propiolonitrile	51	C3HN	001070-71-9	3
3			Propane, 2,2-difluoro-	80	C3H6F2	000420-45-1	2
4			Difluoromethane	52	CH2F2	000075-10-5	1
5			2-Chloroethanol	80	C2H5ClO	000107-07-3	1

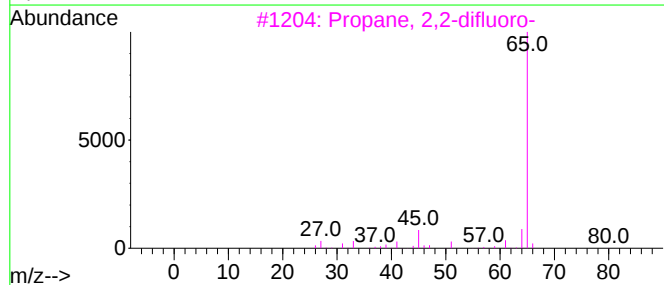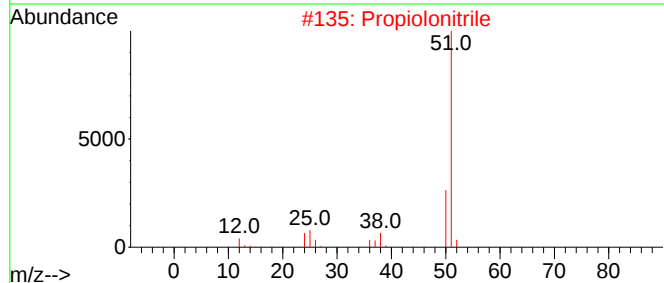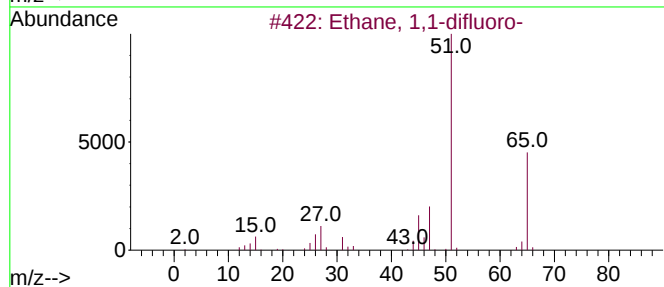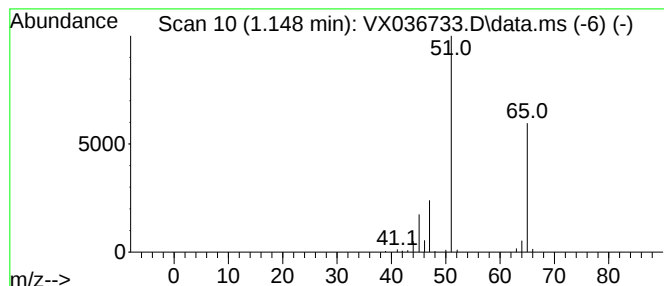

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073123\
Data File : VX036733.D
Acq On : 31 Jul 2023 20:23
Operator : JC/MD
Sample : 03850-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-073123

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethane, 1,1-dif...	1.148	8.8	ug/l	67428	1	5.550	381075	50.0