

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
 Data File : VX042780.D
 Acq On : 31 Jul 2024 17:57
 Operator : JC/MD
 Sample : P3398-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E08L0

Quant Time: Aug 01 02:19:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Aug 01 01:44:51 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	152132	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	128435	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	50538	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	32106	34.737	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.480%
7) Chloroethane-d5	1.648	69	18278	47.992	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.980%
11) 1,1-Dichloroethene-d2	2.294	65	22883	50.249	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	100.500%
21) 2-Butanone-d5	4.464	46	84428	123.249	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	123.250%
24) Chloroform-d	5.056	84	104645	51.727	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.460%
26) 1,2-Dichloroethane-d4	5.958	65	74282	56.914	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	113.820%
32) Benzene-d6	5.970	84	193874	54.390	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.780%
36) 1,2-Dichloropropane-d6	7.311	67	61390	58.192	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	116.380%
41) Toluene-d8	8.647	98	164865	51.586	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.180%
43) trans-1,3-Dichloroprop...	8.951	79	24149	48.916	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.840%
47) 2-Hexanone-d5	9.384	63	54663	115.893	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	115.890%
56) 1,1,2,2-Tetrachloroeth...	11.195	84	85333	56.179	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	112.360%
66) 1,2-Dichlorobenzene-d4	12.323	152	48873	51.170	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.340%
Target Compounds						
13) Acetone	2.392	43	1463	2.732	ug/L	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
Data File : VX042780.D
Acq On : 31 Jul 2024 17:57
Operator : JC/MD
Sample : P3398-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E08L0

Quant Time: Aug 01 02:19:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Aug 01 01:44:51 2024
Response via : Initial Calibration

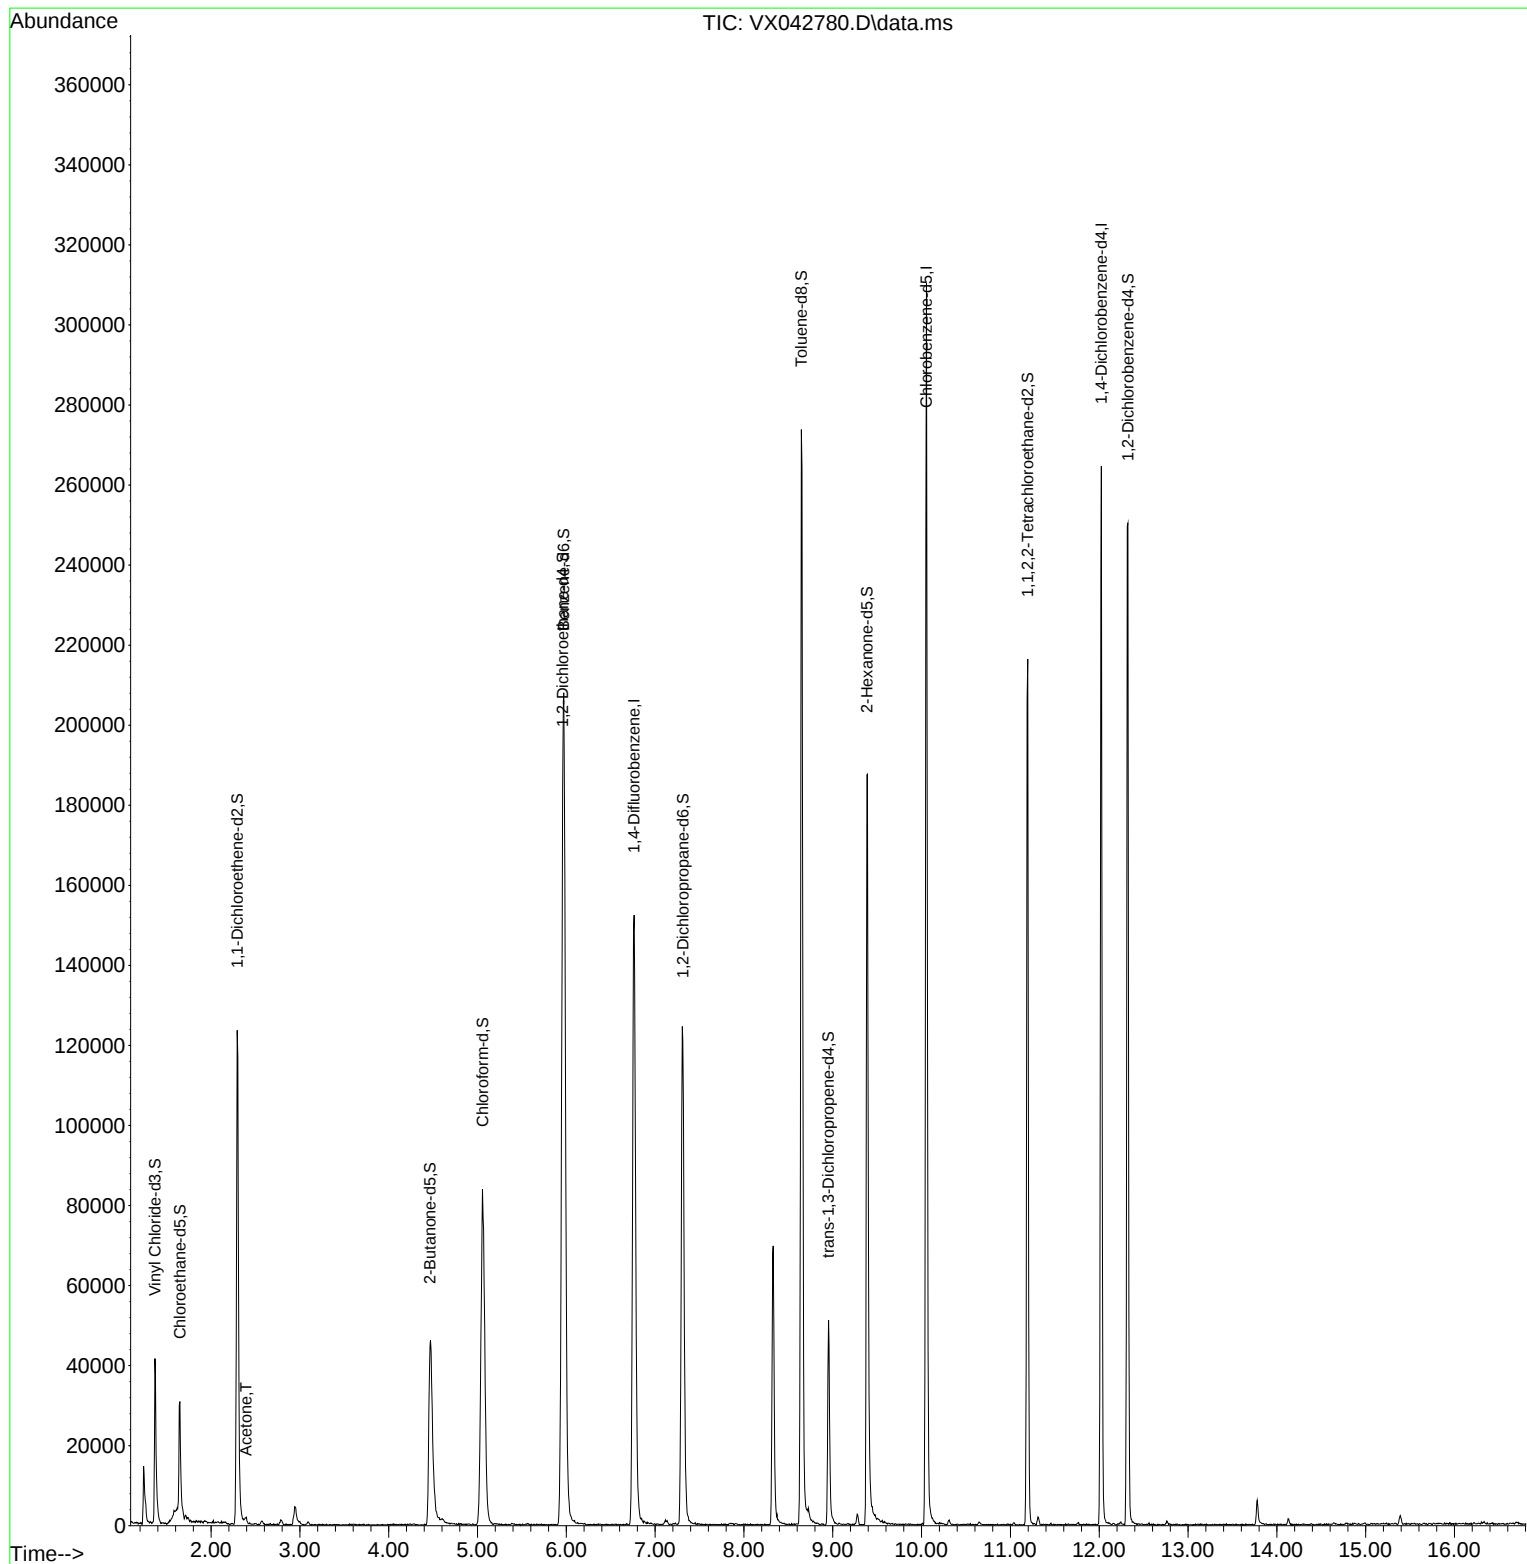

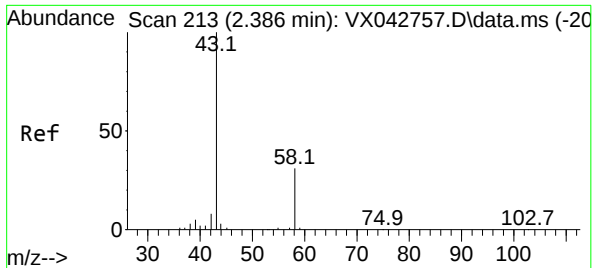

#13
 Acetone
 Concen: 2.732 ug/L
 RT: 2.392 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX042780.D
 Acq: 31 Jul 2024 17:57

Instrument :
 MSVOA_X
 ClientSampleId :
 E08L0

Tgt Ion: 43 Resp: 1463
 Ion Ratio Lower Upper
 43 100
 58 5.9 0.0 62.4

