

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
 Data File : VX042759.D
 Acq On : 31 Jul 2024 09:38
 Operator : JC/MD
 Sample : VX0731WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK712

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

Signal : TIC: VX042759.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	54	rBV	35773	41272	9.96%	1.293%
2	1.660	90	94	107	rVB	22151	34059	8.22%	1.067%
3	2.050	154	158	160	rBV	147	248	0.06%	0.008%
4	2.239	185	189	193	rBV	162	332	0.08%	0.010%
5	2.306	193	200	210	rVB	93867	145962	35.21%	4.573%
6	2.386	210	213	217	rVB2	370	617	0.15%	0.019%
7	2.465	223	226	227	rBV	178	136	0.03%	0.004%
8	2.508	231	233	234	rBV	290	212	0.05%	0.007%
9	2.727	268	269	272	rBB	198	131	0.03%	0.004%
10	2.782	275	278	284	rBV2	760	1086	0.26%	0.034%
11	2.940	301	304	307	rBV	337	319	0.08%	0.010%
12	3.093	326	329	333	rBV2	375	703	0.17%	0.022%
13	3.599	410	412	413	rBV	230	164	0.04%	0.005%
14	3.629	416	417	419	rBB	249	134	0.03%	0.004%
15	4.458	545	553	573	rBV	26817	77282	18.64%	2.421%
16	4.708	593	594	599	rBB	143	135	0.03%	0.004%
17	5.056	640	651	671	rBV	60737	177809	42.90%	5.571%
18	5.385	703	705	711	rVB2	292	403	0.10%	0.013%
19	5.446	714	715	717	rBB2	198	134	0.03%	0.004%
20	5.477	717	720	721	rBV2	210	187	0.05%	0.006%
21	5.544	729	731	732	rBV2	186	172	0.04%	0.005%
22	5.666	749	751	755	rBV2	185	282	0.07%	0.009%
23	5.970	788	801	817	rBV2	138503	414507	100.00%	12.986%
24	6.318	857	858	861	rBV2	158	161	0.04%	0.005%
25	6.367	863	866	869	rBB	146	165	0.04%	0.005%
26	6.446	876	879	881	rBV	175	165	0.04%	0.005%
27	6.757	922	930	947	rBV	119077	287871	69.45%	9.019%
28	7.117	982	989	996	rBB5	1551	3273	0.79%	0.103%
29	7.306	1009	1020	1038	rBV	80389	183149	44.18%	5.738%
30	7.458	1043	1045	1046	rVB	273	182	0.04%	0.006%
31	7.519	1053	1055	1057	rBV	175	140	0.03%	0.004%
32	7.836	1103	1107	1108	rBB	128	168	0.04%	0.005%
33	7.952	1125	1126	1128	rBV	167	137	0.03%	0.004%
34	8.196	1163	1166	1168	rBB	137	134	0.03%	0.004%
35	8.324	1181	1187	1201	rBV	54889	89550	21.60%	2.806%
36	8.574	1226	1228	1229	rBV	353	245	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
 Data File : VX042759.D
 Acq On : 31 Jul 2024 09:38
 Operator : JC/MD
 Sample : VX0731WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK712

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

37	8.647	1233	1240	1249	rBV	216375	335411	80.92%	10.508%
38	8.952	1285	1290	1303	rBV	40518	60826	14.67%	1.906%
39	9.153	1321	1323	1326	rVB	272	245	0.06%	0.008%
40	9.208	1331	1332	1337	rVB	206	177	0.04%	0.006%
41	9.281	1341	1344	1347	rBB	769	808	0.19%	0.025%
42	9.384	1356	1361	1379	rBV	114909	172623	41.65%	5.408%
43	9.610	1397	1398	1401	rBV2	399	316	0.08%	0.010%
44	9.970	1454	1457	1459	rBB2	219	155	0.04%	0.005%
45	10.055	1465	1471	1488	rBV	241909	340213	82.08%	10.659%
46	10.305	1509	1512	1518	rBB	666	943	0.23%	0.030%
47	10.372	1521	1523	1526	rBB	133	151	0.04%	0.005%
48	10.646	1564	1568	1574	rBV2	914	1650	0.40%	0.052%
49	10.805	1591	1594	1597	rBV	192	234	0.06%	0.007%
50	10.896	1606	1609	1611	rBB	112	146	0.04%	0.005%
51	10.963	1617	1620	1624	rBV	653	725	0.17%	0.023%
52	11.189	1652	1657	1666	rBV	159522	207458	50.05%	6.499%
53	11.293	1671	1674	1677	rBB	241	228	0.06%	0.007%
54	11.457	1696	1701	1704	rBV	709	975	0.24%	0.031%
55	11.506	1707	1709	1710	rBB	204	144	0.03%	0.005%
56	11.762	1747	1751	1754	rBB	584	736	0.18%	0.023%
57	11.969	1783	1785	1788	rBV2	683	844	0.20%	0.026%
58	12.024	1788	1794	1806	rVV	224419	299793	72.33%	9.392%
59	12.317	1837	1842	1849	rBV	229501	289599	69.87%	9.073%
60	12.494	1869	1871	1876	rBB	145	243	0.06%	0.008%
61	12.768	1911	1916	1918	rBB	242	324	0.08%	0.010%
62	12.902	1935	1938	1943	rBB	156	210	0.05%	0.007%
63	13.006	1952	1955	1961	rBB	175	366	0.09%	0.011%
64	13.085	1967	1968	1971	rBV	149	144	0.03%	0.005%
65	13.122	1971	1974	1977	rVB	891	820	0.20%	0.026%
66	13.250	1994	1995	1999	rBB	106	136	0.03%	0.004%
67	13.304	2002	2004	2008	rBB	225	236	0.06%	0.007%
68	13.591	2049	2051	2055	rBV	477	569	0.14%	0.018%
69	13.682	2063	2066	2068	rBV	157	201	0.05%	0.006%
70	13.743	2072	2076	2078	rBB	146	140	0.03%	0.004%
71	13.786	2079	2083	2087	rBV	695	1094	0.26%	0.034%
72	13.877	2097	2098	2101	rBV	146	130	0.03%	0.004%
73	13.963	2109	2112	2115	rBV3	621	796	0.19%	0.025%
74	14.127	2136	2139	2144	rBB2	1888	2291	0.55%	0.072%
75	14.353	2173	2176	2181	rBV	153	255	0.06%	0.008%
76	14.603	2214	2217	2220	rBB	203	241	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
 Data File : VX042759.D
 Acq On : 31 Jul 2024 09:38
 Operator : JC/MD
 Sample : VX0731WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK712

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
 Title : VOC Analysis

77	14.664	2224	2227	2229	rBV	241	202	0.05%	0.006%
78	14.810	2250	2251	2253	rVV	231	145	0.03%	0.005%
79	14.847	2256	2257	2259	rVB	236	130	0.03%	0.004%
80	14.877	2260	2262	2263	rBV	214	146	0.04%	0.005%
81	14.981	2277	2279	2281	rBV	213	230	0.06%	0.007%
82	15.078	2292	2295	2299	rVB2	202	266	0.06%	0.008%
83	15.109	2299	2300	2302	rBV	261	153	0.04%	0.005%
84	15.146	2304	2306	2309	rBV	327	416	0.10%	0.013%
85	15.200	2313	2315	2318	rBV	213	296	0.07%	0.009%
86	15.267	2323	2326	2328	rBV	193	175	0.04%	0.005%
87	15.286	2328	2329	2332	rBV	261	305	0.07%	0.010%
88	15.389	2343	2346	2350	rBV	1216	1522	0.37%	0.048%
89	15.487	2360	2362	2364	rBV2	454	351	0.08%	0.011%
90	15.530	2367	2369	2372	rBV	448	435	0.10%	0.014%
91	15.639	2383	2387	2388	rBV	211	240	0.06%	0.008%
92	15.737	2400	2403	2404	rBV	352	289	0.07%	0.009%
93	15.786	2408	2411	2413	rBB	226	186	0.04%	0.006%
94	15.804	2413	2414	2419	rBV3	207	364	0.09%	0.011%
95	16.042	2450	2453	2456	rBV	183	200	0.05%	0.006%
96	16.078	2456	2459	2462	rVB	374	422	0.10%	0.013%
97	16.298	2494	2495	2497	rBB	289	200	0.05%	0.006%
98	16.328	2497	2500	2501	rBV	252	212	0.05%	0.007%
99	16.426	2515	2516	2518	rBV	277	218	0.05%	0.007%
100	16.609	2543	2546	2550	rBV	426	601	0.14%	0.019%




Sum of corrected areas: 3191926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
Data File : VX042759.D
Acq On : 31 Jul 2024 09:38
Operator : JC/MD
Sample : VX0731WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK712

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

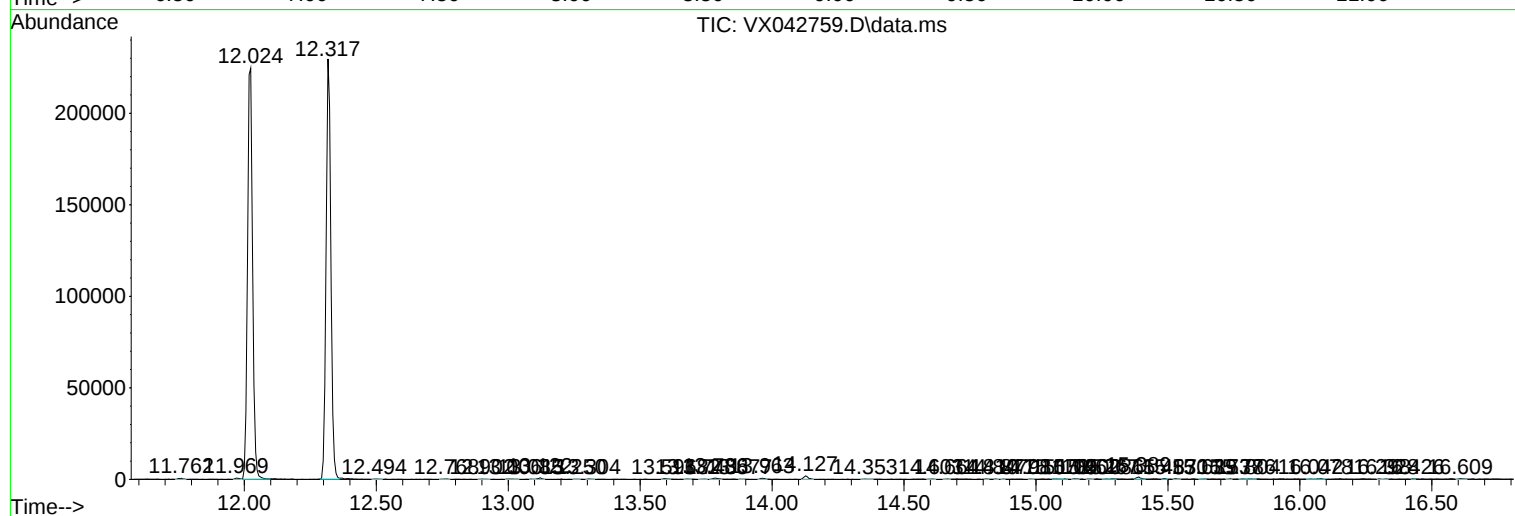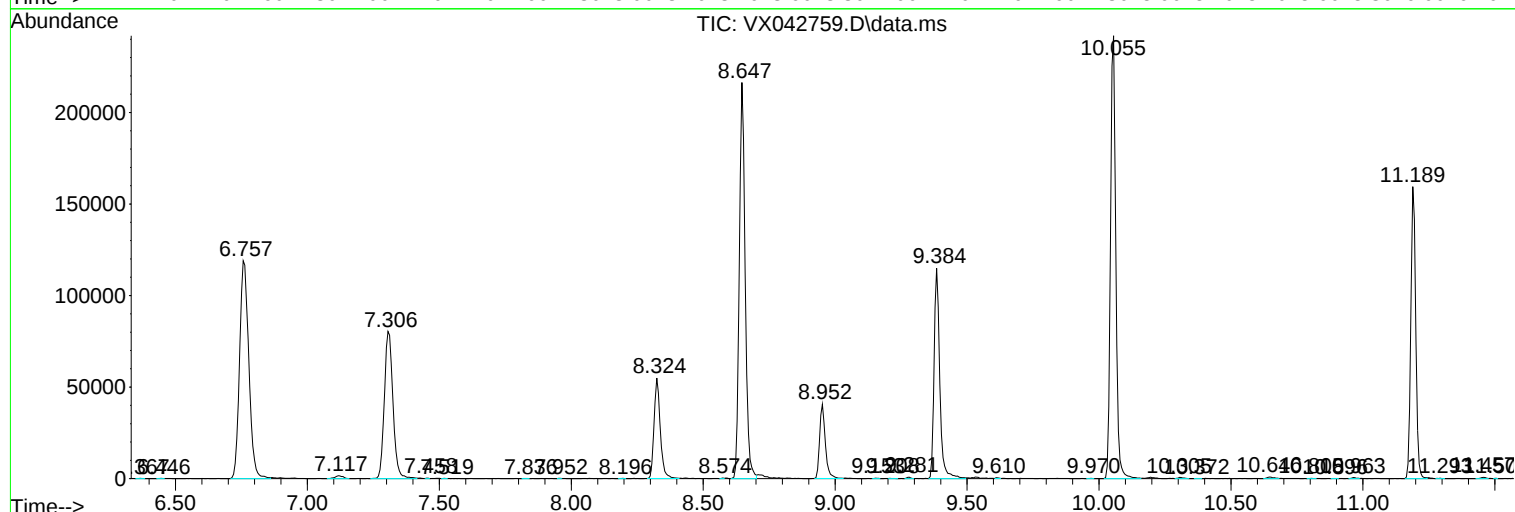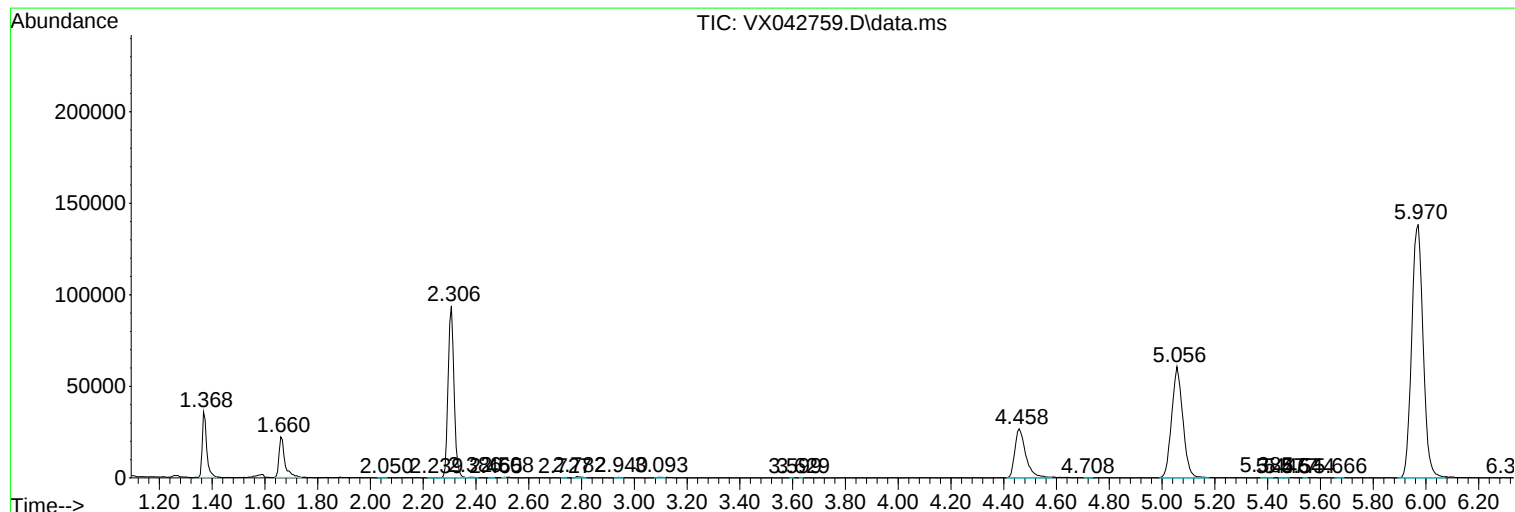

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
Data File : VX042759.D
Acq On : 31 Jul 2024 09:38
Operator : JC/MD
Sample : VX0731WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK712

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXMLM072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
Data File : VX042759.D
Acq On : 31 Jul 2024 09:38
Operator : JC/MD
Sample : VX0731WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK712

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML072624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc