
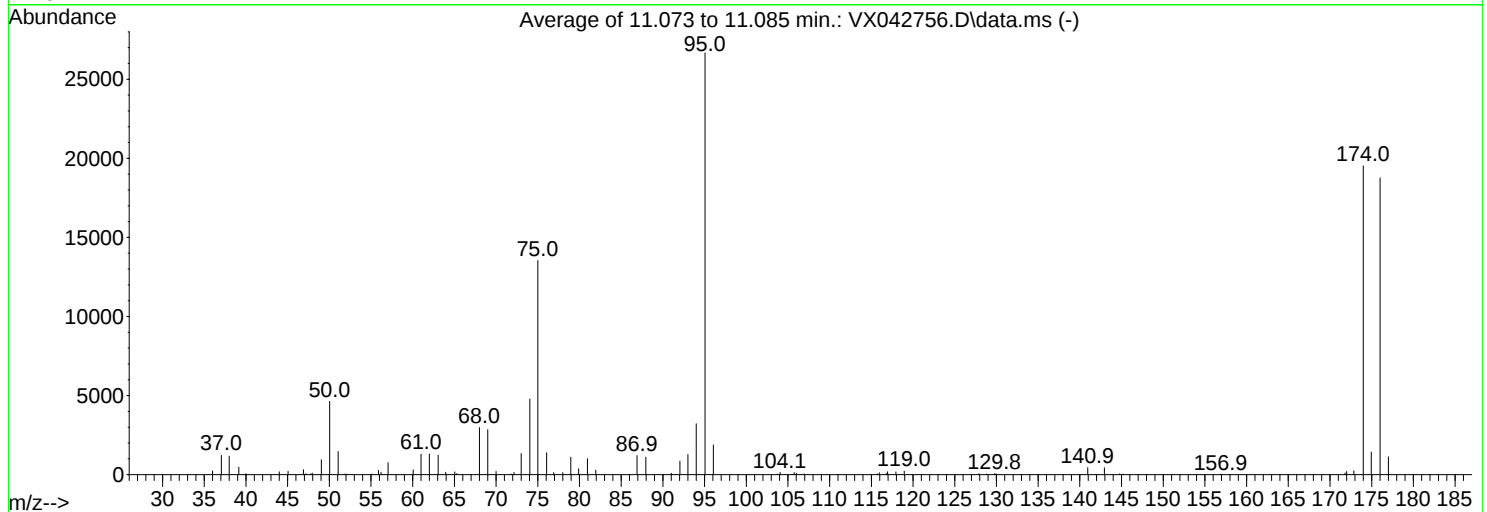


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX073124\
Data File : VX042756.D
Acq On : 31 Jul 2024 08:06
Operator : JC/MD
Sample : BFB689
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB689

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM072624WMA.M
Title : VOC Analysis
Last Update : Thu Aug 01 01:44:51 2024

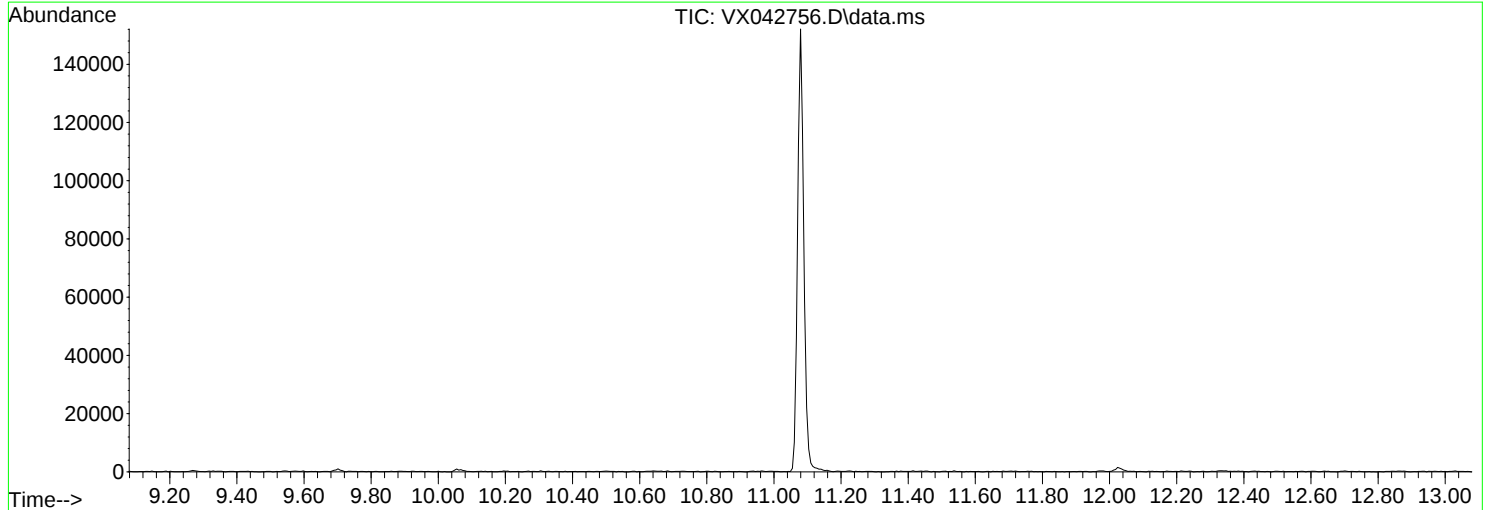

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	4632	PASS
75	95	30	80	50.8	13538	PASS
95	95	100	100	100.0	26672	PASS
96	95	5	9	7.1	1882	PASS
173	174	0.00	2	1.2	243	PASS
174	95	50	120	73.2	19526	PASS
175	174	5	9	7.3	1429	PASS
176	174	95	101	96.1	18768	PASS
177	176	5	9	6.0	1126	PASS

m/z	Abundance
40.10	77.0
44.20	69.0

Instrument :
MSVOA_X
ClientSampleId :
BFB689

m/z	Abundance
36.10	324.0
37.10	1333.0
38.00	1374.0
39.20	544.0
40.00	137.0
44.00	310.0
45.10	197.0
47.00	378.0
47.80	157.0
49.00	869.0
50.00	4482.0
51.00	1243.0
51.90	56.0
52.20	73.0
55.10	107.0
55.90	416.0
57.10	646.0
60.10	239.0
61.00	1079.0
62.00	1143.0
63.00	1152.0
63.90	126.0
65.10	343.0
68.00	2630.0
69.00	2804.0
70.00	185.0
72.20	104.0
73.10	1228.0
74.10	4948.0
75.00	13327.0
76.10	1569.0
76.80	94.0
78.00	115.0
78.90	994.0
79.90	288.0
81.00	950.0
82.00	246.0
86.80	1112.0
87.90	1171.0
91.00	141.0
92.00	735.0
93.00	1019.0
94.00	3051.0
95.00	24112.0
96.00	1679.0
103.70	112.0
104.10	133.0
105.70	160.0
107.00	79.0
116.00	177.0
116.80	200.0
117.90	131.0
119.00	175.0
127.90	71.0
128.80	66.0
129.80	70.0
141.00	375.0
141.90	54.0
142.90	338.0
145.20	79.0
171.80	292.0
172.90	215.0
174.00	14667.0
175.00	1245.0
176.00	14152.0
177.00	1000.0

Instrument :
MSVOA_X
ClientSampleId :
BFB689

m/z	Abundance
35.90	217.0
37.10	1426.0
38.00	1355.0
39.10	621.0
40.00	123.0
44.00	249.0
45.00	302.0
46.80	285.0
47.20	171.0
48.00	172.0
49.00	1048.0
50.00	5694.0
51.00	1889.0
51.90	83.0
55.90	395.0
57.10	852.0
60.00	305.0
61.00	1486.0
62.00	1991.0
63.10	1362.0
64.00	149.0
65.30	200.0
68.00	3469.0
69.00	3272.0
69.90	310.0
71.80	122.0
72.20	158.0
73.00	1556.0
74.00	5485.0
75.00	15309.0
76.00	1498.0
76.90	164.0
78.00	93.0
79.00	1453.0
79.90	550.0
80.90	1213.0
81.90	338.0
86.90	1441.0
88.00	1250.0
91.00	137.0
92.10	1144.0
93.00	1455.0
94.00	4098.0
95.10	31272.0
96.10	2593.0
104.00	184.0
106.00	271.0
106.90	60.0
115.90	174.0
117.00	254.0
118.00	172.0
119.00	344.0
127.90	128.0
128.80	67.0
130.00	126.0
141.00	429.0
142.90	450.0
144.80	68.0
172.00	339.0
172.80	287.0
174.00	23376.0
175.00	1891.0
176.00	23448.0
177.00	1287.0

Instrument :
MSVOA_X
ClientSampleId :
BFB689

m/z	Abundance
36.10	162.0
37.00	925.0
38.10	771.0
39.10	233.0
40.00	138.0
44.20	191.0
45.10	126.0
46.90	289.0
47.90	143.0
49.10	912.0
50.10	3720.0
51.10	1285.0
56.20	432.0
57.00	778.0
60.00	366.0
61.00	1315.0
62.10	780.0
63.00	1202.0
64.00	183.0
64.90	171.0
68.00	2834.0
69.00	2469.0
70.10	126.0
72.00	154.0
72.90	1225.0
74.00	3888.0
75.00	11977.0
76.10	1094.0
77.00	150.0
78.00	201.0
78.90	858.0
79.90	274.0
80.90	875.0
81.90	274.0
87.00	1064.0
88.00	881.0
92.00	704.0
93.00	1341.0
94.00	2510.0
95.10	24632.0
96.10	1373.0
104.00	104.0
105.80	222.0
115.70	155.0
116.90	303.0
117.90	217.0
118.80	153.0
129.80	132.0
140.90	532.0
143.00	513.0
144.70	97.0
156.90	60.0
172.00	270.0
172.80	226.0
174.00	20536.0
174.90	1152.0
176.00	18704.0
177.00	1090.0

Instrument :
MSVOA_X
ClientSampleId :
BFB689