


Instrument :
MSVOA_X
ClientSampleId :

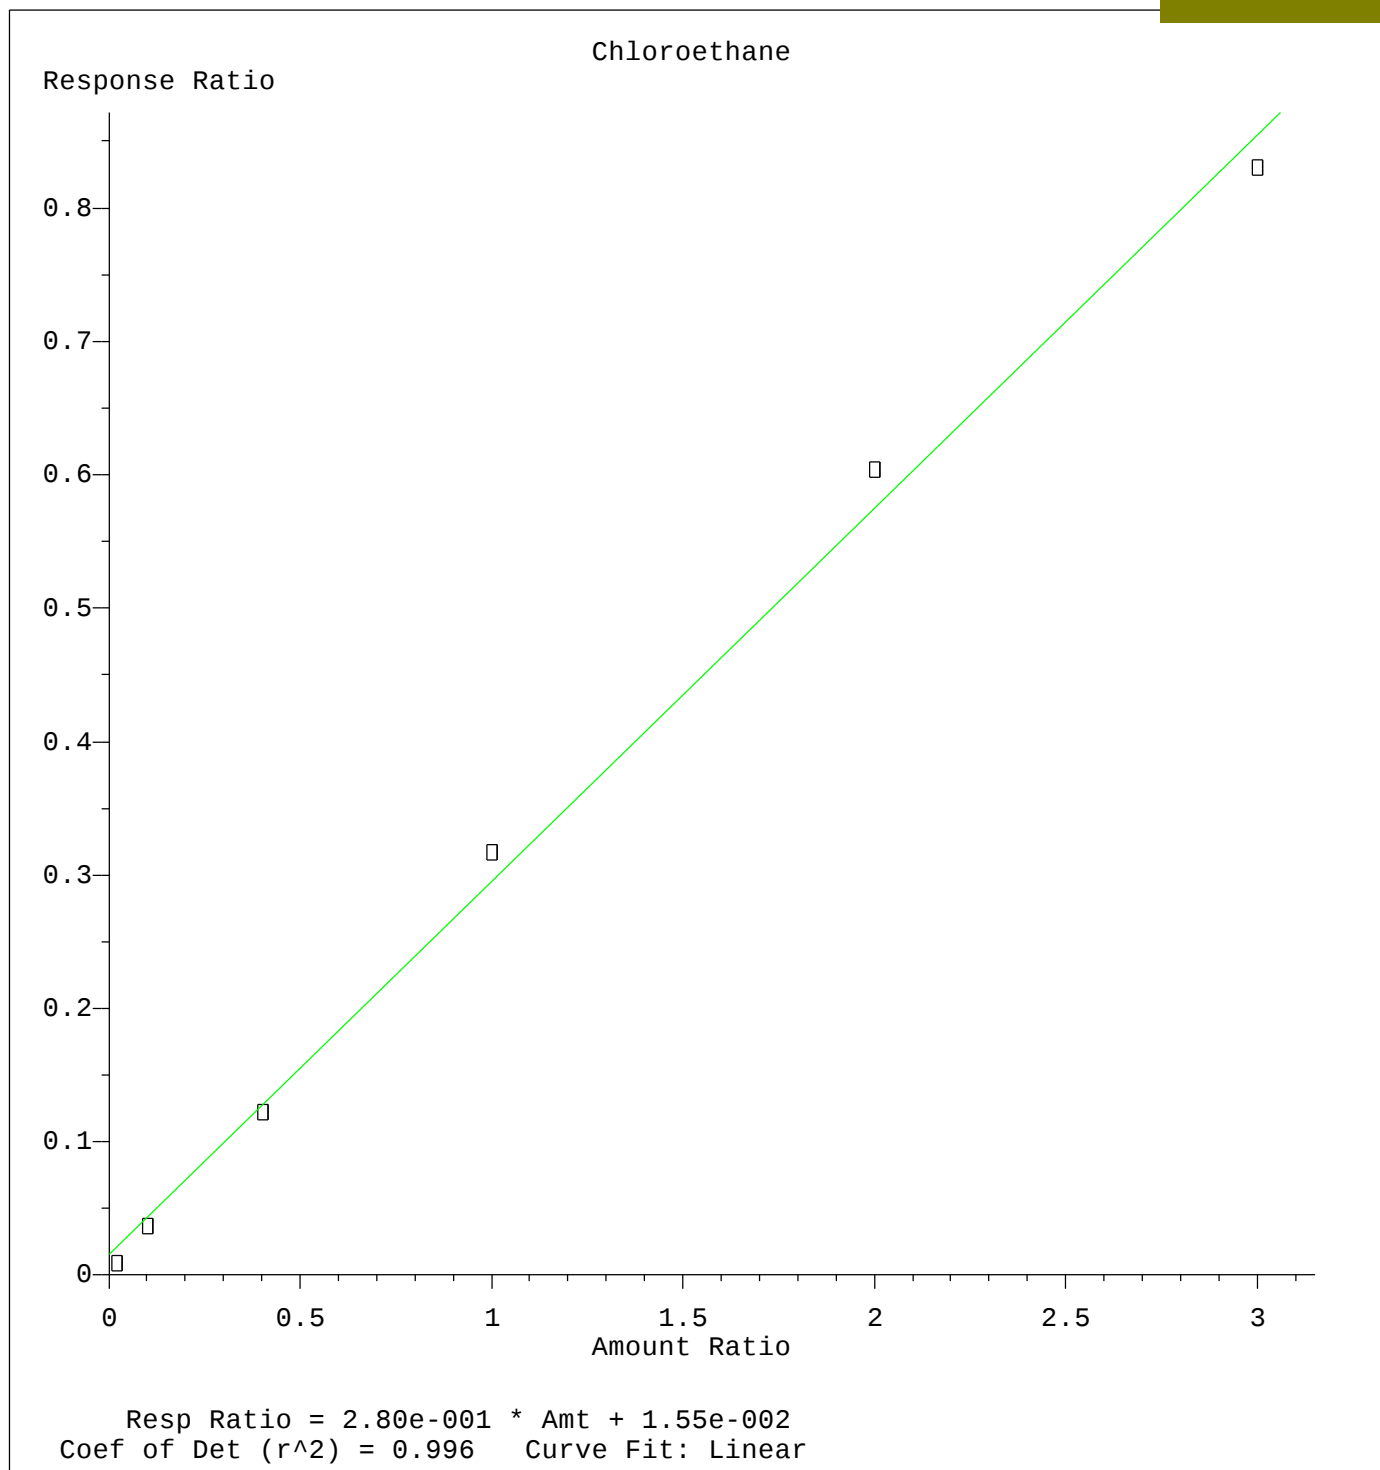


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Calibration Table Last Updated: Fri Aug 02 01:55:00 2019

Instrument :
MSVOA_X
ClientSampleId :

Tert butyl alcohol

Response Ratio

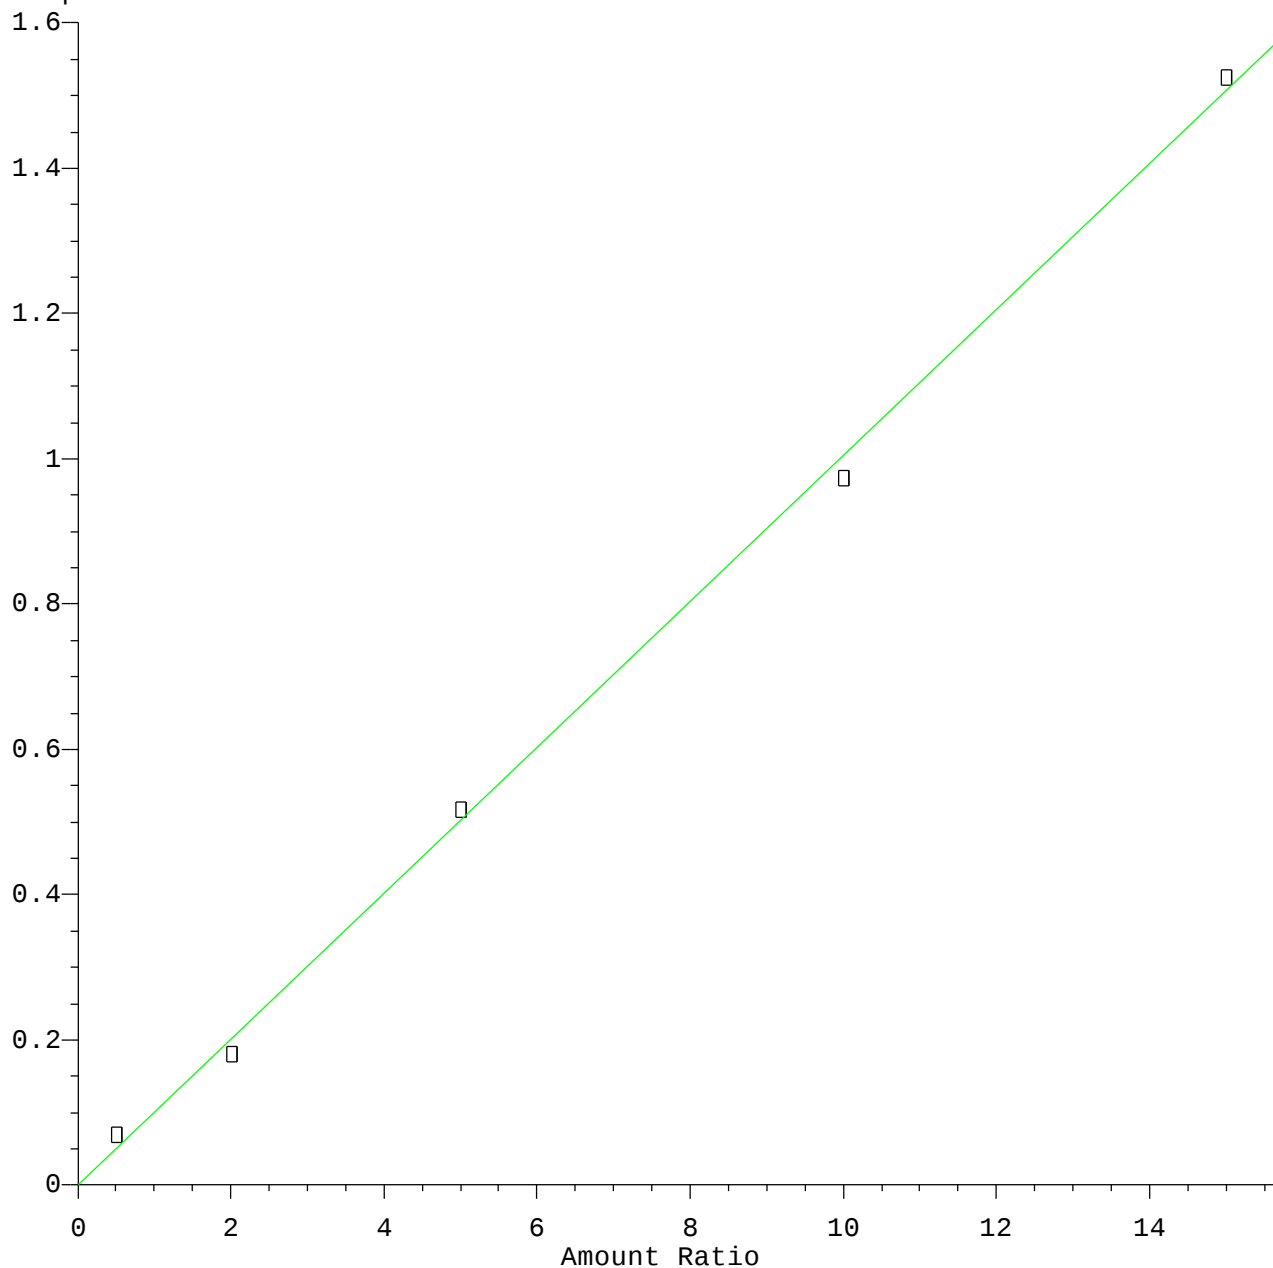


Resp Ratio = $1.00e-001 * \text{Amt} - 4.58e-005$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Calibration Table Last Updated: Fri Aug 02 01:55:00 2019

Instrument :
MSVOA_X
ClientSampleId :

Acrolein

Response Ratio

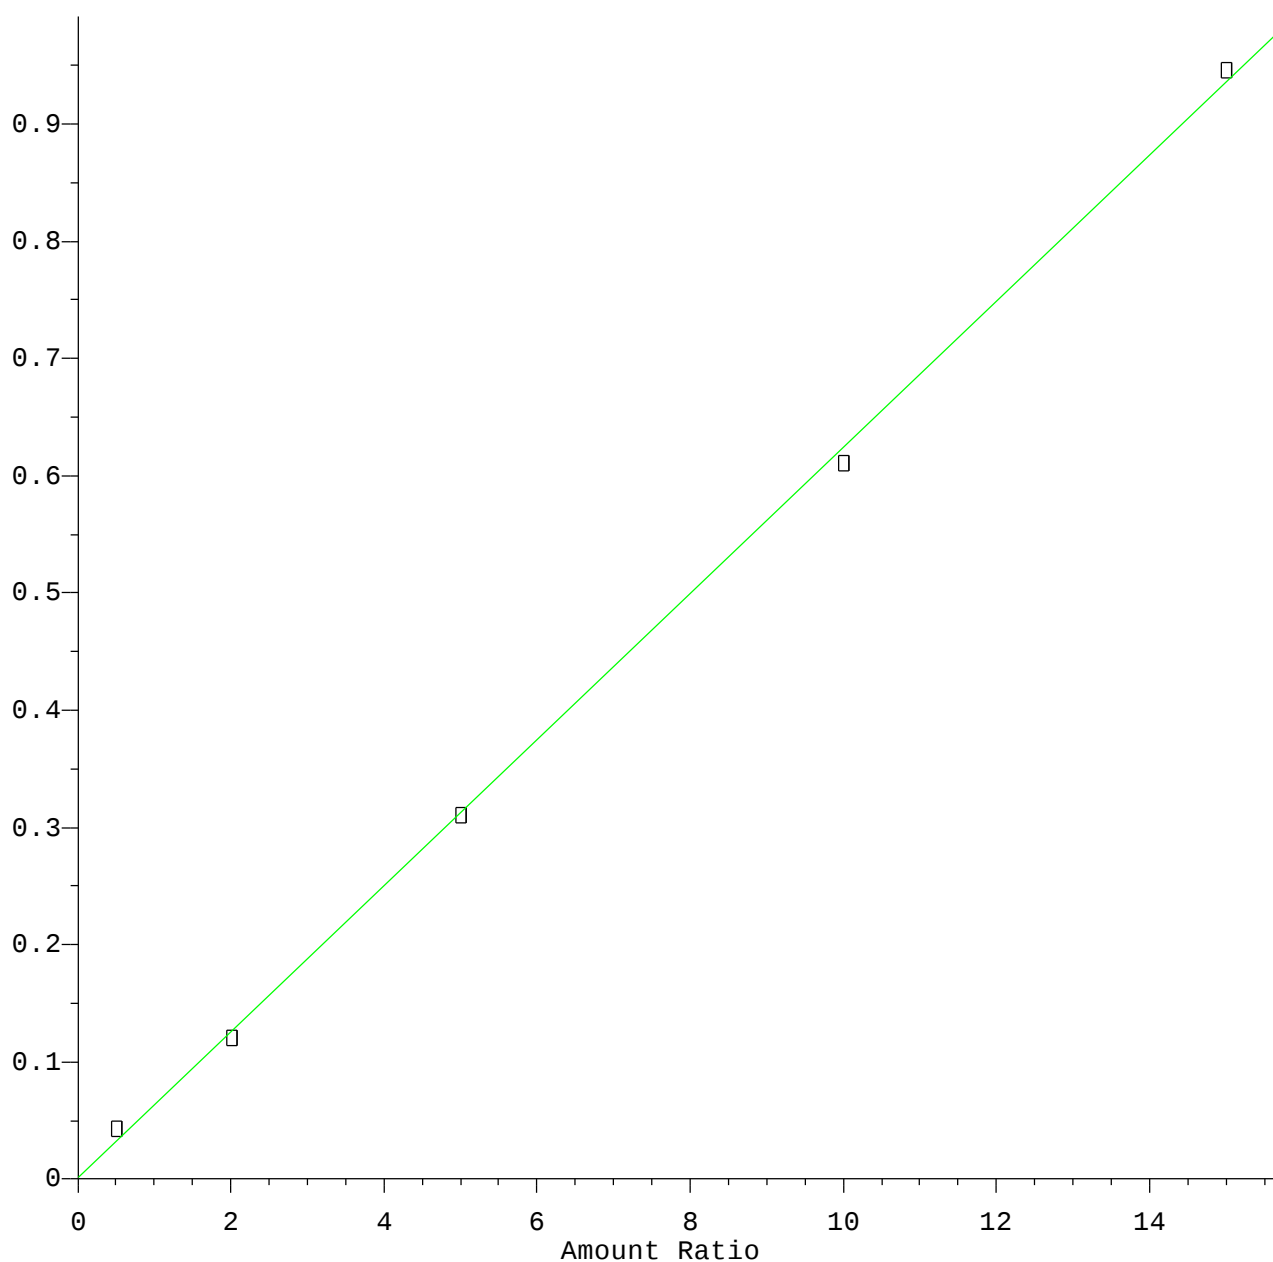


Resp Ratio = $6.23 \times 10^{-2} \times \text{Amt} + 5.27 \times 10^{-4}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Calibration Table Last Updated: Fri Aug 02 01:55:00 2019

Instrument :
MSVOA_X
ClientSampleId :

t-1,3-Dichloropropene


Response Ratio

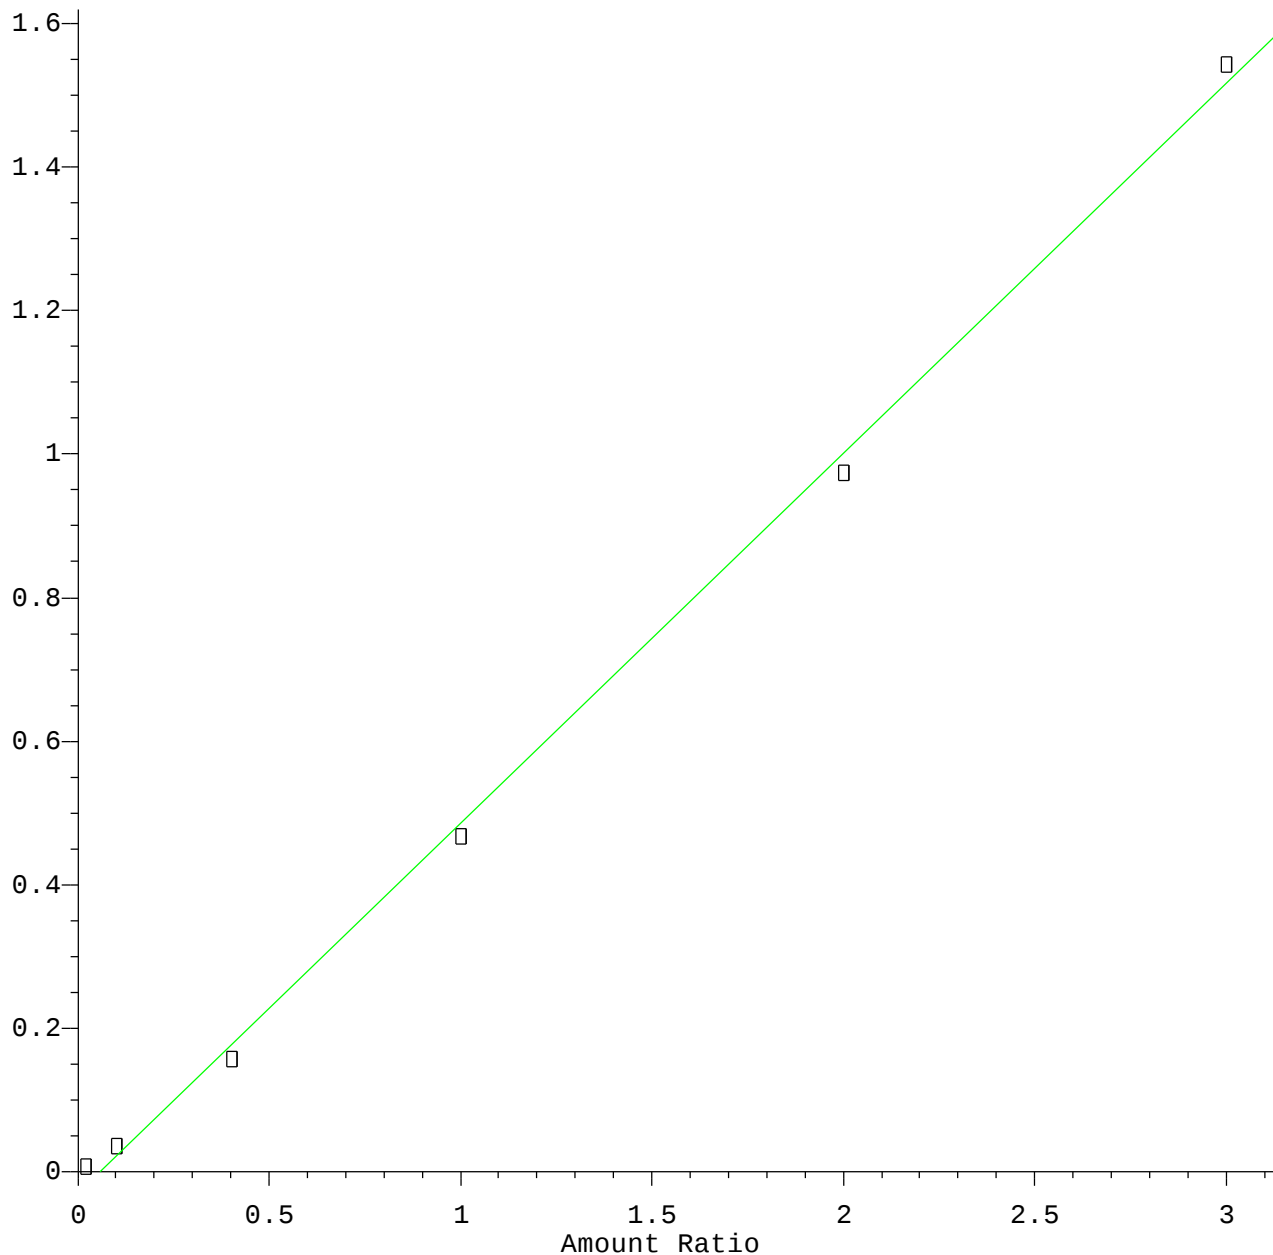

Resp Ratio = $5.15 \times 10^{-1} \times \text{Amt} - 2.92 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Calibration Table Last Updated: Fri Aug 02 01:55:00 2019

Instrument :
MSVOA_X
ClientSampleId :

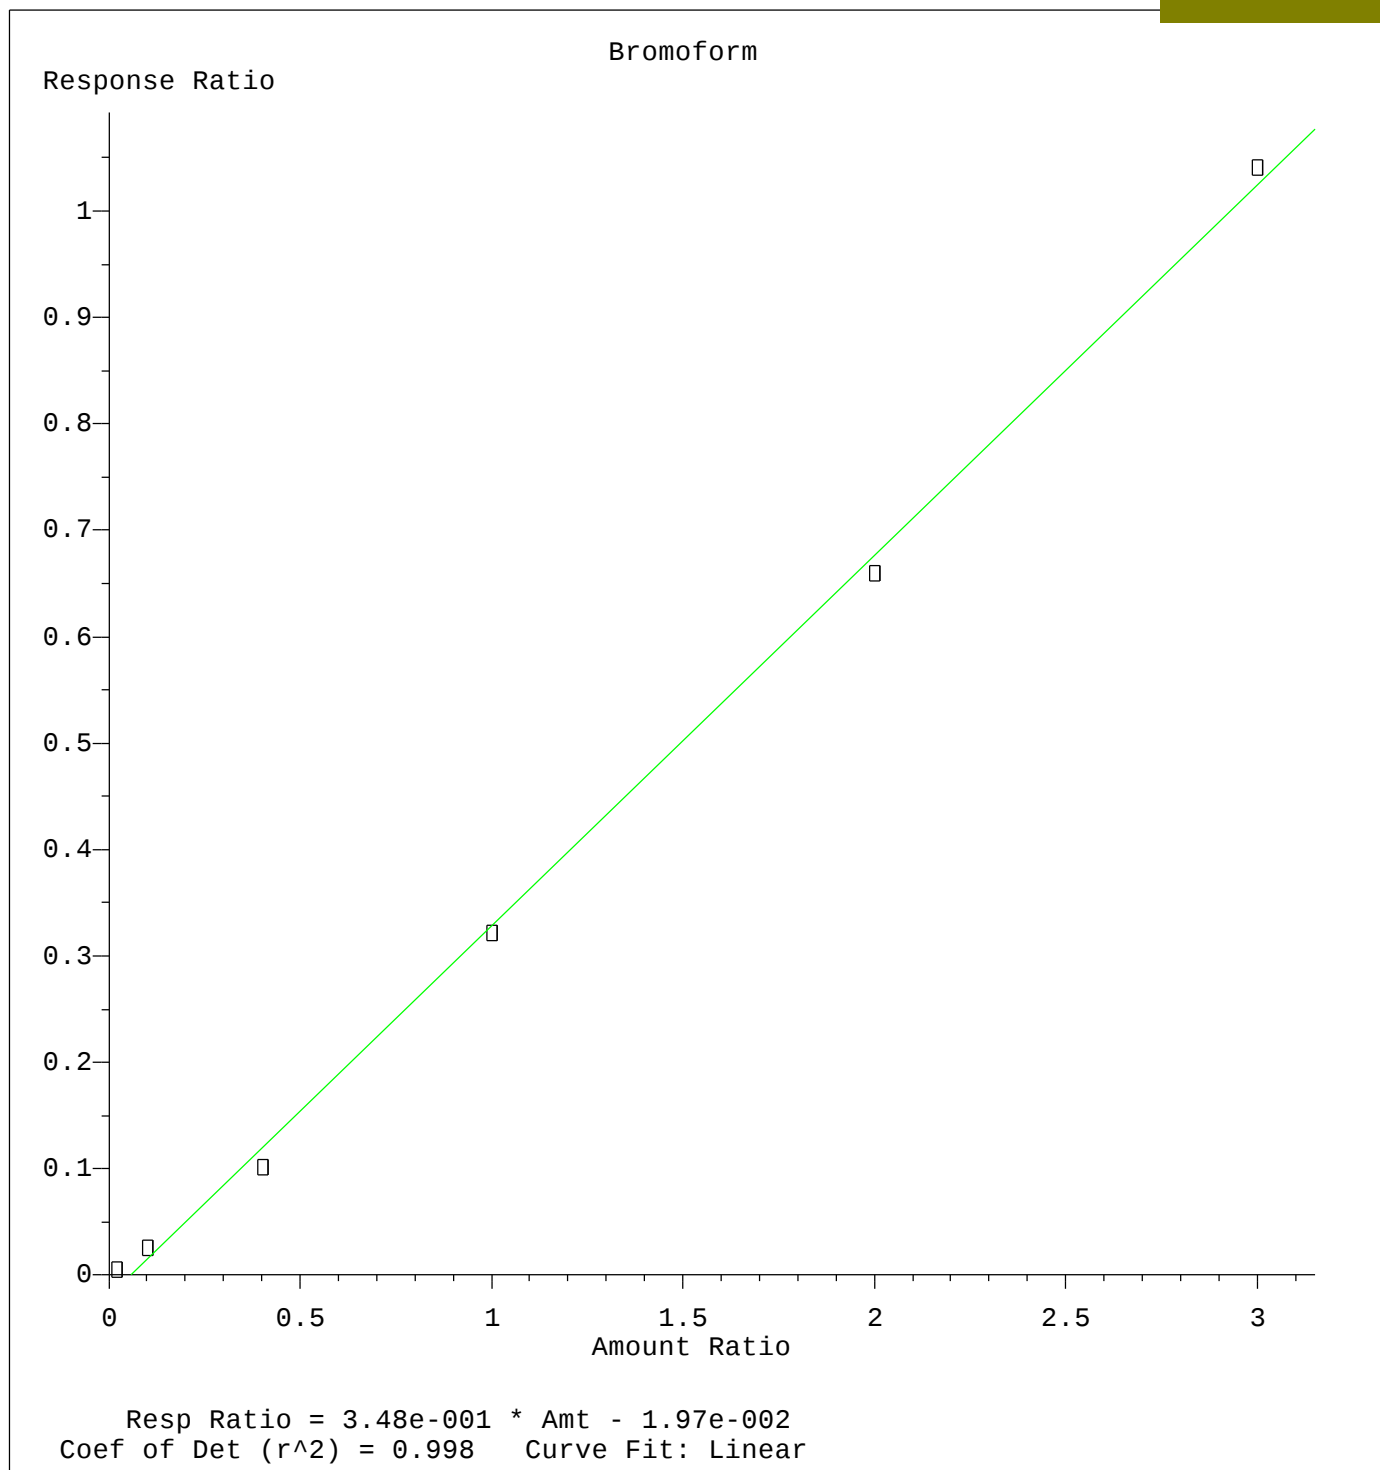


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Calibration Table Last Updated: Fri Aug 02 01:55:00 2019

Instrument :
MSVOA_X
ClientSampleId :

trans-1,4-Dichloro-2-butene

Response Ratio

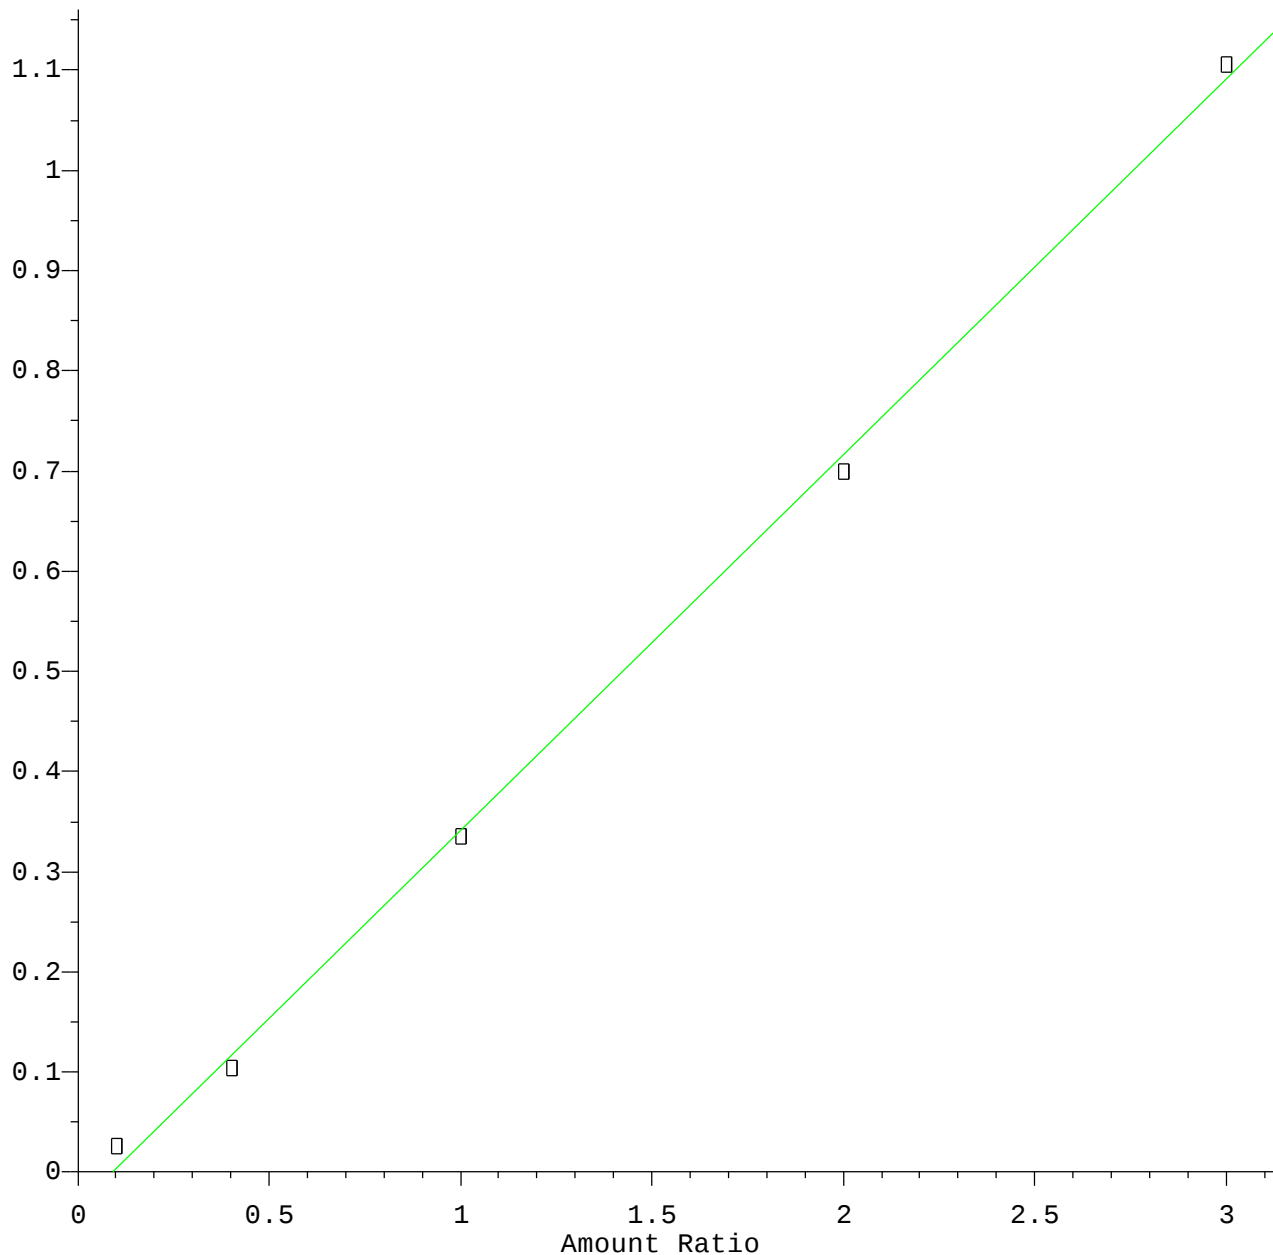

Resp Ratio = $3.75 \times 10^{-1} \times \text{Amt} - 3.40 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X080119W.M
Calibration Table Last Updated: Fri Aug 02 01:55:00 2019