

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080123\
 Data File : VX036753.D
 Acq On : 01 Aug 2023 17:03
 Operator : JC/MD
 Sample : 03856-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LEA-11D

Quant Time: Aug 02 06:25:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 21 12:14:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	130473	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	236974	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	216958	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	97878	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	88155	45.663	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	91.320%
35) Dibromofluoromethane	5.385	113	74998	46.044	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.080%
50) Toluene-d8	8.647	98	282457	48.900	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.800%
62) 4-Bromofluorobenzene	11.079	95	104593	47.995	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.980%
Target Compounds						
					Qvalue	
44) Trichloroethene	7.135	130	1004	0.544	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080123\
Data File : VX036753.D
Acq On : 01 Aug 2023 17:03
Operator : JC/MD
Sample : 03856-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
LEA-11D

Quant Time: Aug 02 06:25:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 21 12:14:12 2023
Response via : Initial Calibration




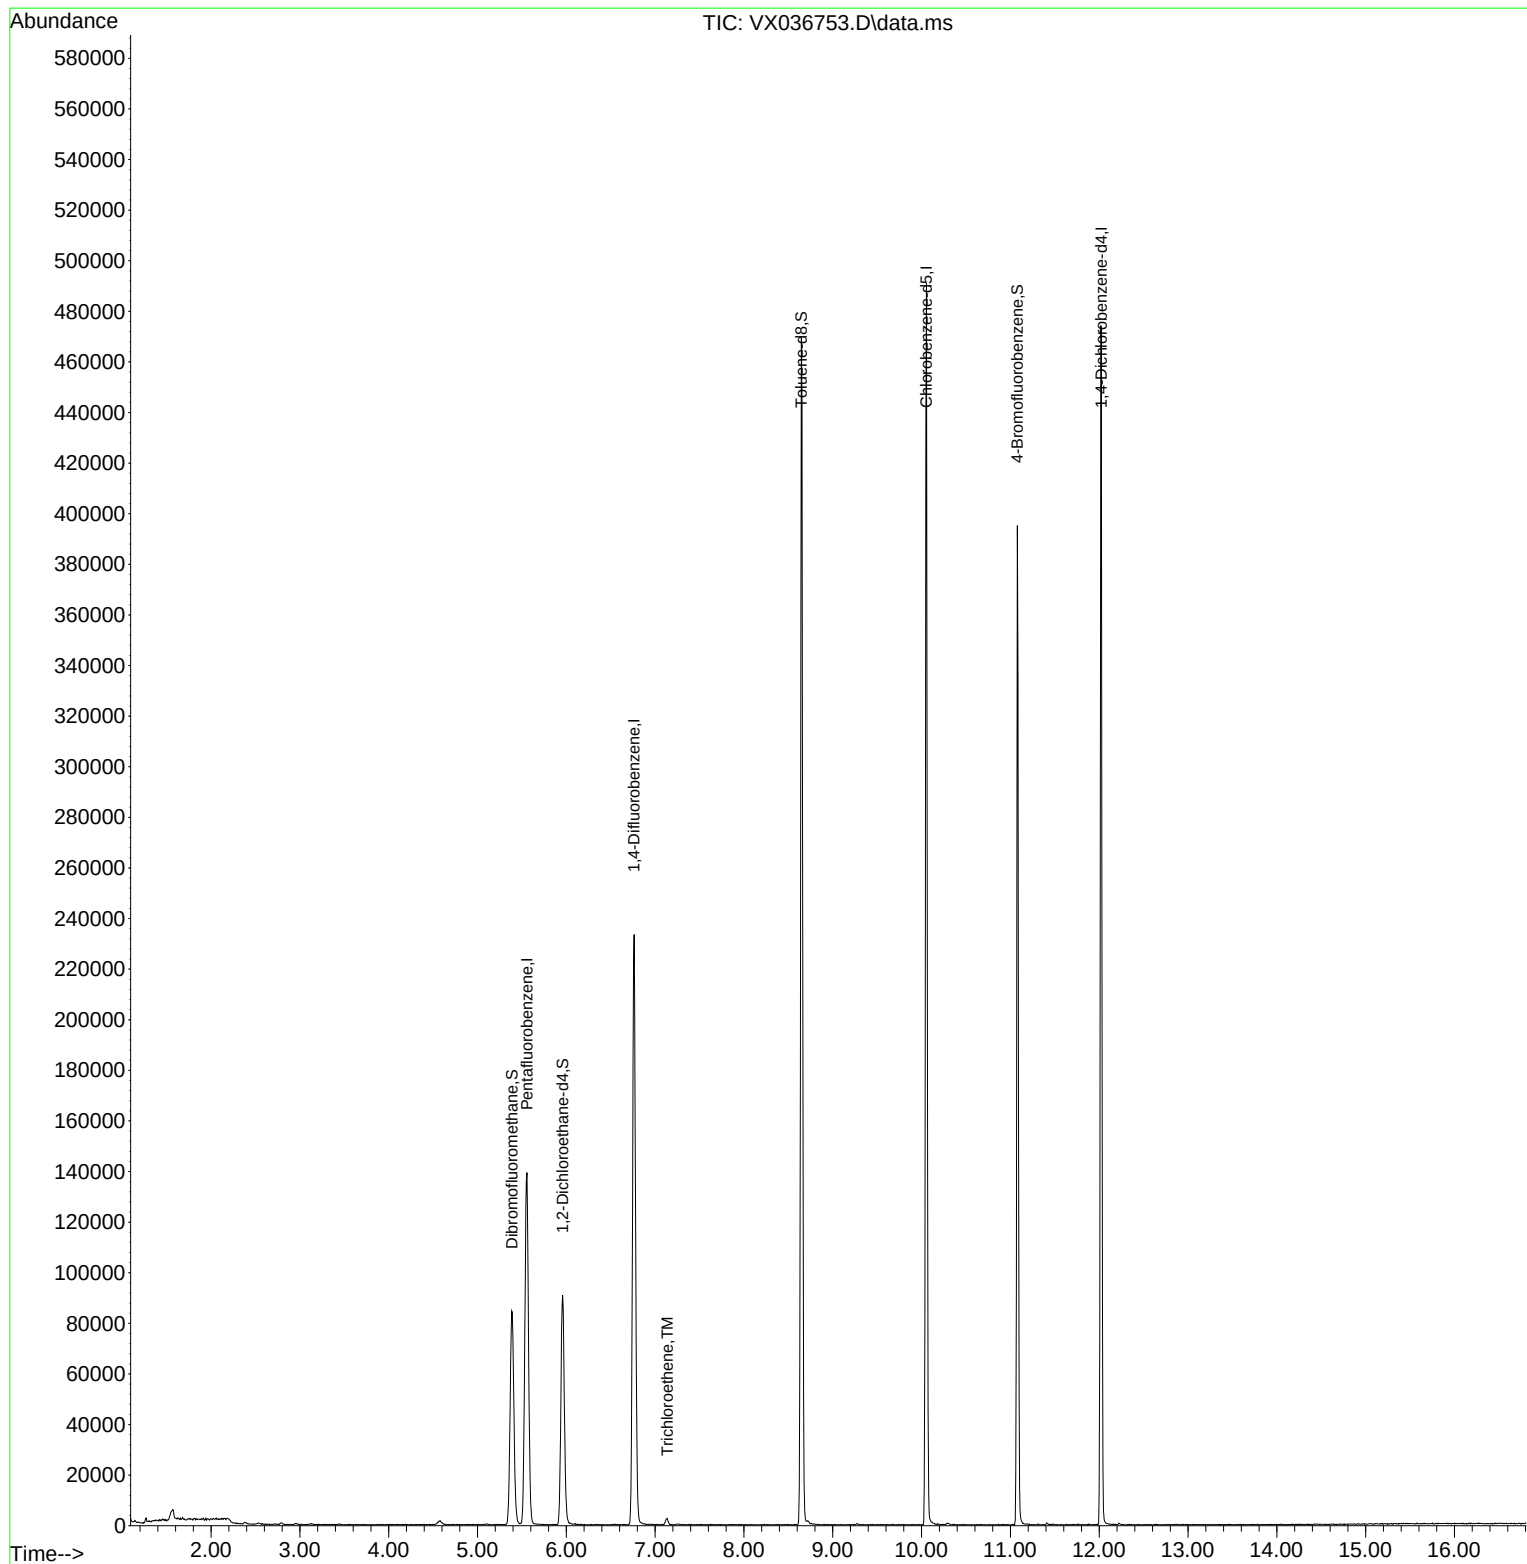


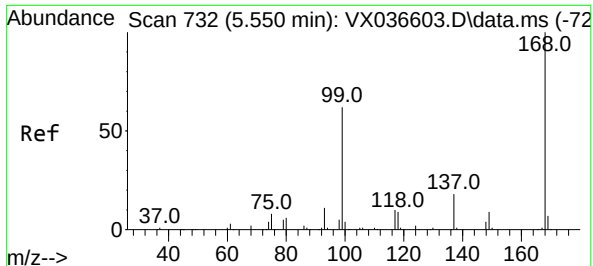

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 711
Delta R.T. 0.006 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03




Instrument :
MSVOA_X
ClientSampleId :
LEA-11D


Tgt Ion:168 Resp: 130473
Ion Ratio Lower Upper
168 100
99 60.7 56.6 85.0

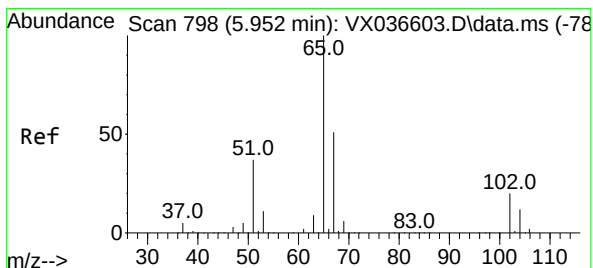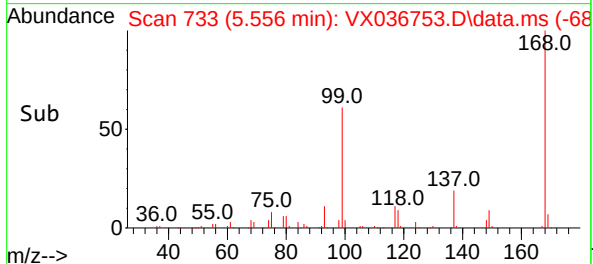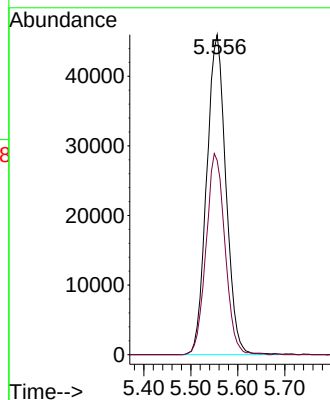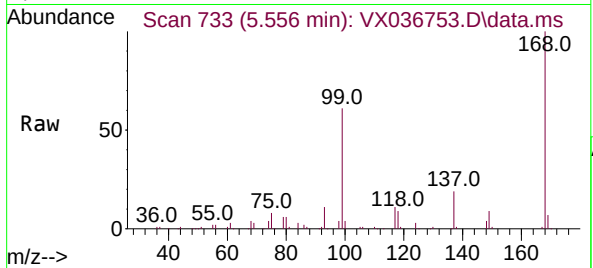

#33
1,2-Dichloroethane-d4
Concen: 45.663 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.006 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03

Tgt Ion: 65 Resp: 88155
Ion Ratio Lower Upper
65 100
67 52.0 0.0 100.2


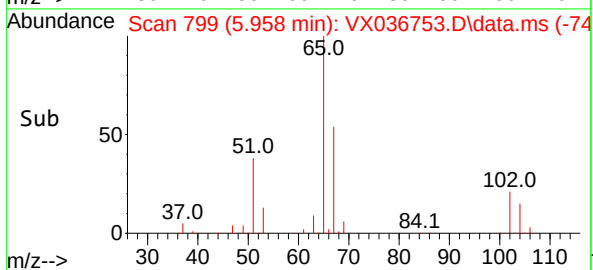
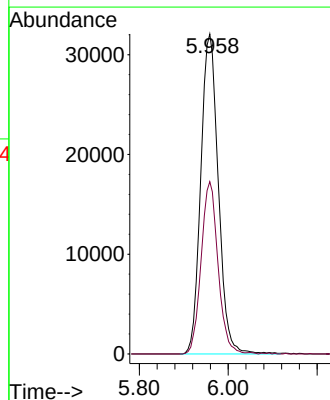
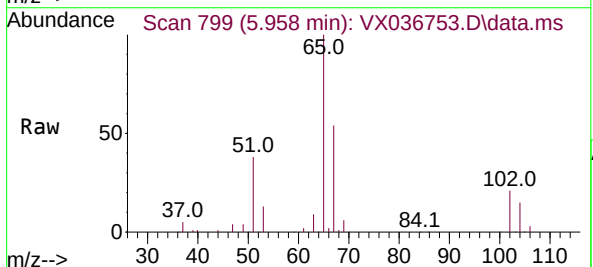


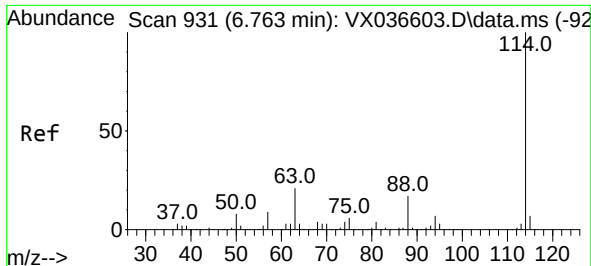

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03




Instrument :
MSVOA_X
ClientSampleId :
LEA-11D


Tgt Ion:114 Resp: 236974
Ion Ratio Lower Upper
114 100
63 21.0 0.0 45.0
88 16.6 0.0 36.6

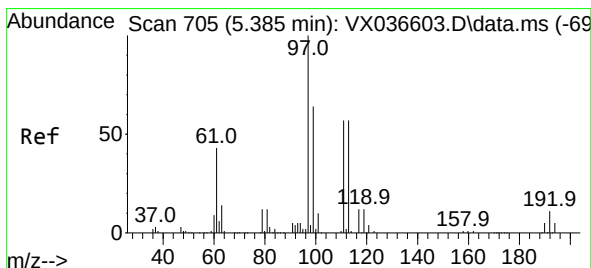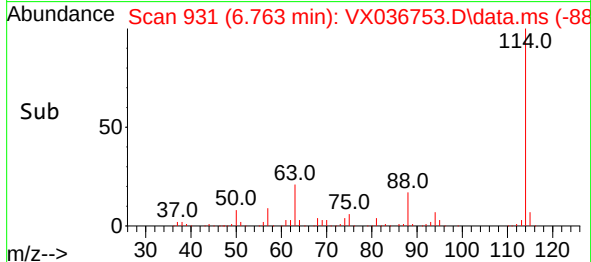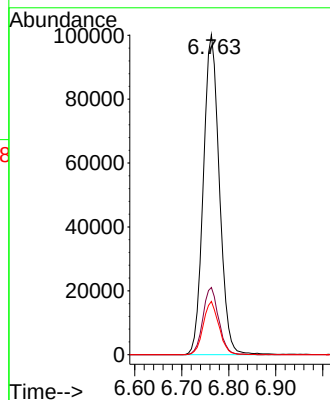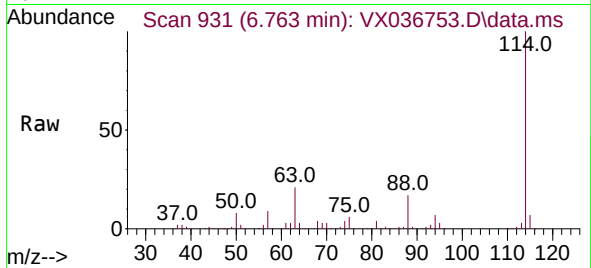

#35
Dibromofluoromethane
Concen: 46.044 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03

Tgt Ion:113 Resp: 74998
Ion Ratio Lower Upper
113 100
111 103.0 82.9 124.3
192 18.1 13.3 19.9


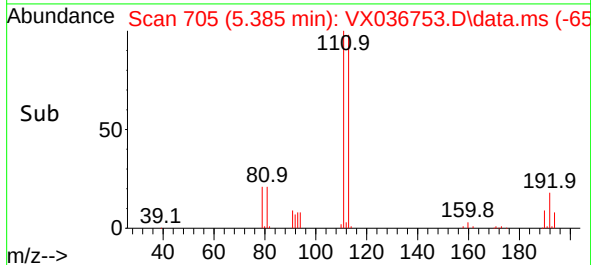
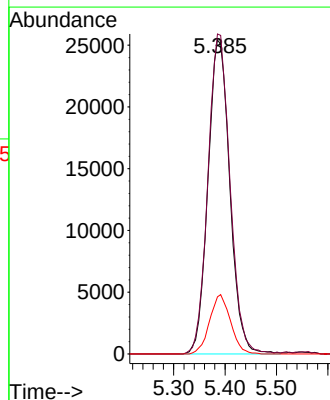
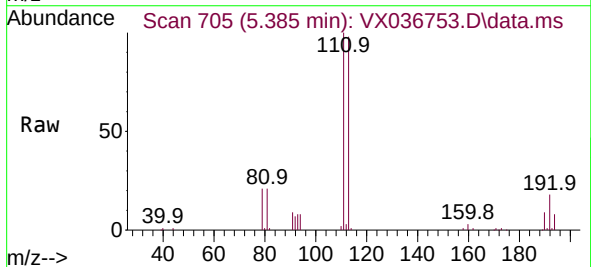


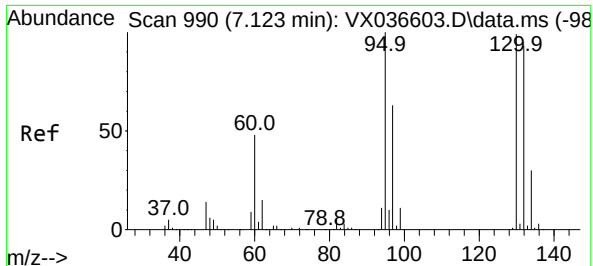

#44
Trichloroethene
Concen: 0.544 ug/l
RT: 7.135 min Scan# 991
Delta R.T. 0.012 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03




Instrument :
MSVOA_X
ClientSampleId :
LEA-11D


Tgt Ion:130 Resp: 1004
Ion Ratio Lower Upper
130 100
95 88.4 0.0 204.4

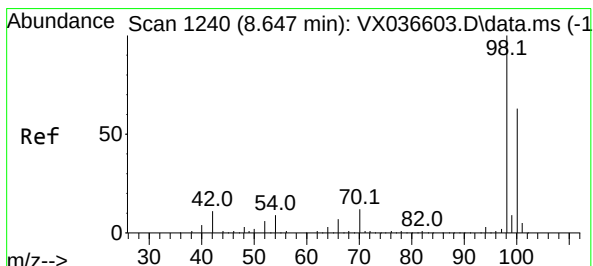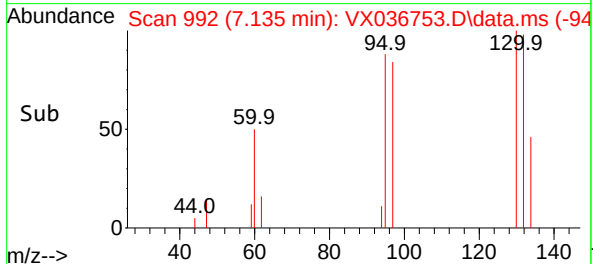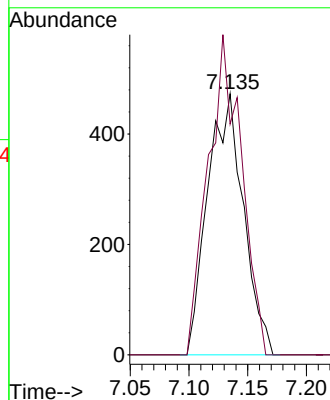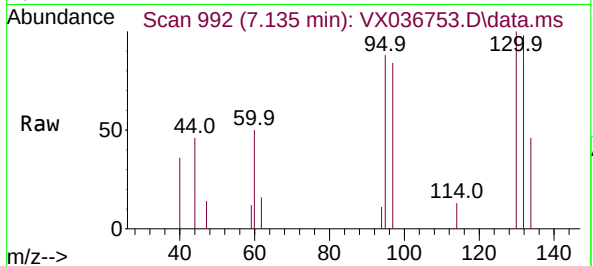

#50
Toluene-d8
Concen: 48.900 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03

Tgt Ion: 98 Resp: 282457
Ion Ratio Lower Upper
98 100
100 66.1 53.1 79.7


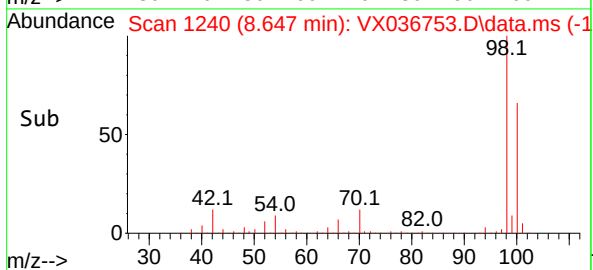
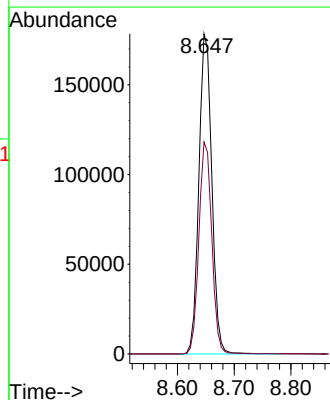
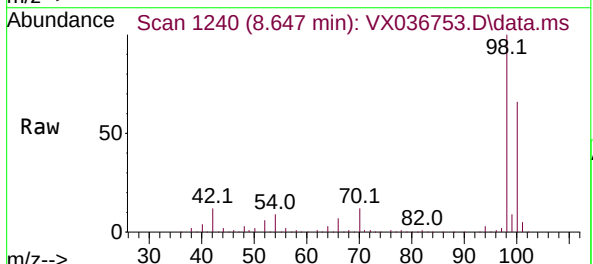


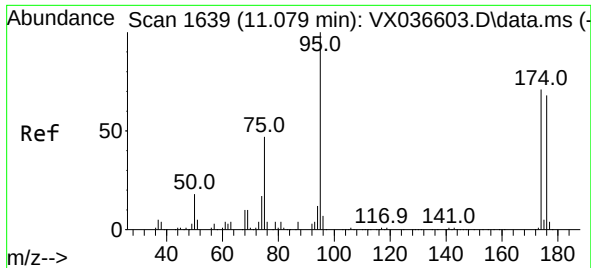

#62
4-Bromofluorobenzene
Concen: 47.995 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03




Instrument :
MSVOA_X
ClientSampleId :
LEA-11D


Tgt Ion: 95 Resp: 104593
Ion Ratio Lower Upper
95 100
174 73.4 0.0 135.6
176 71.5 0.0 131.0

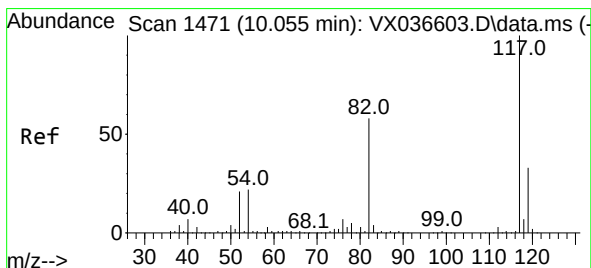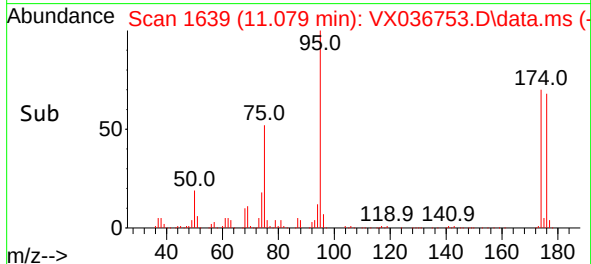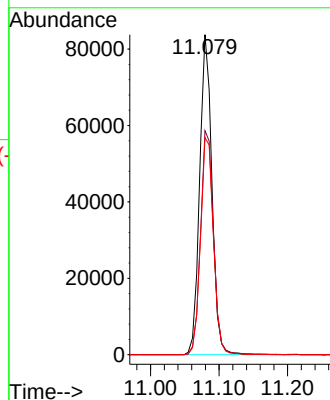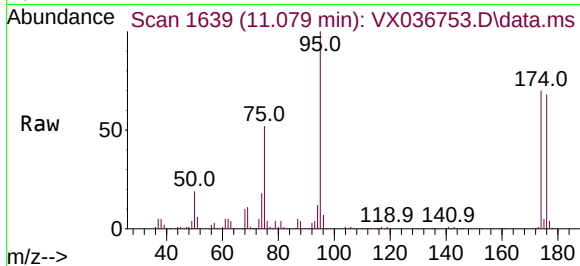

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX036753.D
Acq: 01 Aug 2023 17:03

Tgt Ion: 117 Resp: 216958
Ion Ratio Lower Upper
117 100
82 56.4 46.2 69.4
119 32.4 25.5 38.3

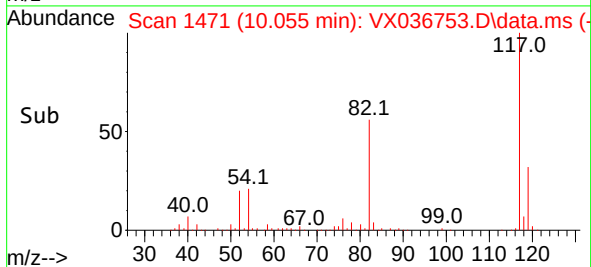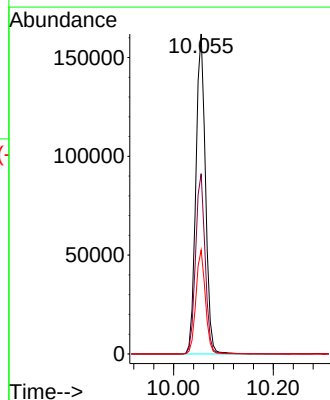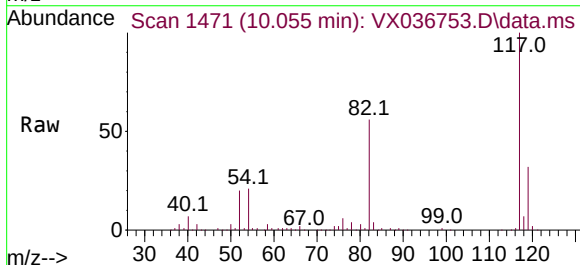

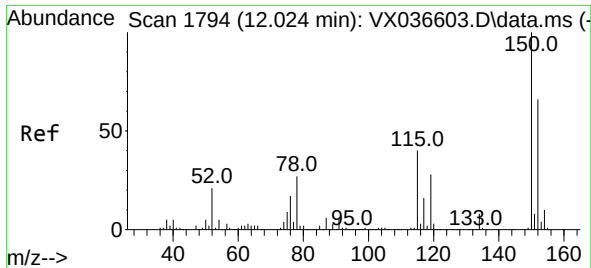

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX036753.D


Acq: 01 Aug 2023 17:03

Instrument :

MSVOA_X

ClientSampleId :

LEA-11D

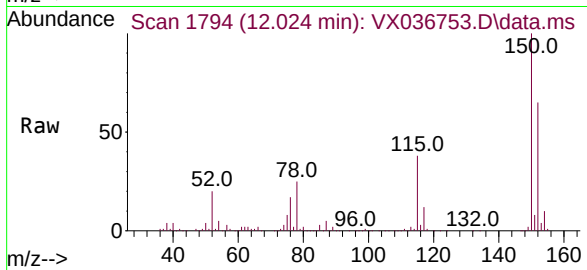

Tgt Ion:152 Resp: 97878

Ion Ratio Lower Upper

152 100

115 61.3 43.3 129.9

150 157.5 0.0 345.0

