

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080123\
 Data File : VX036756.D
 Acq On : 01 Aug 2023 18:14
 Operator : JC/MD
 Sample : 03775-03ME 10X
 Misc : 4.96g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BUILDING-A-8-(0-5)ME

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
 Title : SW846 8260

Signal : TIC: VX036756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.556	69	77	79	rBV6	4084	8890	1.13%	0.186%
2	4.574	562	572	581	rBV2	3114	9707	1.24%	0.203%
3	5.385	692	705	721	rBV	89663	264105	33.68%	5.536%
4	5.550	721	732	749	rVB	149024	421863	53.80%	8.843%
5	5.958	789	799	806	rBV	95376	252519	32.20%	5.293%
6	6.043	806	813	827	rVB2	47662	130497	16.64%	2.735%
7	6.763	921	931	946	rBV	246344	577653	73.66%	12.108%
8	8.647	1234	1240	1247	rBV	499715	784179	100.00%	16.437%
9	8.720	1247	1252	1266	rVB	54816	85649	10.92%	1.795%
10	10.055	1465	1471	1487	rBV	514269	693085	88.38%	14.528%
11	10.195	1490	1494	1501	rVB	6331	8960	1.14%	0.188%
12	10.299	1506	1511	1519	rVV	22135	31299	3.99%	0.656%
13	10.652	1562	1569	1580	rBV3	23603	43901	5.60%	0.920%
14	11.079	1634	1639	1652	rBV	412917	517081	65.94%	10.838%
15	12.018	1788	1793	1802	rBV	475357	625384	79.75%	13.108%
16	12.414	1853	1858	1868	rBV	52100	68935	8.79%	1.445%
17	13.774	2076	2081	2092	rBV	172317	212410	27.09%	4.452%
18	14.639	2218	2223	2230	rVB	13597	18125	2.31%	0.380%
19	14.780	2241	2246	2254	rVB2	13201	16596	2.12%	0.348%




Sum of corrected areas: 4770838

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080123\
Data File : VX036756.D
Acq On : 01 Aug 2023 18:14
Operator : JC/MD
Sample : 03775-03ME 10X
Misc : 4.96g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-8-(0-5)ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

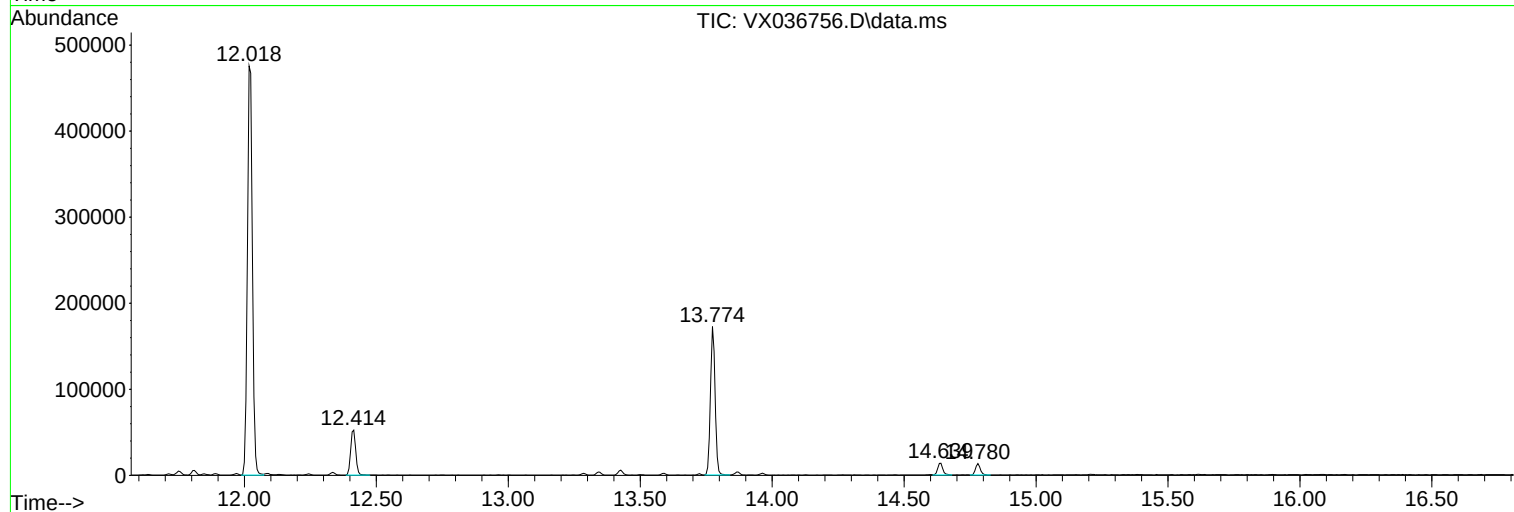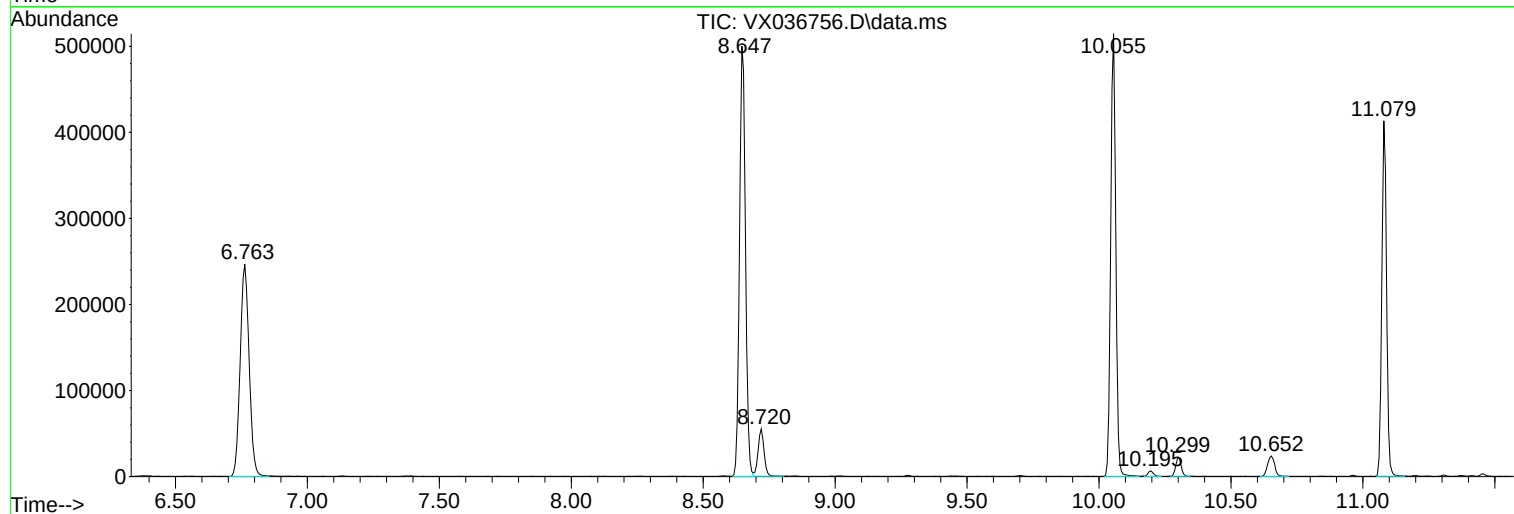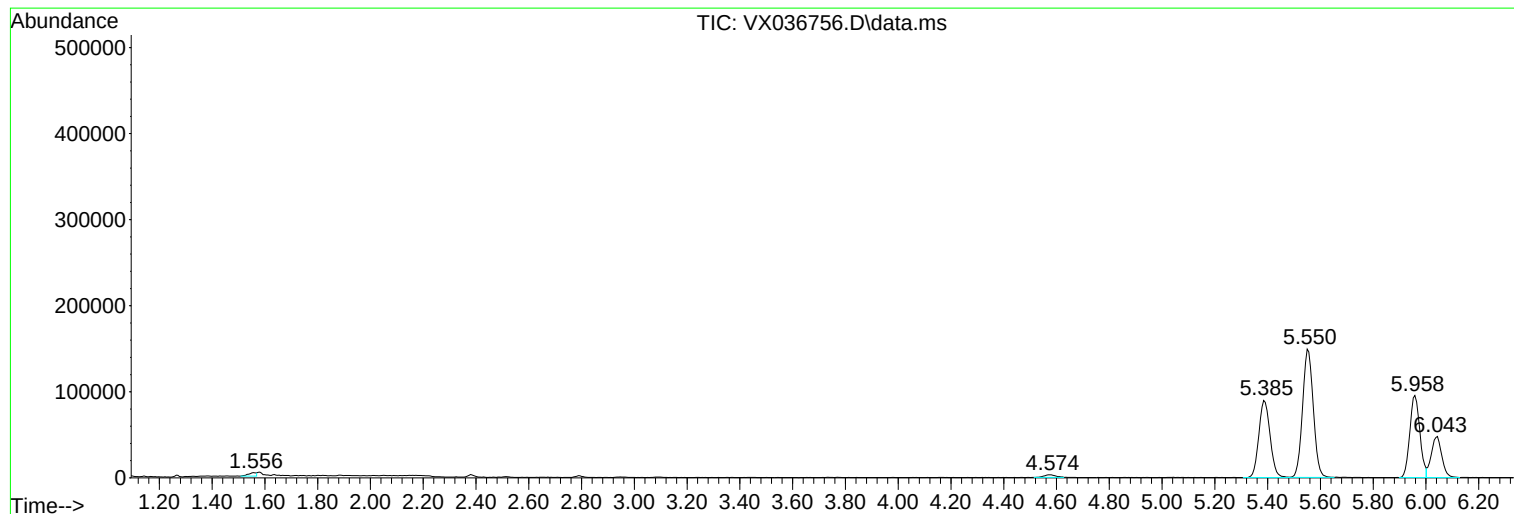

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080123\
Data File : VX036756.D
Acq On : 01 Aug 2023 18:14
Operator : JC/MD
Sample : 03775-03ME 10X
Misc : 4.96g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-8-(0-5)ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080123\
Data File : VX036756.D
Acq On : 01 Aug 2023 18:14
Operator : JC/MD
Sample : 03775-03ME 10X
Misc : 4.96g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BUILDING-A-8-(0-5)ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------