
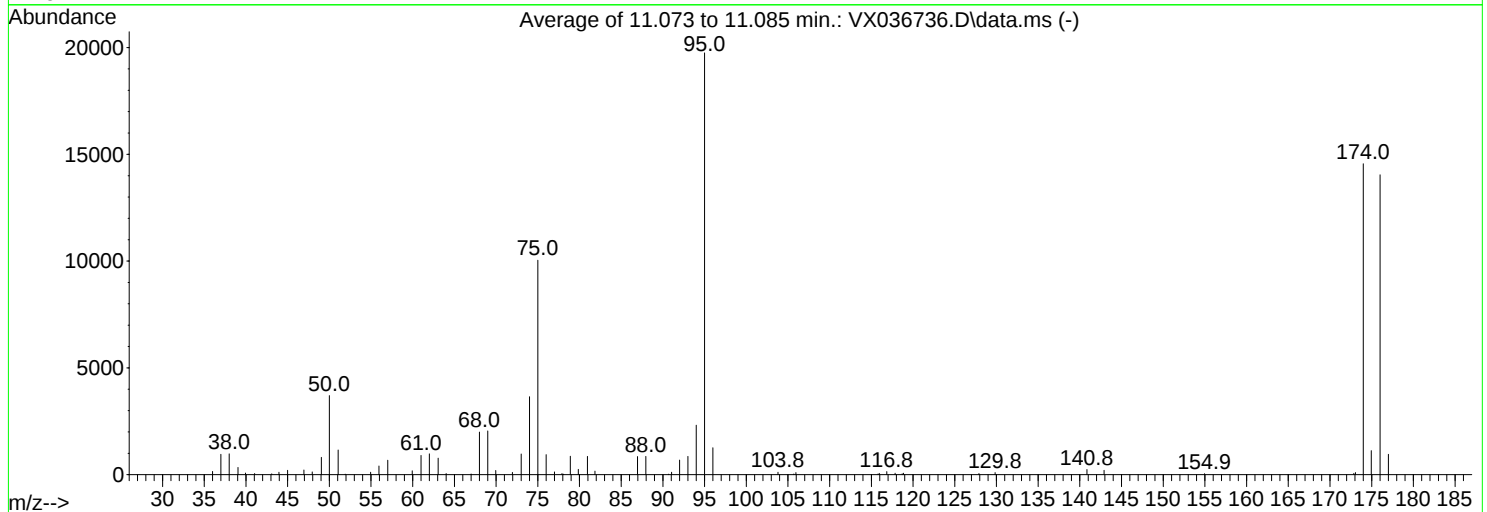


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080123\
Data File : VX036736.D
Acq On : 01 Aug 2023 08:58
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Title : SW846 8260
Last Update : Fri Jul 21 12:14:12 2023

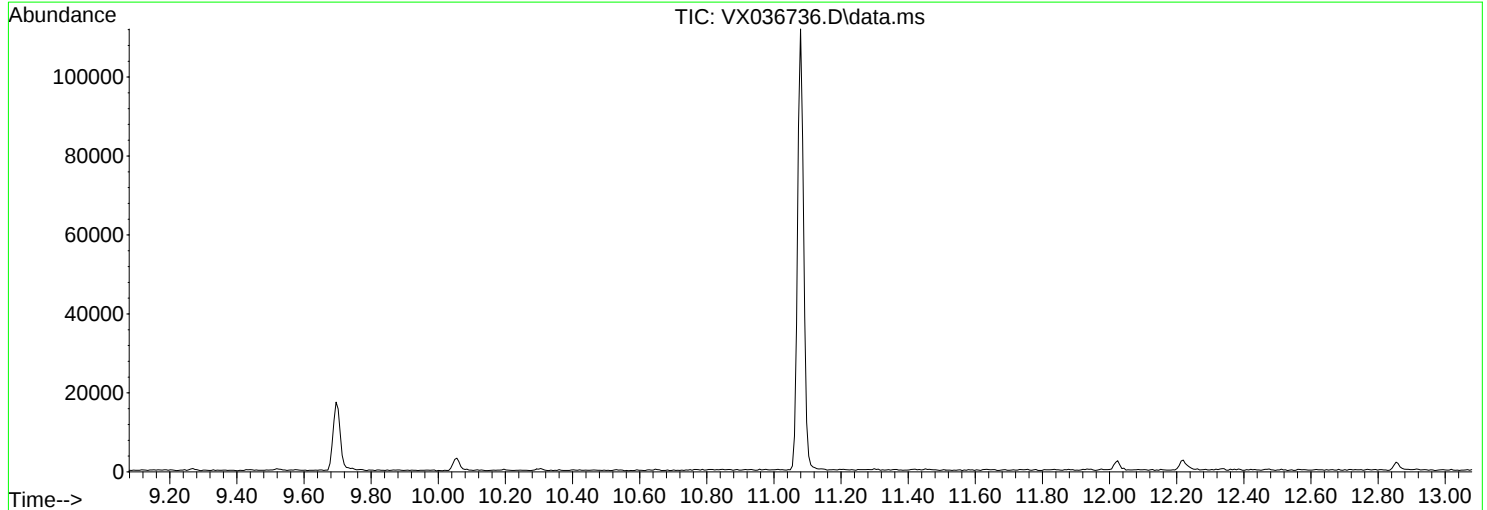

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	3698	PASS
75	95	30	60	50.8	10041	PASS
95	95	100	100	100.0	19752	PASS
96	95	5	9	6.4	1257	PASS
173	174	0.00	2	0.7	98	PASS
174	95	50	100	73.7	14556	PASS
175	174	5	9	7.7	1121	PASS
176	174	95	101	96.5	14044	PASS
177	176	5	9	6.8	950	PASS