

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
 Data File : VX042826.D
 Acq On : 02 Aug 2024 05:25
 Operator : JC/MD
 Sample : P3430-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 925-K1-WPO-0-0.25-073124

Quant Time: Aug 02 08:29:46 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 01 16:40:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	79643	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	156317	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	152527	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	64635	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	64710	50.573	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 101.140%			
35) Dibromofluoromethane	5.385	113	53055	49.132	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 98.260%			
50) Toluene-d8	8.647	98	189751	48.411	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 96.820%			
62) 4-Bromofluorobenzene	11.079	95	71388	49.838	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 99.680%			
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.142	85	11660	9.239	ug/l	98
3) Chloromethane	1.300	50	431	Below Cal	#	43
4) Vinyl Chloride	1.374	62	321351	325.304	ug/l	97
7) Trichlorofluoromethane	2.136	101	289	0.218	ug/l	99
9) 1,1,2-Trichlorotrifluo...	2.319	101	154218	154.210	ug/l	99
11) Tert butyl alcohol	2.953	59	119	Below Cal	#	78
12) 1,1-Dichloroethene	2.319	96	9307	9.601	ug/l #	70
16) Acetone	2.392	43	2509	5.400	ug/l	91
18) Methyl Acetate	2.703	43	306	0.262	ug/l #	53
20) Methylene Chloride	2.794	84	480	Below Cal	#	68
21) trans-1,2-Dichloroethene	3.093	96	21926	21.922	ug/l	84
24) 1,1-Dichloroethane	3.605	63	21191	12.211	ug/l	99
25) 2-Butanone	4.574	43	229	0.335	ug/l #	60
27) cis-1,2-Dichloroethene	4.489	96	3067376	2623.520	ug/l	81
29) Tetrahydrofuran	5.031	42	620	1.458	ug/l #	87
31) Cyclohexane	5.550	56	1757	1.246	ug/l #	1
32) 1,1,1-Trichloroethane	5.373	97	2990	1.745	ug/l #	93
36) 1,1-Dichloropropene	5.550	75	6658	4.754	ug/l #	52
38) Carbon Tetrachloride	5.550	117	8748	5.420	ug/l #	17
39) Methylcyclohexane	7.129	83	683	0.389	ug/l #	1
40) Benzene	6.043	78	5083	1.157	ug/l	93
41) Methacrylonitrile	5.038	41	275	0.364	ug/l #	33
42) 1,2-Dichloroethane	6.092	62	1194	0.752	ug/l #	77
44) Trichloroethene	7.129	130	54701	47.551	ug/l	93
52) Toluene	8.720	92	7852	2.754	ug/l	98
55) 1,1,2-Trichloroethane	9.153	97	573	0.497	ug/l #	84
60) Dibromochloromethane	9.275	129	2056	1.760	ug/l #	11
64) Tetrachloroethene	9.275	164	1901	1.840	ug/l	96
65) Chlorobenzene	10.085	112	1976	0.587	ug/l	95
76) 1,2,3-Trichloropropane	11.079	75	38252	25.900	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	38252	76.658	ug/l #	5
86) p-Isopropyltoluene	12.012	119	1010	0.232	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042826.D
Acq On : 02 Aug 2024 05:25
Operator : JC/MD
Sample : P3430-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124

Quant Time: Aug 02 08:29:46 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260
QLast Update : Thu Aug 01 16:40:12 2024
Response via : Initial Calibration




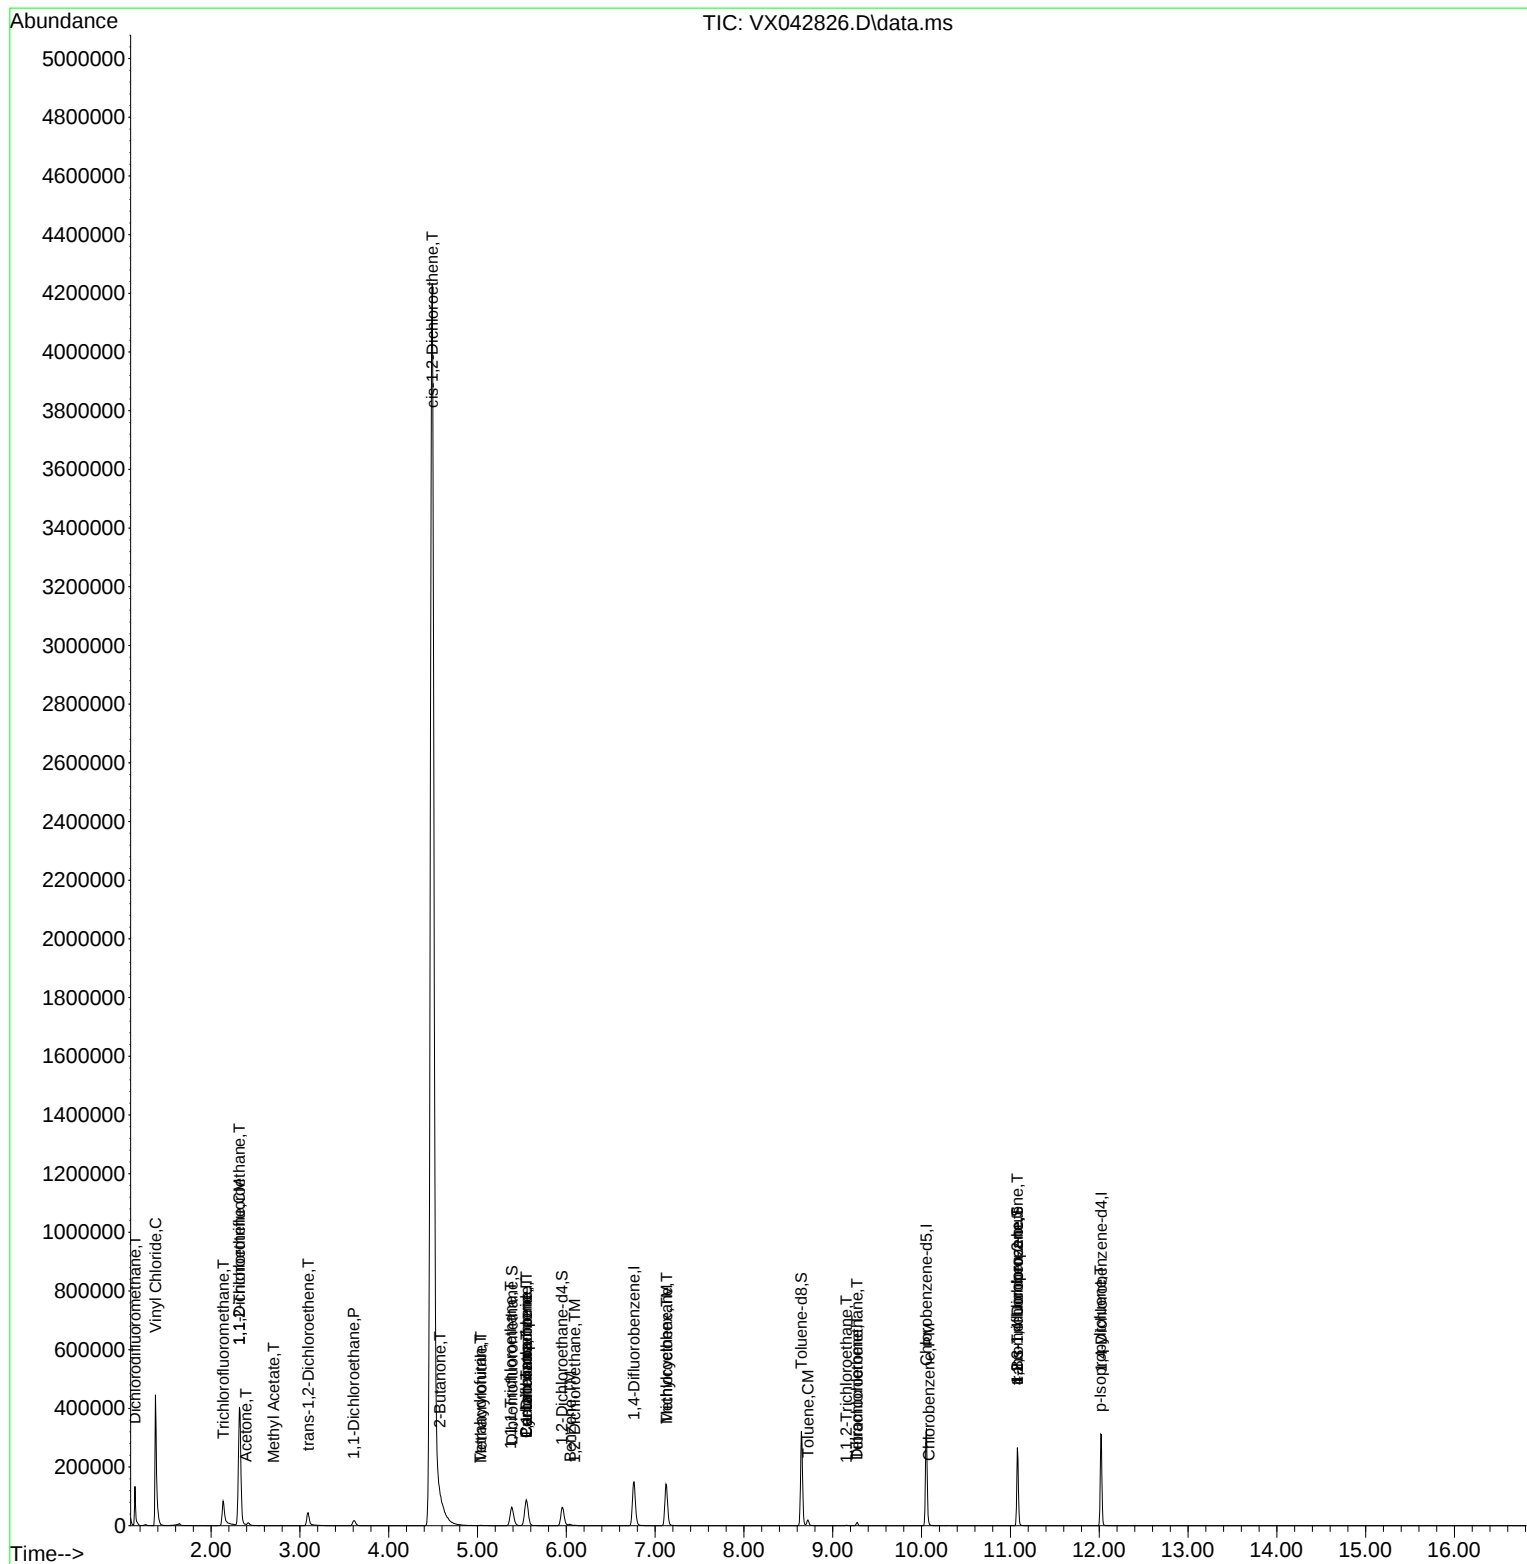


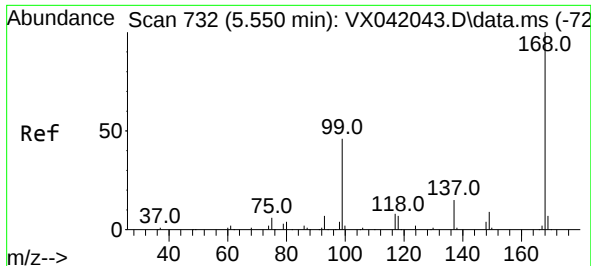

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion:168 Resp: 79643
Ion Ratio Lower Upper
168 100
99 66.4 56.6 85.0



#2
Dichlorodifluoromethane
Concen: 9.239 ug/l
RT: 1.142 min Scan# 9
Delta R.T. -0.024 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 85 Resp: 11660
Ion Ratio Lower Upper
85 100
87 34.5 16.7 50.1


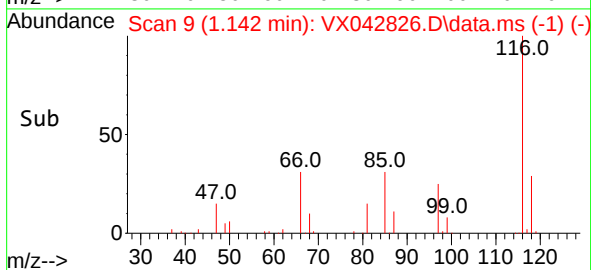




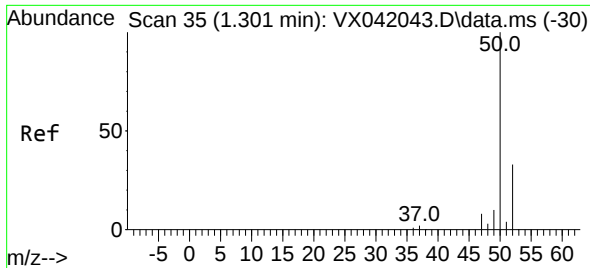

#3
Chloromethane
Concen: Below Cal
RT: 1.300 min Scan# 31
Delta R.T. -0.007 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion: 50 Resp: 431
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#

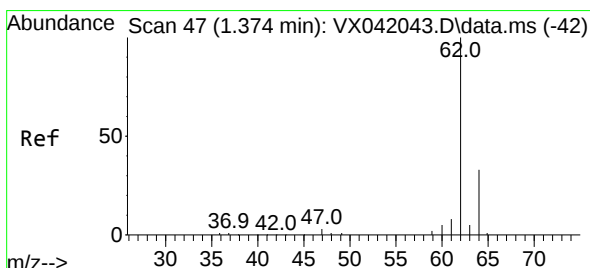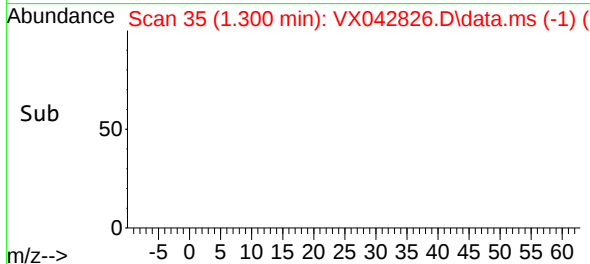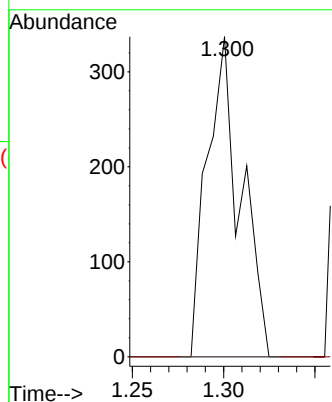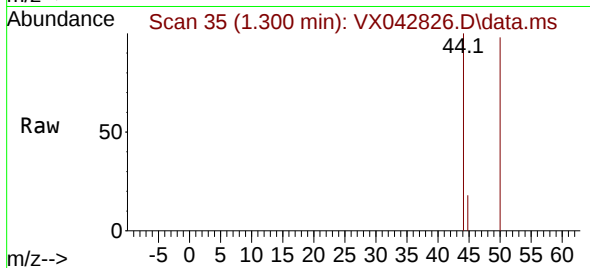

#4
Vinyl Chloride
Concen: 325.304 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 62 Resp: 321351
Ion Ratio Lower Upper
62 100
64 33.4 25.4 38.0


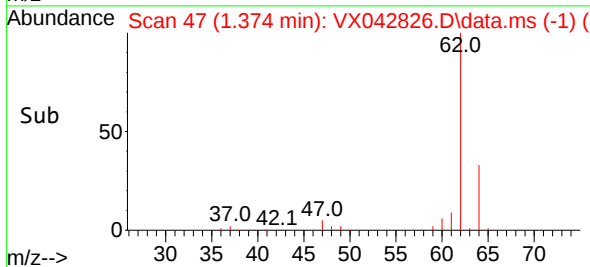
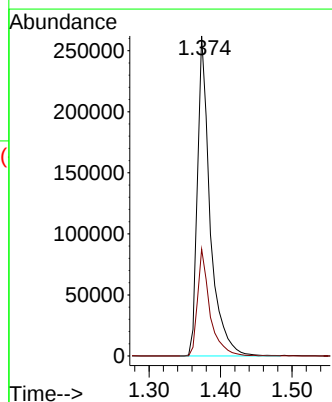
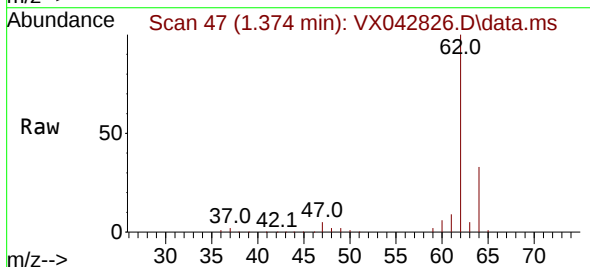




#7
 Trichlorofluoromethane
 Concen: 0.218 ug/l
 RT: 2.136 min Scan# 11
 Delta R.T. 0.269 min
 Lab File: VX042826.D
 Acq: 02 Aug 2024 05:25




Instrument :
 MSVOA_X
 ClientSampleId :
 925-K1-WPO-0-0.25-073124


Tgt Ion:101 Resp: 289
 Ion Ratio Lower Upper
 101 100
 103 65.0 51.4 77.2



#9
 1,1,2-Trichlorotrifluoroethane
 Concen: 154.210 ug/l
 RT: 2.319 min Scan# 202
 Delta R.T. 0.007 min
 Lab File: VX042826.D
 Acq: 02 Aug 2024 05:25

Tgt Ion:101 Resp: 154218
 Ion Ratio Lower Upper
 101 100
 85 45.0 37.0 55.6
 151 72.8 58.6 87.8





#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.953 min Scan# 30

Delta R.T. -0.054 min

Lab File: VX042826.D

Acq: 02 Aug 2024 05:25

Instrument :

MSVOA_X

ClientSampleId :





925-K1-WPO-0-0.25-073124

Tgt Ion: 59 Resp: 119

Ion Ratio Lower Upper

59 100

57 0.0 6.0 9.0#



#12

1,1-Dichloroethene

Concen: 9.601 ug/l

RT: 2.319 min Scan# 202

Delta R.T. 0.013 min

Lab File: VX042826.D

Acq: 02 Aug 2024 05:25




Tgt Ion: 96 Resp: 9307


Ion Ratio Lower Upper

96 100

61 131.6 144.6 216.8#

98 50.7 50.4 75.6



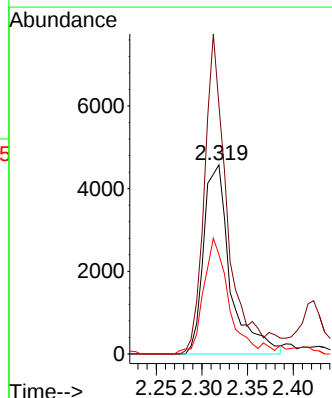





#16
Acetone
Concen: 5.400 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion: 43 Resp: 2509
Ion Ratio Lower Upper
43 100
58 32.0 21.9 32.9

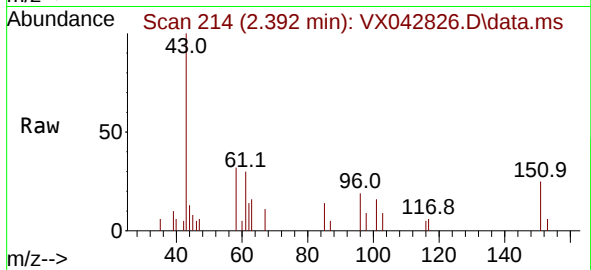

#18
Methyl Acetate
Concen: 0.262 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 43 Resp: 306
Ion Ratio Lower Upper
43 100
74 0.0 17.8 26.8#









#20
Methylene Chloride
Concen: Below Cal
RT: 2.794 min Scan# 21
Delta R.T. 0.012 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion: 84	Resp: 480
Ion Ratio	Lower Upper
84 100	
49 92.2	103.6 155.4#
51 24.1	33.8 50.6#
86 34.3	49.4 74.0#



#21
trans-1,2-Dichloroethene
Concen: 21.922 ug/l
RT: 3.093 min Scan# 329
Delta R.T. 0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 96	Resp: 21926
Ion Ratio	Lower Upper
96 100	
61 122.3	119.2 178.8
98 64.3	48.7 73.1


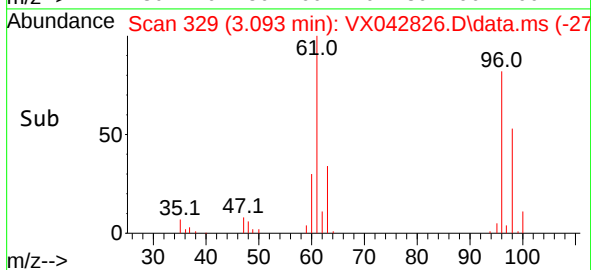






#24
1,1-Dichloroethane
Concen: 12.211 ug/l
RT: 3.605 min Scan# 413
Delta R.T. -0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion:	63	Resp:	21191
Ion	Ratio	Lower	Upper
63	100		
98	6.5	3.3	9.8
100	5.3	2.1	6.5

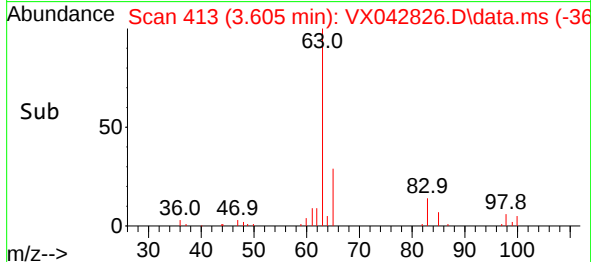

#25
2-Butanone
Concen: 0.335 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion:	43	Resp:	229
Ion	Ratio	Lower	Upper
43	100		
72	4.5	19.4	29.2#

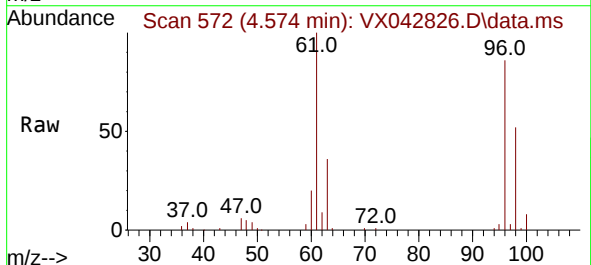



#27

cis-1,2-Dichloroethene

Concen: 2623.520 ug/l

RT: 4.489 min Scan# 51

Delta R.T. -0.000 min

Lab File: VX042826.D

Acq: 02 Aug 2024 05:25

Instrument :





MSVOA_X

ClientSampleId :

925-K1-WPO-0-0.25-073124

Tgt Ion: 96 Resp: 3067376

Ion	Ratio	Lower	Upper
96	100		
61	120.7	0.0	312.2
98	64.7	0.0	129.0

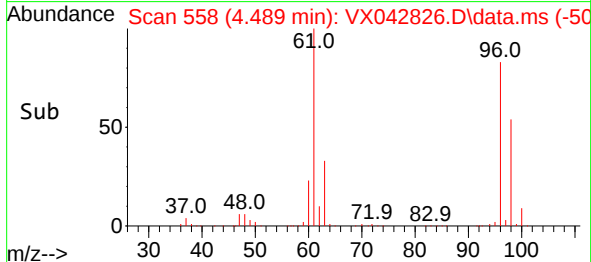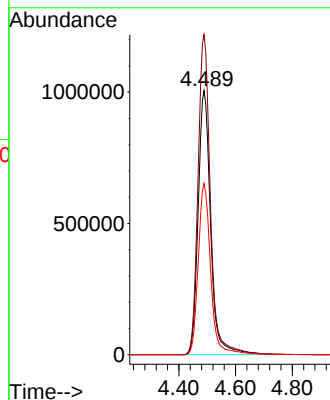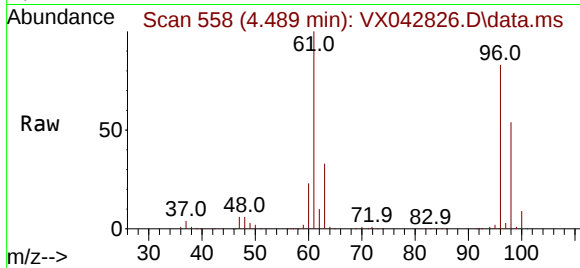

#29

Tetrahydrofuran

Concen: 1.458 ug/l

RT: 5.031 min Scan# 647




Delta R.T. 0.012 min


Lab File: VX042826.D

Acq: 02 Aug 2024 05:25

Tgt Ion: 42 Resp: 620

Ion	Ratio	Lower	Upper
42	100		
72	51.5	34.2	51.4#
71	33.1	32.2	48.2


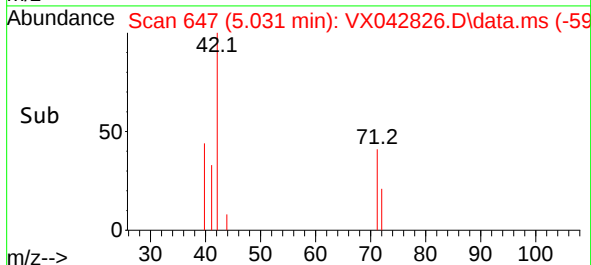
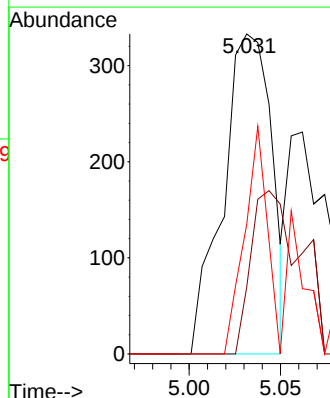
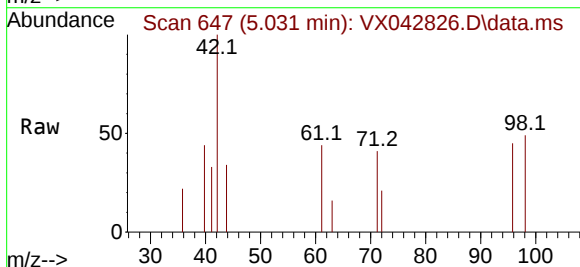




#31
Cyclohexane
Concen: 1.246 ug/l
RT: 5.550 min Scan# 718
Delta R.T. 0.086 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion: 56 Resp: 1757
Ion Ratio Lower Upper
56 100
69 188.8 23.4 35.2#
84 149.7 65.9 98.9#

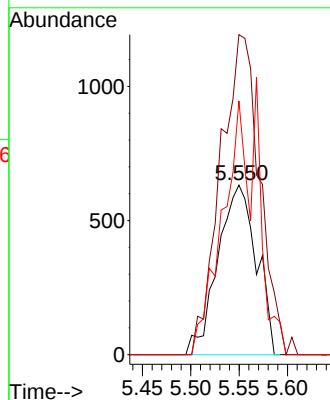

#32
1,1,1-Trichloroethane
Concen: 1.745 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 97 Resp: 2990
Ion Ratio Lower Upper
97 100
99 64.1 51.1 76.7
61 55.9 36.4 54.6#



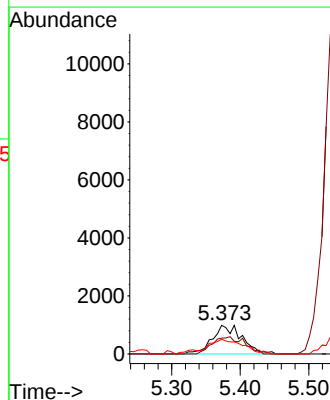





#33
 1,2-Dichloroethane-d4
 Concen: 50.573 ug/l
 RT: 5.952 min Scan# 799
 Delta R.T. -0.006 min
 Lab File: VX042826.D
 Acq: 02 Aug 2024 05:25




Instrument :
 MSVOA_X
 ClientSampleId :
 925-K1-WPO-0-0.25-073124


Tgt Ion: 65 Resp: 64710
 Ion Ratio Lower Upper
 65 100
 67 50.1 0.0 100.2

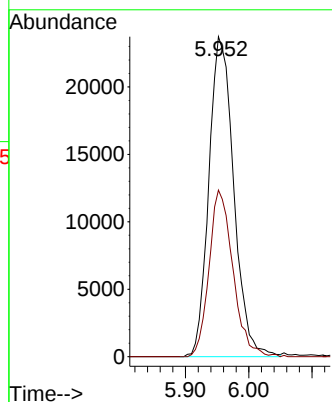

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 931
 Delta R.T. -0.000 min
 Lab File: VX042826.D
 Acq: 02 Aug 2024 05:25

Tgt Ion: 114 Resp: 156317
 Ion Ratio Lower Upper
 114 100
 63 18.3 0.0 45.0
 88 15.5 0.0 36.6


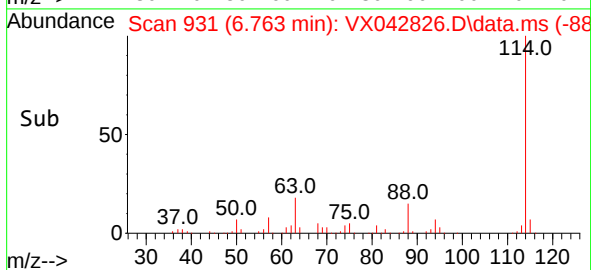






#35
Dibromofluoromethane
Concen: 49.132 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion:	113	Resp:	53055
Ion	Ratio	Lower	Upper
113	100		
111	102.1	82.9	124.3
192	17.2	13.3	19.9

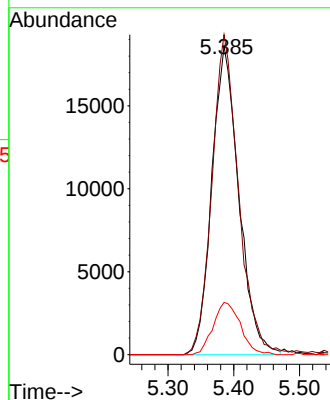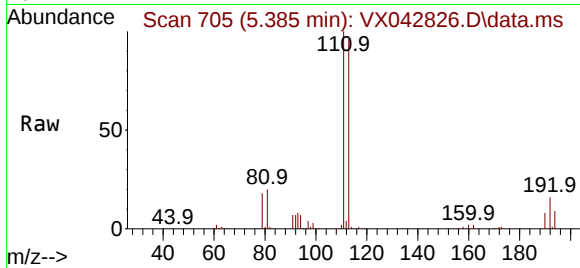

#36
1,1-Dichloropropene
Concen: 4.754 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.140 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25


Tgt Ion:	75	Resp:	6658
Ion	Ratio	Lower	Upper
75	100		
110	10.3	17.0	50.9#
77	0.0	24.7	37.1#

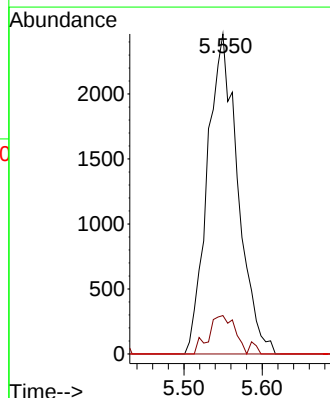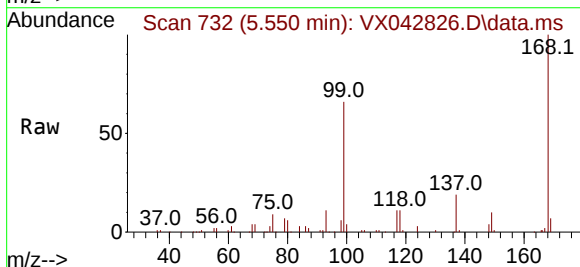






#38
Carbon Tetrachloride
Concen: 5.420 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124







Tgt Ion: 117 Resp: 8748
Ion Ratio Lower Upper
117 100
119 7.0 78.2 117.2#
121 0.0 24.4 36.6#



#39
Methylcyclohexane
Concen: 0.389 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.250 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 83 Resp: 683
Ion Ratio Lower Upper
83 100
55 0.0 64.6 97.0#
98 138.8 36.7 55.1#


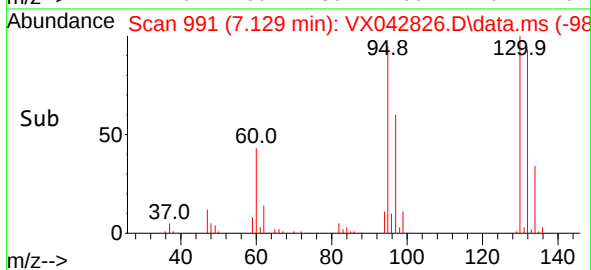






#40
Benzene
Concen: 1.157 ug/l
RT: 6.043 min Scan# 812
Delta R.T. 0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion: 78 Resp: 5083
Ion Ratio Lower Upper
78 100
77 20.6 19.3 28.9

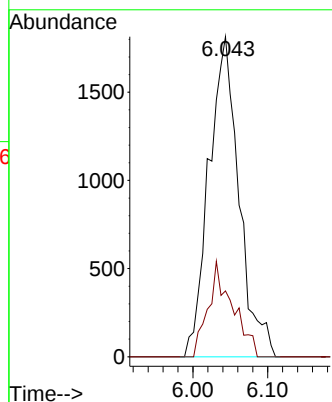

#41
Methacrylonitrile
Concen: 0.364 ug/l
RT: 5.038 min Scan# 648
Delta R.T. 0.110 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 41 Resp: 275
Ion Ratio Lower Upper
41 100
39 16.4 45.2 67.8#
67 0.0 52.6 78.8#
52 0.0 22.7 34.1#

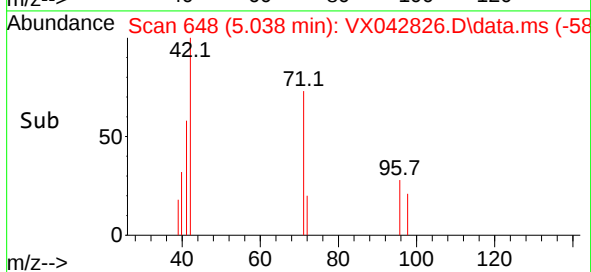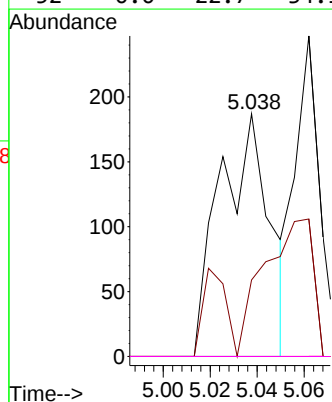



#42

1,2-Dichloroethane

Concen: 0.752 ug/l

RT: 6.092 min Scan# 81

Delta R.T. 0.006 min

Lab File: VX042826.D

Acq: 02 Aug 2024 05:25

Instrument :

MSVOA_X

ClientSampleId :





925-K1-WPO-0-0.25-073124

Tgt Ion: 62 Resp: 1194

Ion Ratio Lower Upper

62 100

98 0.0 0.0 16.0

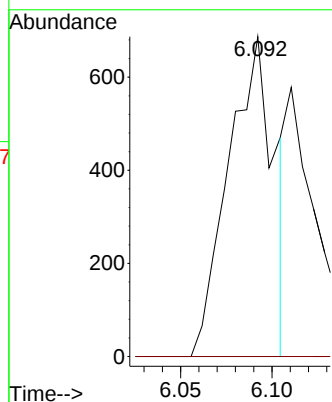

#44

Trichloroethene

Concen: 47.551 ug/l

RT: 7.129 min Scan# 991

Delta R.T. -0.000 min

Lab File: VX042826.D




Acq: 02 Aug 2024 05:25


Tgt Ion:130 Resp: 54701

Ion Ratio Lower Upper

130 100

95 95.5 0.0 204.4









#50
Toluene-d8
Concen: 48.411 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion: 98 Resp: 189751
Ion Ratio Lower Upper
98 100
100 66.7 53.1 79.7

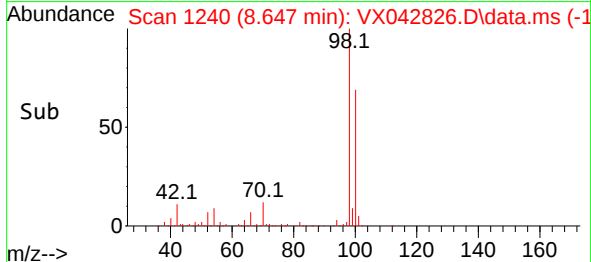

#52
Toluene
Concen: 2.754 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 92 Resp: 7852
Ion Ratio Lower Upper
92 100
91 165.3 134.2 201.2


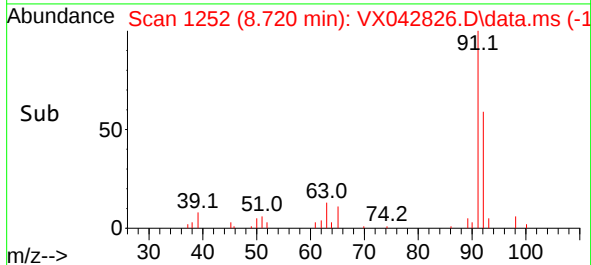




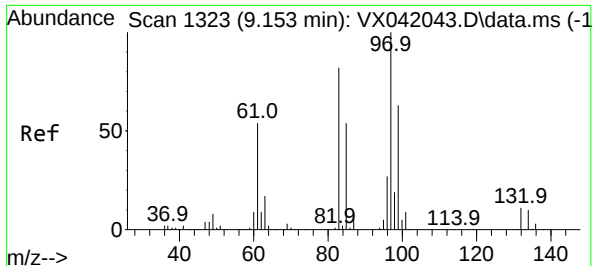

#55
 1,1,2-Trichloroethane
 Concen: 0.497 ug/l
 RT: 9.153 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: VX042826.D
 Acq: 02 Aug 2024 05:25




Instrument :
 MSVOA_X
 ClientSampleId :
 925-K1-WPO-0-0.25-073124


Tgt Ion: 97	Resp:	573	
Ion	Ratio	Lower	Upper
97	100		
83	64.8	65.8	98.8#
85	37.1	41.6	62.4#
99	65.0	47.8	71.8

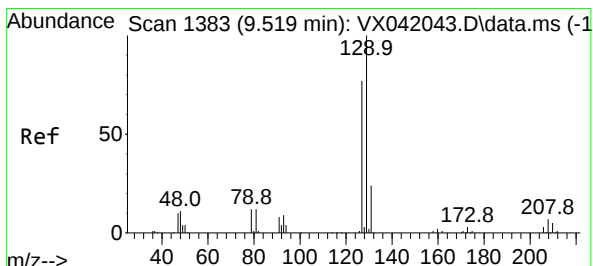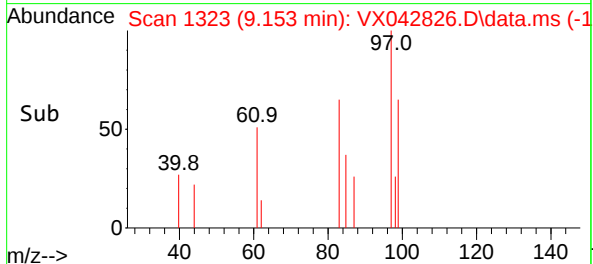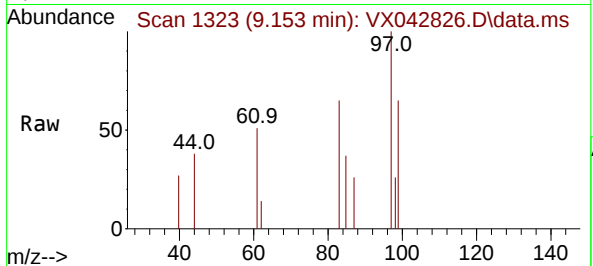

#60
 Dibromochloromethane
 Concen: 1.760 ug/l
 RT: 9.275 min Scan# 1343
 Delta R.T. -0.250 min
 Lab File: VX042826.D
 Acq: 02 Aug 2024 05:25

Tgt Ion:129	Resp:	2056	
Ion	Ratio	Lower	Upper
129	100		
127	0.0	38.8	116.4#


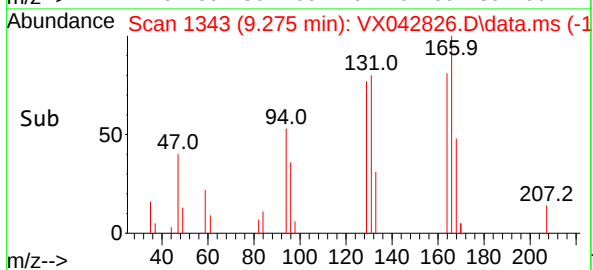

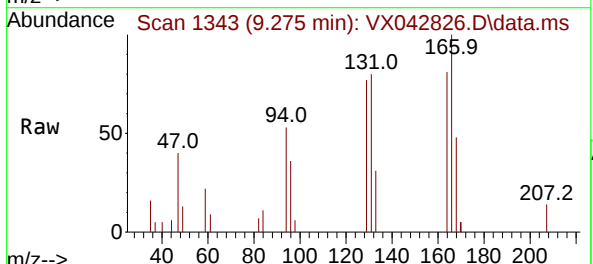




#62
4-Bromofluorobenzene
Concen: 49.838 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion: 95 Resp: 71388
Ion Ratio Lower Upper
95 100
174 72.3 0.0 135.6
176 68.3 0.0 131.0

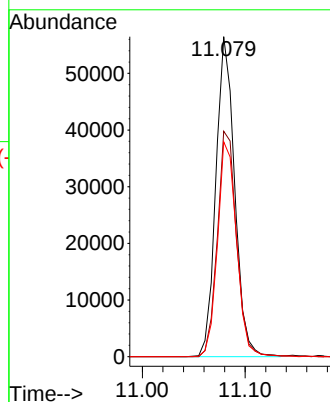

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 117 Resp: 152527
Ion Ratio Lower Upper
117 100
82 55.6 46.2 69.4
119 32.8 25.5 38.3


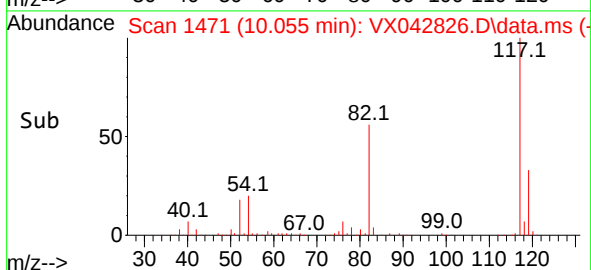
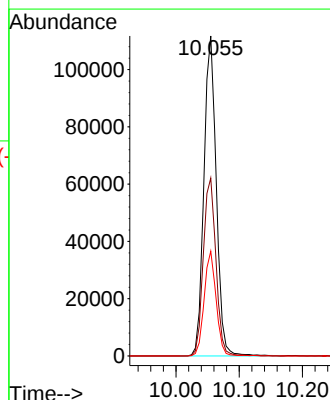





#64
Tetrachloroethene
Concen: 1.840 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25




Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124


Tgt Ion:164	Resp:	1901
Ion	Ratio	Lower Upper
164	100	
166	123.8	102.7 154.1
129	95.3	80.4 120.6
131	98.8	76.5 114.7

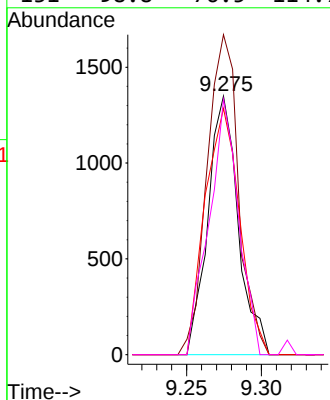

#65
Chlorobenzene
Concen: 0.587 ug/l
RT: 10.085 min Scan# 1476
Delta R.T. 0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion:112	Resp:	1976
Ion	Ratio	Lower Upper
112	100	
114	34.7	25.7 38.5

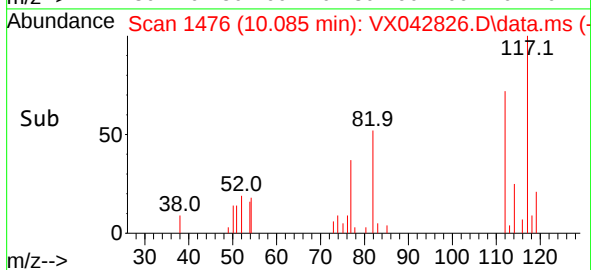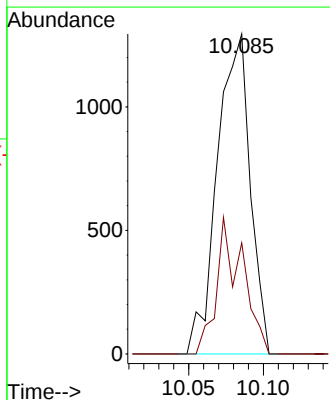



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX042826.D

Acq: 02 Aug 2024 05:25

Instrument :

MSVOA_X

ClientSampleId :

925-K1-WPO-0-0.25-073124





Tgt Ion:152 Resp: 64635

Ion Ratio Lower Upper

152 100

115 65.1 43.3 129.9

150 160.5 0.0 345.0

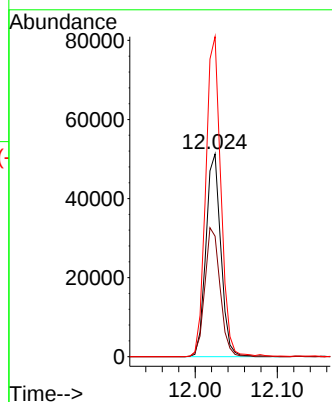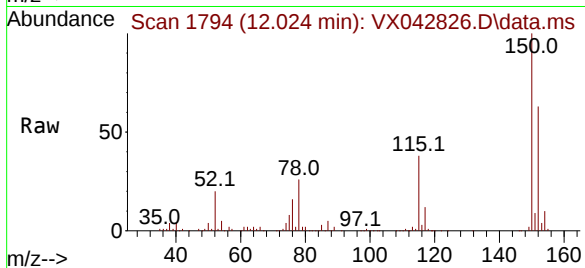

#76

1,2,3-Trichloropropane

Concen: 25.900 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX042826.D




Acq: 02 Aug 2024 05:25


Tgt Ion: 75 Resp: 38252

Ion Ratio Lower Upper

75 100

77 1.0 19.1 57.5#


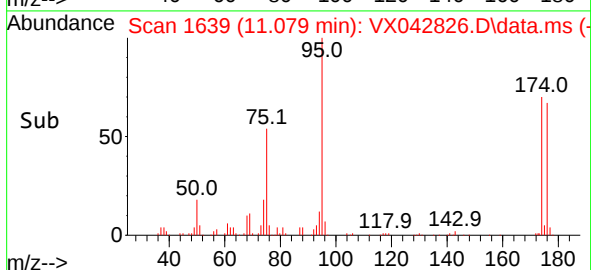

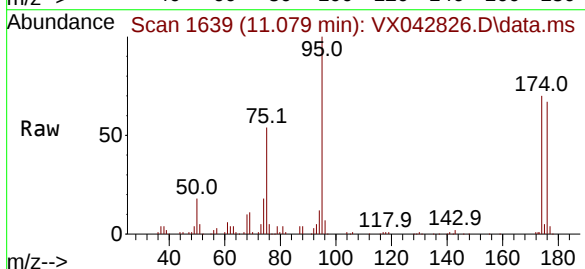




#81
trans-1,4-Dichloro-2-butene
Concen: 76.658 ug/l
RT: 11.079 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Instrument :
MSVOA_X
ClientSampleId :
925-K1-WPO-0-0.25-073124

Tgt Ion: 75 Resp: 38252
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

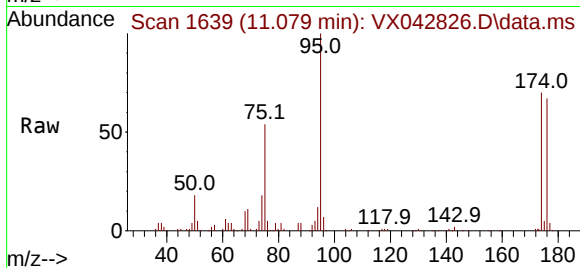

#86
p-Isopropyltoluene
Concen: 0.232 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. 0.006 min
Lab File: VX042826.D
Acq: 02 Aug 2024 05:25

Tgt Ion: 119 Resp: 1010
Ion Ratio Lower Upper
119 100
134 27.9 12.8 38.3
91 38.0 13.1 39.3

