

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
 Data File : VX042820.D
 Acq On : 02 Aug 2024 03:05
 Operator : JC/MD
 Sample : P3426-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 927-K1-WS-073124

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
 Title : SW846 8260

Signal : TIC: VX042820.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	13	rBV	39741	34067	8.42%	1.406%
2	1.374	41	47	51	rBV	11982	14504	3.59%	0.599%
3	1.648	85	92	97	rVB6	5919	13328	3.30%	0.550%
4	2.130	166	171	179	rVB3	11051	17606	4.35%	0.727%
5	2.319	196	202	210	rBV3	12358	22561	5.58%	0.931%
6	4.483	548	557	575	rBV	51656	142289	35.18%	5.873%
7	5.385	695	705	719	rBV2	53675	154958	38.31%	6.396%
8	5.550	723	732	744	rBV	77127	212681	52.59%	8.779%
9	5.958	790	799	811	rBV	56416	153123	37.86%	6.321%
10	6.757	921	930	950	rBV	128159	312207	77.19%	12.887%
11	7.129	983	991	1001	rBV3	16774	37162	9.19%	1.534%
12	8.647	1234	1240	1248	rBV	260762	404447	100.00%	16.695%
13	8.720	1248	1252	1261	rVB	6059	12065	2.98%	0.498%
14	10.055	1465	1471	1487	rBV	258178	359617	88.92%	14.844%
15	11.079	1634	1639	1655	rBV	192899	250216	61.87%	10.328%
16	12.024	1788	1794	1804	rBV	214993	281795	69.67%	11.632%




Sum of corrected areas: 2422626

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042820.D
Acq On : 02 Aug 2024 03:05
Operator : JC/MD
Sample : P3426-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WS-073124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

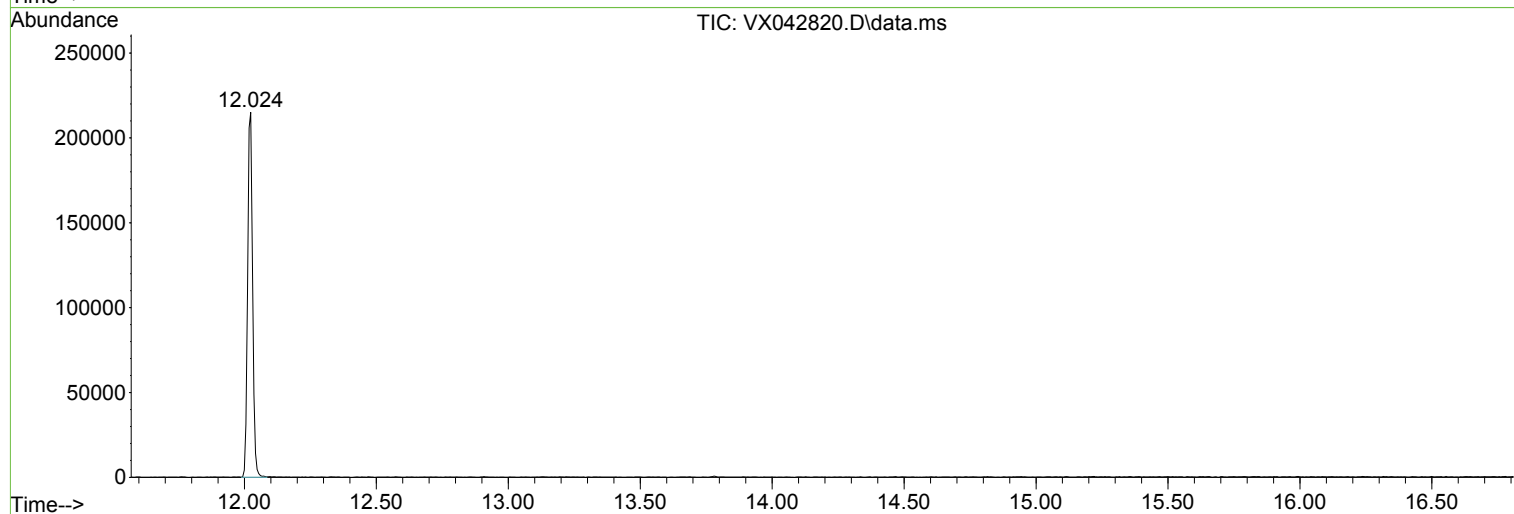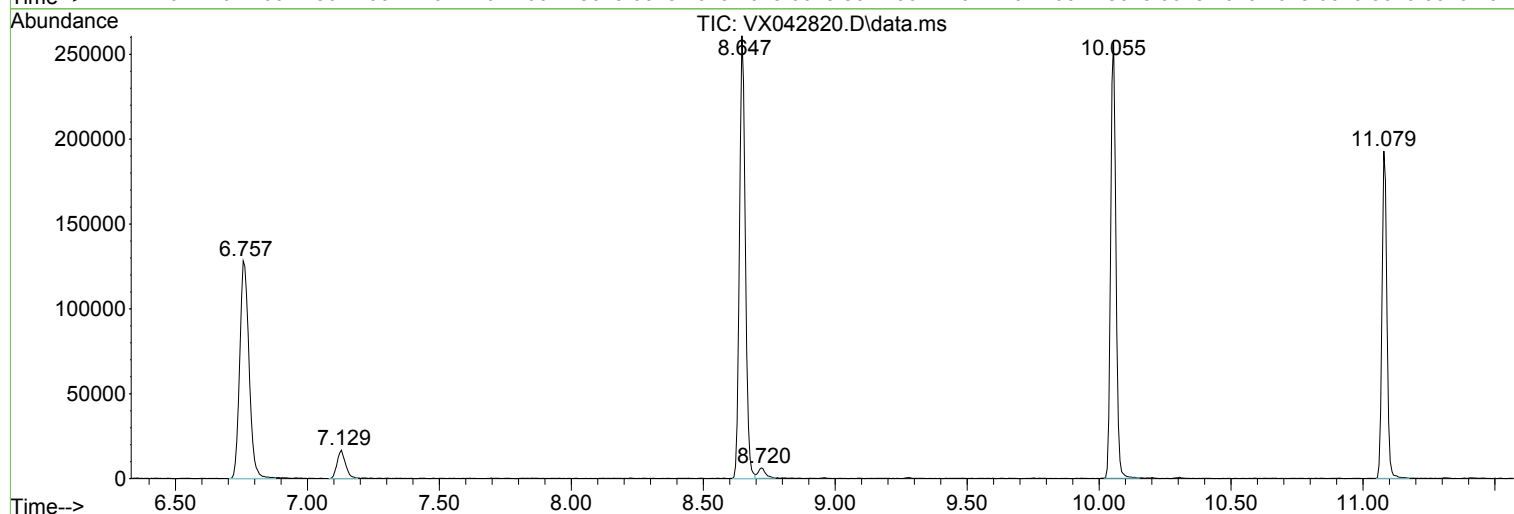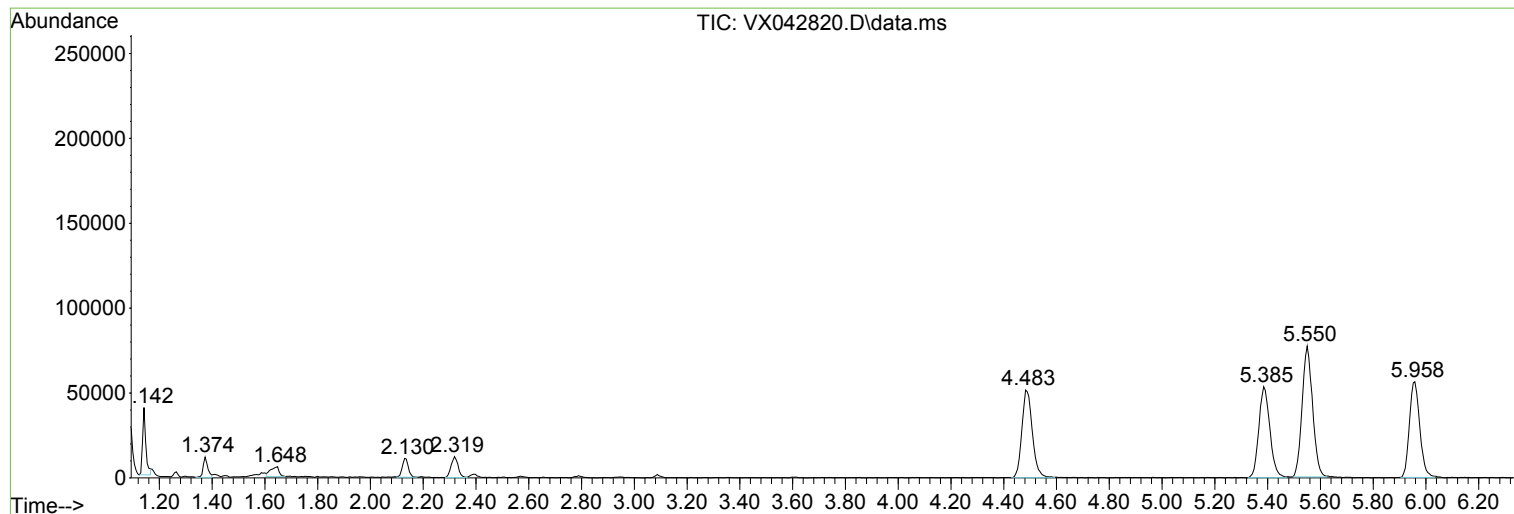

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042820.D
Acq On : 02 Aug 2024 03:05
Operator : JC/MD
Sample : P3426-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WS-073124










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethene, chlorotrifluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.142	8.01 ug/l	34067	Pentafluorobenzene	5.550

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethene, chlorotrifluoro-	116	C2ClF3	000079-38-9	95
2			5-Chloro-1-methylimidazole	116	C4H5ClN2	000872-49-1	17
3			1,2,5-Thiadiazole-3,4-diamine	116	C2H4N4S	055904-36-4	5
4			1-Propene, 1-(ethylthio)-2-methyl-	116	C6H12S	027482-14-0	5
5			3-Ethylthiolane	116	C6H12S	062184-67-2	5

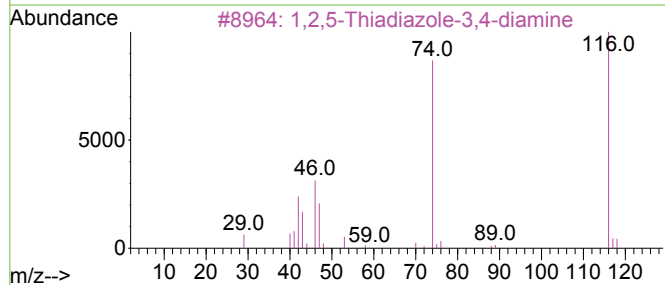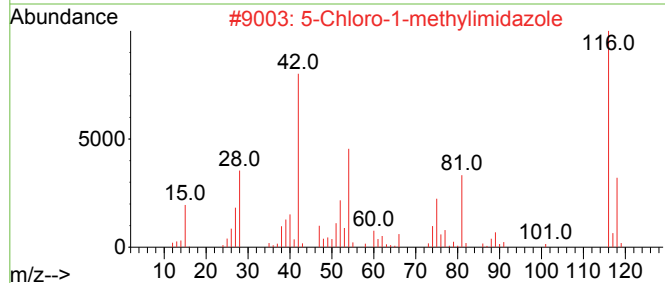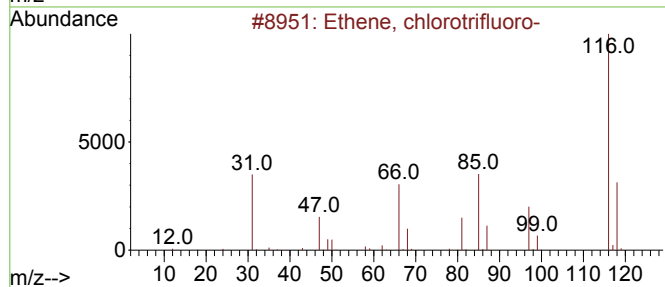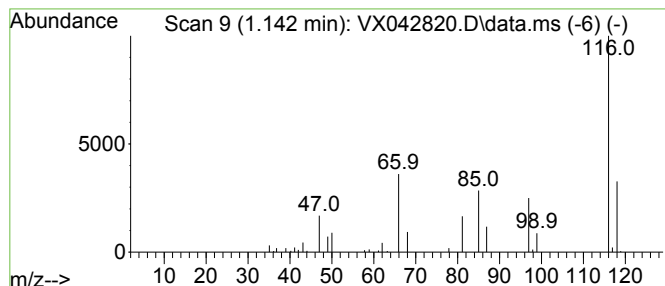

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042820.D
Acq On : 02 Aug 2024 03:05
Operator : JC/MD
Sample : P3426-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WS-073124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, chlorot...	1.142	8.0	ug/l	34067	1	5.550	212681	50.0