

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
 Data File : VX042822.D
 Acq On : 02 Aug 2024 03:52
 Operator : JC/MD
 Sample : P3430-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 927-K1-WPO-0-0.25-073124

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
 Title : SW846 8260

Signal : TIC: VX042822.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	12	rBV	21757	18047	5.63%	0.973%
2	1.172	12	14	18	rVB2	4389	4899	1.53%	0.264%
3	1.374	43	47	52	rBV	8093	9974	3.11%	0.538%
4	1.599	69	84	85	rBV4	2917	7134	2.22%	0.385%
5	1.636	85	90	95	rVB6	5613	9139	2.85%	0.493%
6	2.130	167	171	178	rVB3	7224	11077	3.45%	0.597%
7	2.392	207	214	221	rVB	1782	3398	1.06%	0.183%
8	4.489	547	558	569	rBV4	5749	16065	5.01%	0.866%
9	5.025	640	646	651	rBV4	2654	7214	2.25%	0.389%
10	5.385	695	705	718	rBV	46227	134252	41.85%	7.240%
11	5.550	721	732	747	rVV	58385	164082	51.15%	8.849%
12	5.958	790	799	811	rBV2	48754	134166	41.82%	7.236%
13	6.757	922	930	944	rBV	103068	249138	77.66%	13.436%
14	7.135	985	992	1002	rVB4	2741	6395	1.99%	0.345%
15	8.647	1233	1240	1248	rBV	203977	320804	100.00%	17.301%
16	8.720	1248	1252	1261	rVB	8809	15442	4.81%	0.833%
17	10.055	1465	1471	1482	rBV	213191	293590	91.52%	15.834%
18	11.079	1634	1639	1649	rBV	161961	208342	64.94%	11.236%
19	12.018	1788	1793	1802	rBV	184397	236993	73.87%	12.781%
20	13.121	1970	1974	1978	rBV3	3078	4066	1.27%	0.219%




Sum of corrected areas: 1854217

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042822.D
Acq On : 02 Aug 2024 03:52
Operator : JC/MD
Sample : P3430-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

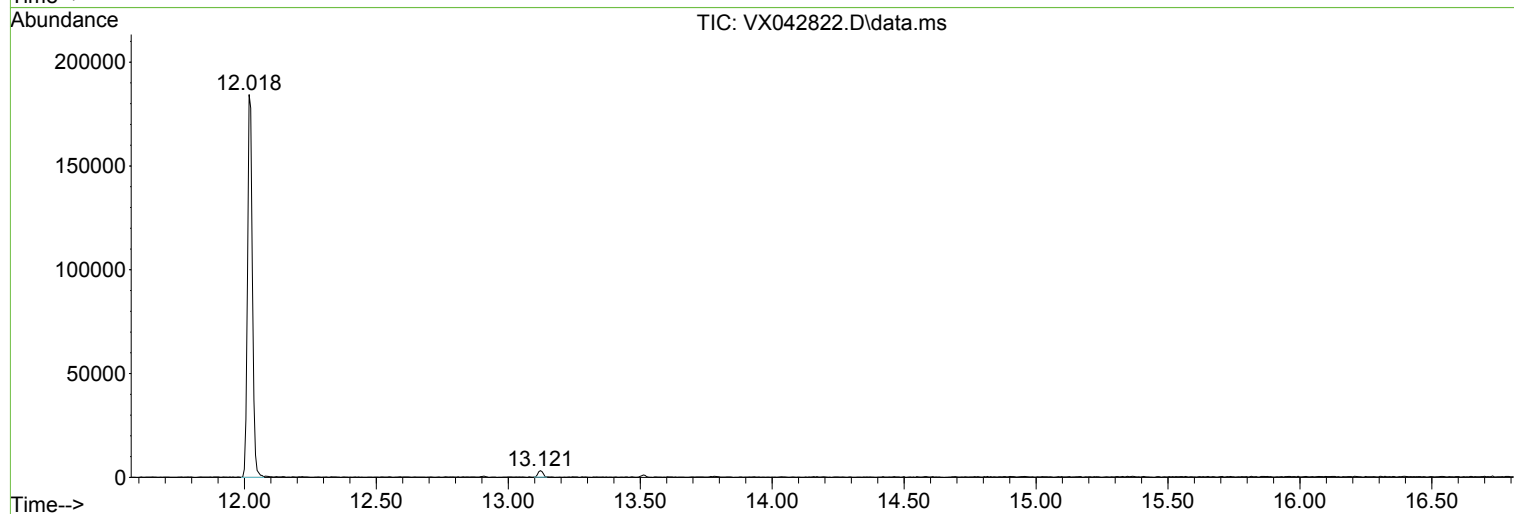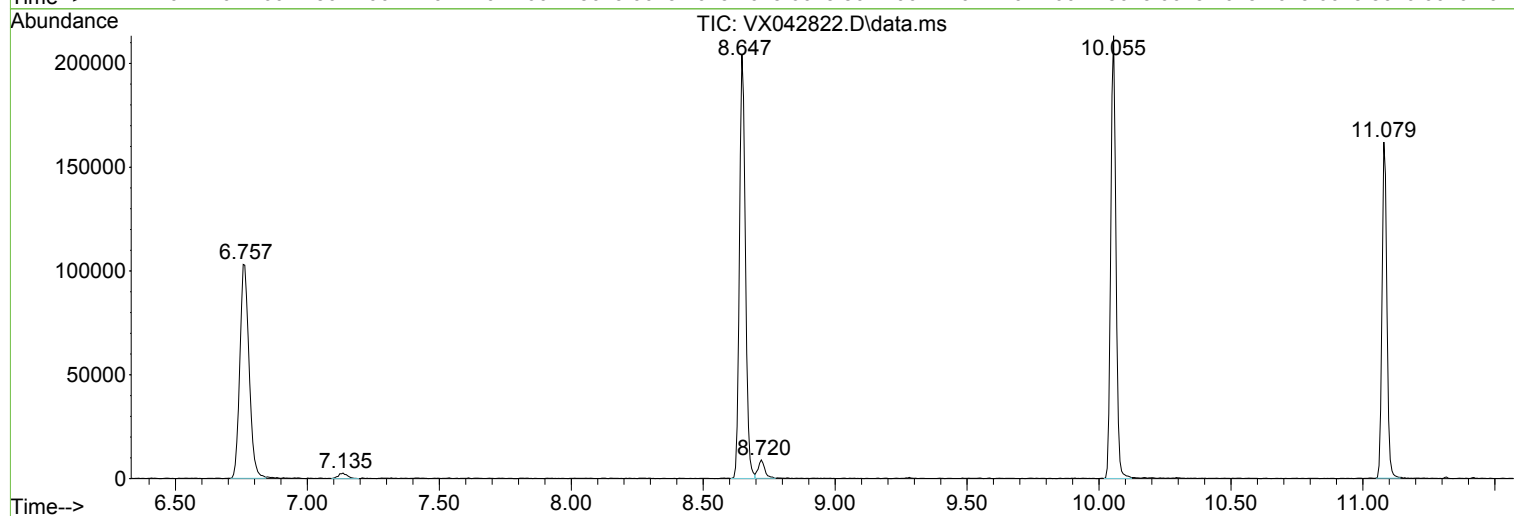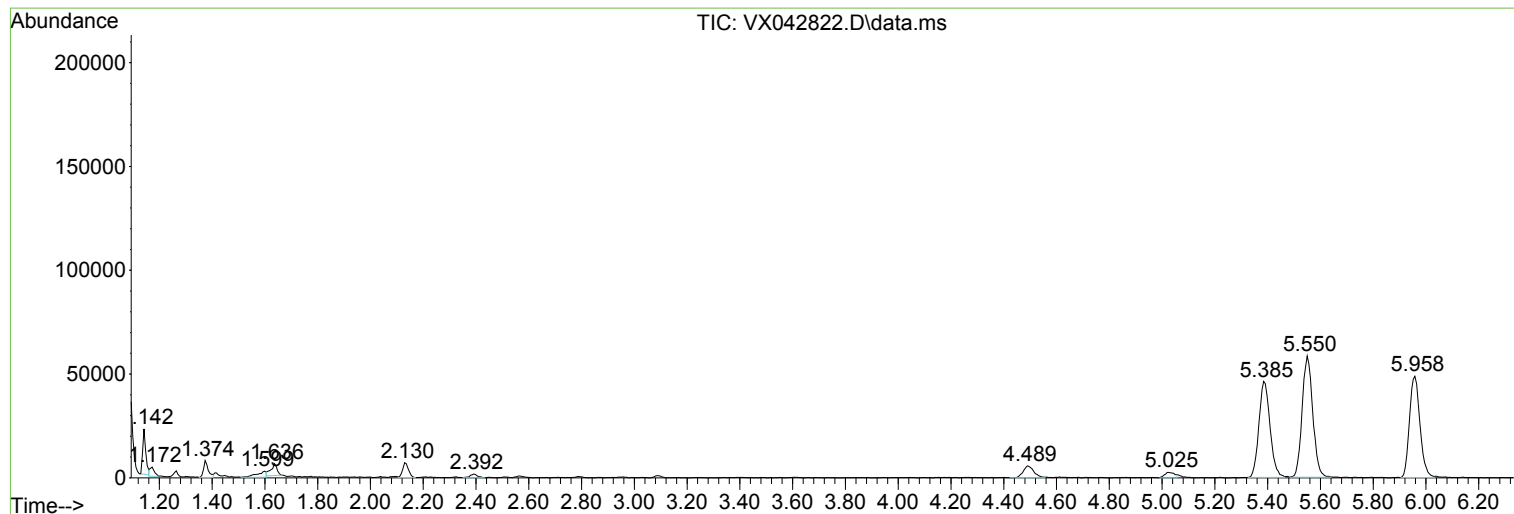

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042822.D
Acq On : 02 Aug 2024 03:52
Operator : JC/MD
Sample : P3430-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethene, chlorotrifluoro- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.142	5.50 ug/l	18047	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethene, chlorotrifluoro-	116	C2ClF3	000079-38-9	96
2			Pyrazole, 4-chloro-3-methyl-	116	C4H5ClN2	015878-08-7	9
3			1,2,5-Thiadiazole-3,4-diamine	116	C2H4N4S	055904-36-4	9
4			5-Chloro-1-methylimidazole	116	C4H5ClN2	000872-49-1	9
5			1-Propene, 1-(ethylthio)-2-methyl-	116	C6H12S	027482-14-0	5

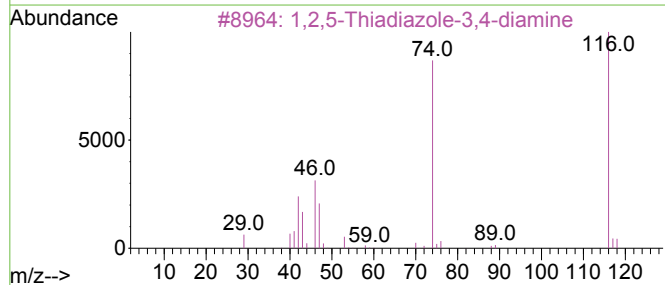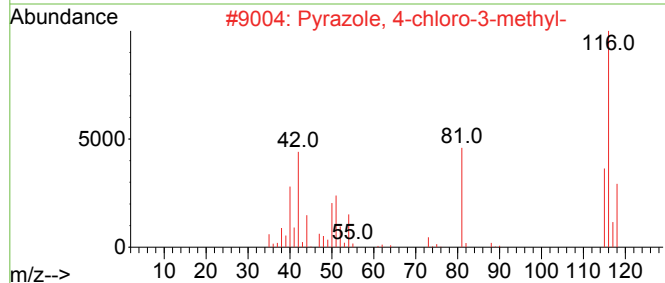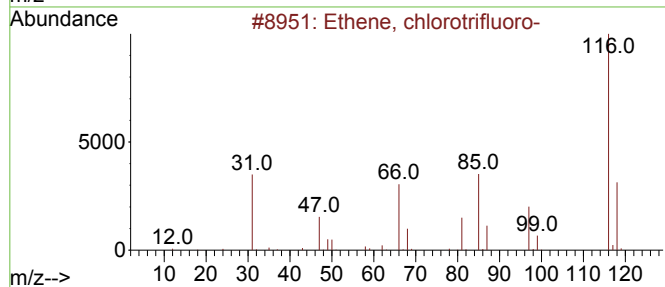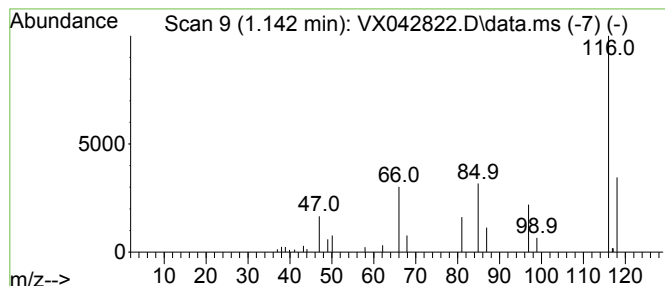

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX080124\
Data File : VX042822.D
Acq On : 02 Aug 2024 03:52
Operator : JC/MD
Sample : P3430-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
927-K1-WPO-0-0.25-073124

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X080124W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethene, chlorot...	1.142	5.5	ug/l	18047	1	5.556	164082	50.0